

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031379.D
 Acq On : 06 Jun 2023 16:40
 Operator : SY/MD
 Sample : 02990-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C38

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031379.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	42978	47578	8.60%	1.160%
2	1.352	92	97	104	rBV	17449	19840	3.59%	0.484%
3	1.387	104	108	115	rVB2	8171	8572	1.55%	0.209%
4	1.532	146	153	164	rVB	48939	57528	10.40%	1.402%
5	2.063	306	318	330	rBV	85822	127467	23.04%	3.107%
6	2.124	330	337	350	rVB3	6441	13324	2.41%	0.325%
7	2.709	505	519	537	rBV3	11133	23920	4.32%	0.583%
8	3.802	848	859	893	rBV	81566	281234	50.84%	6.855%
9	4.259	986	1001	1024	rBV2	76391	202759	36.66%	4.942%
10	4.966	1202	1221	1246	rBV3	159510	428013	77.38%	10.433%
11	5.545	1388	1401	1422	rBV	112012	234828	42.45%	5.724%
12	5.841	1480	1493	1515	rBV6	22801	54086	9.78%	1.318%
13	5.998	1529	1542	1564	rBV2	105722	226417	40.93%	5.519%
14	6.921	1818	1829	1856	rBV2	41215	86584	15.65%	2.111%
15	7.252	1921	1932	1957	rBV2	154037	283660	51.28%	6.914%
16	7.561	2018	2028	2050	rBV2	27012	54786	9.90%	1.335%
17	7.911	2120	2137	2160	rBV	193538	342507	61.92%	8.349%
18	8.034	2165	2175	2212	rBV2	252535	553124	100.00%	13.483%
19	8.792	2397	2411	2433	rBV	187912	327437	59.20%	7.982%
20	10.162	2825	2837	2858	rVB	87009	142772	25.81%	3.480%
21	10.332	2881	2890	2899	rBV3	8454	12807	2.32%	0.312%
22	11.191	3144	3157	3185	rBV	176705	289687	52.37%	7.061%
23	11.567	3264	3274	3289	rBV	179014	283515	51.26%	6.911%




Sum of corrected areas: 4102445

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031379.D
Acq On : 06 Jun 2023 16:40
Operator : SY/MD
Sample : 02990-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

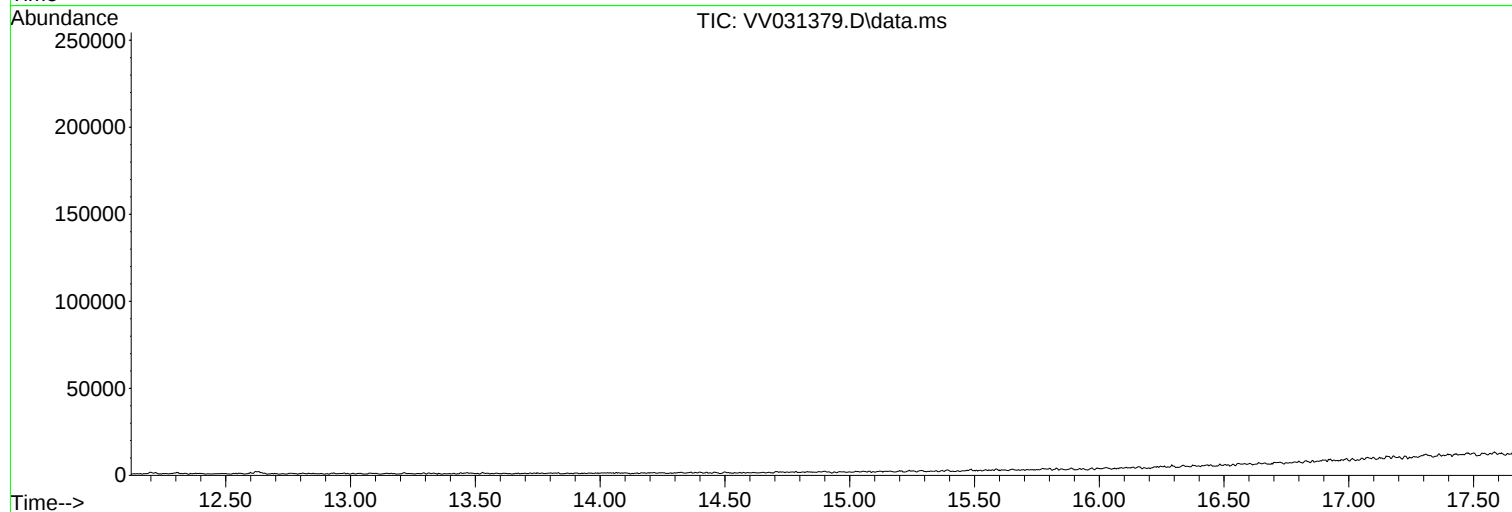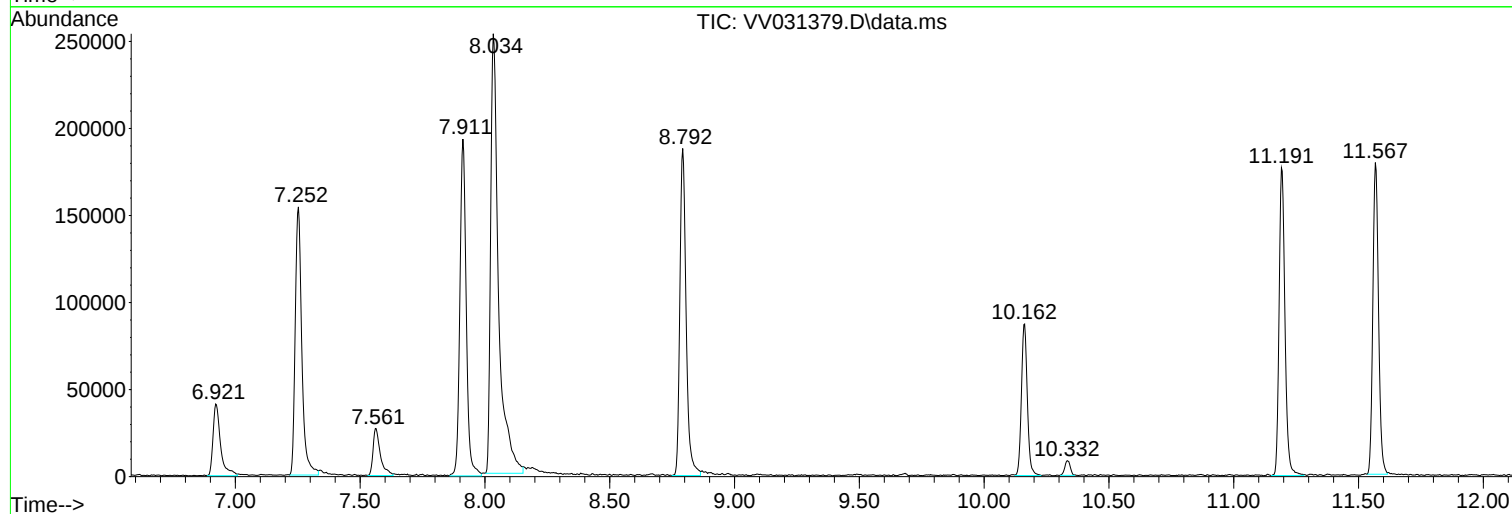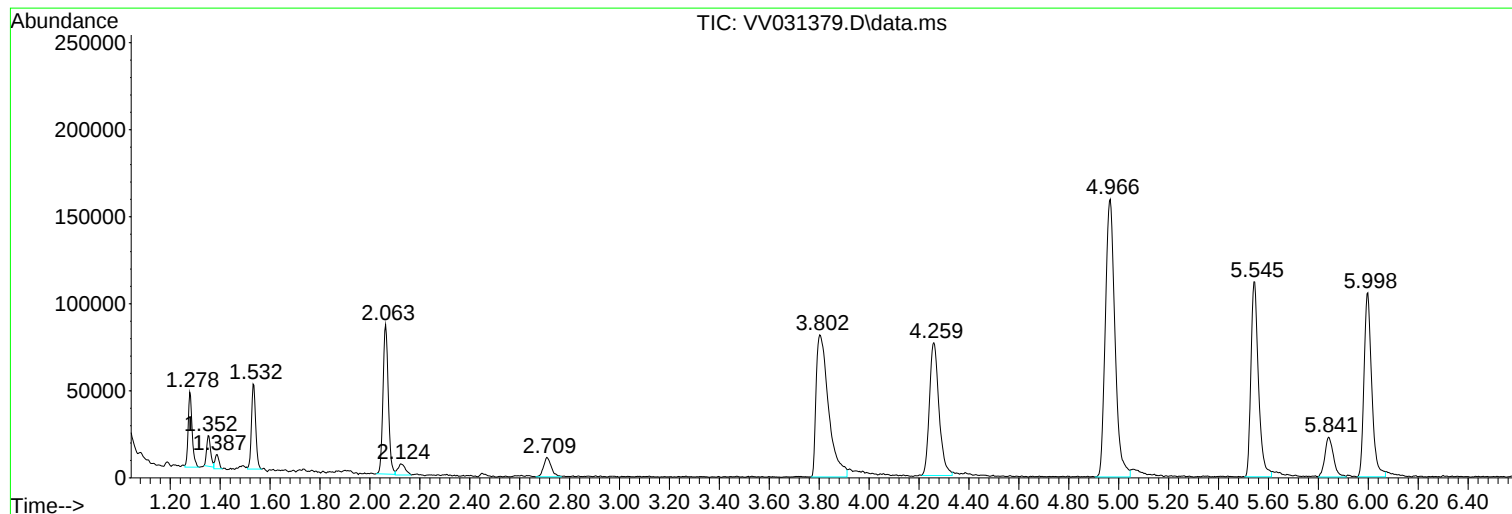

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031379.D
Acq On : 06 Jun 2023 16:40
Operator : SY/MD
Sample : 02990-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031379.D
Acq On : 06 Jun 2023 16:40
Operator : SY/MD
Sample : 02990-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C38

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc