

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031380.D
 Acq On : 06 Jun 2023 17:02
 Operator : SY/MD
 Sample : 02990-11
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C39

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV031380.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	40458	46392	8.17%	1.066%
2	1.532	147	153	167	rVB	50221	61356	10.81%	1.410%
3	2.063	308	318	330	rBV	81761	121752	21.45%	2.798%
4	2.127	331	338	351	rVB3	7427	14336	2.53%	0.329%
5	2.712	506	520	534	rBV3	13300	28770	5.07%	0.661%
6	3.802	849	859	897	rBV2	75497	242220	42.67%	5.567%
7	4.259	986	1001	1024	rBV	80065	207505	36.55%	4.769%
8	4.963	1205	1220	1246	rBV2	168601	448000	78.91%	10.296%
9	5.542	1386	1400	1423	rBV	109398	235055	41.40%	5.402%
10	5.838	1480	1492	1511	rBV9	14667	37134	6.54%	0.853%
11	5.995	1526	1541	1560	rBV	113143	238535	42.02%	5.482%
12	6.921	1820	1829	1850	rBV	45628	88343	15.56%	2.030%
13	7.252	1919	1932	1950	rBV	160397	293136	51.63%	6.737%
14	7.561	2018	2028	2042	rBV2	30732	58038	10.22%	1.334%
15	7.912	2119	2137	2157	rBV	322130	563345	99.23%	12.946%
16	8.034	2165	2175	2209	rBV2	263333	567716	100.00%	13.047%
17	8.793	2395	2411	2437	rBV	189803	334311	58.89%	7.683%
18	10.159	2821	2836	2853	rBV	93830	151527	26.69%	3.482%
19	10.333	2881	2890	2902	rBV3	8222	11864	2.09%	0.273%
20	11.191	3143	3157	3180	rBV	184045	295313	52.02%	6.787%
21	11.567	3263	3274	3294	rBV	190530	306734	54.03%	7.049%




Sum of corrected areas: 4351382

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031380.D
Acq On : 06 Jun 2023 17:02
Operator : SY/MD
Sample : 02990-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

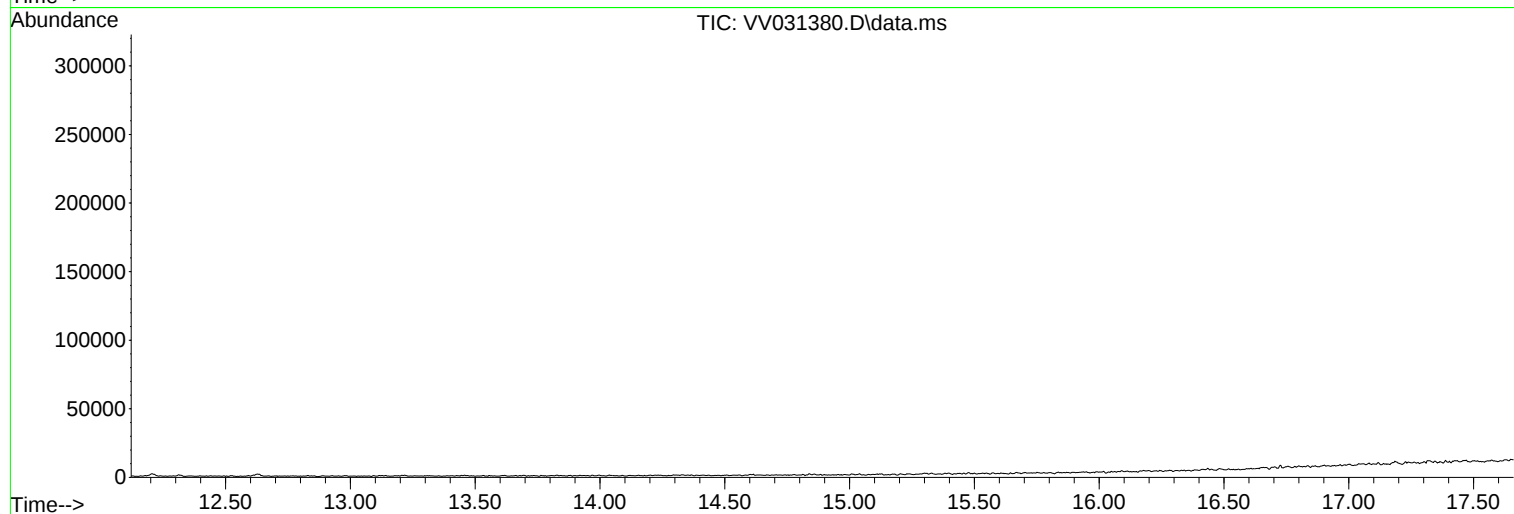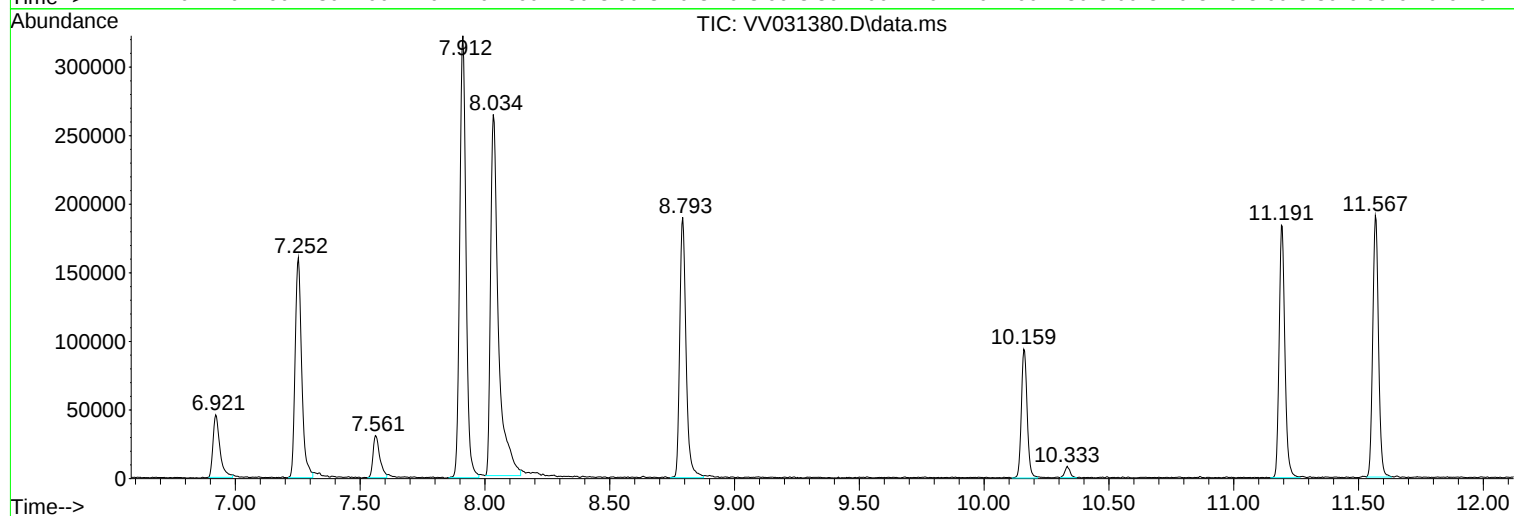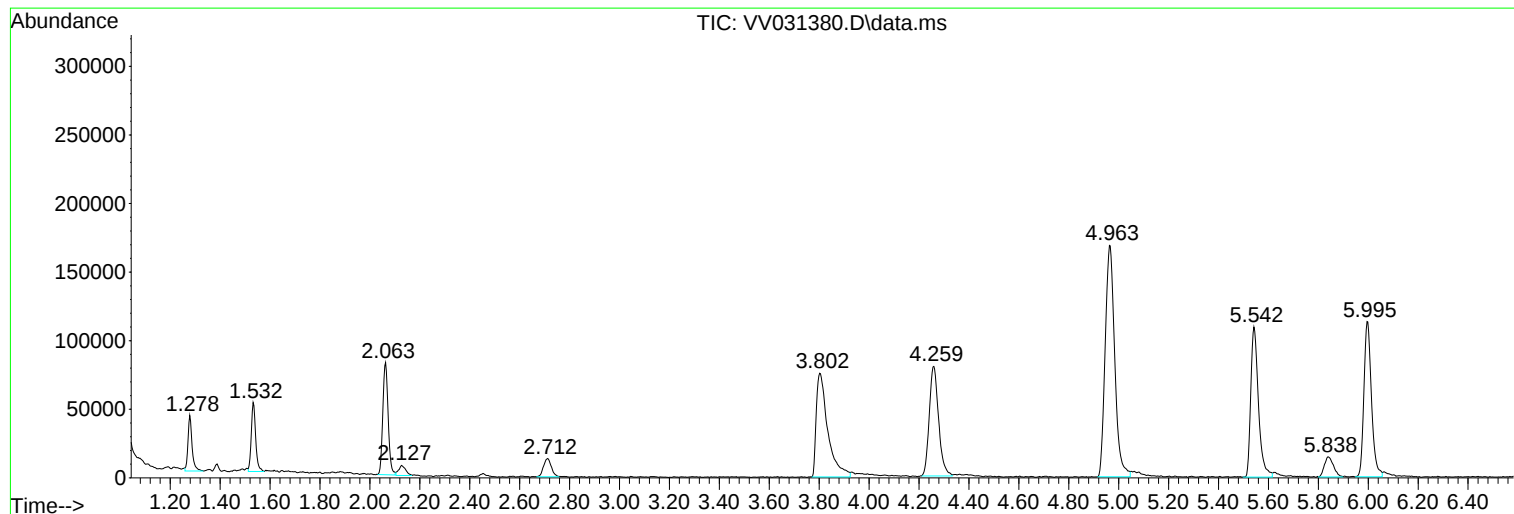

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031380.D
Acq On : 06 Jun 2023 17:02
Operator : SY/MD
Sample : 02990-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031380.D
Acq On : 06 Jun 2023 17:02
Operator : SY/MD
Sample : 02990-11
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C39

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc