

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031381.D
 Acq On : 06 Jun 2023 17:27
 Operator : SY/MD
 Sample : 02990-12 4X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C43

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031381.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	70702	74527	8.86%	1.425%
2	1.532	146	153	167	rVB	66541	79499	9.45%	1.520%
3	2.060	305	317	331	rBV	134148	201942	24.00%	3.861%
4	2.452	430	439	451	rVB3	7689	13112	1.56%	0.251%
5	3.818	851	864	906	rBV	66292	259753	30.87%	4.966%
6	4.256	985	1000	1028	rBV2	97959	254460	30.24%	4.865%
7	4.966	1204	1221	1244	rBV3	203685	530698	63.06%	10.146%
8	5.542	1387	1400	1419	rBV	157766	329353	39.14%	6.296%
9	5.841	1478	1493	1505	rBV10	11824	29422	3.50%	0.562%
10	5.995	1526	1541	1559	rBV2	130257	274285	32.59%	5.244%
11	6.921	1817	1829	1851	rBV3	47747	97896	11.63%	1.872%
12	7.249	1920	1931	1947	rBV	207550	373922	44.43%	7.148%
13	7.561	2015	2028	2051	rBV2	31790	63227	7.51%	1.209%
14	7.911	2122	2137	2164	rBV	479542	841531	100.00%	16.088%
15	8.037	2166	2176	2211	rVV2	239973	531777	63.19%	10.166%
16	8.792	2399	2411	2433	rBV	244557	421866	50.13%	8.065%
17	10.159	2824	2836	2855	rBV	89594	147710	17.55%	2.824%
18	10.333	2879	2890	2901	rBV2	5528	8857	1.05%	0.169%
19	11.191	3146	3157	3177	rBV	221043	360360	42.82%	6.889%
20	11.567	3262	3274	3292	rBV	209671	336640	40.00%	6.436%




Sum of corrected areas: 5230837

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031381.D
Acq On : 06 Jun 2023 17:27
Operator : SY/MD
Sample : 02990-12 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

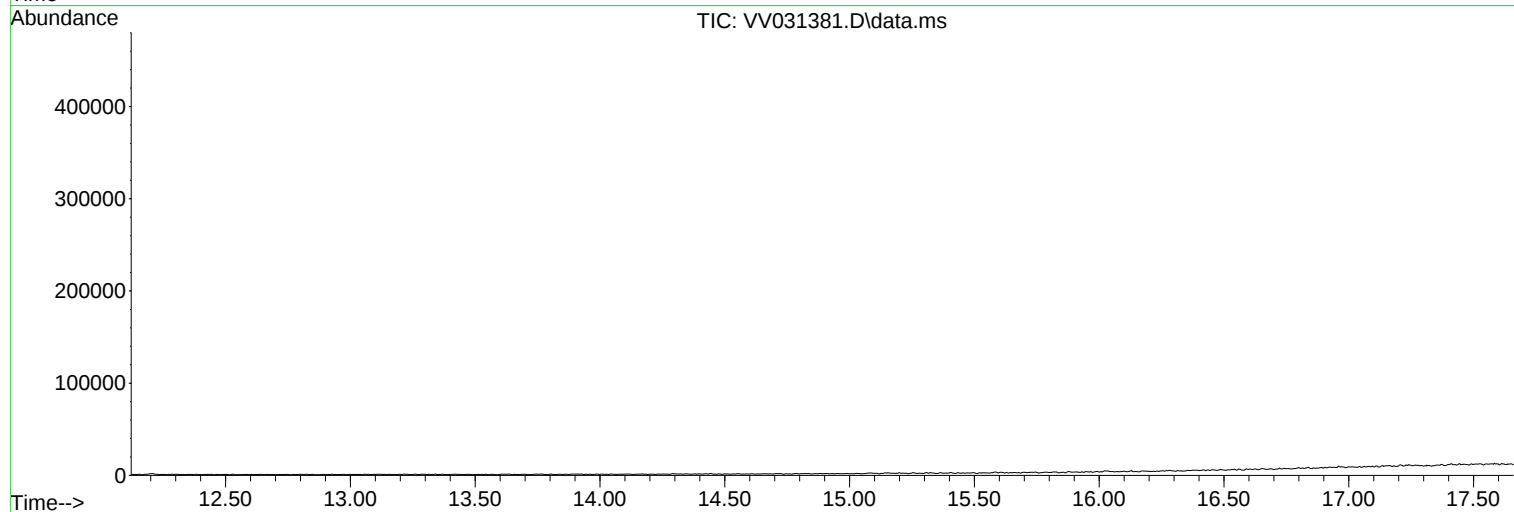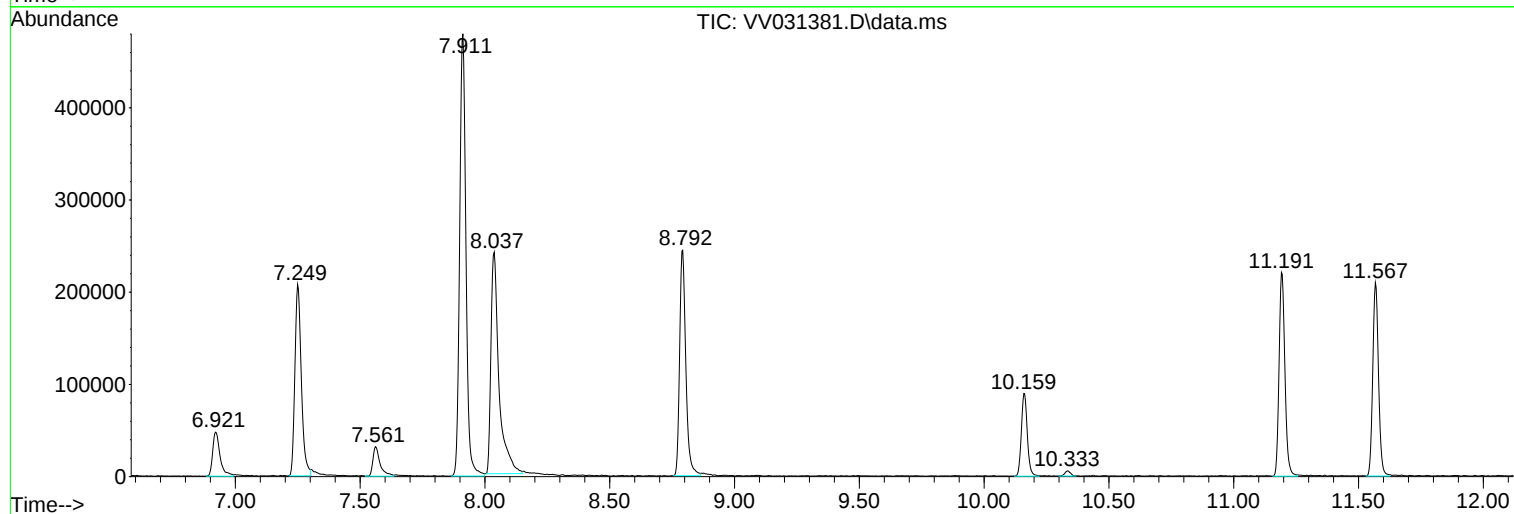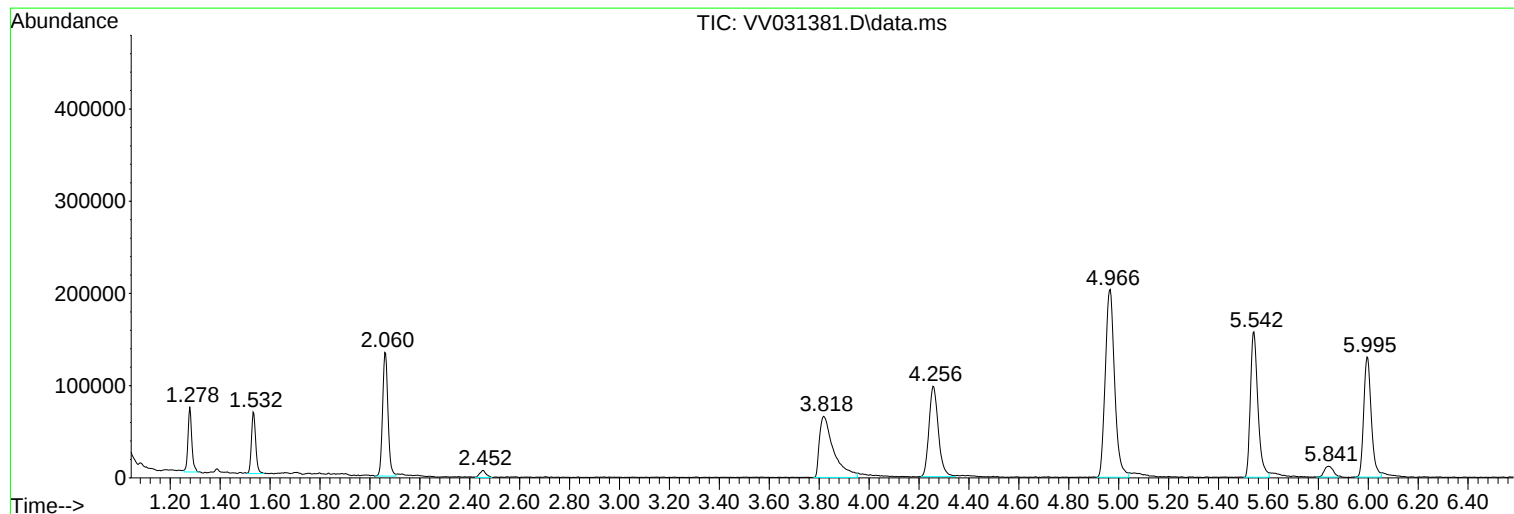

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031381.D
Acq On : 06 Jun 2023 17:27
Operator : SY/MD
Sample : 02990-12 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031381.D
Acq On : 06 Jun 2023 17:27
Operator : SY/MD
Sample : 02990-12 4X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C43

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc