

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
 Data File : VV031384.D
 Acq On : 06 Jun 2023 18:40
 Operator : SY/MD
 Sample : VIBLK303
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK303

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV031384.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	67	74	85	rVB	64676	70041	13.85%	1.737%
2	1.532	146	153	166	rVB	63775	76265	15.08%	1.891%
3	2.060	307	317	337	rVB	133887	198229	39.21%	4.916%
4	2.449	430	438	455	rVB3	12179	23439	4.64%	0.581%
5	3.828	854	867	903	rBV2	39834	181306	35.86%	4.497%
6	4.256	984	1000	1023	rBV2	91249	239729	47.42%	5.945%
7	4.963	1205	1220	1248	rBV2	193828	505571	100.00%	12.539%
8	5.542	1382	1400	1420	rBV	148857	317146	62.73%	7.865%
9	5.838	1480	1492	1504	rBV	6112	13403	2.65%	0.332%
10	5.995	1524	1541	1574	rBV	120563	265610	52.54%	6.587%
11	6.921	1818	1829	1856	rBV2	45475	93070	18.41%	2.308%
12	7.249	1920	1931	1953	rBV	199903	361723	71.55%	8.971%
13	7.561	2017	2028	2047	rBV	26728	56097	11.10%	1.391%
14	8.037	2166	2176	2223	rBV2	181688	445252	88.07%	11.043%
15	8.792	2399	2411	2444	rBV	232025	407480	80.60%	10.106%
16	10.159	2826	2836	2850	rBV2	77703	127272	25.17%	3.156%
17	11.191	3145	3157	3182	rBV	206993	340389	67.33%	8.442%
18	11.567	3262	3274	3297	rBV	190091	310100	61.34%	7.691%




Sum of corrected areas: 4032122

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031384.D
Acq On : 06 Jun 2023 18:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

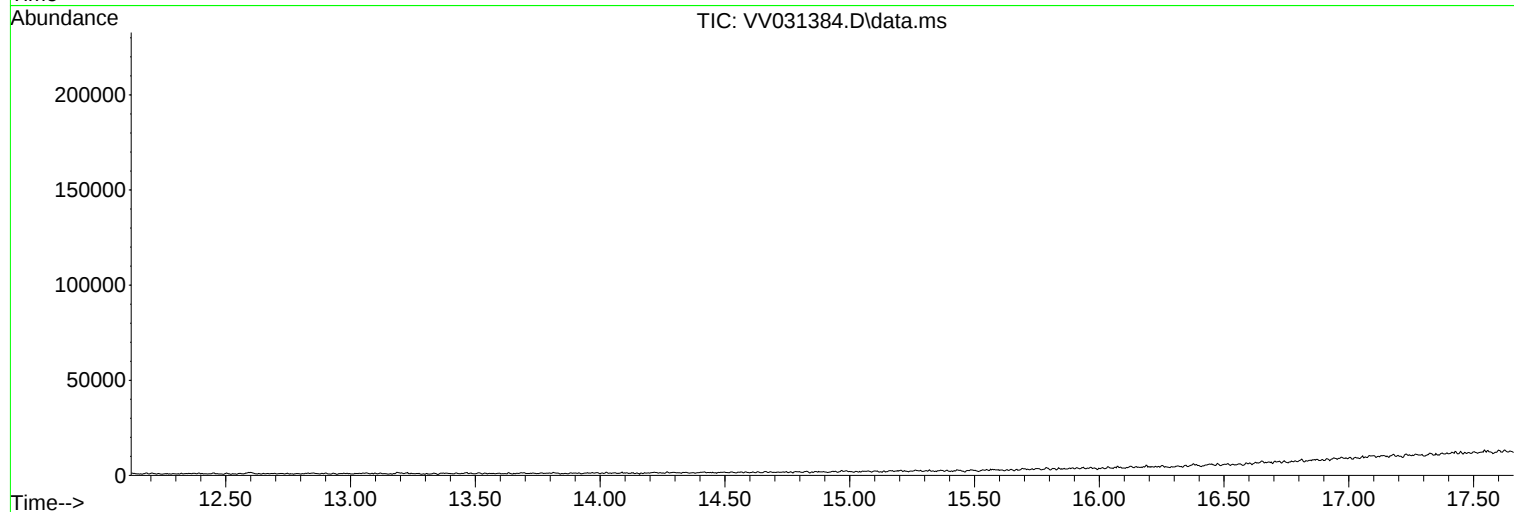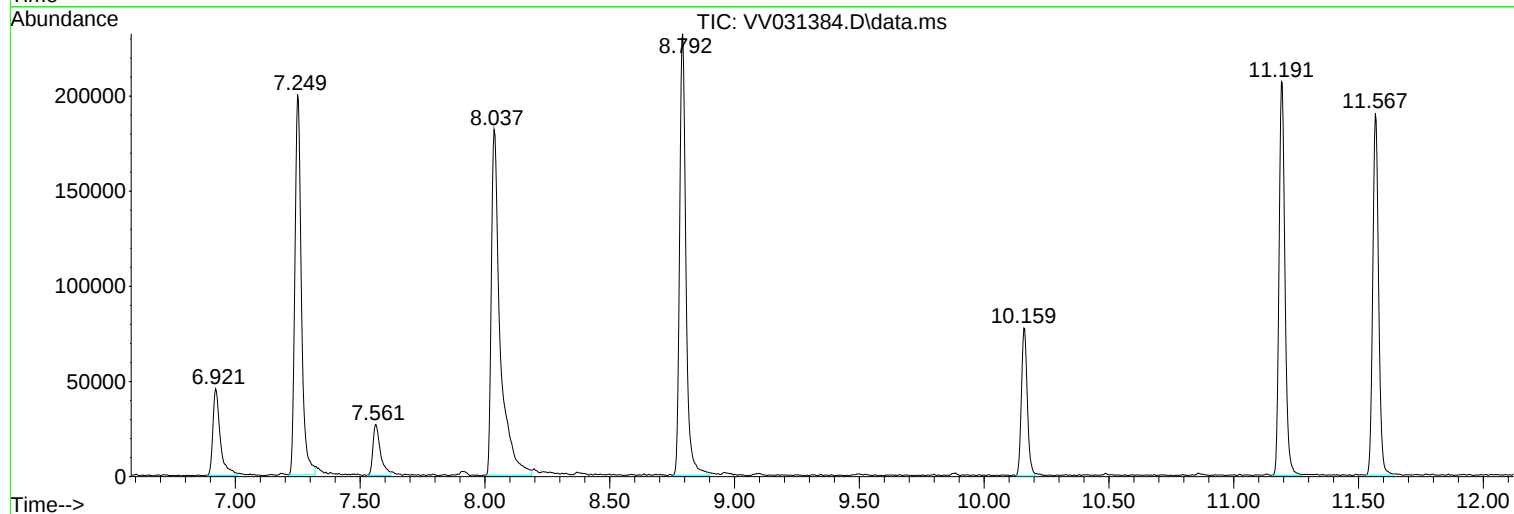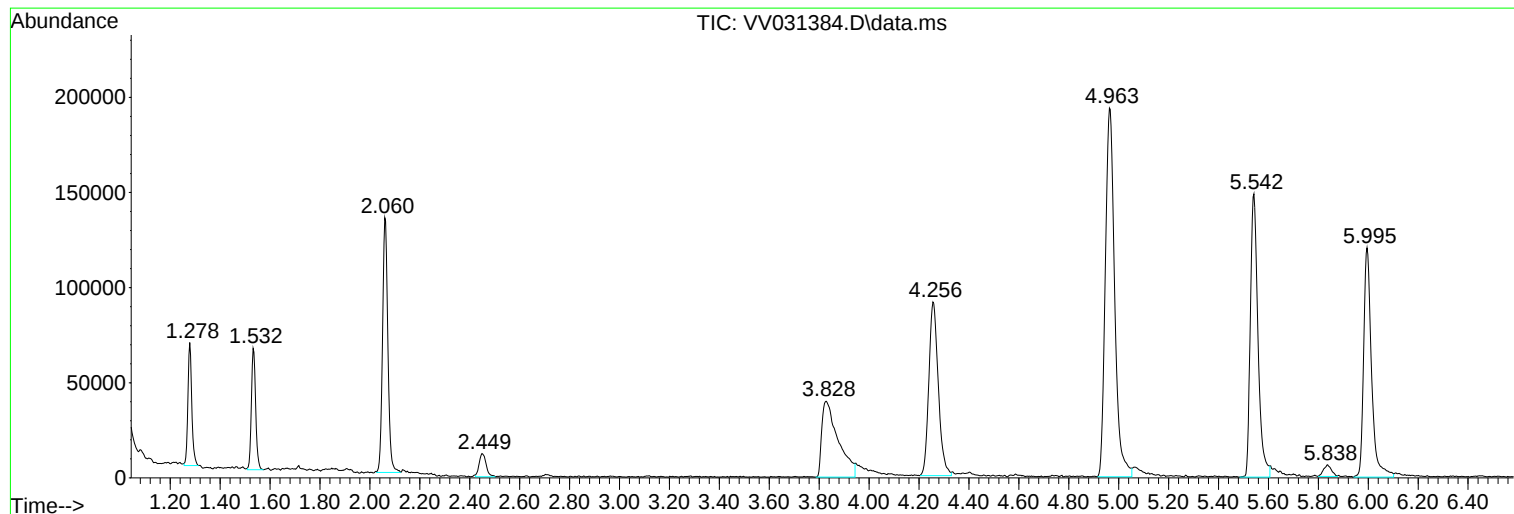

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031384.D
Acq On : 06 Jun 2023 18:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031384.D
Acq On : 06 Jun 2023 18:40
Operator : SY/MD
Sample : VIBLK303
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK303

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc