


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060623\
Data File : VV031361.D
Acq On : 06 Jun 2023 08:59
Operator : SY/MD
Sample : BFB271
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB271

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060123WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Wed Jun 07 01:59:39 2023

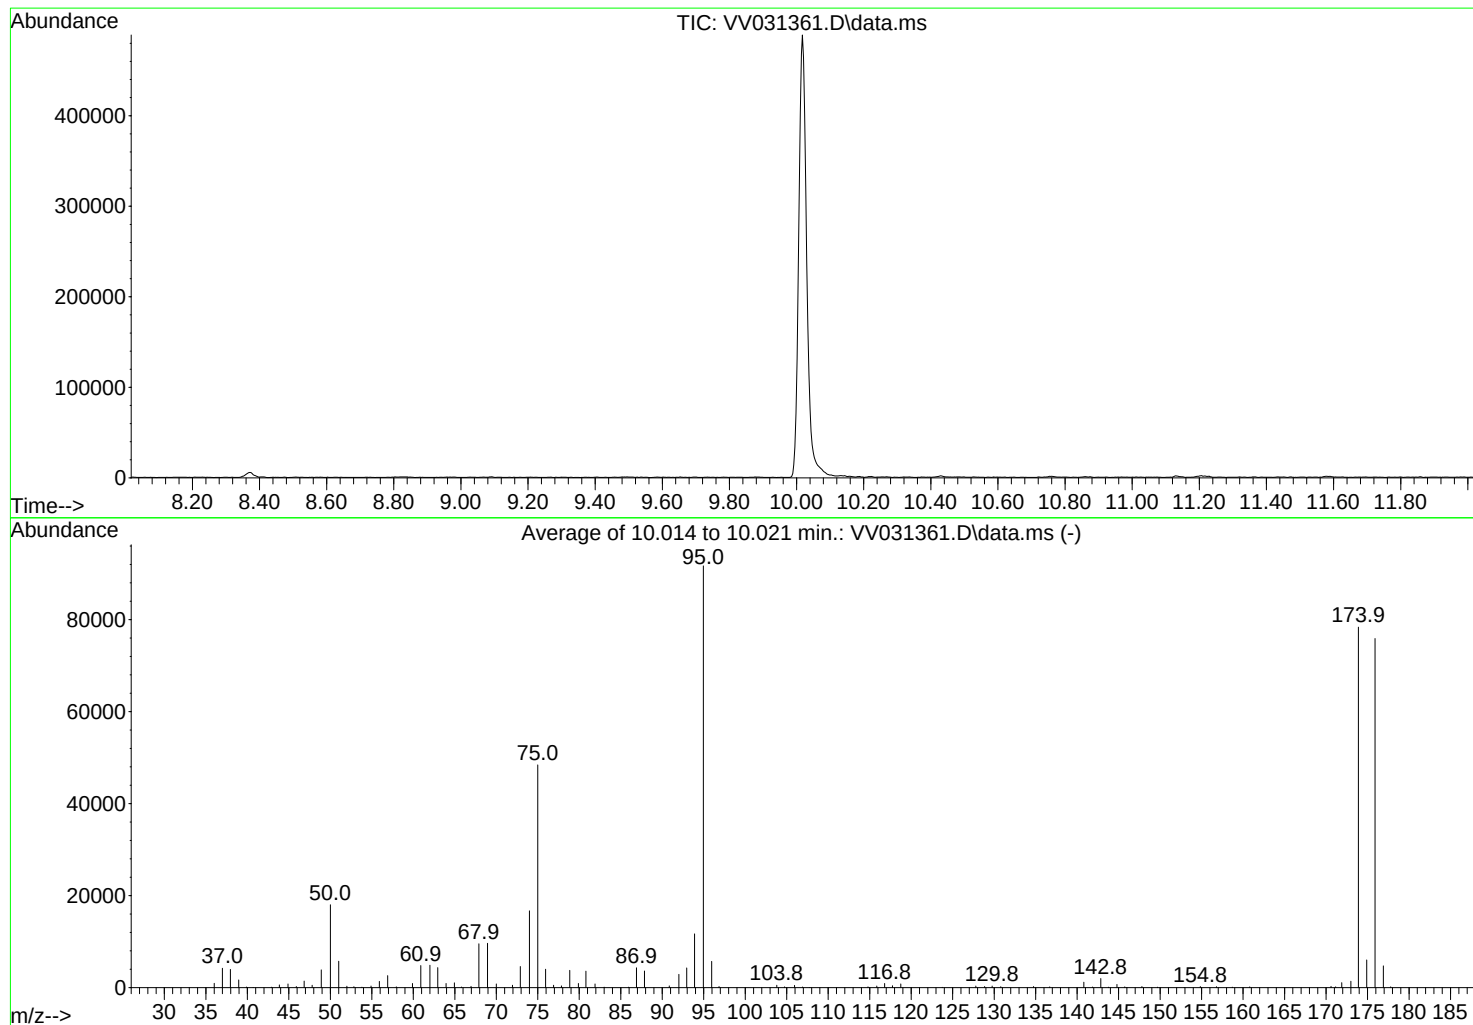

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2778

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.6	18019	PASS
75	95	30	80	52.8	48424	PASS
95	95	100	100	100.0	91704	PASS
96	95	5	9	6.2	5700	PASS
173	174	0.00	2	1.8	1379	PASS
174	95	50	120	85.5	78376	PASS
175	174	5	9	7.7	6014	PASS
176	174	95	105	96.8	75891	PASS
177	176	5	10	6.2	4729	PASS

Scan 2778 (9.972 min): VV031361.D\data.ms
BFB271

m/z	Abundance
39.90	231.0
43.80	324.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	968.0
37.00	4395.0
37.90	3942.0
38.90	1645.0
39.90	335.0
40.70	122.0
42.90	142.0
43.90	923.0
44.90	829.0
45.90	263.0
46.80	1306.0
47.80	538.0
48.90	3865.0
50.00	18752.0
51.00	5599.0
52.00	341.0
52.80	167.0
54.90	374.0
55.90	1367.0
56.90	2730.0
57.90	199.0
59.90	953.0
60.90	4579.0
62.00	4741.0
62.90	4135.0
64.00	843.0
65.00	1015.0
65.80	139.0
66.90	242.0
67.90	9316.0
69.00	9760.0
70.00	829.0
72.00	585.0
72.90	4462.0
74.00	16920.0
75.00	47560.0
76.00	3885.0
76.90	564.0
77.90	346.0
78.90	3717.0
79.90	878.0
80.80	3603.0
81.90	742.0
85.90	165.0
86.90	4156.0
87.90	3541.0
90.80	403.0
92.00	2832.0
93.00	4233.0
93.90	11734.0
94.90	90888.0
95.90	5638.0
96.90	324.0
103.80	464.0
104.80	184.0
106.00	510.0
106.90	143.0
114.80	183.0
115.90	358.0
116.80	931.0
117.70	388.0
118.80	769.0
123.80	129.0
127.80	333.0
128.80	262.0
129.70	323.0
130.80	172.0
134.70	224.0
136.70	193.0
140.80	1103.0
141.90	147.0
142.80	2096.0
143.90	104.0
144.80	732.0
145.80	209.0
147.80	248.0
149.70	106.0
152.90	115.0
154.80	253.0
156.80	198.0
158.70	120.0
160.80	172.0
170.70	316.0
171.90	1002.0
173.00	1301.0
173.90	76952.0
174.90	6118.0
175.90	73992.0
176.90	4639.0
177.80	190.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	937.0
37.00	4385.0
37.90	4033.0
39.00	1714.0
39.90	387.0
42.90	135.0
43.90	950.0
44.90	852.0
45.90	277.0
46.90	1483.0
47.80	554.0
48.90	3979.0
50.00	18736.0
51.00	5923.0
52.00	313.0
52.80	204.0
53.80	128.0
54.90	368.0
55.90	1421.0
56.90	2736.0
57.90	179.0
59.90	944.0
60.90	5000.0
62.00	5080.0
63.00	4532.0
64.00	906.0
65.00	1074.0
65.80	146.0
67.00	262.0
67.90	9799.0
68.90	9960.0
70.00	865.0
72.00	541.0
72.90	4781.0
74.00	17168.0
75.00	49976.0
75.90	4164.0
76.90	539.0
77.90	398.0
78.80	3872.0
79.90	956.0
80.80	3726.0
81.90	826.0
83.00	146.0
86.00	113.0
86.90	4488.0
87.90	3812.0
90.90	416.0
92.00	2928.0
93.00	4405.0
93.90	12225.0
94.90	94464.0
95.90	5855.0
96.90	258.0
103.80	553.0
104.80	187.0
106.00	522.0
106.90	165.0
114.80	170.0
115.90	336.0
116.80	902.0
117.70	400.0
118.80	825.0
123.70	140.0
127.80	357.0
128.80	246.0
129.80	377.0
130.80	232.0
134.70	229.0
136.70	157.0
140.80	1280.0
141.90	133.0
142.80	2054.0
143.80	118.0
144.80	702.0
145.80	194.0
147.80	234.0
149.70	125.0
154.90	261.0
156.80	232.0
158.70	128.0
160.80	183.0
170.60	268.0
171.10	244.0
171.90	1125.0
173.00	1425.0
173.90	80632.0
174.90	6187.0
175.90	78480.0
176.90	4818.0
177.80	204.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271

m/z	Abundance
36.00	899.0
37.00	3873.0
38.00	3899.0
39.00	1680.0
40.00	398.0
43.90	882.0
44.90	770.0
45.90	227.0
46.90	1463.0
47.80	521.0
48.90	3718.0
50.00	16568.0
51.00	5682.0
52.00	260.0
52.90	234.0
53.80	170.0
54.90	316.0
55.90	1307.0
56.90	2361.0
58.00	126.0
59.90	830.0
60.90	4803.0
62.00	4819.0
63.00	4368.0
63.90	941.0
64.90	1077.0
65.80	180.0
67.00	288.0
67.90	9480.0
68.90	9163.0
70.00	762.0
71.90	489.0
72.90	4554.0
74.00	16008.0
75.00	47736.0
75.90	3974.0
76.90	498.0
77.80	464.0
78.80	3651.0
79.90	918.0
80.80	3472.0
81.90	817.0
83.00	182.0
86.90	4327.0
87.80	3484.0
90.90	388.0
92.00	2869.0
92.90	4228.0
93.90	11138.0
95.00	89760.0
96.00	5607.0
96.80	195.0
103.80	522.0
104.70	184.0
105.90	410.0
106.90	152.0
107.80	136.0
114.80	162.0
115.70	322.0
116.80	849.0
117.80	427.0
118.70	777.0
127.80	355.0
128.90	195.0
129.80	388.0
130.80	228.0
134.80	233.0
136.70	137.0
140.80	1167.0
141.80	103.0
142.90	1844.0
143.70	127.0
144.80	610.0
145.70	164.0
146.00	162.0
147.80	240.0
149.70	137.0
154.90	235.0
156.80	204.0
158.70	110.0
160.80	166.0
170.50	254.0
171.20	295.0
171.90	1127.0
173.00	1411.0
173.90	77544.0
174.90	5736.0
175.90	75200.0
176.90	4731.0
177.80	184.0

Instrument :
MSVOA_V
ClientSampleId :
BFB271