




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
 Data File : VV038760.D
 Acq On : 06 Jun 2025 10:55
 Operator : SY/MD
 Sample : Q2117-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
 Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Jun 13 10:50:34 2025
 Response via : Initial Calibration

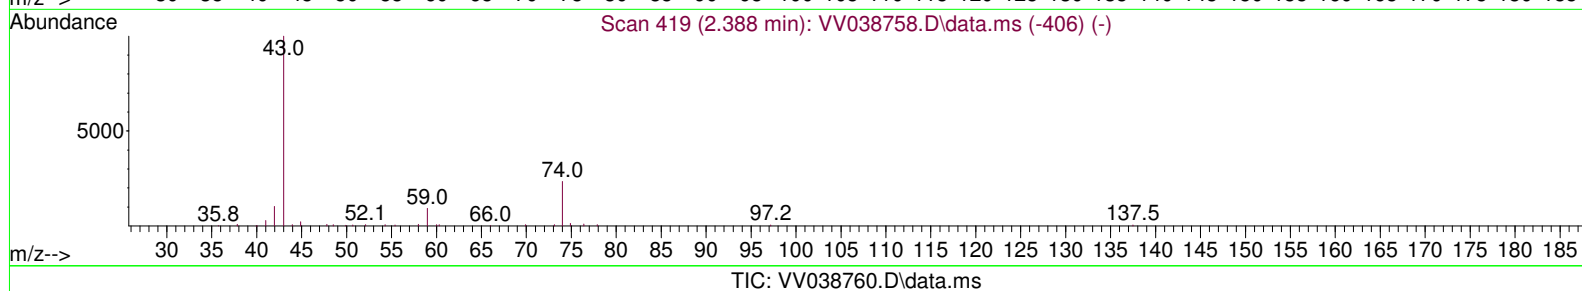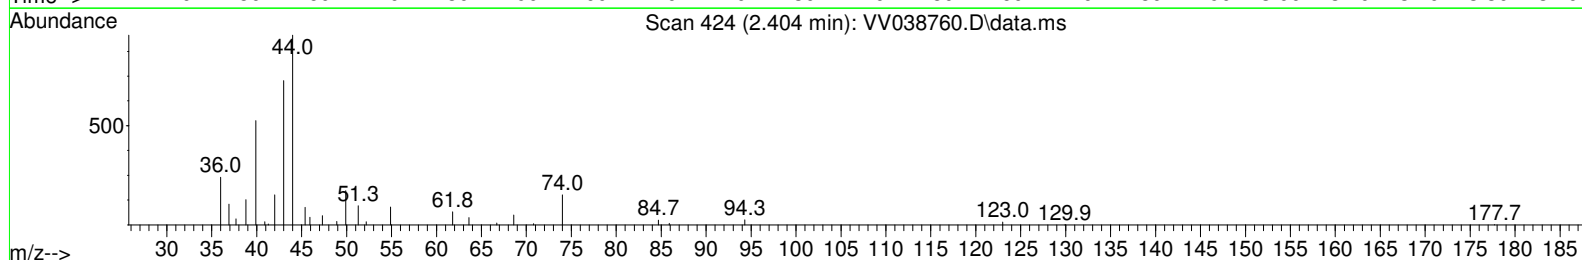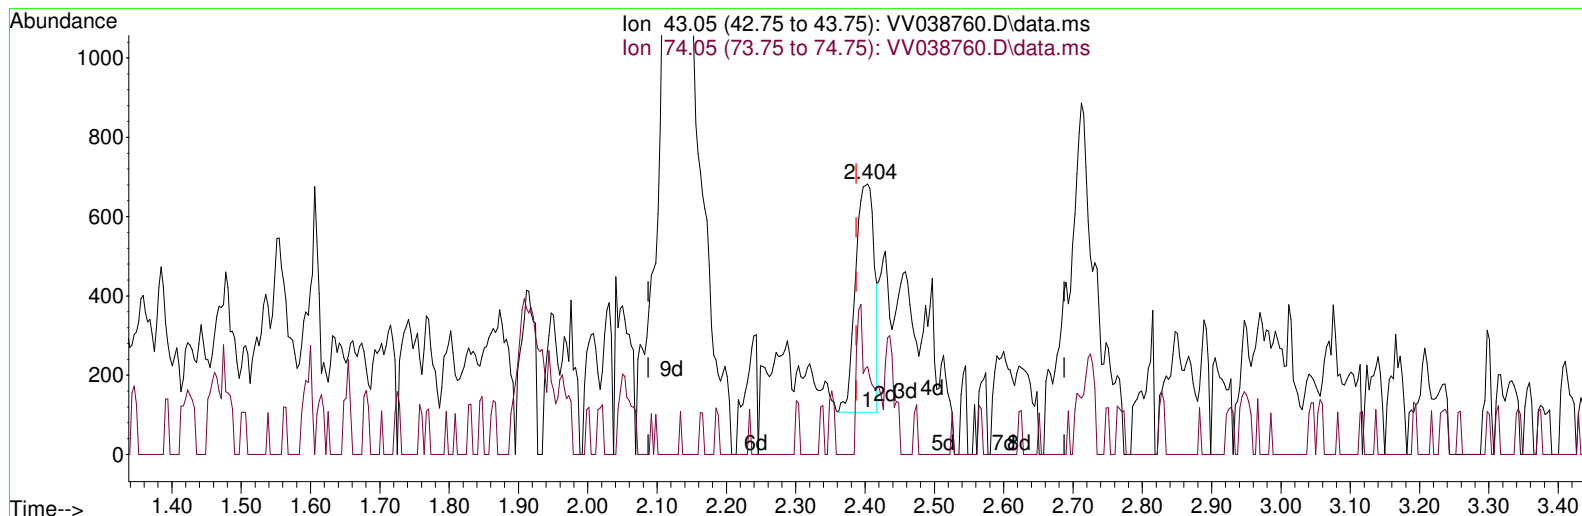

(15) Methyl Acetate (T)

2.404min (+ 0.016) 0.13 ug/L

response 1074

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	23.20	50.09#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

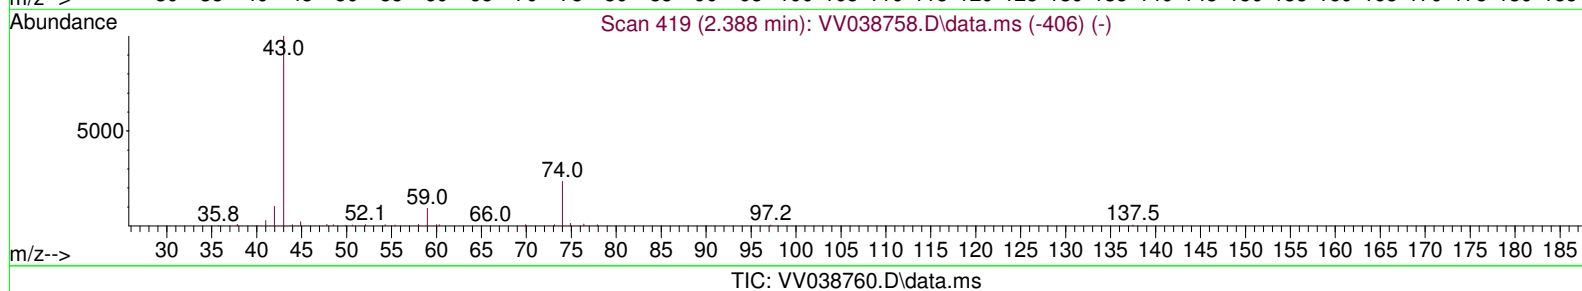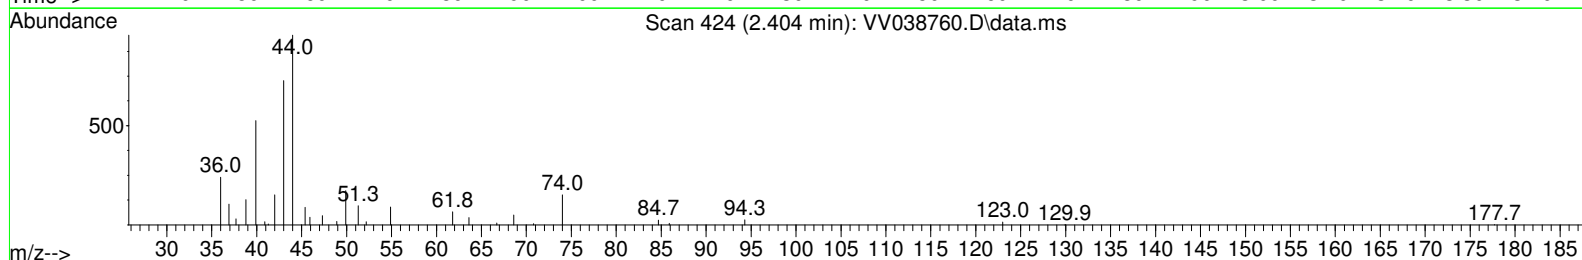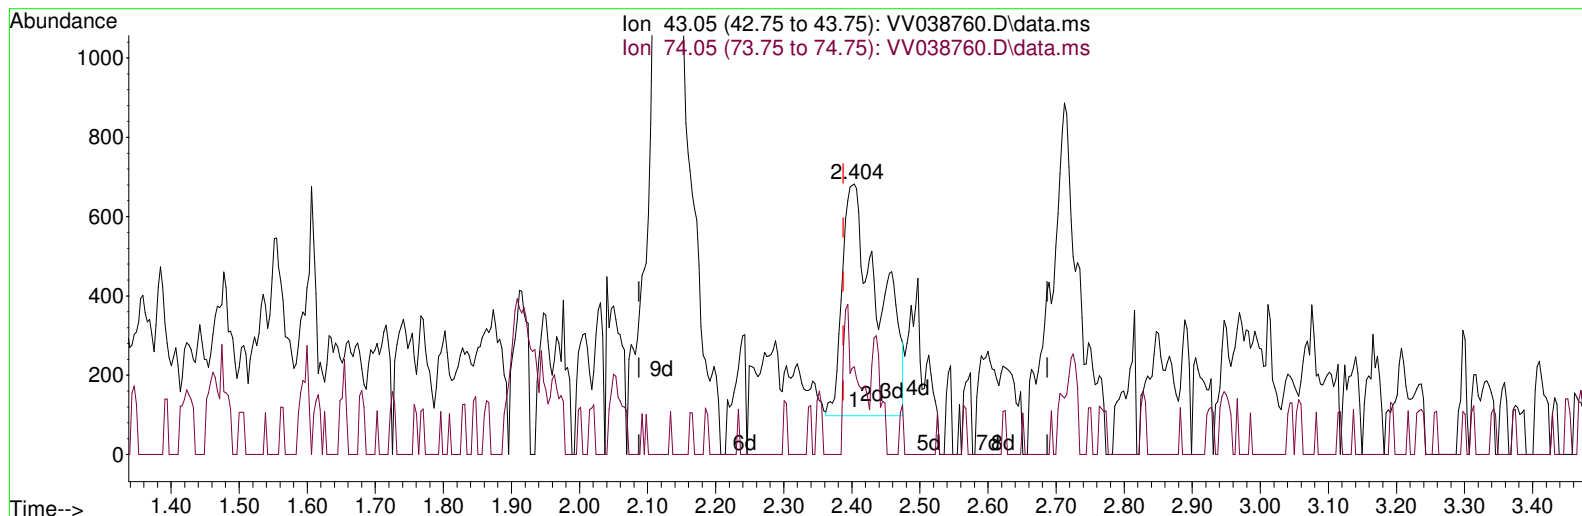

(15) Methyl Acetate (T)

2.404min (+ 0.016) 0.26 ug/L m

response 2150

Ion	Exp%	Act%
43.05	100.00	100.00
74.05	23.20	25.02
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

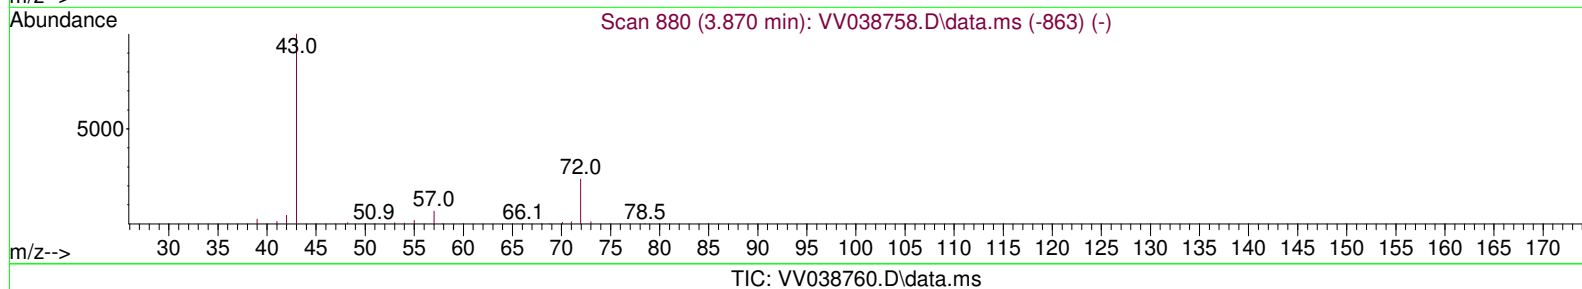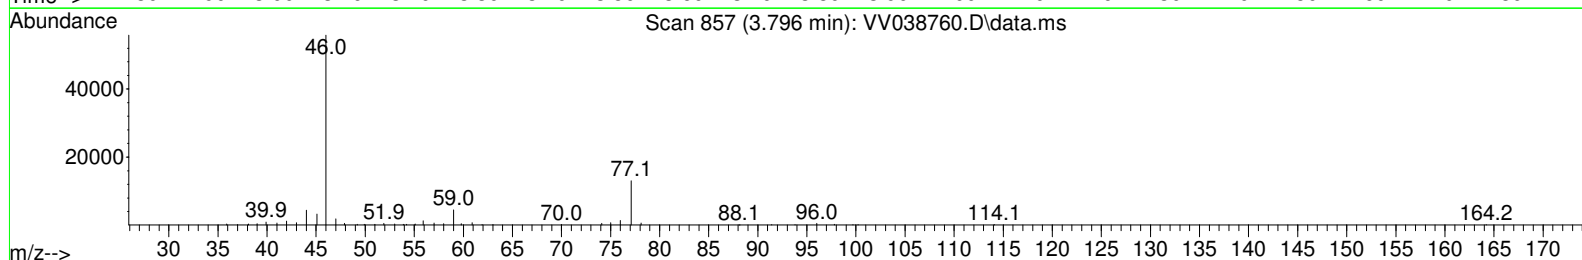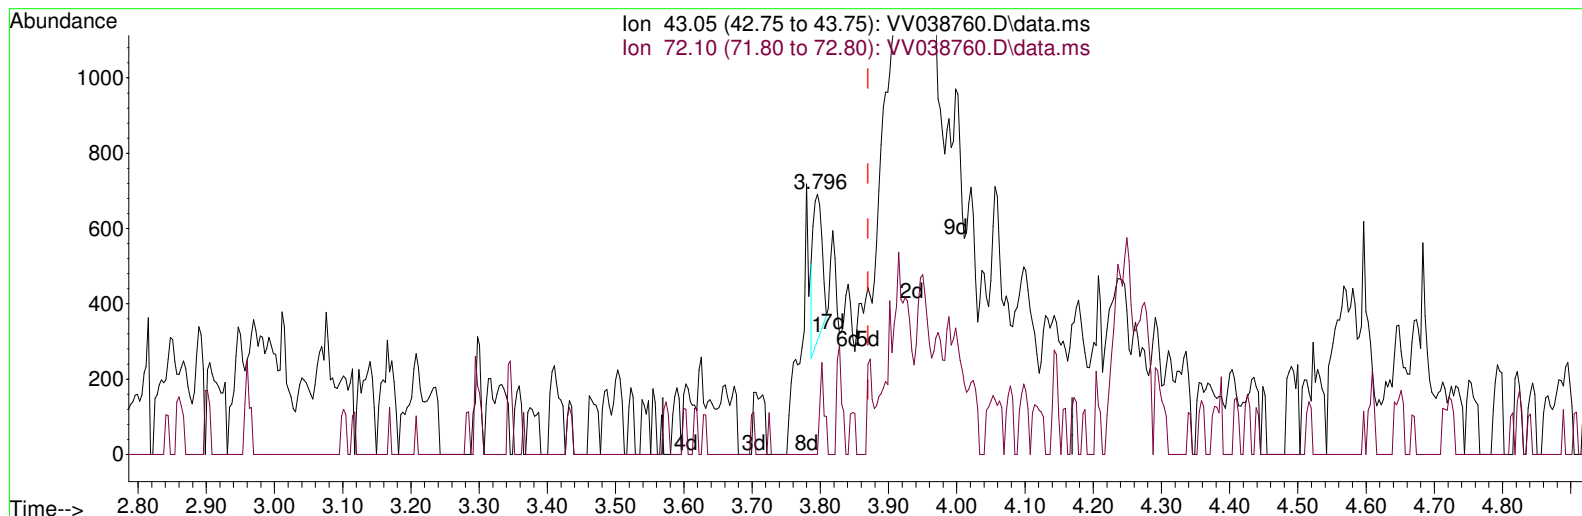

(21) 2-Butanone (T)

3.796min (-0.074) 0.08 ug/L

response 356

Ion	Exp%	Act%
43.05	100.00	100.00
72.10	23.70	30.90
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

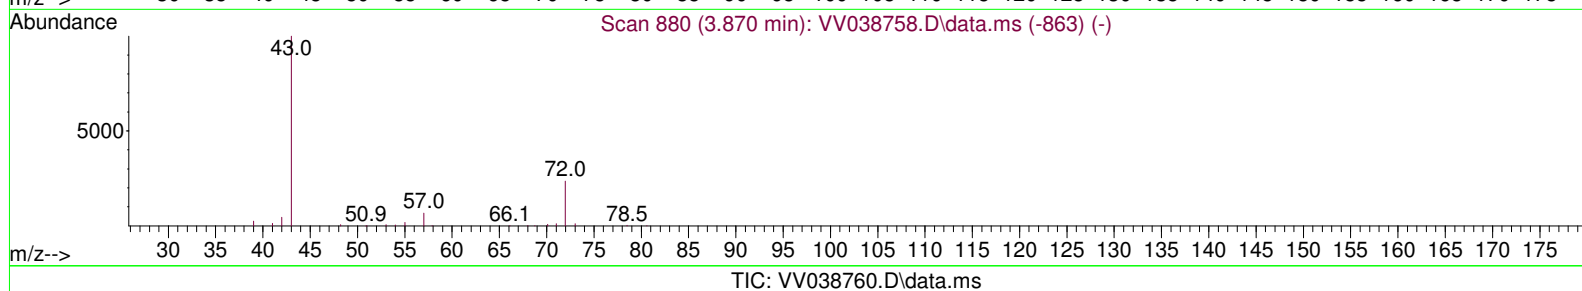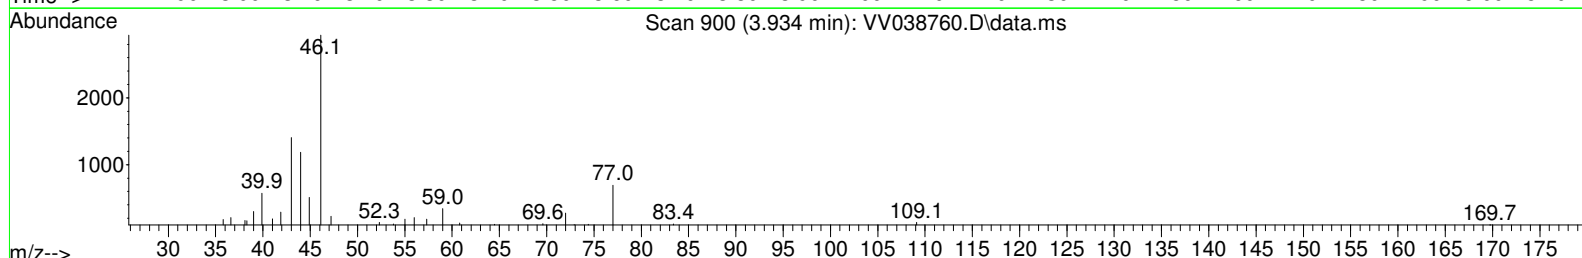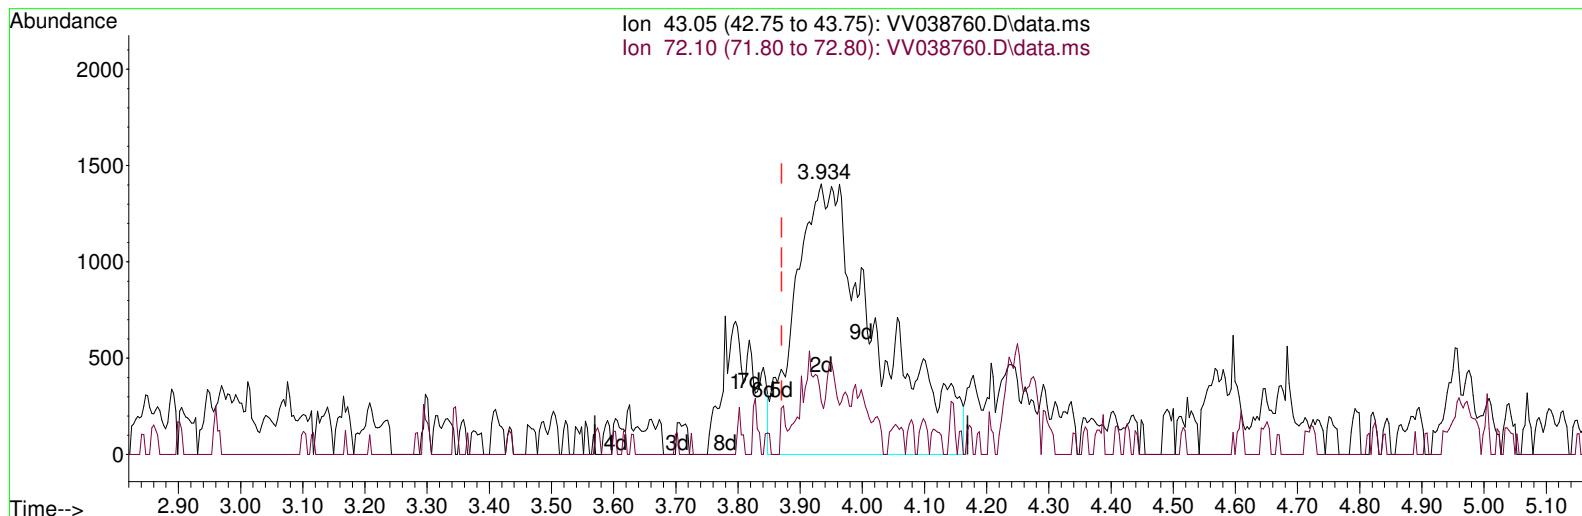

(21) 2-Butanone (T)

3.934min (+ 0.064) 2.97 ug/L m

response 12993

Ion	Exp%	Act%
-----	------	------

43.05	100.00	100.00
-------	--------	--------

72.10	23.70	0.85#
-------	-------	-------

0.00	0.00	0.00
------	------	------

0.00	0.00	0.00
------	------	------




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

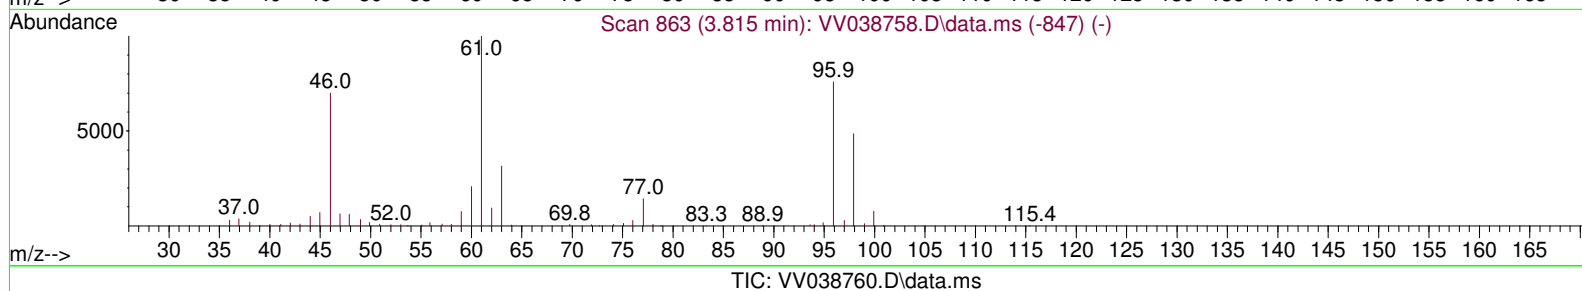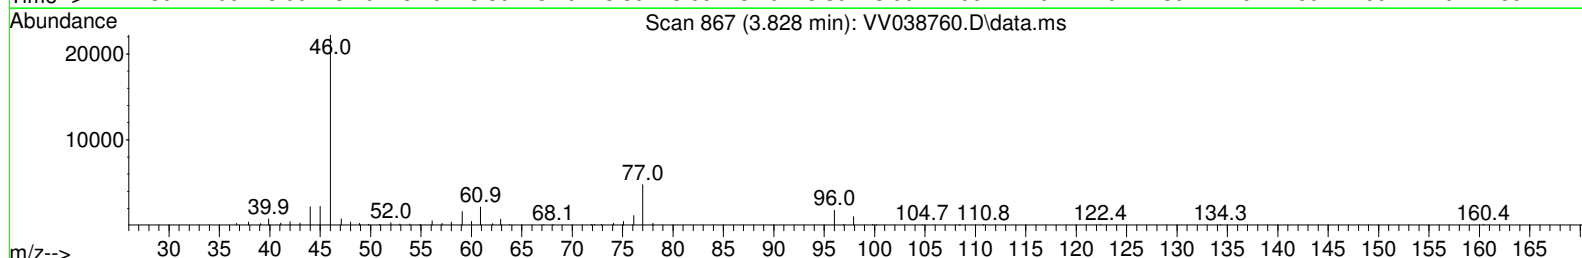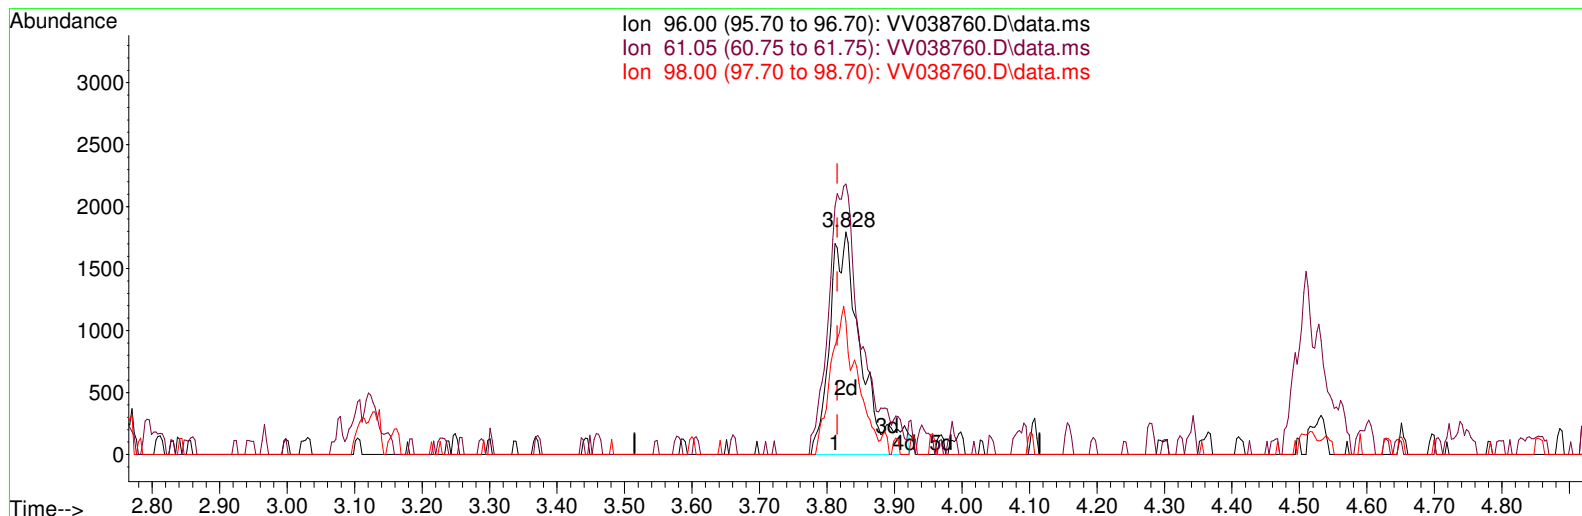

(22) cis-1,2-Dichloroethene (T)

3.828min (+ 0.013) 0.26 ug/L m

response 5793

Ion	Exp%	Act%
96.00	100.00	100.00
61.05	119.40	121.63
98.00	65.20	59.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

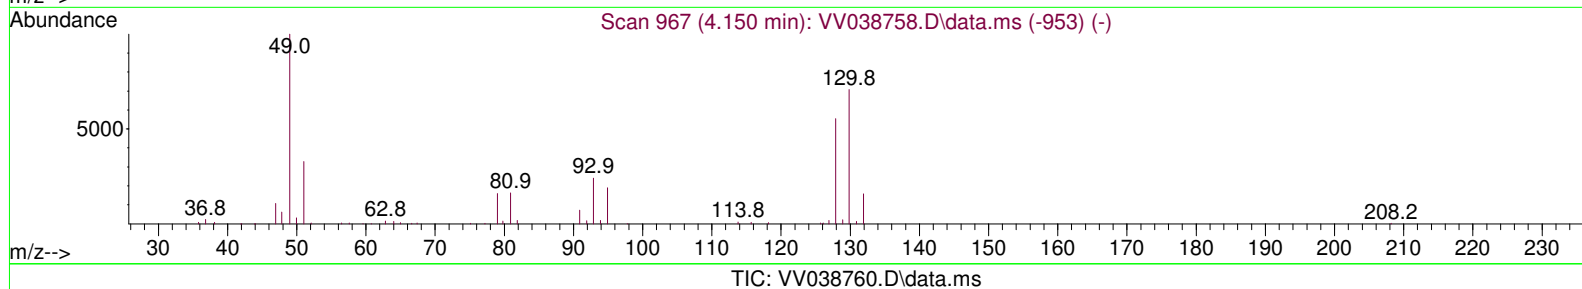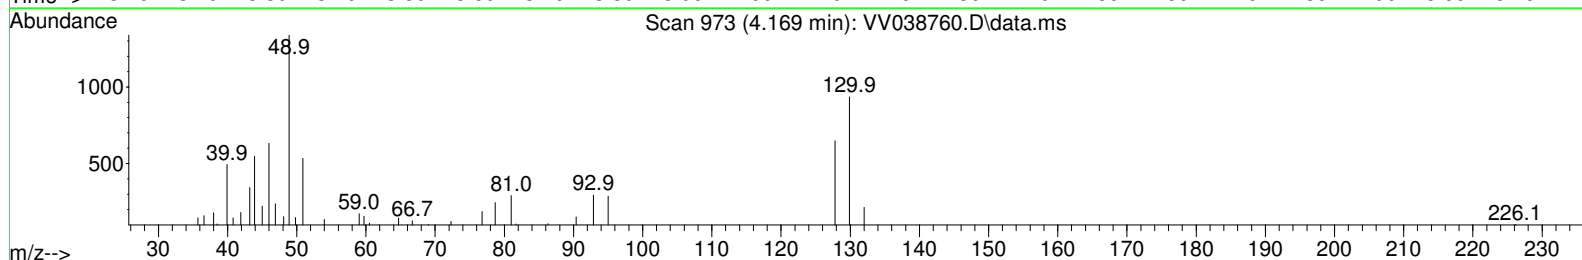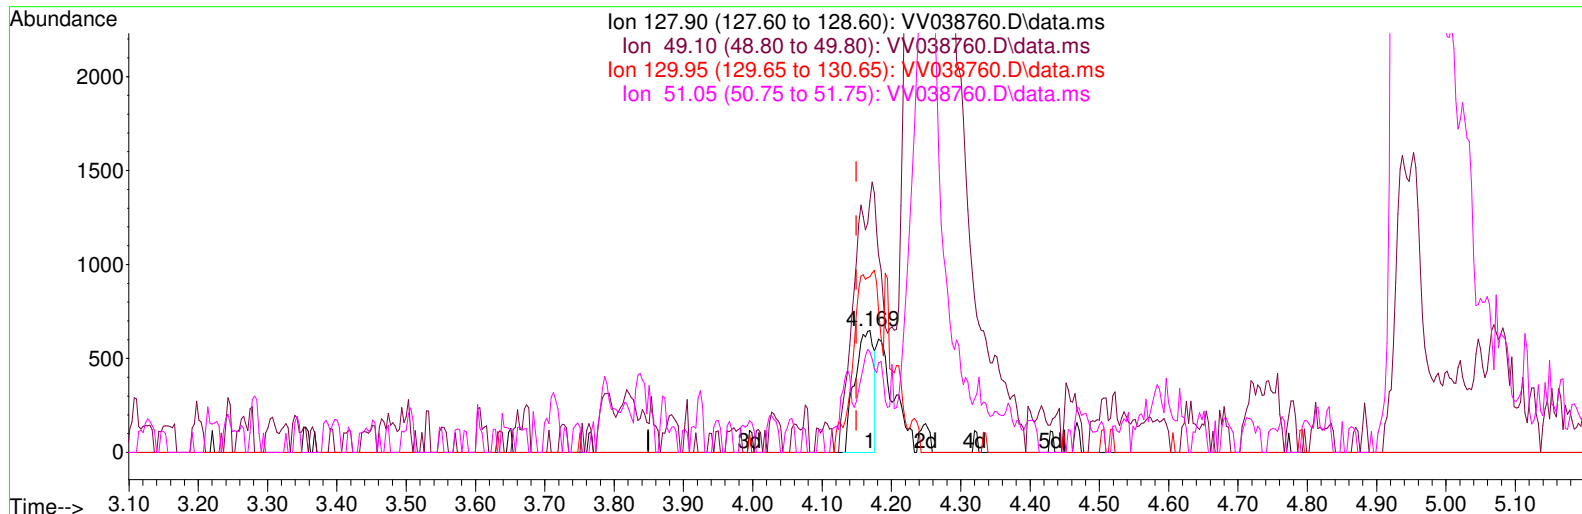

(23) Bromochloromethane (T)

4.169min (+ 0.019) 0.12 ug/L

response 1214

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	165.70	228.81#
129.95	128.90	144.07
51.05	54.30	82.28#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

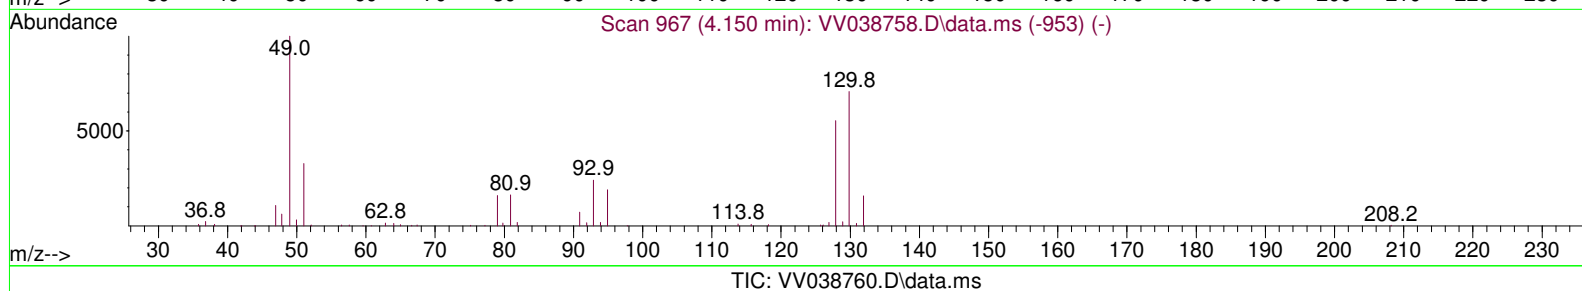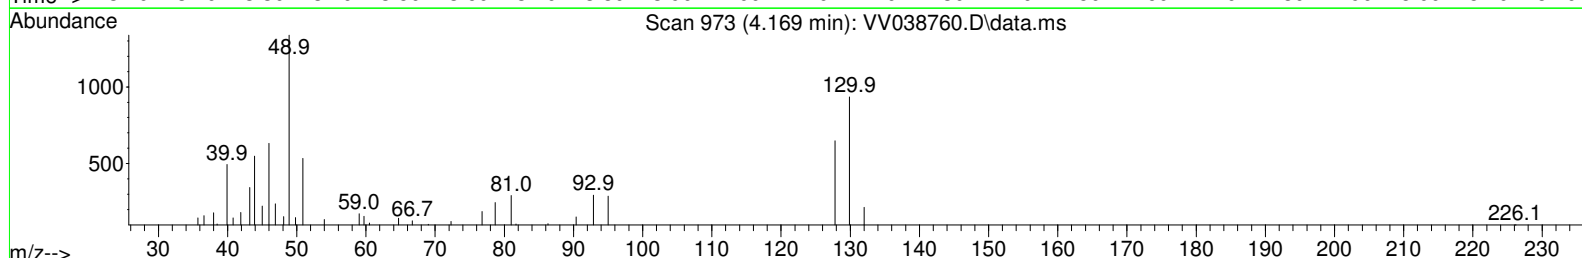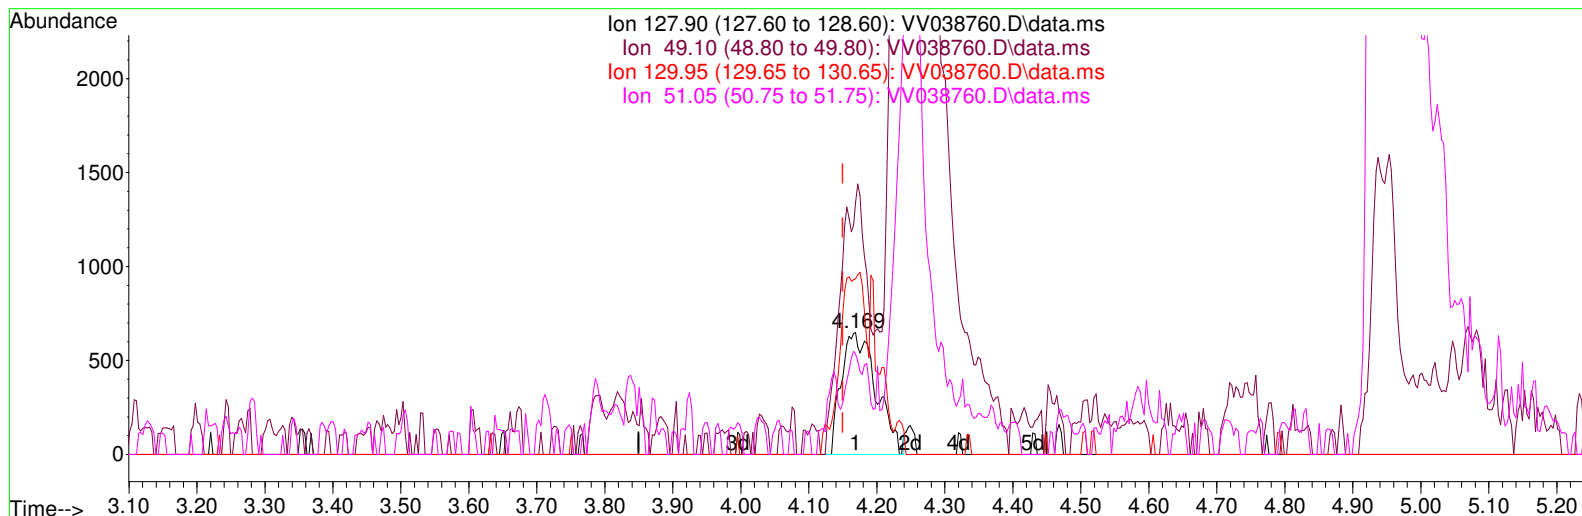

(23) Bromochloromethane (T)

4.169min (+ 0.019) 0.23 ug/L m

response 2318

Ion	Exp%	Act%
127.90	100.00	100.00
49.10	165.70	206.16
129.95	128.90	144.07
51.05	54.30	82.28#




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

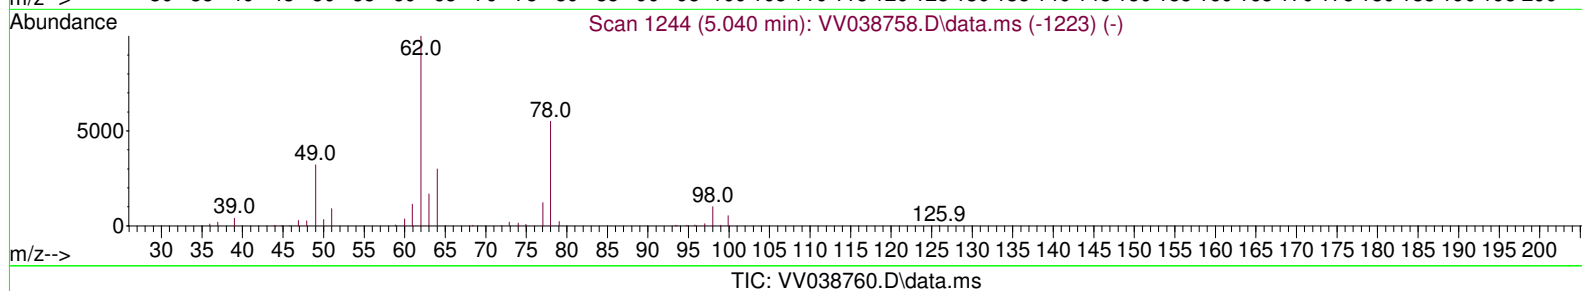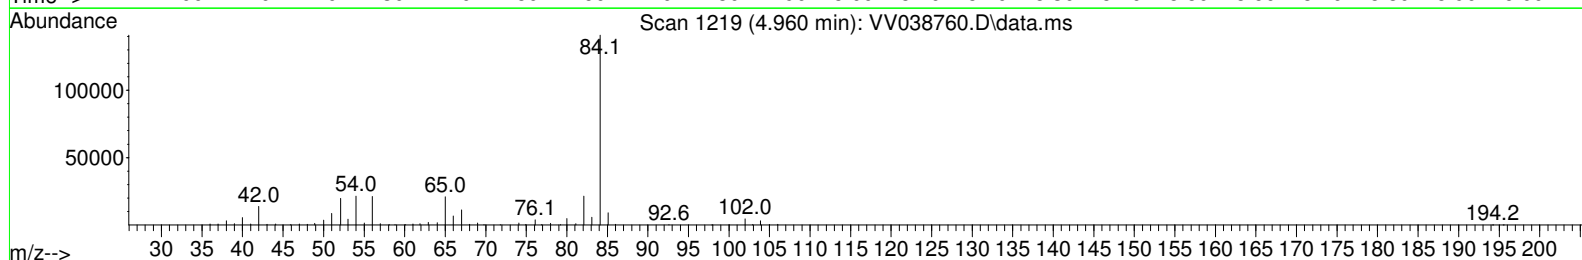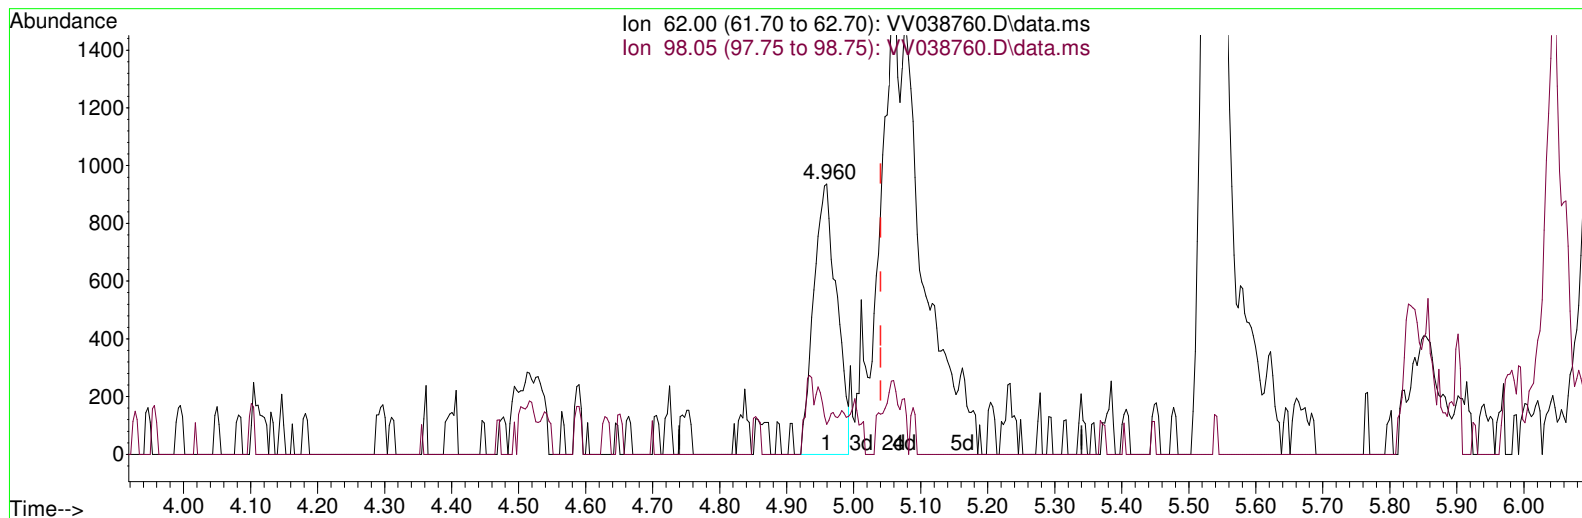

(27) 1,2-Dichloroethane (T)

4.960min (-0.080) 0.09 ug/L

response 2231

Ion	Exp%	Act%
62.00	100.00	100.00
98.05	9.60	11.11
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

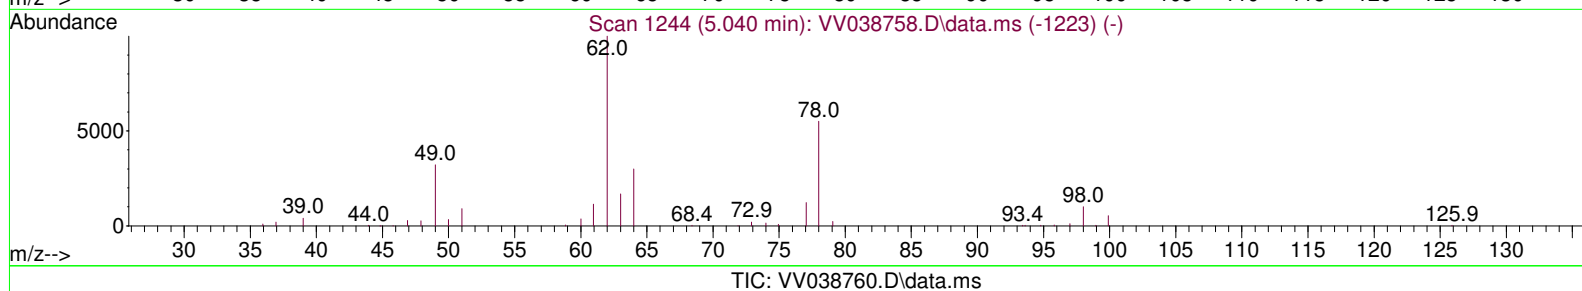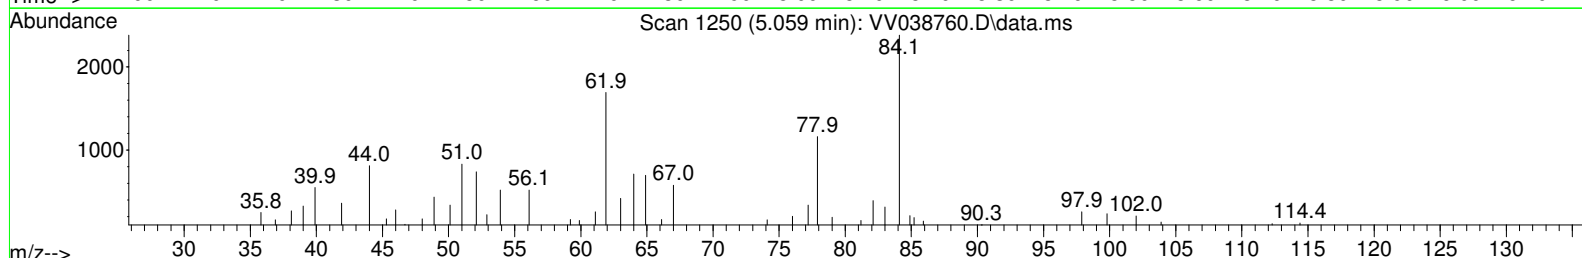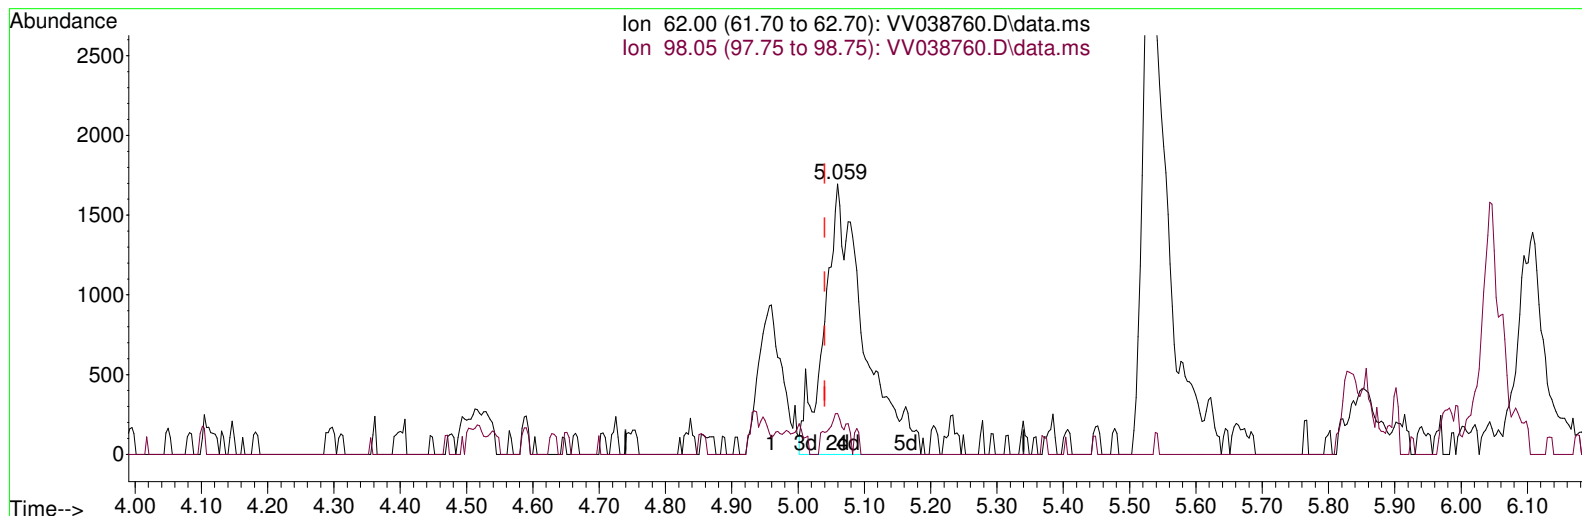

(27) 1,2-Dichloroethane (T)

5.059min (+ 0.019) 0.28 ug/L m

response 6989

Ion	Exp%	Act%
62.00	100.00	100.00
98.05	9.60	15.10#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

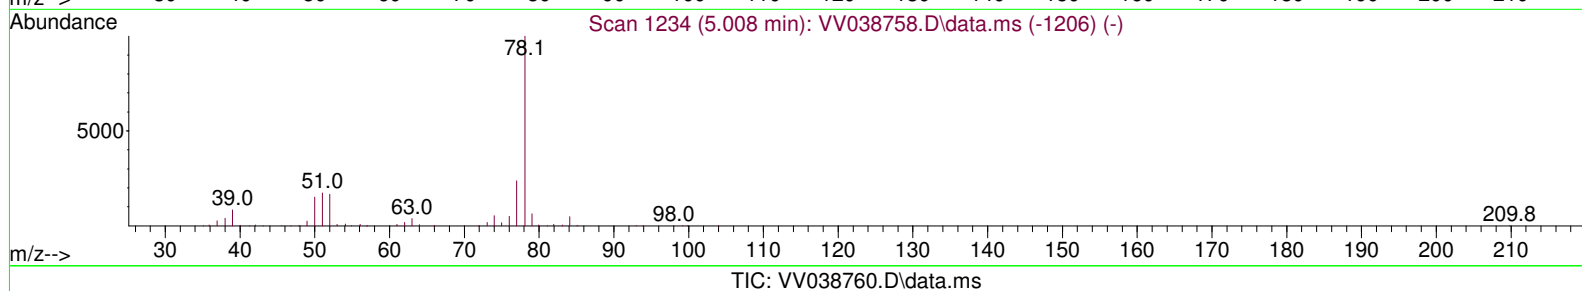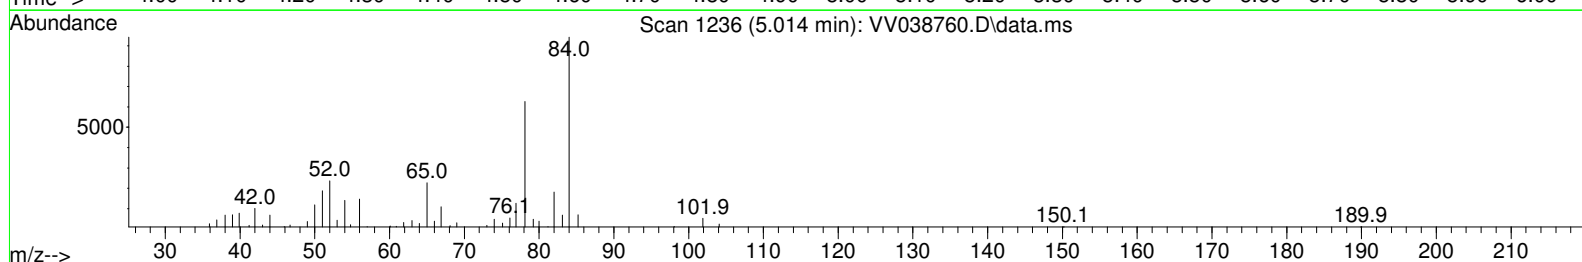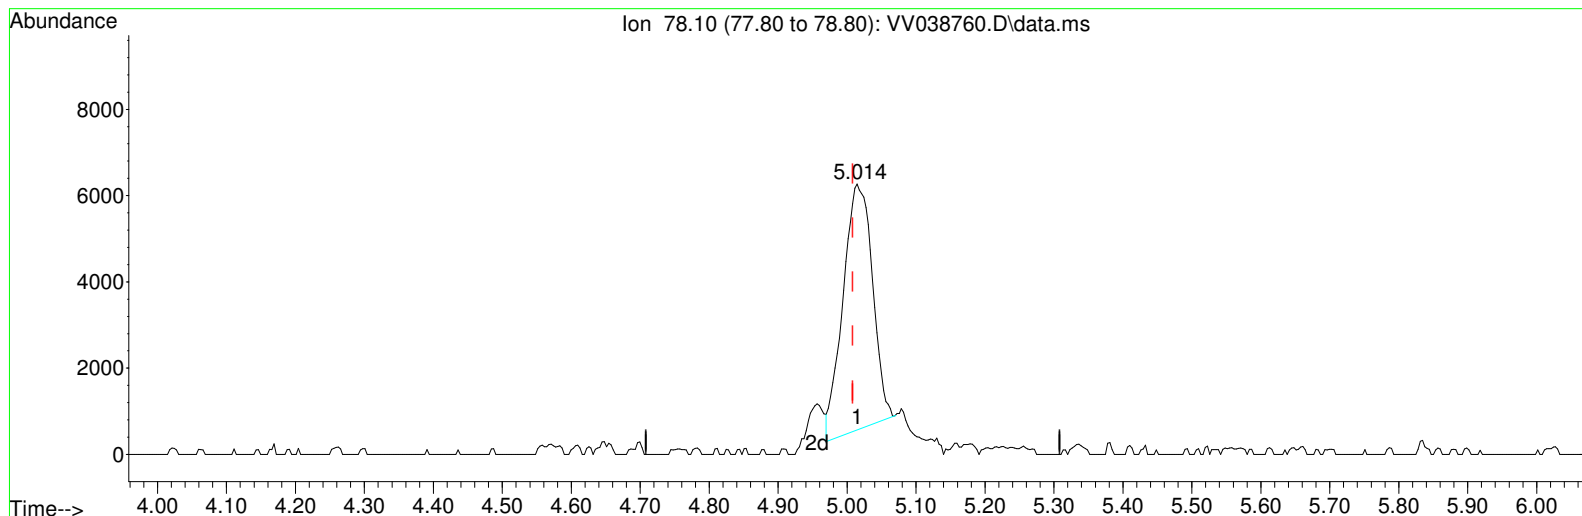

(33) Benzene (T)

5.014min (+ 0.006) 0.19 ug/L

response 16934

Ion	Exp%	Act%
78.10	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

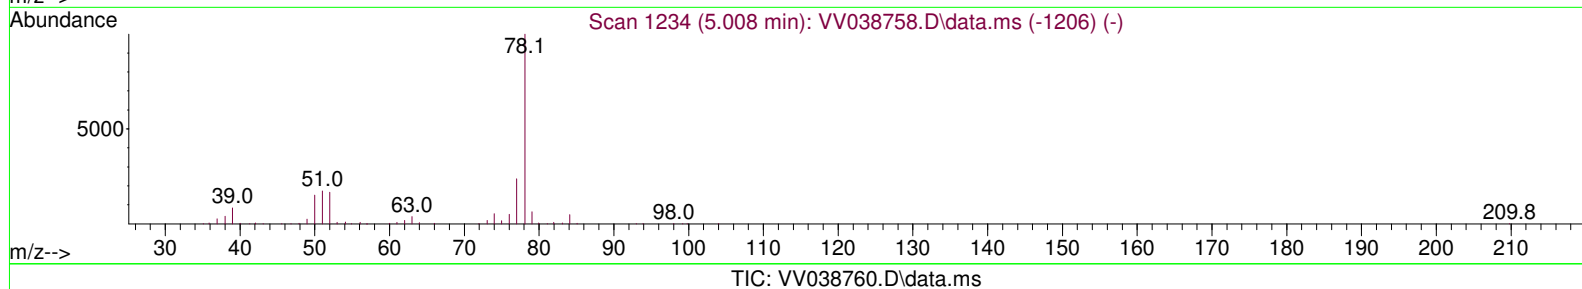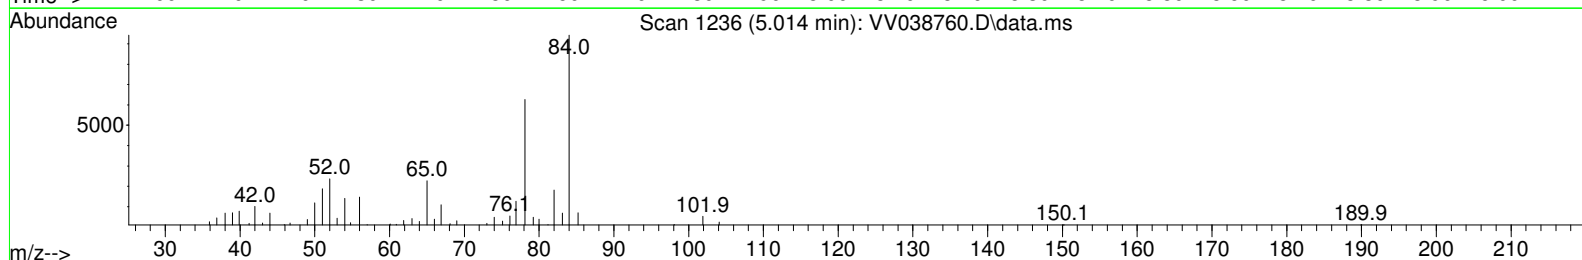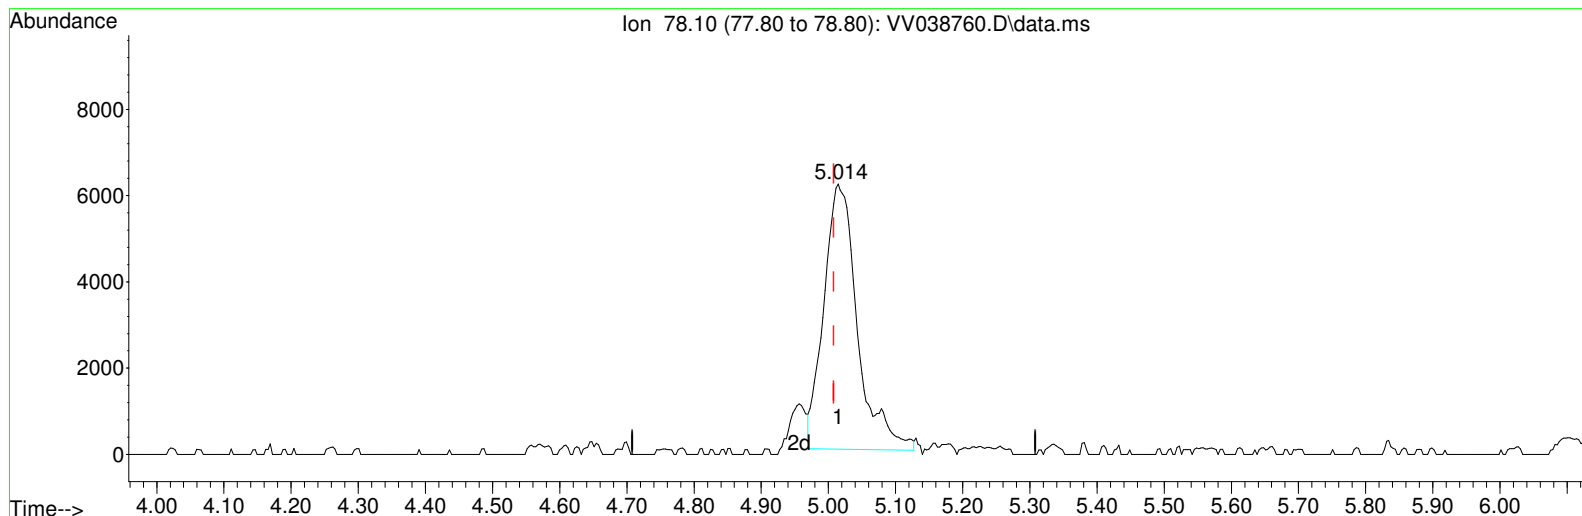

TIC: VV038760.D\data.ms

(33) Benzene (T)

5.014min (+ 0.006) 0.23 ug/L m

response 21346

Ion	Exp%	Act%
78.10	100.00	100.00
0.00	0.00	0.00
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

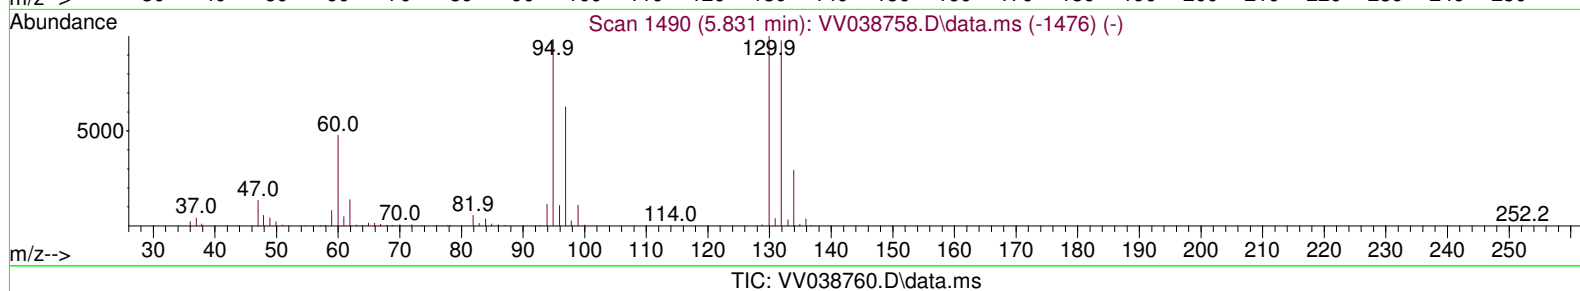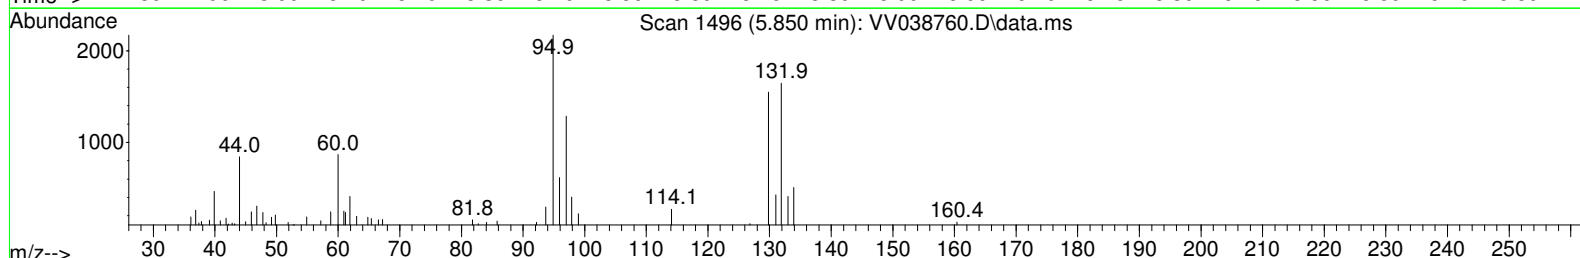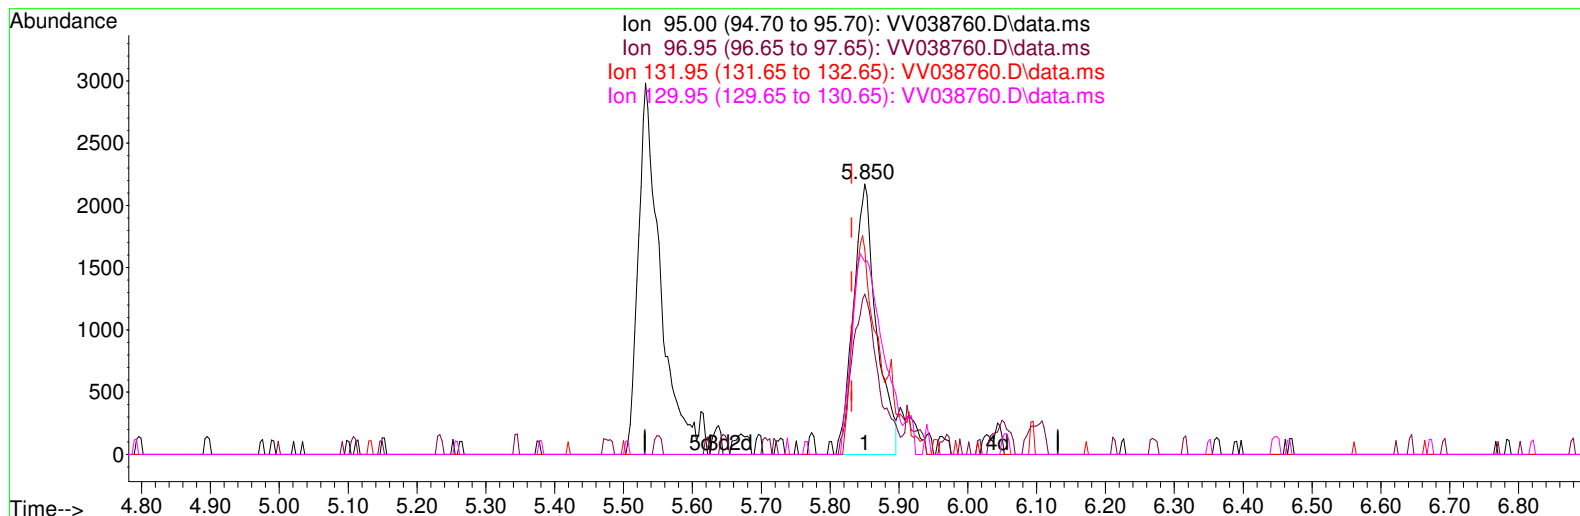

(34) Trichloroethene (T)

5.850min (+ 0.019) 0.22 ug/L

response 5036

Ion	Exp%	Act%
95.00	100.00	100.00
96.95	62.20	59.28
131.95	91.40	75.77
129.95	95.60	71.30


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

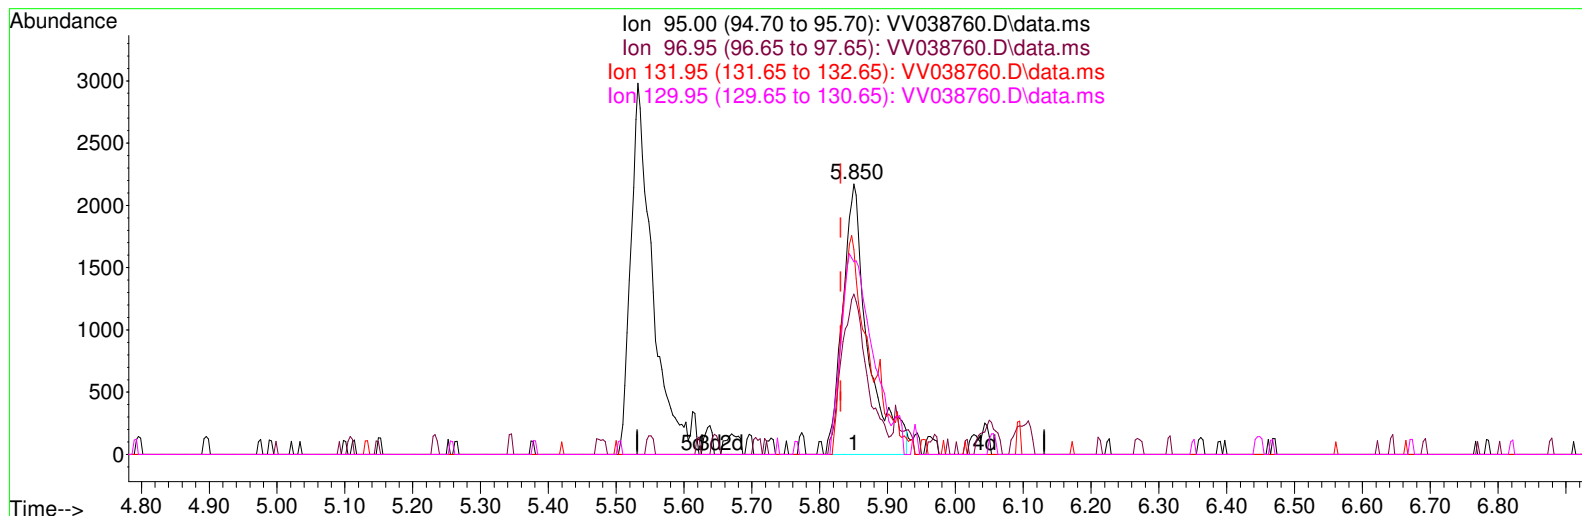




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

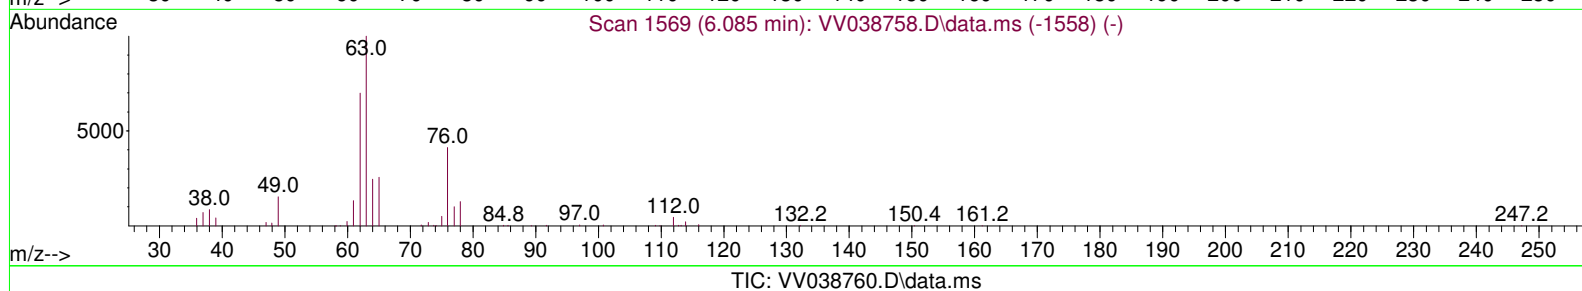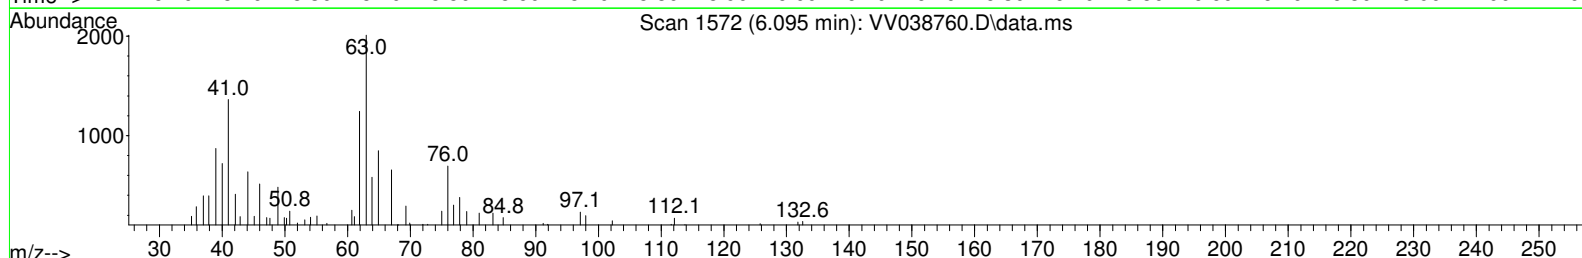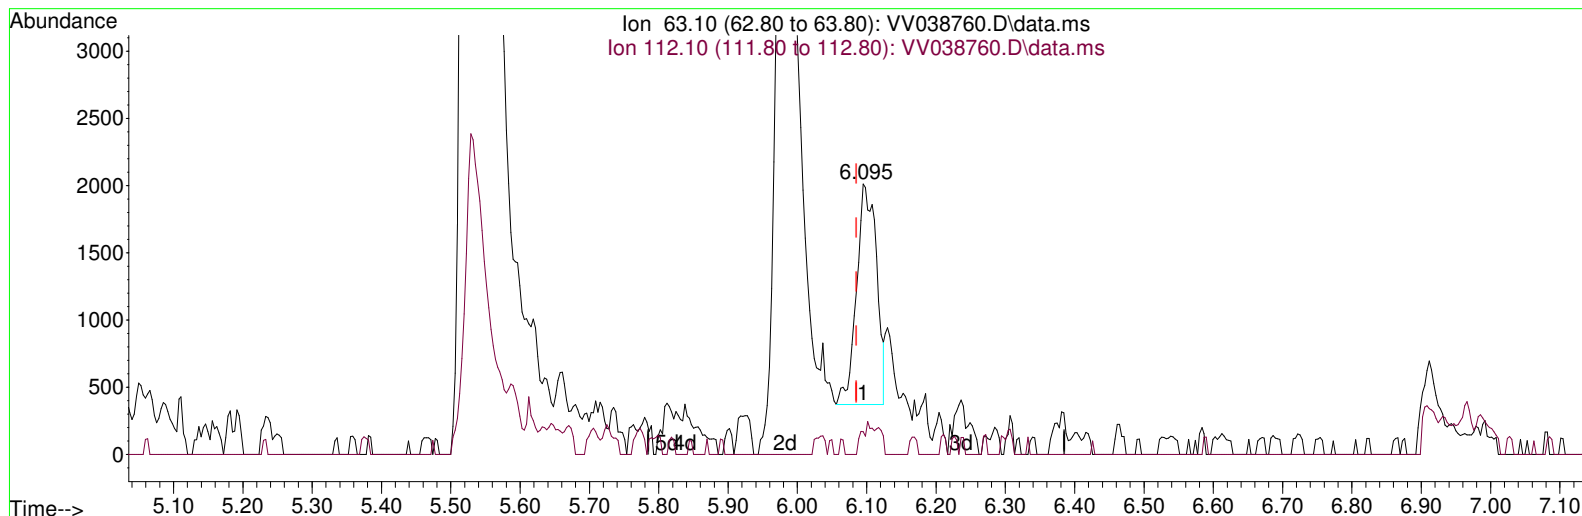

(37) 1,2-Dichloropropane (T)

6.095min (+ 0.010) 0.14 ug/L

response 3275

Ion	Exp%	Act%
63.10	100.00	100.00
112.10	4.50	8.27#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

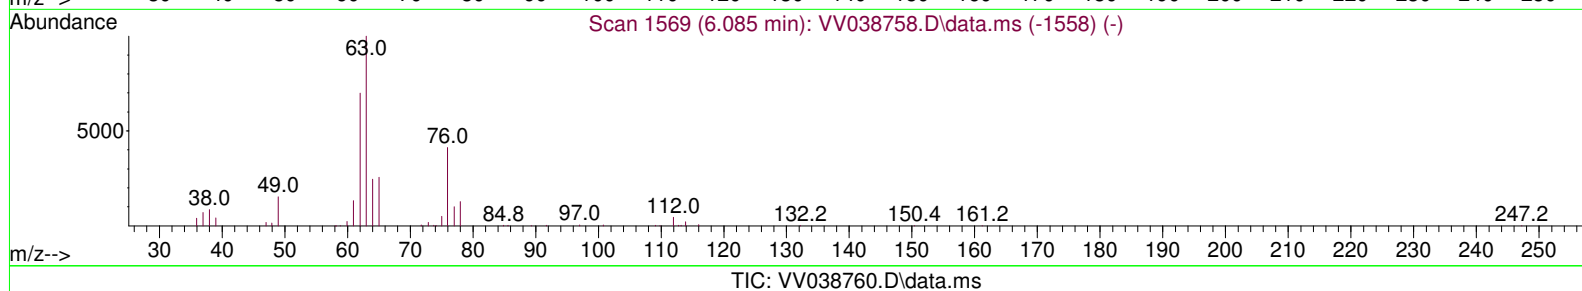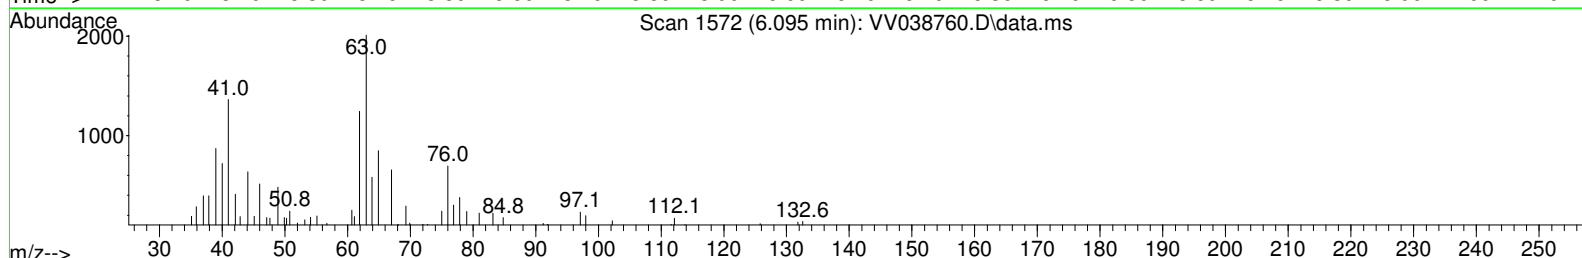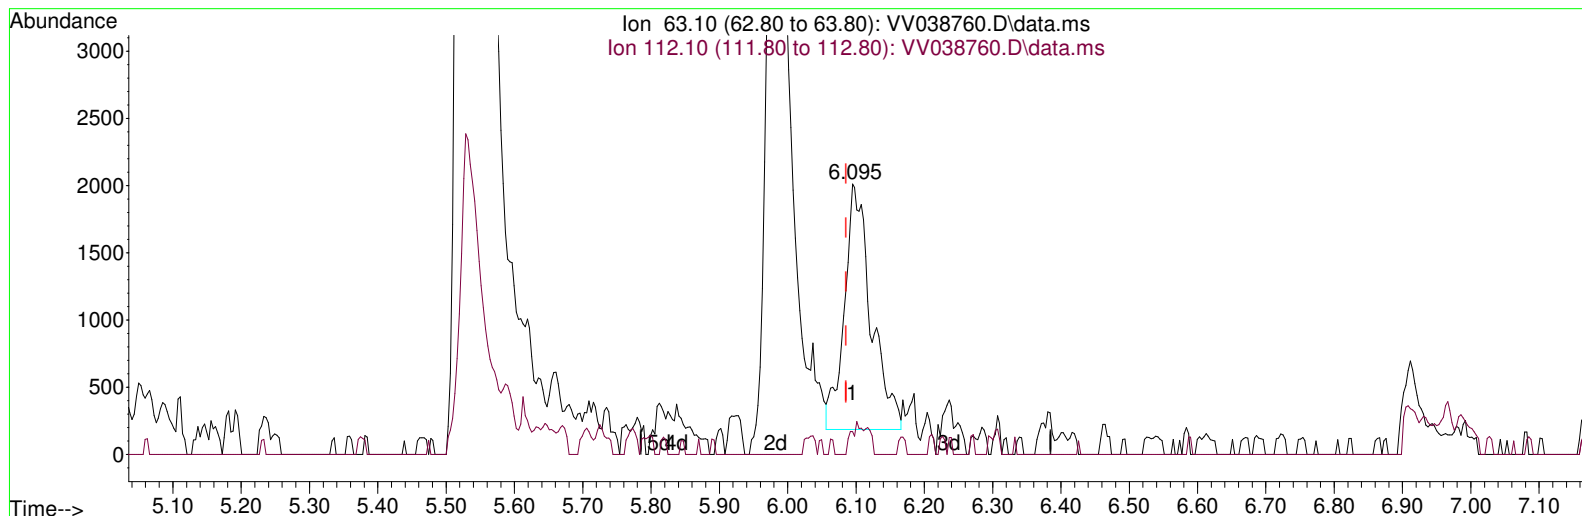

(37) 1,2-Dichloropropane (T)

6.095min (+ 0.010) 0.21 ug/L m

response 4963

Ion	Exp%	Act%
63.10	100.00	100.00
112.10	4.50	5.46#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

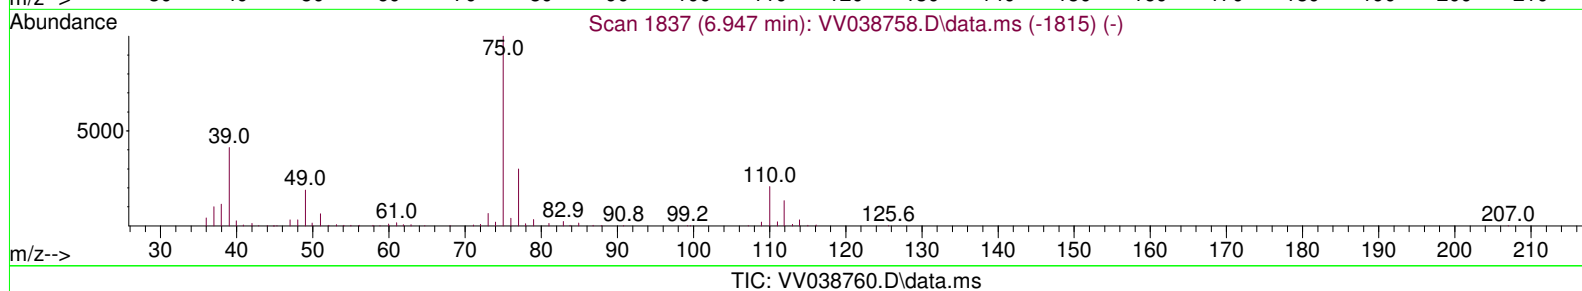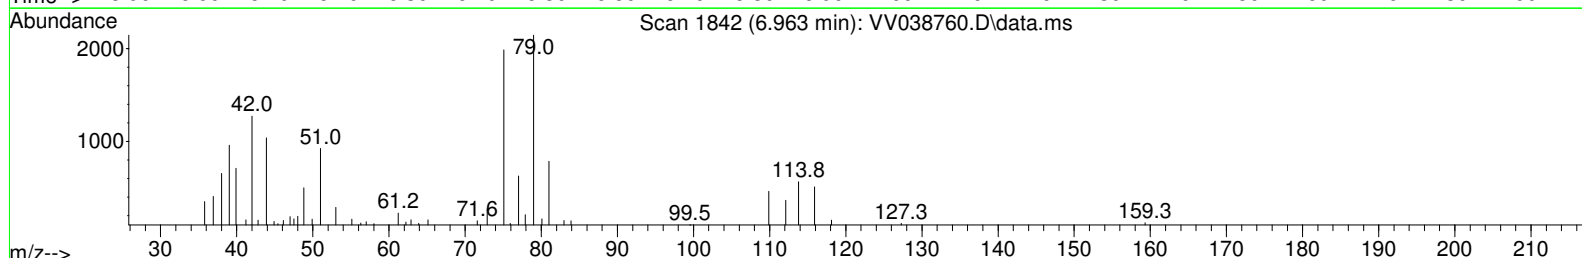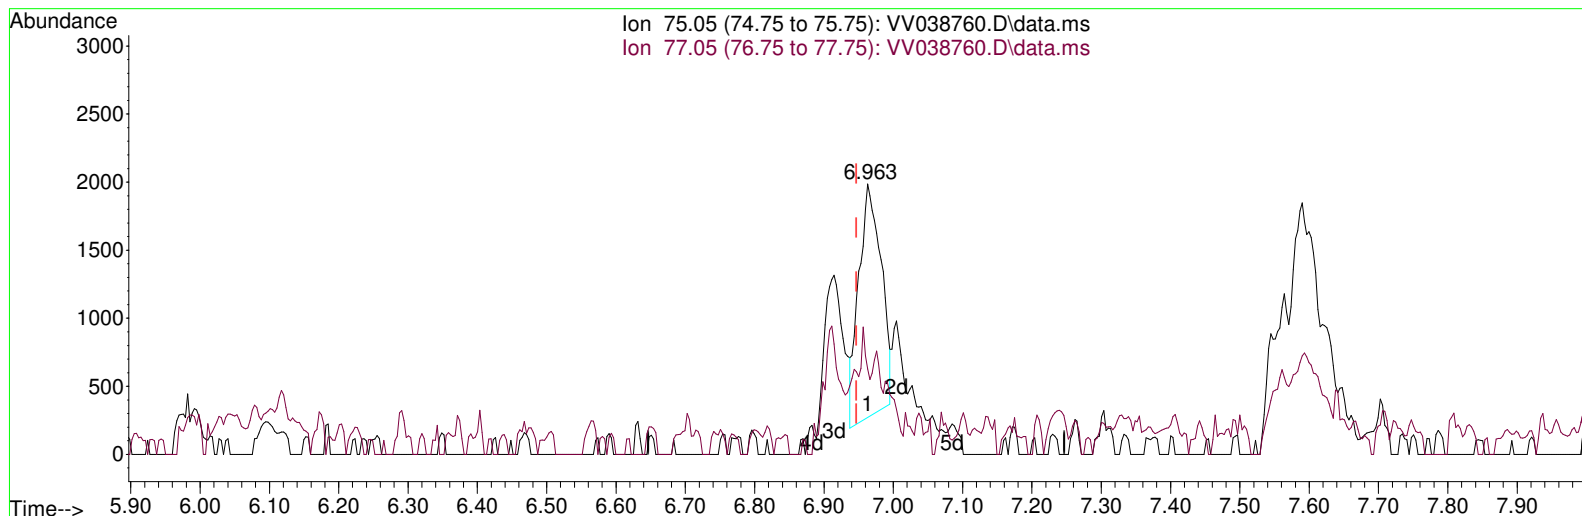

(39) cis-1,3-Dichloropropene (T)

6.963min (+ 0.016) 0.12 ug/L

response 3846

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	30.40	31.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

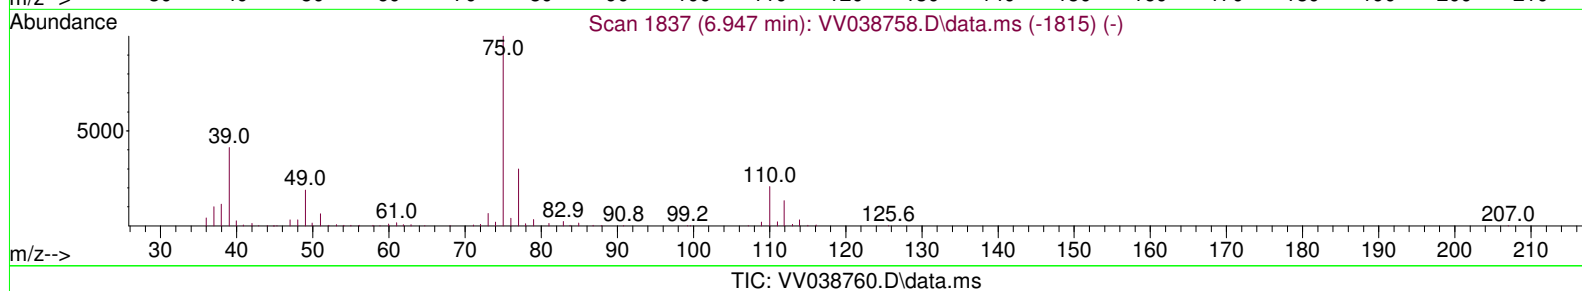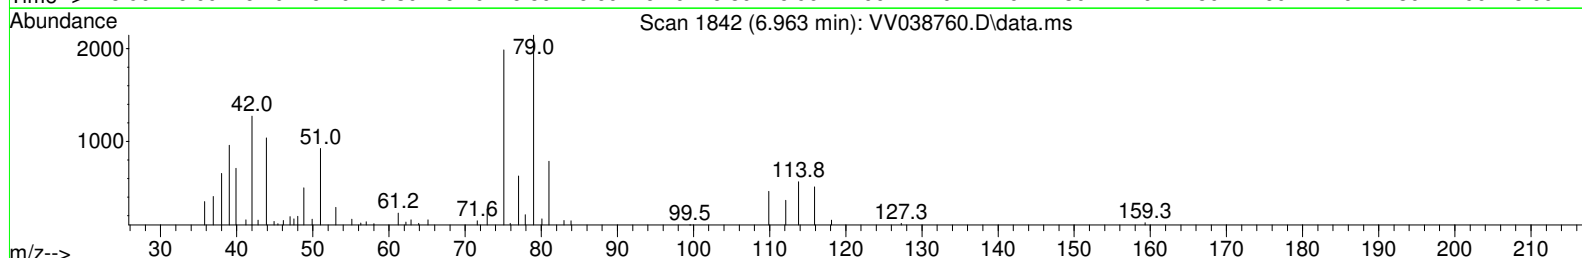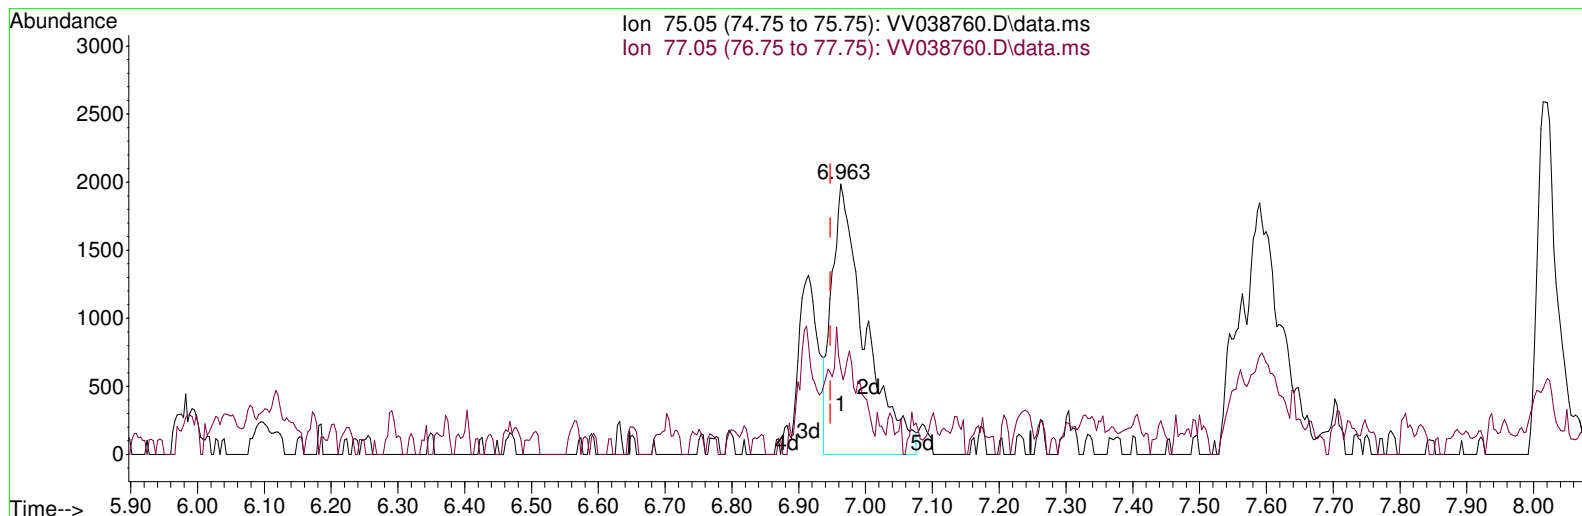

(39) cis-1,3-Dichloropropene (T)

6.963min (+ 0.016) 0.22 ug/L m

response 6884

Ion	Exp%	Act%
75.05	100.00	100.00
77.05	30.40	31.62
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

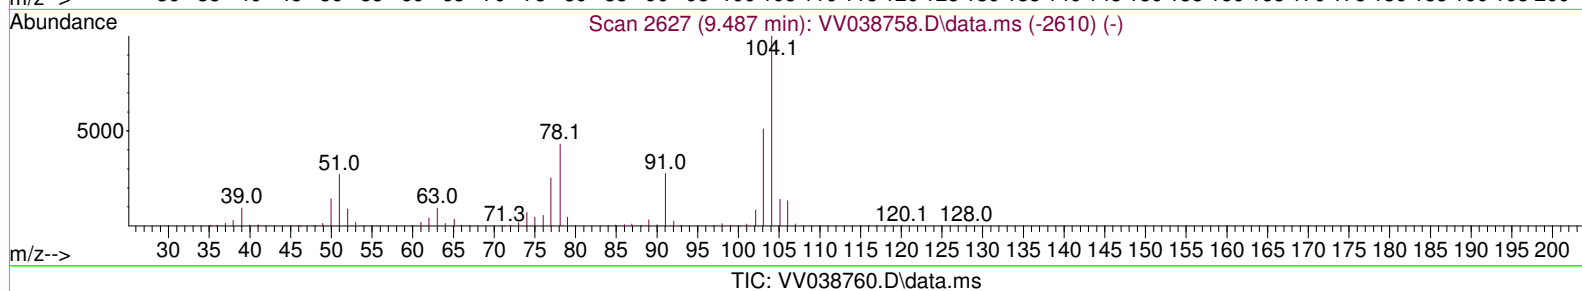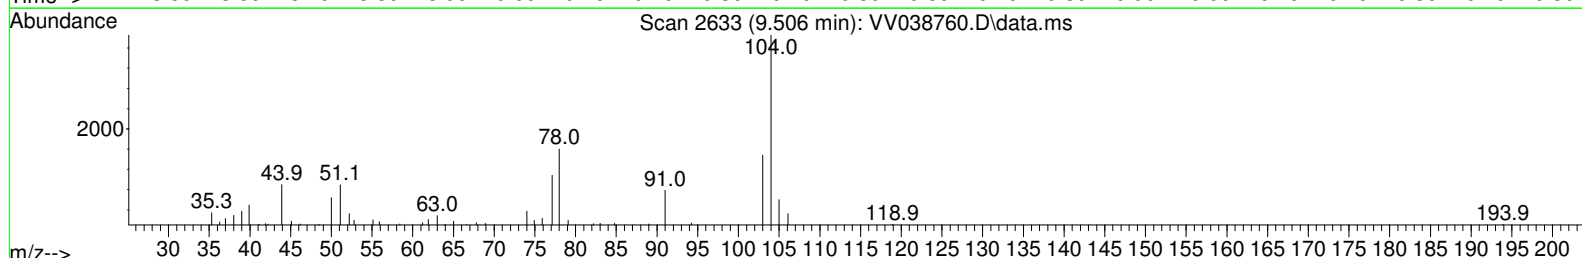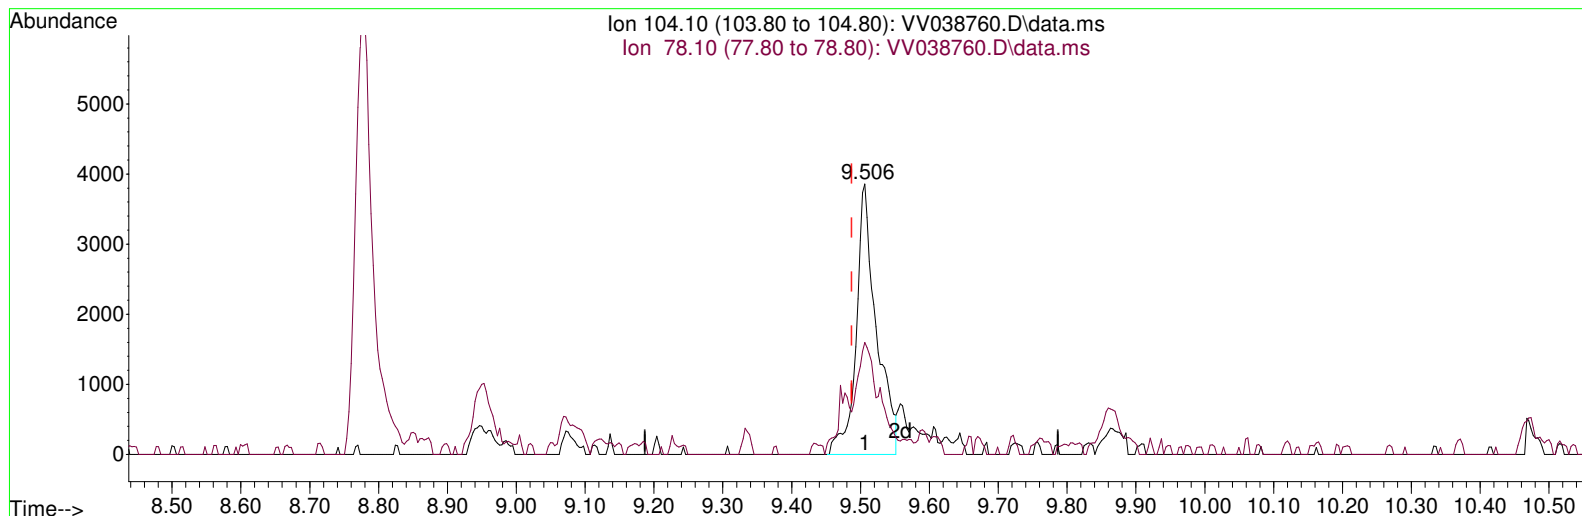

(55) Styrene (T)

9.506min (+ 0.019) 0.13 ug/L

response 7822

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	43.60	41.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

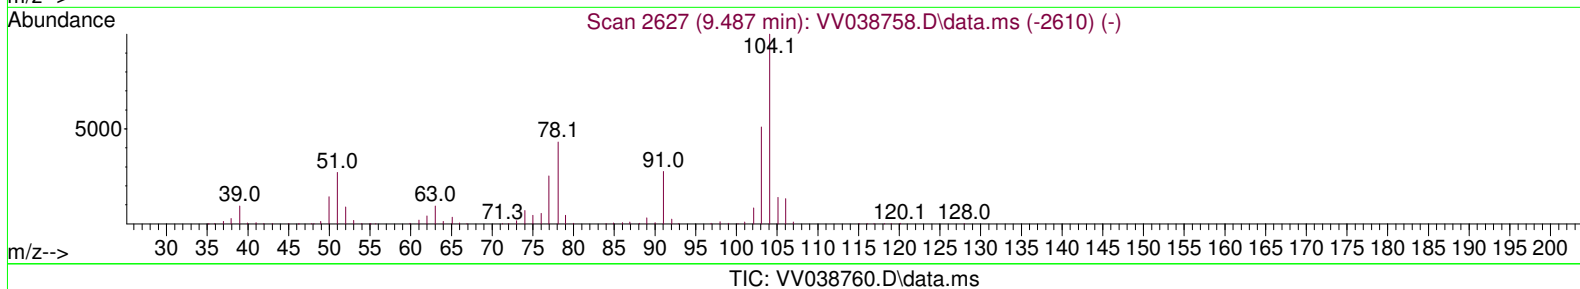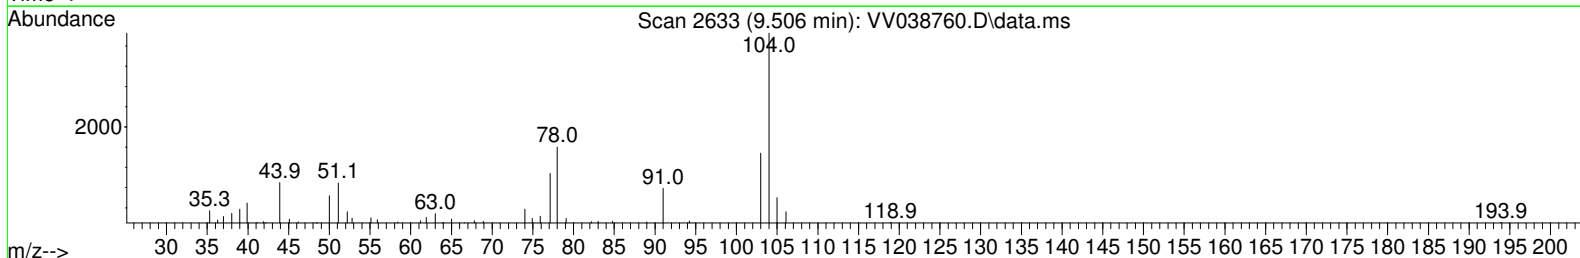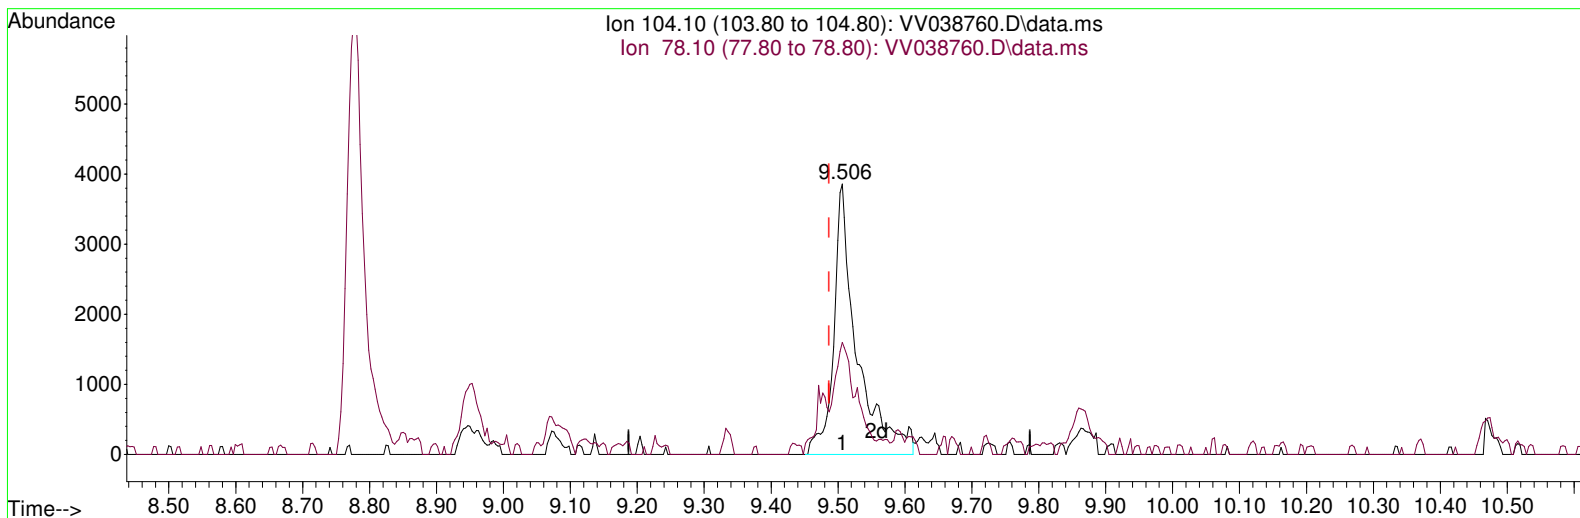

(55) Styrene (T)

9.506min (+ 0.019) 0.16 ug/L m

response 9231

Ion	Exp%	Act%
104.10	100.00	100.00
78.10	43.60	41.46
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

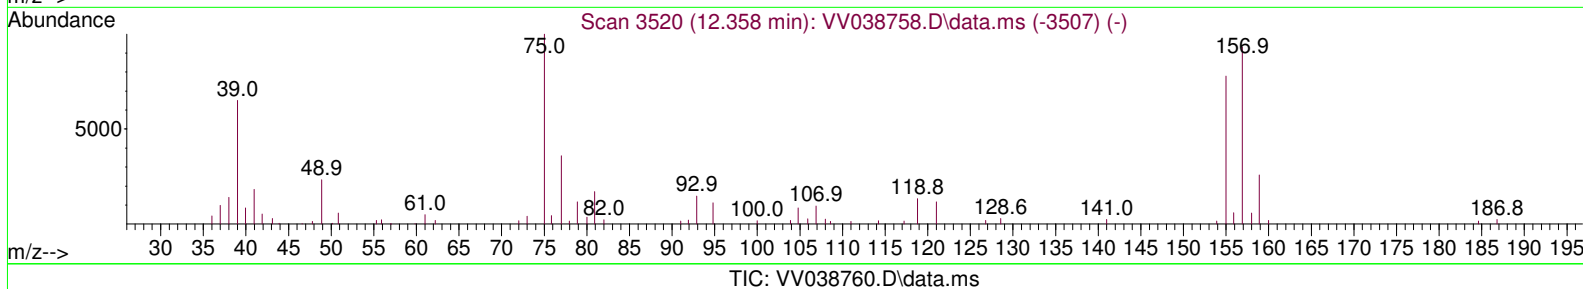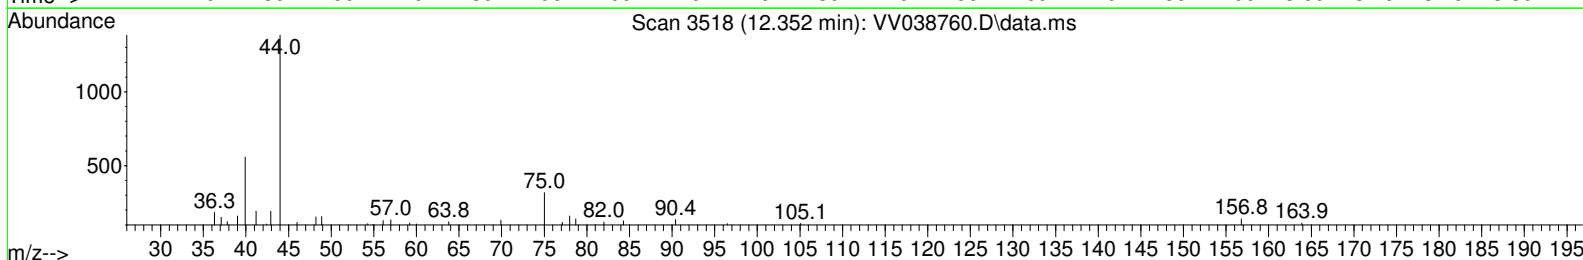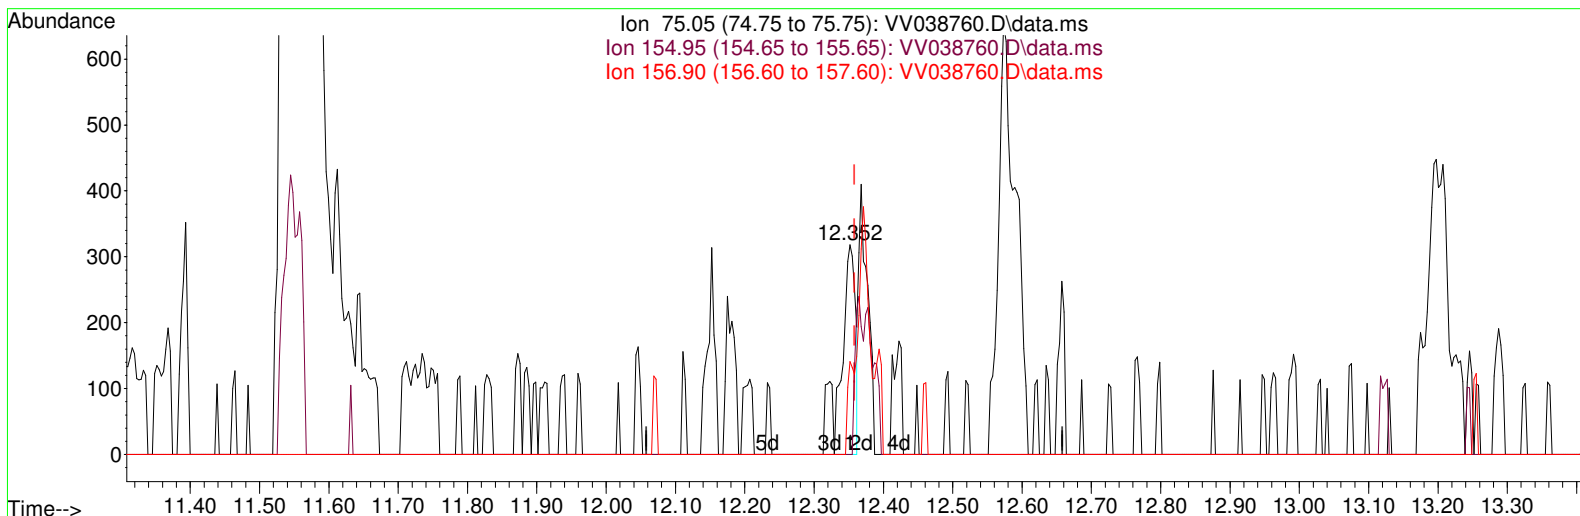

(68) 1,2-Dibromo-3-chloropropane (T)

12.352min (-0.006) 0.18 ug/L

response 392

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	75.40	0.00#
156.90	96.10	44.34#
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038760.D
Acq On : 06 Jun 2025 10:55
Operator : SY/MD
Sample : Q2117-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
MDL-WATER-QT2-2025-04

Manual IntegrationsAPPROVED

Reviewed By :Amit Patel 06/13/2025
Supervised By :Mahesh Dadoda 06/13/2025

Quant Time: Jun 13 10:57:49 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Jun 13 10:50:34 2025
Response via : Initial Calibration

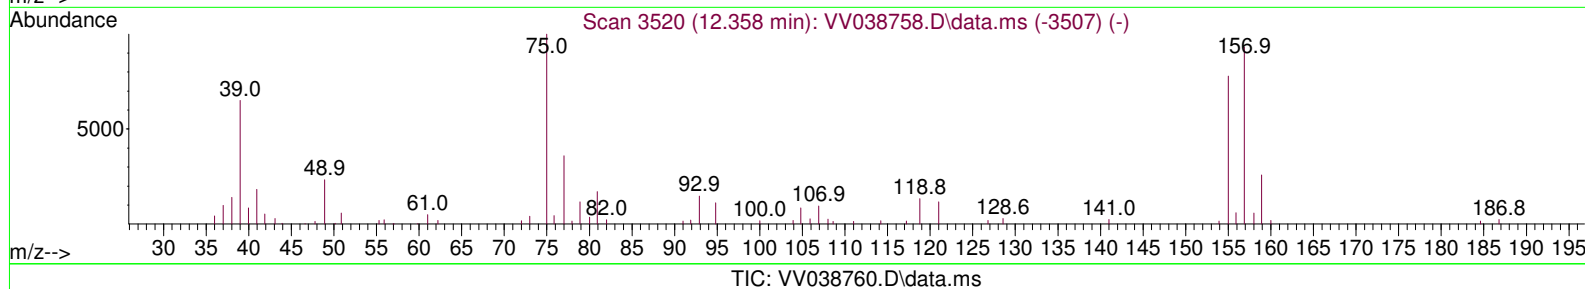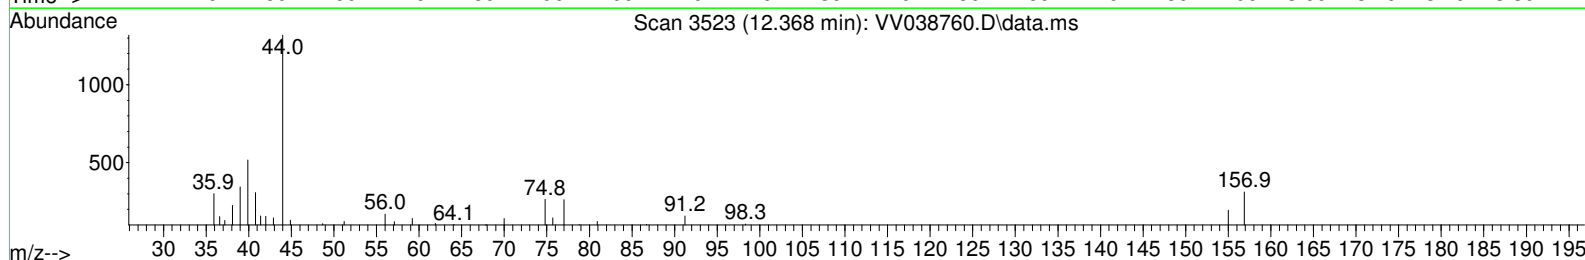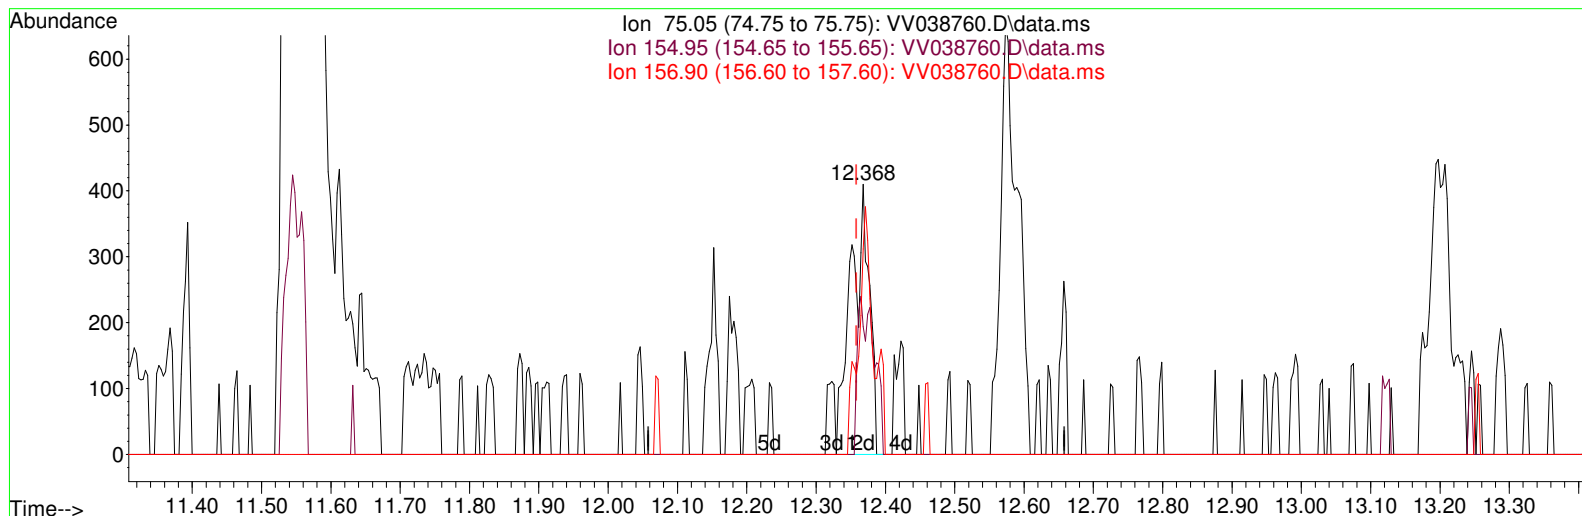

(68) 1,2-Dibromo-3-chloropropane (T)

12.368min (+ 0.010) 0.34 ug/L m

response 758

Ion	Exp%	Act%
75.05	100.00	100.00
154.95	75.40	73.21
156.90	96.10	117.74#
0.00	0.00	0.00