
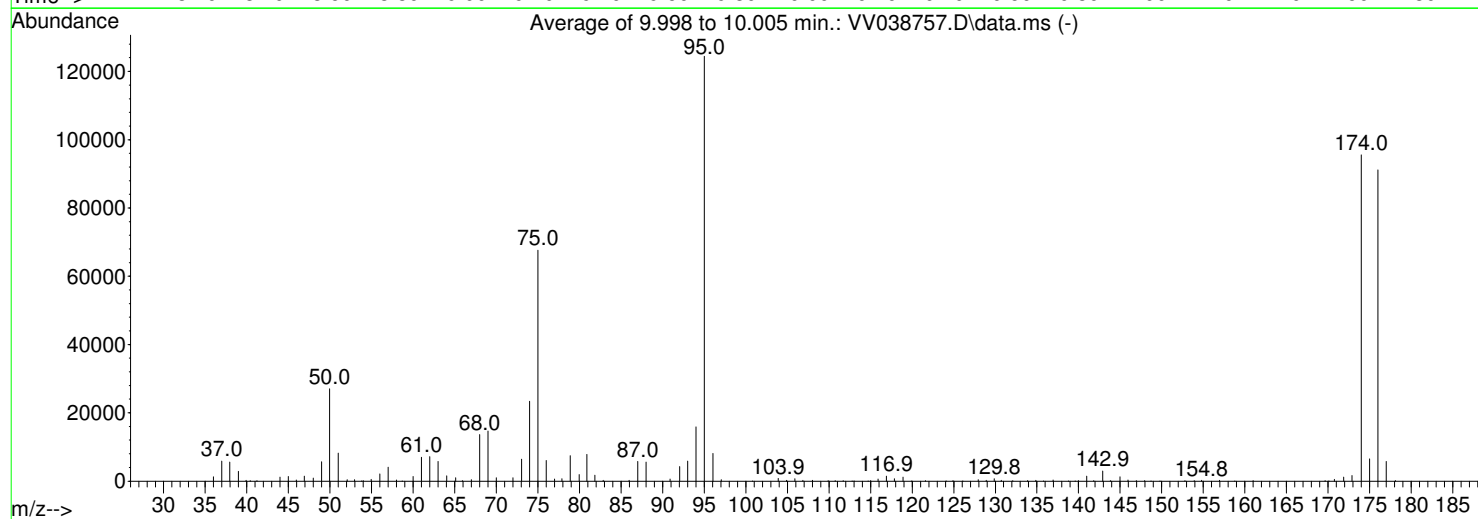


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV060625\
Data File : VV038757.D
Acq On : 06 Jun 2025 07:58
Operator : SY/MD
Sample : BFB208
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB208

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR060425WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Jun 13 10:50:34 2025

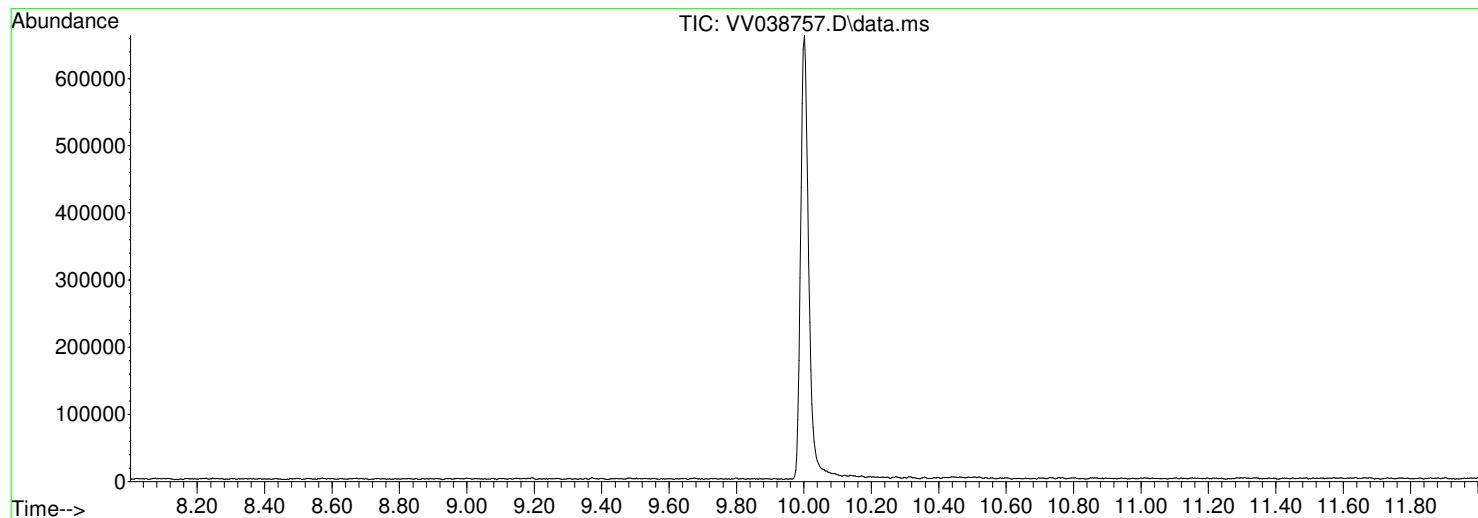

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2774

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	21.7	27035	PASS
75	95	30	80	54.3	67613	PASS
95	95	100	100	100.0	124429	PASS
96	95	5	9	6.5	8084	PASS
173	174	0.00	2	1.7	1668	PASS
174	95	50	120	76.8	95555	PASS
175	174	5	9	6.8	6477	PASS
176	174	95	105	95.4	91120	PASS
177	176	5	10	6.4	5793	PASS

m/z	Abundance
35.40	134.0
36.20	129.0
37.00	107.0
37.90	130.0
39.10	207.0
39.90	388.0
41.70	118.0
43.00	137.0
44.00	726.0
45.00	144.0
47.10	141.0
49.80	141.0
51.00	108.0
57.00	110.0
59.10	108.0
63.20	101.0
67.00	121.0
74.40	189.0
77.00	154.0
77.90	105.0
81.80	101.0
109.00	107.0
119.50	112.0
200.70	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.10	191.0
36.00	1669.0
37.00	6228.0
38.00	5704.0
39.00	3141.0
40.00	633.0
41.10	189.0
41.90	102.0
43.00	173.0
44.00	1767.0
45.00	1563.0
45.90	312.0
46.90	1672.0
48.00	956.0
49.00	5967.0
50.00	27376.0
51.00	8425.0
52.20	420.0
53.00	422.0
53.80	197.0
54.90	496.0
56.00	2091.0
57.00	4263.0
57.90	331.0
58.70	105.0
60.00	1368.0
61.00	7089.0
62.00	6976.0
63.00	5921.0
64.00	1771.0
65.10	1037.0
66.00	186.0
67.10	475.0
68.00	14011.0
69.00	14897.0
70.00	1012.0
72.00	944.0
73.00	6436.0
74.00	23632.0
75.00	67696.0
76.00	6340.0
76.90	866.0
78.00	739.0
78.90	7754.0
79.90	1904.0
80.90	7643.0
81.90	1641.0
82.80	208.0
85.90	331.0
87.00	5167.0
88.00	5696.0
90.90	532.0
92.00	4316.0
93.00	5956.0
94.00	16361.0
95.00	125512.0
96.00	8458.0
97.10	485.0
103.90	778.0
104.90	217.0
105.90	608.0
106.90	189.0
108.00	287.0
109.90	118.0
110.70	143.0
111.70	139.0
112.80	130.0
115.00	267.0
115.90	554.0
116.90	1518.0
117.90	669.0
118.90	1194.0
121.60	123.0
124.10	127.0
124.90	120.0
128.00	452.0
128.90	256.0
129.90	692.0
130.70	246.0
132.10	122.0
134.00	104.0
134.80	233.0
135.80	166.0
137.00	335.0
138.90	119.0
139.60	132.0
140.00	143.0
141.00	1417.0
141.90	184.0
142.90	3068.0
143.90	158.0
145.00	1263.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

146.00	309.0
146.90	112.0
147.90	165.0
148.70	122.0
153.80	144.0
154.80	283.0
156.90	268.0
161.00	187.0
169.60	128.0
170.10	122.0
170.70	511.0
171.90	1120.0
172.90	1623.0
174.00	93912.0
175.00	6804.0
176.00	87936.0
177.00	5786.0
178.10	198.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
35.20	187.0
36.00	1444.0
37.00	6163.0
38.00	5914.0
39.00	3093.0
39.90	603.0
41.20	137.0
41.70	102.0
43.00	145.0
44.00	1917.0
45.00	1541.0
46.00	332.0
46.90	1626.0
48.00	998.0
49.00	5799.0
50.00	28280.0
51.00	8632.0
52.00	372.0
53.00	411.0
54.00	244.0
55.00	516.0
56.00	2124.0
57.00	4328.0
58.00	285.0
60.00	1378.0
61.00	7342.0
62.00	7405.0
63.00	5974.0
64.00	1541.0
65.10	1027.0
65.90	174.0
67.00	560.0
68.00	14184.0
69.00	15218.0
70.00	1038.0
72.00	998.0
73.00	6583.0
74.00	24216.0
75.00	69616.0
76.00	6118.0
77.00	771.0
77.90	896.0
78.90	7692.0
80.00	1981.0
80.90	8061.0
81.90	1849.0
82.90	278.0
85.90	292.0
87.00	5886.0
88.00	5847.0
90.90	585.0
92.00	4343.0
93.00	6060.0
94.00	16464.0
95.00	127976.0
96.10	8409.0
97.10	439.0
100.80	115.0
103.90	883.0
104.90	276.0
105.90	685.0
106.80	212.0
108.00	290.0
109.90	135.0
110.80	188.0
111.70	170.0
112.80	128.0
115.00	240.0
115.90	598.0
116.90	1455.0
117.80	693.0
118.90	1199.0
119.90	128.0
121.60	155.0
124.10	139.0
124.90	154.0
128.00	484.0
128.90	205.0
129.80	745.0
130.70	241.0
132.10	128.0
133.80	133.0
134.80	202.0
135.80	118.0
137.00	291.0
140.00	150.0
141.00	1483.0
141.80	177.0
142.90	3067.0
143.80	165.0
145.00	1337.0
145.90	335.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

147.00	149.0
147.90	173.0
148.70	105.0
149.80	108.0
152.80	144.0
153.90	159.0
154.80	293.0
157.00	257.0
158.80	113.0
161.00	180.0
169.60	144.0
170.80	546.0
171.90	1311.0
172.90	1731.0
174.00	98688.0
175.00	6648.0
176.00	94016.0
177.00	5979.0
178.10	132.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

m/z	Abundance
36.00	1126.0
37.00	5521.0
38.00	5646.0
39.00	2846.0
39.90	510.0
40.40	432.0
41.30	139.0
41.80	118.0
44.00	1947.0
45.00	1387.0
46.00	341.0
46.90	1614.0
48.00	861.0
49.00	5224.0
50.00	25872.0
51.00	7926.0
51.90	404.0
52.90	357.0
54.00	321.0
55.00	447.0
56.00	2005.0
57.00	3926.0
58.10	269.0
60.00	1329.0
61.00	6518.0
62.00	7082.0
63.00	5692.0
64.10	1400.0
65.10	1001.0
65.80	200.0
67.00	512.0
68.00	12800.0
69.00	13901.0
70.00	974.0
72.00	969.0
73.10	6324.0
74.00	22232.0
75.00	65528.0
76.00	5638.0
77.10	671.0
78.00	937.0
78.90	7053.0
80.00	1830.0
80.90	7786.0
81.90	1931.0
82.90	286.0
86.00	236.0
87.00	6111.0
88.00	5221.0
90.90	589.0
92.10	4184.0
93.00	5670.0
94.00	14936.0
95.00	119800.0
96.10	7386.0
97.00	354.0
100.80	146.0
103.90	803.0
104.90	317.0
105.90	746.0
106.80	212.0
108.00	201.0
109.90	127.0
110.80	230.0
111.70	131.0
113.00	125.0
114.70	221.0
115.90	585.0
116.90	1347.0
117.80	658.0
118.90	1106.0
119.90	138.0
121.60	135.0
124.90	122.0
126.10	102.0
127.90	405.0
128.90	166.0
129.80	620.0
130.70	202.0
132.10	107.0
133.80	144.0
134.90	197.0
136.90	241.0
138.70	110.0
140.00	168.0
141.00	1407.0
142.90	2650.0
143.90	173.0
145.00	1308.0
145.90	328.0
147.00	145.0
148.00	200.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208

149.80	122.0
152.80	176.0
154.00	209.0
154.80	266.0
157.00	219.0
158.80	160.0
161.00	175.0
169.70	118.0
170.80	542.0
171.90	1218.0
172.90	1651.0
174.00	94064.0
175.00	5979.0
176.00	91408.0
177.00	5614.0

Instrument :
MSVOA_V
ClientSampleId :
BFB208