

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021522.D
 Acq On : 07 Jun 2021 12:12
 Operator : SY/MD
 Sample : M2596-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 08 03:18:02 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 08 03:17:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	470749	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	446346	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	254628	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	159412	51.434	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	102.860%	
7) Chloroethane-d5	1.568	69	113472	49.217	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	98.440%	
11) 1,1-Dichloroethene-d2	2.108	63	206060	38.909	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	77.820%	
21) 2-Butanone-d5	3.886	46	229440	103.236	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	103.240%	
24) Chloroform-d	4.352	84	297677	48.248	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.500%	
26) 1,2-Dichloroethane-d4	5.034	65	178241	50.157	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	100.320%	
32) Benzene-d6	5.053	84	618888	49.564	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	99.120%	
36) 1,2-Dichloropropane-d6	6.072	67	188618	48.914	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	97.820%	
41) Toluene-d8	7.317	98	592721	49.824	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	99.640%	
43) trans-1,3-Dichloroprop...	7.622	79	100806	48.849	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	97.700%	
47) 2-Hexanone-d5	8.088	63	180417	101.894	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	101.890%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	268346	50.133	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	100.260%	
66) 1,2-Dichlorobenzene-d4	11.625	152	261845	49.470	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	98.940%	
Target Compounds						Qvalue
44) trans-1,3-Dichloropropene	7.622	75	4108	0.793	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021522.D
Acq On : 07 Jun 2021 12:12
Operator : SY/MD
Sample : M2596-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Jun 08 03:18:02 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 08 03:17:01 2021
Response via : Initial Calibration

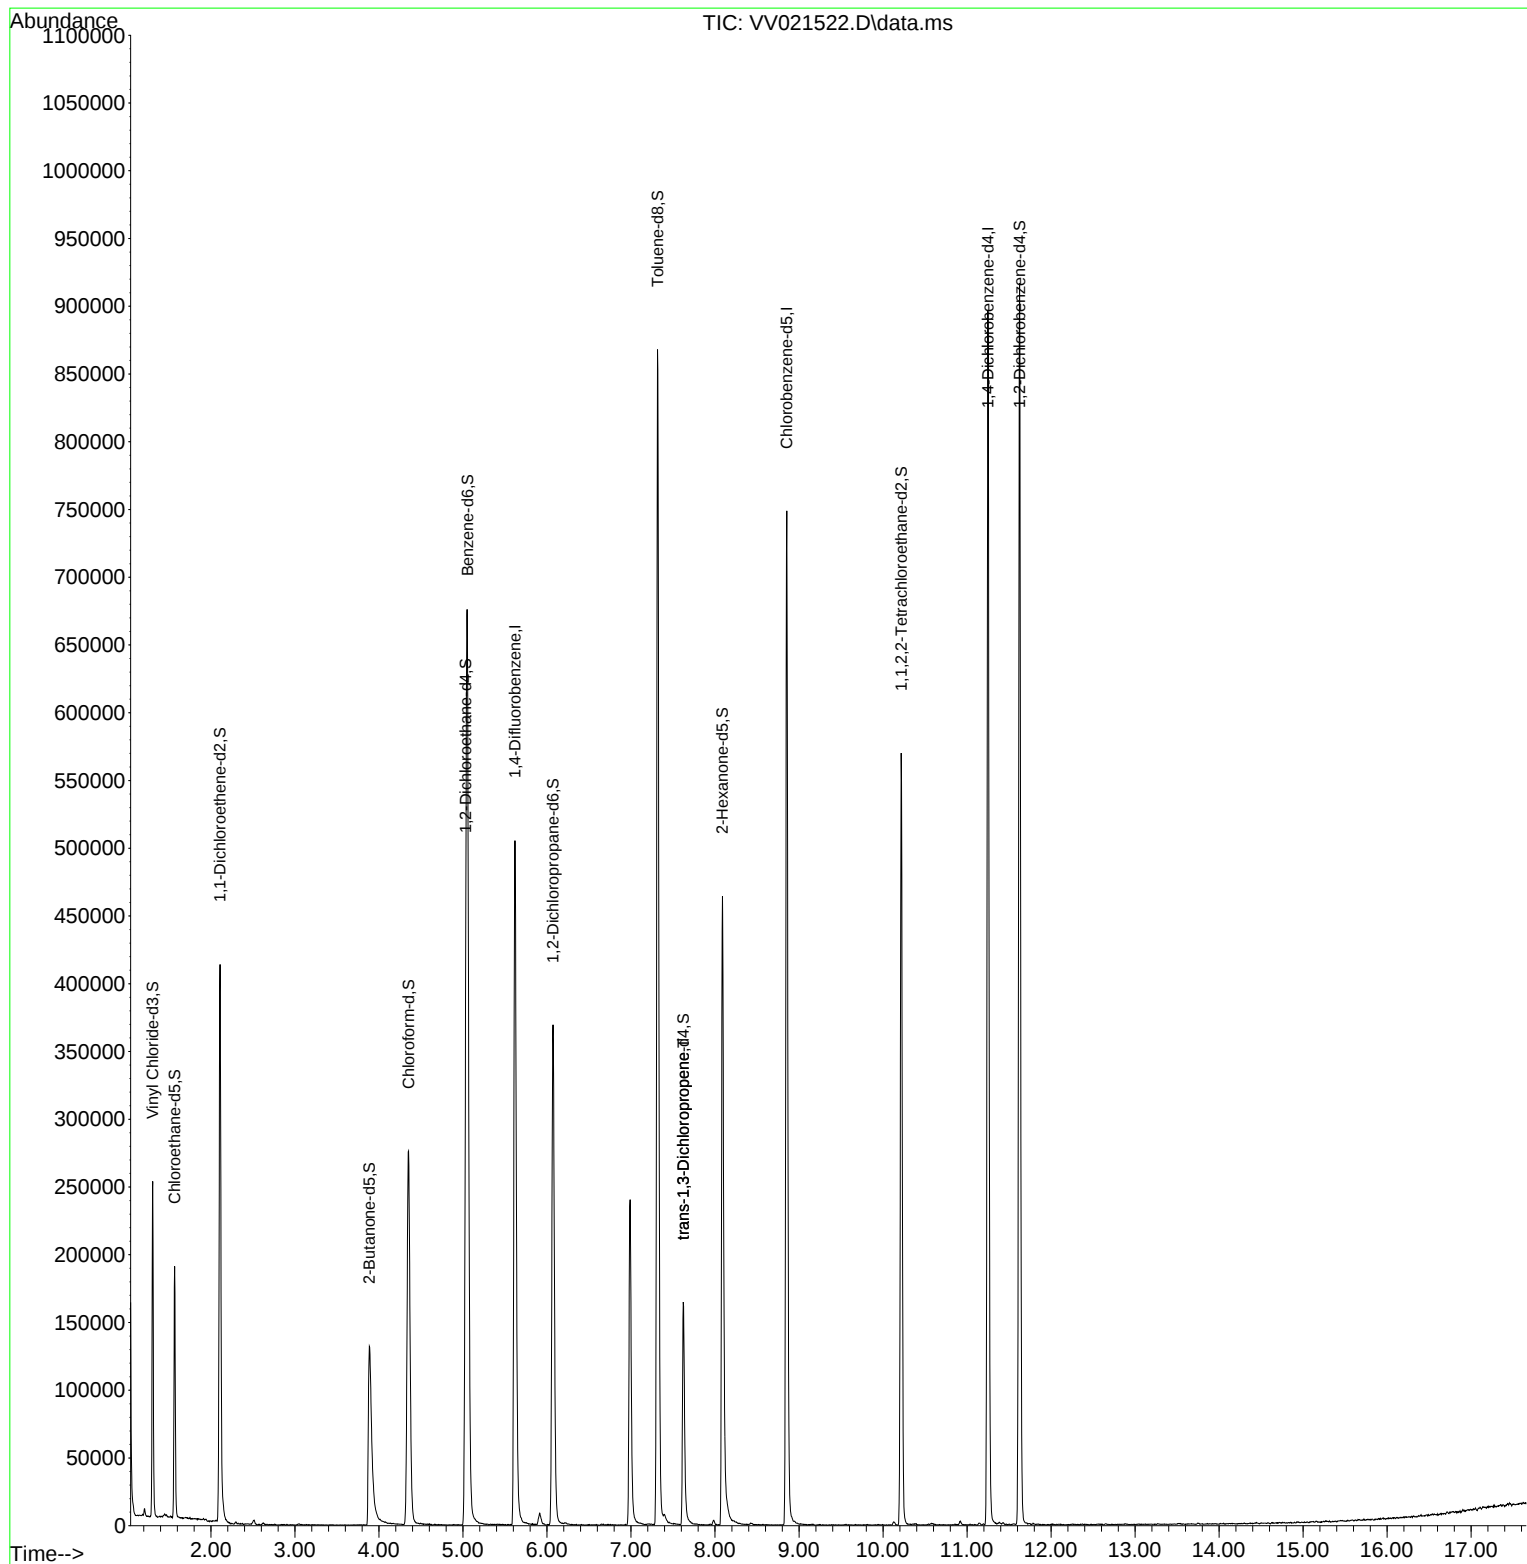

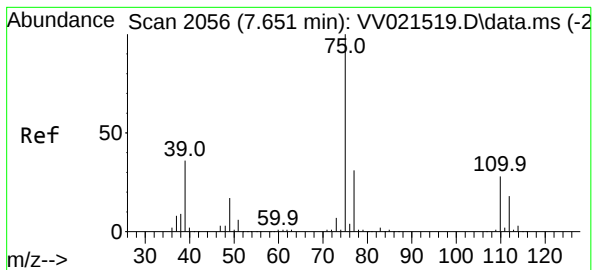

#44
 trans-1,3-Dichloropropene
 Concen: 0.793 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.029 min
 Lab File: VV021522.D
 Acq: 07 Jun 2021 12:12

Instrument :
 MSVOA_V
 ClientSampleId :

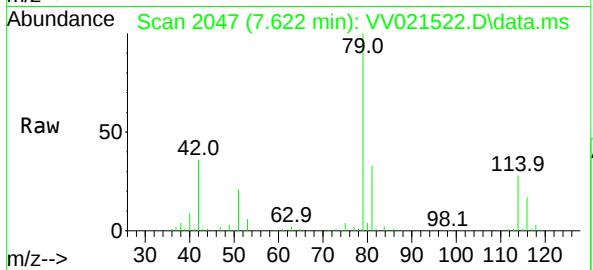

Tgt Ion: 75 Resp: 4108
 Ion Ratio Lower Upper
 75 100
 77 41.3 22.9 42.5

