

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021529.D
 Acq On : 07 Jun 2021 14:58
 Operator : SY/MD
 Sample : M2605-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 08 03:19:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 08 03:17:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	448160	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	427809	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	249330	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	150436	50.984	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	101.960%
7) Chloroethane-d5	1.565	69	95267	43.403	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	86.800%
11) 1,1-Dichloroethene-d2	2.108	63	193703	38.419	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	76.840%
21) 2-Butanone-d5	3.883	46	215882	102.032	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	102.030%
24) Chloroform-d	4.352	84	277173	47.189	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.380%
26) 1,2-Dichloroethane-d4	5.034	65	167258	49.439	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	98.880%
32) Benzene-d6	5.053	84	579225	48.398	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.800%
36) 1,2-Dichloropropane-d6	6.072	67	174365	47.178	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	94.360%
41) Toluene-d8	7.317	98	549020	48.150	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	96.300%
43) trans-1,3-Dichloroprop...	7.622	79	91397	46.209	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.420%
47) 2-Hexanone-d5	8.088	63	168747	99.432	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	99.430%
56) 1,1,2,2-Tetrachloroeth...	10.217	84	246989	48.142	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	96.280%
66) 1,2-Dichlorobenzene-d4	11.625	152	245945	47.453	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	94.900%
Target Compounds						
					Qvalue	
39) cis-1,3-Dichloropropene	6.989	75	5513	1.050	ug/L #	52
61) 1,2,3-Trichloropropane	11.249	75	21650	5.526	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021529.D
Acq On : 07 Jun 2021 14:58
Operator : SY/MD
Sample : M2605-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Jun 08 03:19:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 08 03:17:01 2021
Response via : Initial Calibration




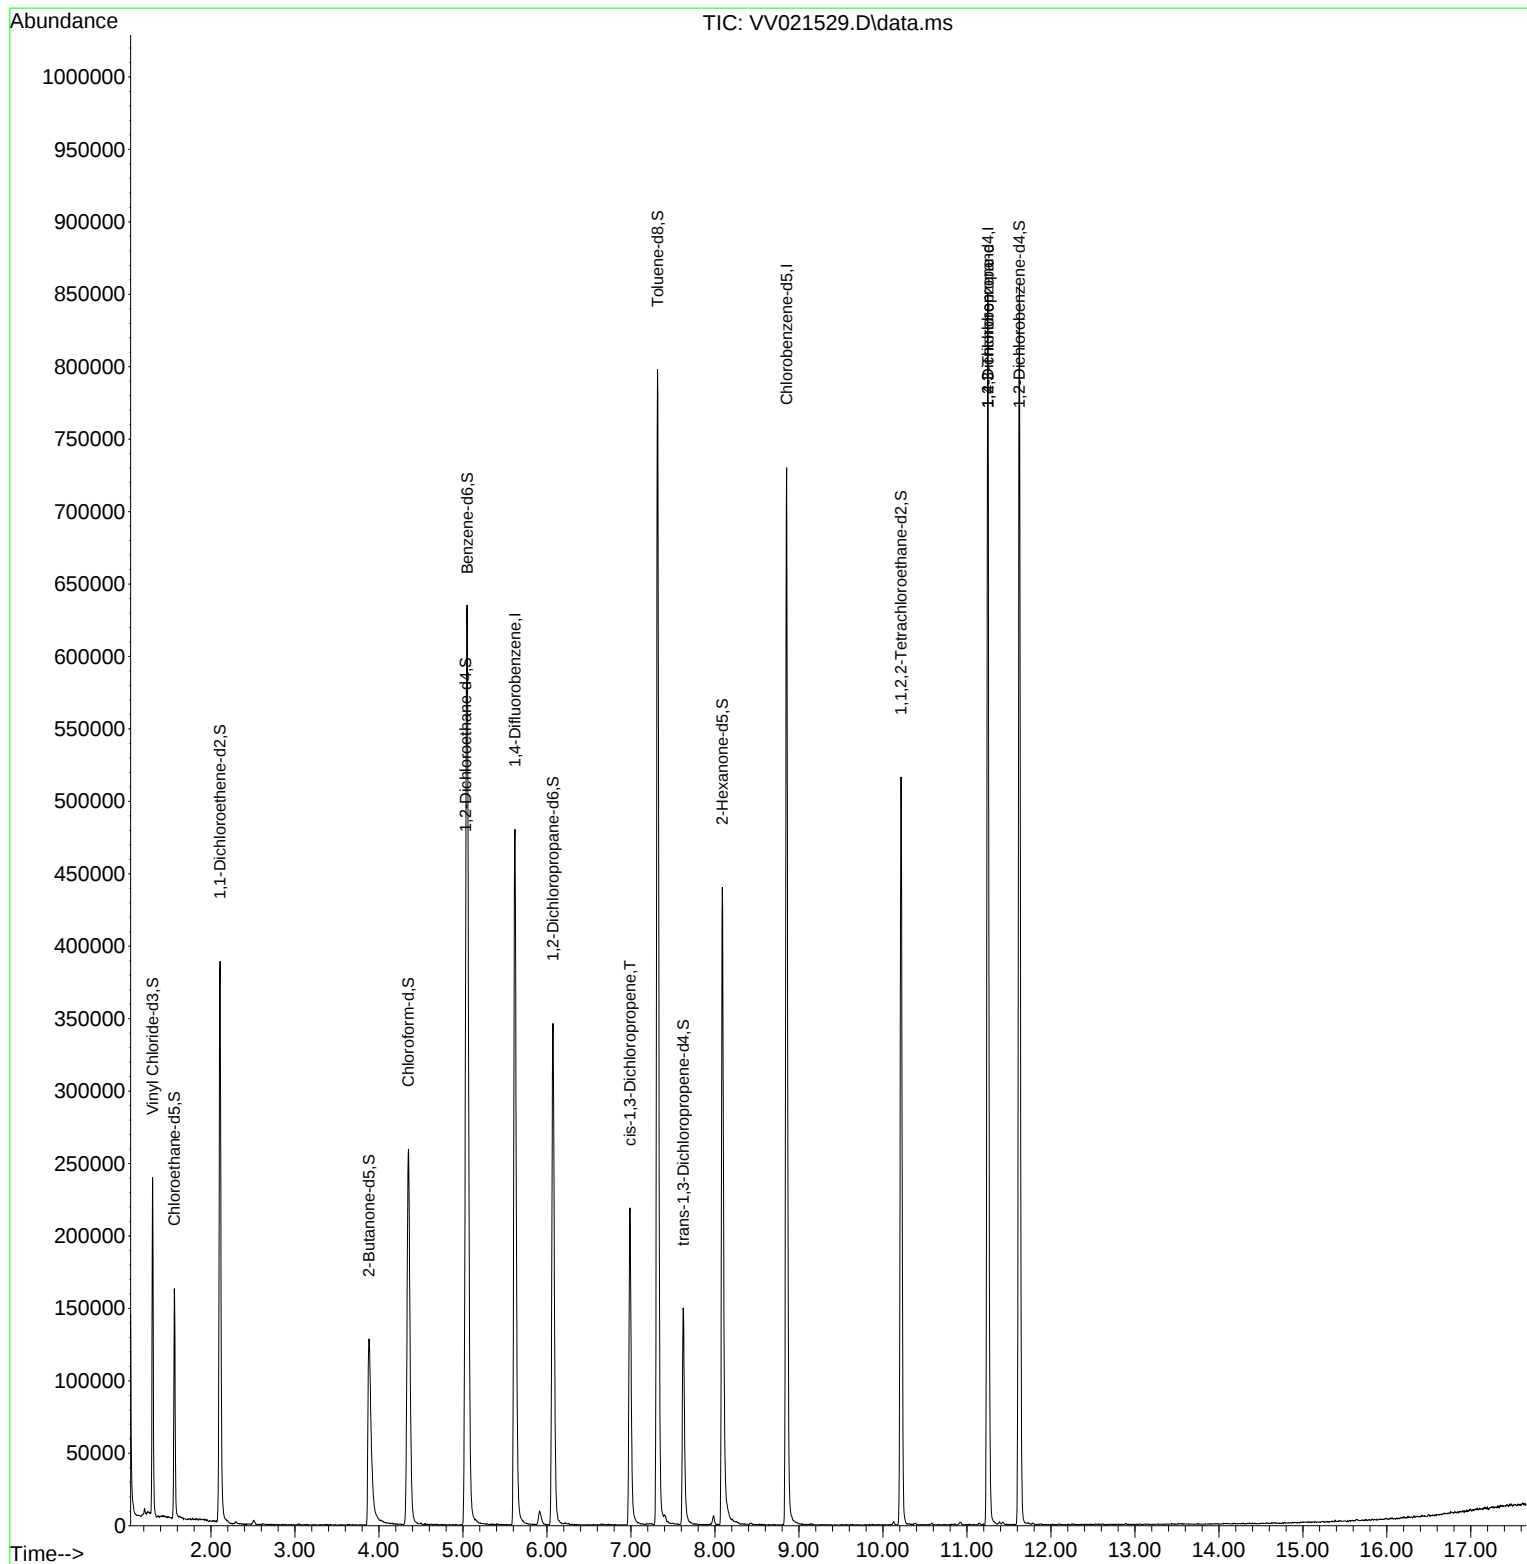


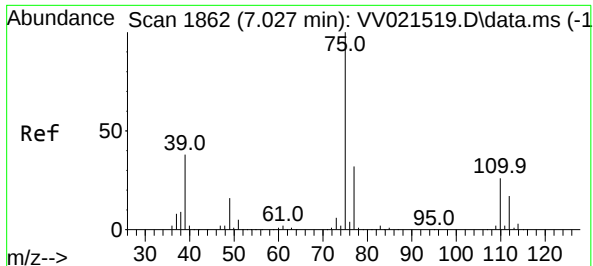

#39
 cis-1,3-Dichloropropene
 Concen: 1.050 ug/L
 RT: 6.989 min Scan# 1850
 Delta R.T. -0.038 min
 Lab File: VV021529.D
 Acq: 07 Jun 2021 14:58

Instrument :
 MSVOA_V
 ClientSampled :

Tgt Ion: 75 Resp: 5513
 Ion Ratio Lower Upper
 75 100
 77 58.1 22.0 41.0#

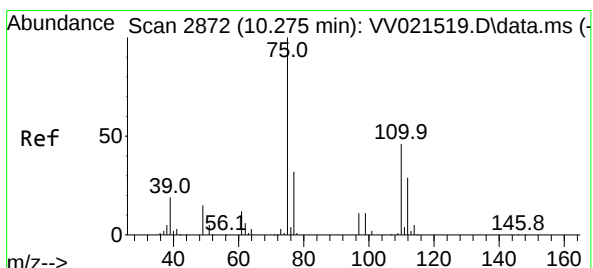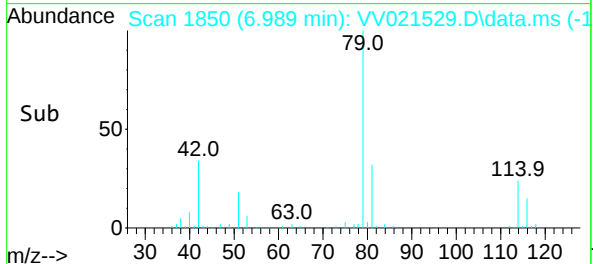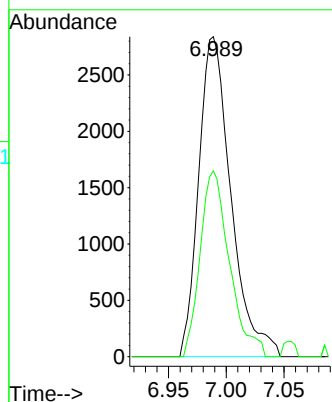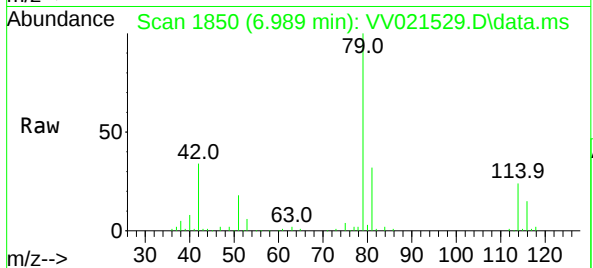

#61
 1,2,3-Trichloropropane
 Concen: 5.526 ug/L
 RT: 11.249 min Scan# 3175
 Delta R.T. 0.974 min
 Lab File: VV021529.D
 Acq: 07 Jun 2021 14:58

Tgt Ion: 75 Resp: 21650
 Ion Ratio Lower Upper
 75 100
 77 34.2 25.9 38.9
 110 3.1 34.8 52.2#

