

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060721\
 Data File : VW021530.D
 Acq On : 07 Jun 2021 15:35
 Operator : SY/MD
 Sample : M2618-08ME
 Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampled :

Quant Time: Jun 08 03:19:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 08 03:17:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	521217	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	499809	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.252	152	286884	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	160108	46.656	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery =	93.320%		
7) Chloroethane-d5	1.564	69	76273	29.879	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery =	59.760%#		
11) 1,1-Dichloroethene-d2	2.088	63	200637	34.216	ug/L	-0.02
Spiked Amount	50.000	Range 60 - 125	Recovery =	68.440%		
21) 2-Butanone-d5	3.892	46	141032	57.313	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery =	57.310%		
24) Chloroform-d	4.342	84	292559	42.827	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	85.660%		
26) 1,2-Dichloroethane-d4	5.027	65	178102	45.265	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	90.540%		
32) Benzene-d6	5.043	84	608724	43.536	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery =	87.080%		
36) 1,2-Dichloropropane-d6	6.066	67	183684	42.540	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery =	85.080%		
41) Toluene-d8	7.313	98	591227	44.383	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	88.760%		
43) trans-1,3-Dichloroprop...	7.622	79	99685	43.139	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery =	86.280%		
47) 2-Hexanone-d5	8.117	63	151660	76.491	ug/L	0.03
Spiked Amount	100.000	Range 45 - 130	Recovery =	76.490%		
56) 1,1,2,2-Tetrachloroeth...	10.223	84	240807	40.176	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery =	80.360%		
66) 1,2-Dichlorobenzene-d4	11.628	152	257707	43.214	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery =	86.420%		
Target Compounds						
44) trans-1,3-Dichloropropene	7.622	75	3621	0.624	ug/L	95
61) 1,2,3-Trichloropropane	11.252	75	25862	5.737	ug/L #	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021530.D
 Acq On : 07 Jun 2021 15:35
 Operator : SY/MD
 Sample : M2618-08ME
 Misc : 4.90g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Jun 08 03:19:24 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 08 03:17:01 2021
 Response via : Initial Calibration




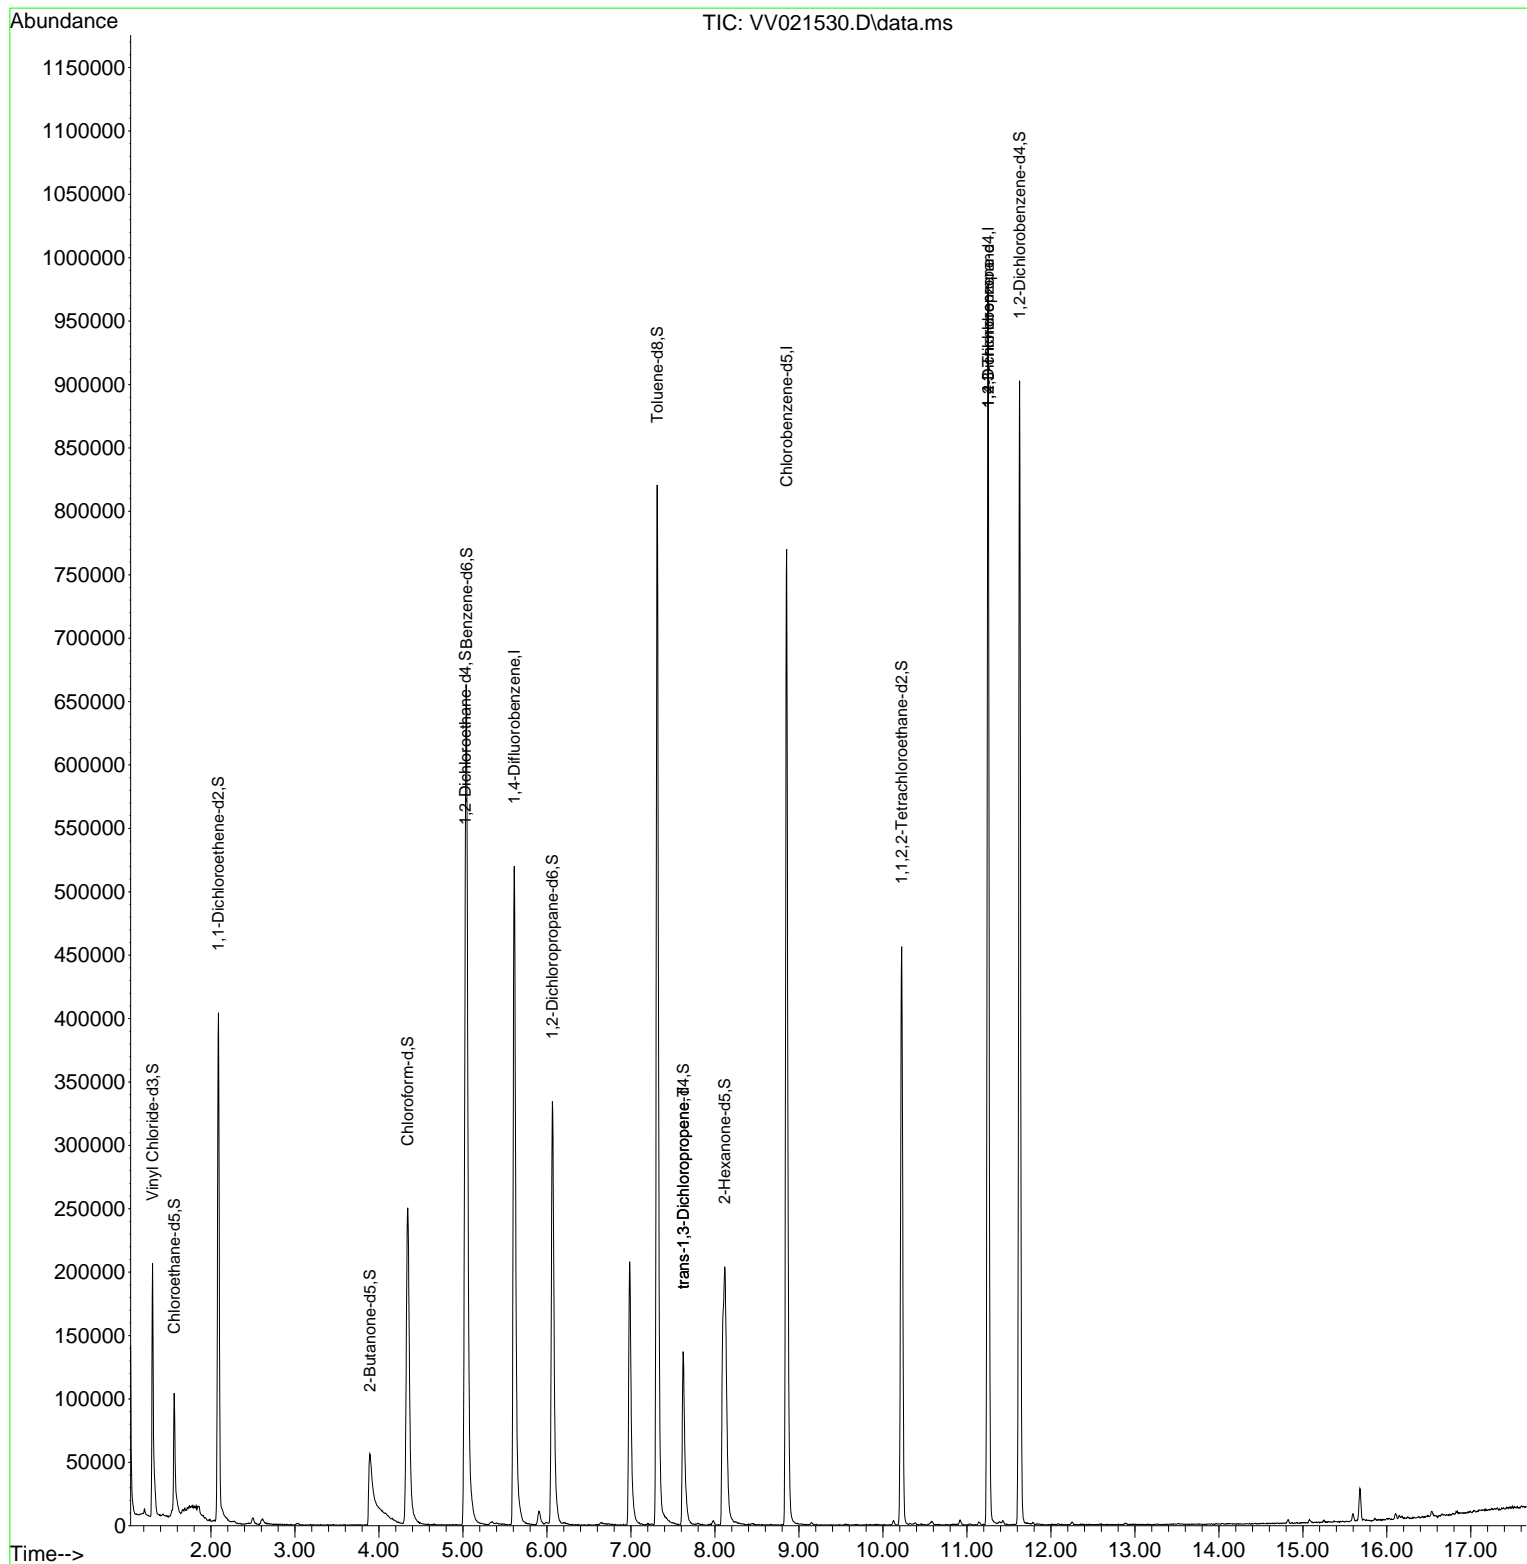


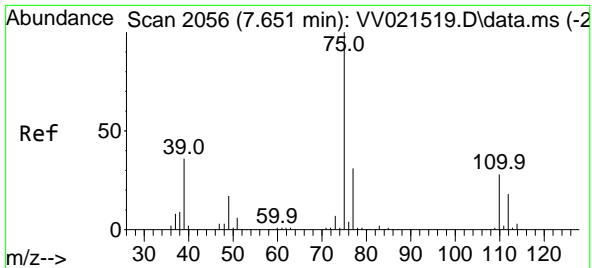

#44
 trans-1,3-Dichloropropene
 Concen: 0.624 ug/L
 RT: 7.622 min Scan# 2047
 Delta R.T. -0.029 min
 Lab File: VV021530.D
 Acq: 07 Jun 2021 15:35

Instrument : MSVOA_V
 ClientSampled :

Tgt Ion: 75 Resp: 3621
 Ion Ratio Lower Upper
 75 100
 77 35.5 22.9 42.5

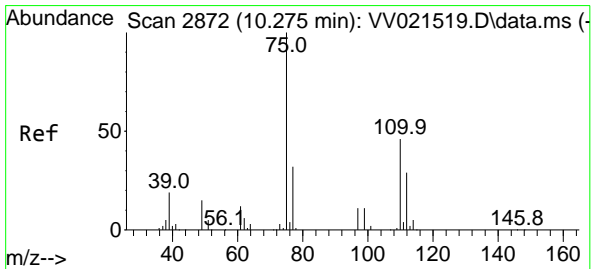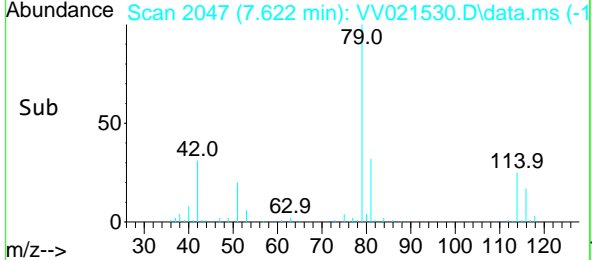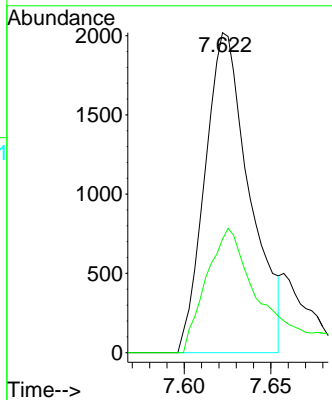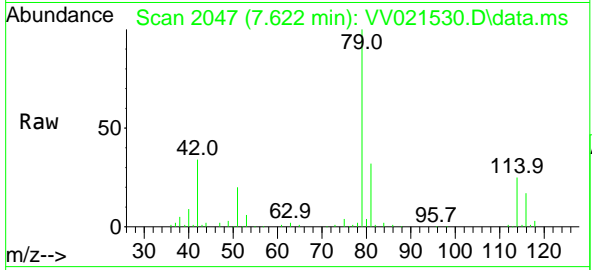

#61
 1,2,3-Trichloropropane
 Concen: 5.737 ug/L
 RT: 11.252 min Scan# 3176
 Delta R.T. 0.977 min
 Lab File: VV021530.D
 Acq: 07 Jun 2021 15:35

Tgt Ion: 75 Resp: 25862
 Ion Ratio Lower Upper
 75 100
 77 31.1 25.9 38.9
 110 2.8 34.8 52.2#

