

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021528.D
 Acq On : 07 Jun 2021 14:34
 Operator : SY/MD
 Sample : M2618-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Jun 08 03:19:05 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Jun 08 03:17:01 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	465070	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	438852	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	251502	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	154641	50.504	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	101.000%	
7) Chloroethane-d5	1.568	69	100367	44.064	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	88.120%	
11) 1,1-Dichloroethene-d2	2.108	63	197261	37.702	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	75.400%	
21) 2-Butanone-d5	3.883	46	206398	94.002	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	94.000%	
24) Chloroform-d	4.352	84	281000	46.101	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	92.200%	
26) 1,2-Dichloroethane-d4	5.034	65	171050	48.721	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	97.440%	
32) Benzene-d6	5.053	84	592495	48.261	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	96.520%	
36) 1,2-Dichloropropane-d6	6.072	67	178255	47.016	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	94.040%	
41) Toluene-d8	7.317	98	563645	48.189	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	96.380%	
43) trans-1,3-Dichloroprop...	7.622	79	95611	47.123	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	94.240%	
47) 2-Hexanone-d5	8.088	63	165662	95.158	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	95.160%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	248934	47.300	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	94.600%	
66) 1,2-Dichlorobenzene-d4	11.625	152	250518	47.918	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	95.840%	
Target Compounds						
					Qvalue	
46) Tetrachloroethene	7.985	164	2776	0.884	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021528.D
Acq On : 07 Jun 2021 14:34
Operator : SY/MD
Sample : M2618-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Jun 08 03:19:05 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 08 03:17:01 2021
Response via : Initial Calibration

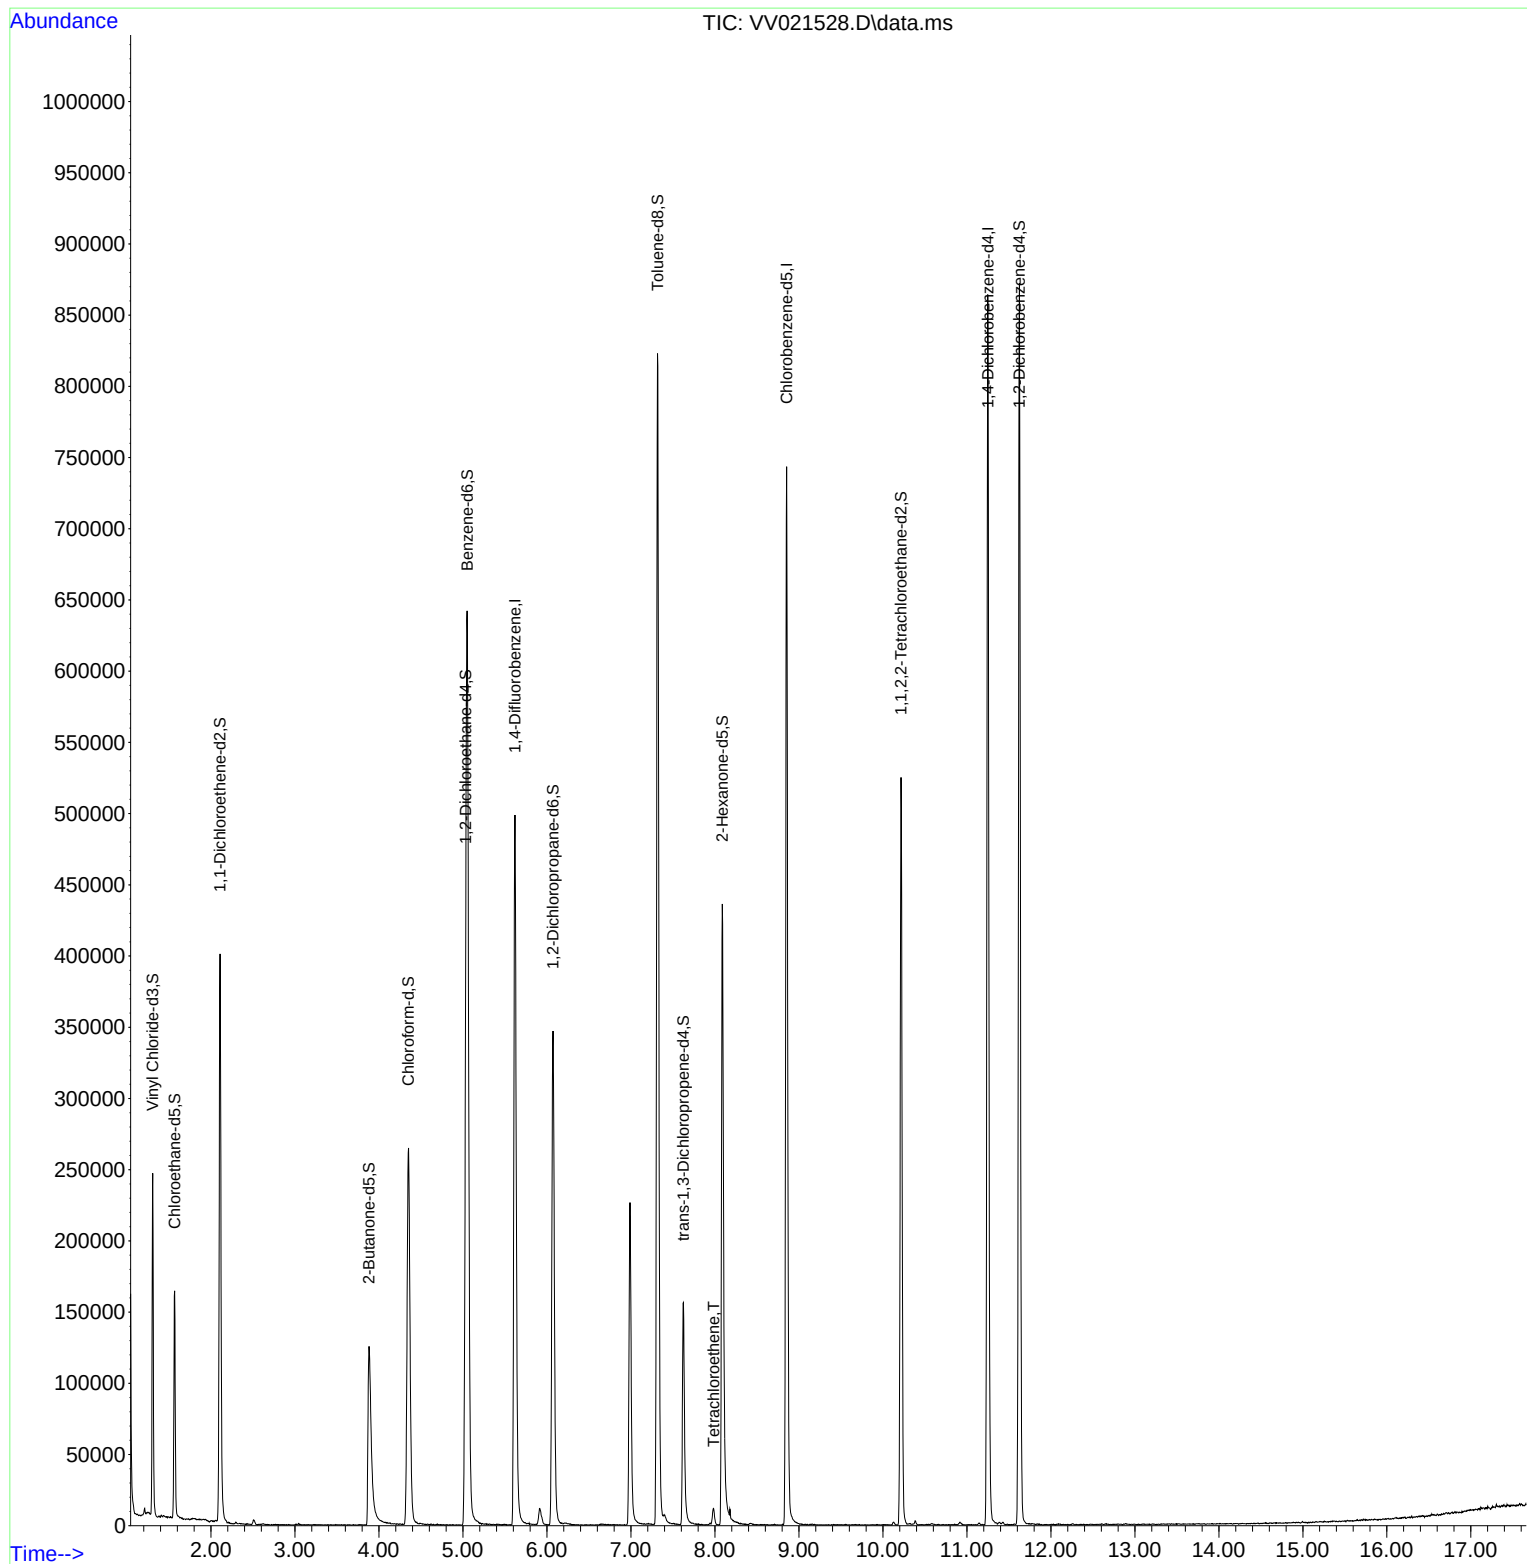

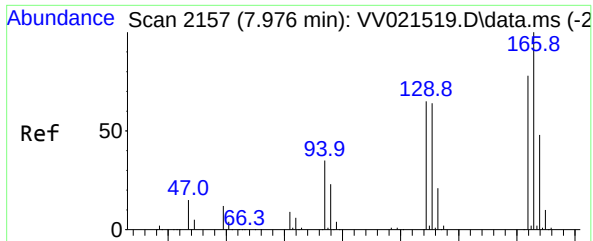

#46
Tetrachloroethene
Concen: 0.884 ug/L
RT: 7.985 min Scan# 2160
Delta R.T. 0.010 min
Lab File: VV021528.D
Acq: 07 Jun 2021 14:34

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

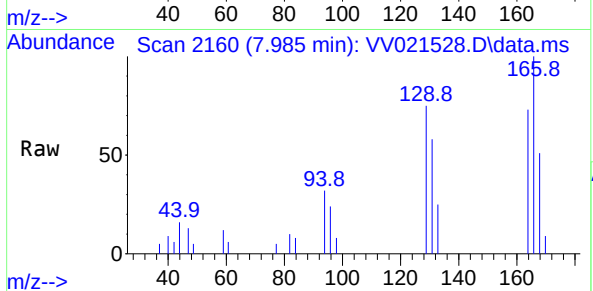

Tgt Ion:164 Resp: 2776

Ion	Ratio	Lower	Upper
164	100		
129	102.3	60.5	112.3
131	79.1	58.7	108.9
166	136.6	88.1	163.5

