

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021520.D
 Acq On : 07 Jun 2021 11:26
 Operator : SY/MD
 Sample : VV0607MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021520.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	277508	283060	15.30%	1.938%
2	1.568	157	164	174	rVB	204518	225658	12.20%	1.545%
3	2.105	322	331	357	rVB	455638	685338	37.05%	4.691%
4	2.510	448	457	464	rBV3	3323	5303	0.29%	0.036%
5	2.606	484	487	488	rBV	513	298	0.02%	0.002%
6	2.757	528	534	541	rBV4	1073	1473	0.08%	0.010%
7	2.796	544	546	548	rVB2	490	181	0.01%	0.001%
8	2.809	548	550	551	rBV2	281	99	0.01%	0.001%
9	2.880	570	572	574	rBV2	152	89	0.00%	0.001%
10	2.973	599	601	606	rBV3	298	286	0.02%	0.002%
11	3.092	636	638	639	rBV	195	89	0.00%	0.001%
12	3.143	652	654	656	rBV	285	121	0.01%	0.001%
13	3.188	666	668	671	rVB2	217	126	0.01%	0.001%
14	3.204	671	673	674	rBV2	232	119	0.01%	0.001%
15	3.336	710	714	717	rVV2	332	249	0.01%	0.002%
16	3.352	717	719	722	rVB3	235	122	0.01%	0.001%
17	3.388	728	730	731	rBV	285	101	0.01%	0.001%
18	3.494	761	763	766	rVB	261	131	0.01%	0.001%
19	3.510	766	768	770	rVB	393	157	0.01%	0.001%
20	3.539	770	777	781	rBV2	264	407	0.02%	0.003%
21	3.561	781	784	785	rBV2	357	99	0.01%	0.001%
22	3.593	790	794	796	rBV2	437	274	0.01%	0.002%
23	3.728	834	836	837	rBV	215	92	0.00%	0.001%
24	3.767	845	848	852	rBV3	440	329	0.02%	0.002%
25	3.841	868	871	873	rVB2	217	99	0.01%	0.001%
26	3.879	873	883	924	rBV	125532	383914	20.76%	2.628%
27	4.346	1011	1028	1056	rBV	291216	725415	39.22%	4.966%
28	4.564	1092	1096	1100	rBV4	606	504	0.03%	0.003%
29	4.760	1155	1157	1161	rVB2	417	234	0.01%	0.002%
30	4.815	1171	1174	1176	rVB2	427	179	0.01%	0.001%
31	4.905	1200	1202	1204	rBV2	281	134	0.01%	0.001%
32	5.043	1227	1245	1277	rBV2	723772	1849562	100.00%	12.661%
33	5.445	1369	1370	1376	rVB2	464	367	0.02%	0.003%
34	5.613	1409	1422	1454	rBV	546204	1093818	59.14%	7.487%
35	5.908	1503	1514	1529	rBV4	9146	18961	1.03%	0.130%
36	6.014	1546	1547	1549	rBV2	383	106	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021520.D
 Acq On : 07 Jun 2021 11:26
 Operator : SY/MD
 Sample : VV0607MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.066	1549	1563	1588	rBV	390552	798907	43.19%	5.469%
38	6.320	1639	1642	1644	rVB4	441	266	0.01%	0.002%
39	6.330	1644	1645	1647	rBV	275	124	0.01%	0.001%
40	6.426	1673	1675	1680	rVB2	333	211	0.01%	0.001%
41	6.490	1693	1695	1701	rVB2	363	364	0.02%	0.002%
42	6.522	1701	1705	1706	rVV2	229	128	0.01%	0.001%
43	6.545	1709	1712	1719	rVB3	609	619	0.03%	0.004%
44	6.606	1729	1731	1732	rBV3	340	86	0.00%	0.001%
45	6.635	1738	1740	1742	rBV	369	154	0.01%	0.001%
46	6.648	1742	1744	1745	rBV	371	213	0.01%	0.001%
47	6.715	1763	1765	1766	rBV	284	82	0.00%	0.001%
48	6.850	1804	1807	1809	rBV	173	83	0.00%	0.001%
49	6.876	1813	1815	1819	rVB	409	227	0.01%	0.002%
50	6.912	1823	1826	1830	rBV	304	299	0.02%	0.002%
51	6.982	1836	1848	1880	rBV	257255	468789	25.35%	3.209%
52	7.313	1938	1951	1971	rBV	932601	1603333	86.69%	10.975%
53	7.619	2036	2046	2077	rBV	177461	314352	17.00%	2.152%
54	7.886	2126	2129	2132	rBV2	449	392	0.02%	0.003%
55	7.924	2139	2141	2143	rBV2	335	189	0.01%	0.001%
56	7.979	2152	2158	2166	rVB4	2417	3208	0.17%	0.022%
57	8.018	2167	2170	2174	rVB3	238	192	0.01%	0.001%
58	8.085	2181	2191	2232	rBV	462120	831247	44.94%	5.690%
59	8.542	2331	2333	2335	rBV	217	131	0.01%	0.001%
60	8.638	2358	2363	2364	rBV	368	266	0.01%	0.002%
61	8.677	2373	2375	2379	rVB3	597	278	0.02%	0.002%
62	8.699	2379	2382	2383	rBV	251	138	0.01%	0.001%
63	8.709	2383	2385	2389	rVB2	268	123	0.01%	0.001%
64	8.741	2393	2395	2398	rBV2	436	221	0.01%	0.002%
65	8.850	2417	2429	2464	rBV	810544	1317303	71.22%	9.017%
66	9.117	2509	2512	2513	rVB2	443	200	0.01%	0.001%
67	9.127	2513	2515	2516	rBV2	466	204	0.01%	0.001%
68	9.140	2517	2519	2530	rVB4	1081	1247	0.07%	0.009%
69	9.265	2556	2558	2561	rBV2	250	91	0.00%	0.001%
70	9.294	2565	2567	2570	rVB	338	190	0.01%	0.001%
71	9.368	2587	2590	2594	rBV3	281	260	0.01%	0.002%
72	9.445	2612	2614	2617	rBV2	216	101	0.01%	0.001%
73	9.497	2627	2630	2634	rVB2	287	212	0.01%	0.001%
74	9.526	2636	2639	2640	rBV	439	178	0.01%	0.001%
75	9.635	2670	2673	2677	rBV3	422	340	0.02%	0.002%
76	9.673	2681	2685	2687	rBV3	480	312	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021520.D
 Acq On : 07 Jun 2021 11:26
 Operator : SY/MD
 Sample : VV0607MBL01
 Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK187

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.786	2718	2720	2725	rVB2	287	170	0.01%	0.001%
78	9.809	2725	2727	2729	rBV2	232	106	0.01%	0.001%
79	9.847	2735	2739	2741	rBV3	454	332	0.02%	0.002%
80	9.956	2772	2773	2775	rVB	449	124	0.01%	0.001%
81	9.995	2782	2785	2787	rBV	249	149	0.01%	0.001%
82	10.127	2819	2826	2834	rVB6	2492	4104	0.22%	0.028%
83	10.217	2840	2854	2874	rBV	569777	904376	48.90%	6.191%
84	10.448	2924	2926	2931	rVB3	403	285	0.02%	0.002%
85	10.474	2932	2934	2936	rBV2	208	83	0.00%	0.001%
86	10.529	2948	2951	2953	rBV2	588	404	0.02%	0.003%
87	10.657	2986	2991	2992	rBV	397	297	0.02%	0.002%
88	10.754	3019	3021	3023	rVB	457	169	0.01%	0.001%
89	10.850	3049	3051	3057	rVB2	737	618	0.03%	0.004%
90	10.876	3057	3059	3063	rVB	322	184	0.01%	0.001%
91	10.918	3065	3072	3085	rVB5	3724	5362	0.29%	0.037%
92	11.069	3116	3119	3123	rBV2	326	320	0.02%	0.002%
93	11.249	3163	3175	3206	rBV	969381	1493047	80.72%	10.220%
94	11.558	3270	3271	3272	rBV	427	89	0.00%	0.001%
95	11.622	3279	3291	3313	rBV	987466	1557521	84.21%	10.662%
96	11.915	3381	3382	3388	rBV2	394	303	0.02%	0.002%
97	12.648	3605	3610	3621	rVB8	2651	4021	0.22%	0.028%
98	12.924	3694	3696	3701	rBV4	620	474	0.03%	0.003%
99	13.268	3797	3803	3813	rVB5	3938	5451	0.29%	0.037%
100	13.513	3872	3879	3890	rVB2	5167	8087	0.44%	0.055%




Sum of corrected areas: 14608830

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021520.D
Acq On : 07 Jun 2021 11:26
Operator : SY/MD
Sample : VV0607MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

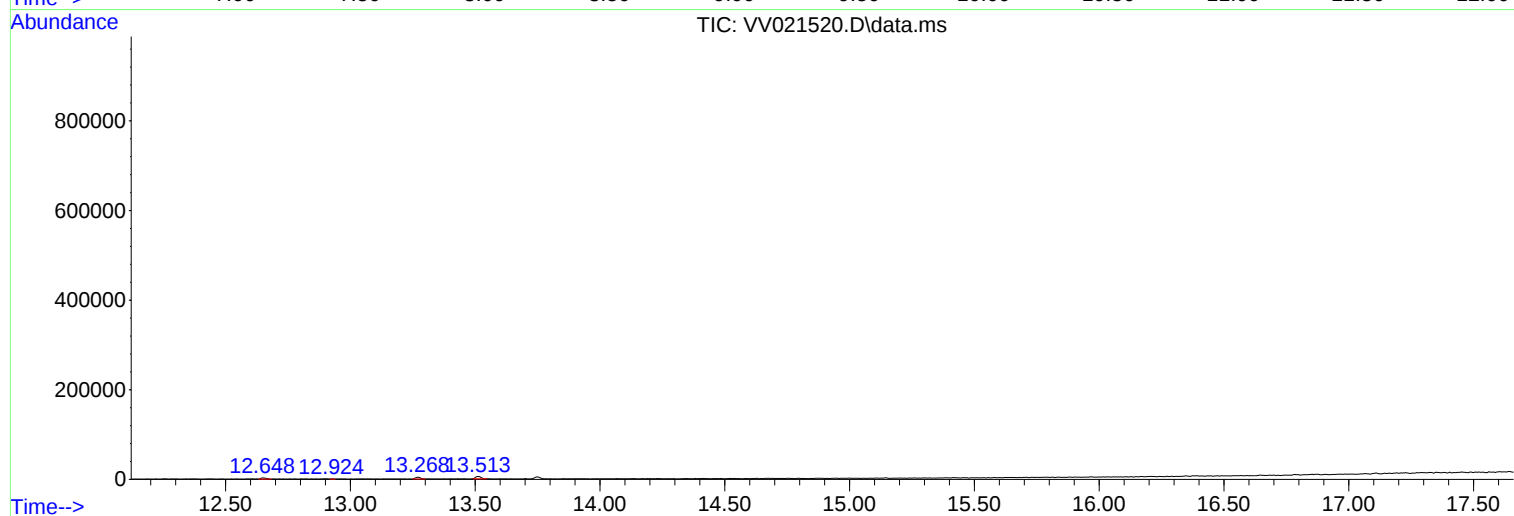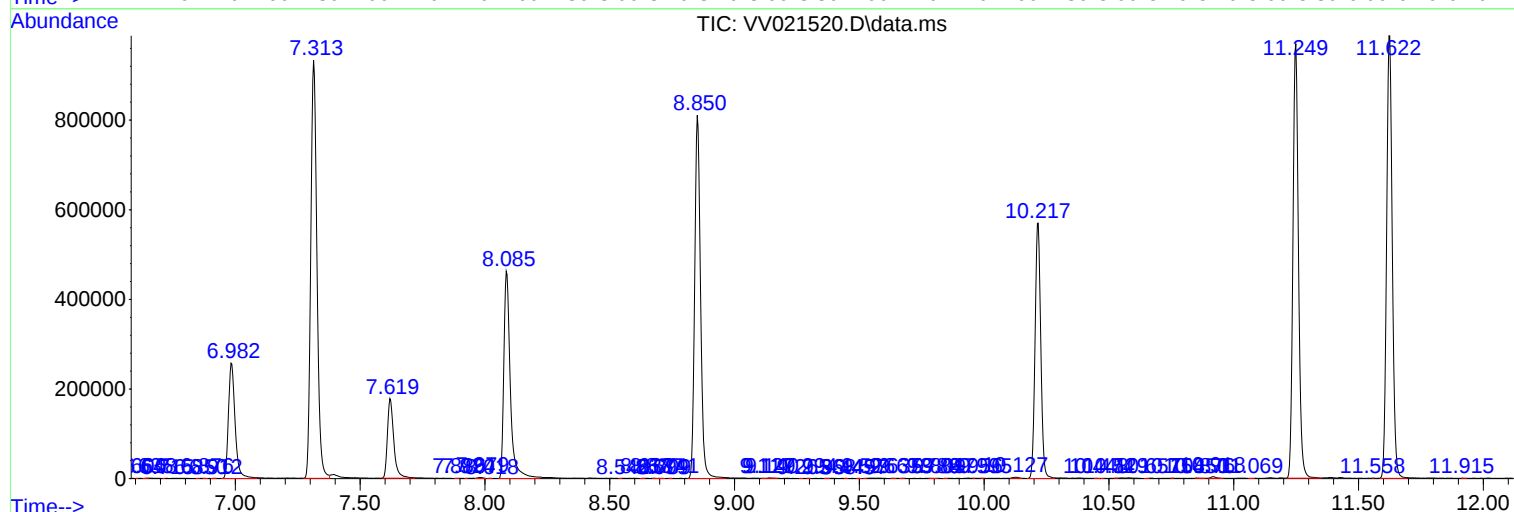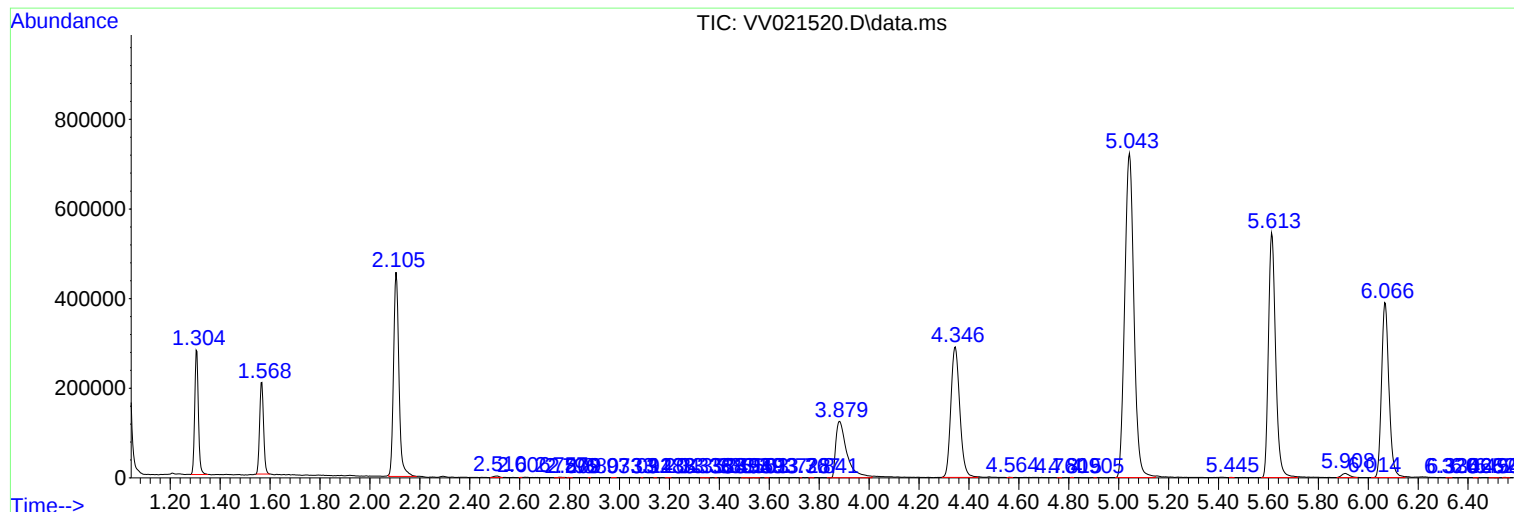

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021520.D
Acq On : 07 Jun 2021 11:26
Operator : SY/MD
Sample : VV0607MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021520.D
Acq On : 07 Jun 2021 11:26
Operator : SY/MD
Sample : VV0607MBL01
Misc : 5.0g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK187

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
