

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021521.D
 Acq On : 07 Jun 2021 11:49
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK188

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021521.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	77	83	95	rVB	275087	268738	14.87%	1.883%
2	1.568	157	164	179	rBV	188321	203739	11.28%	1.428%
3	2.108	323	332	361	rVB	431775	655756	36.30%	4.596%
4	2.606	483	487	489	rBV3	616	415	0.02%	0.003%
5	2.767	534	537	539	rBV	561	412	0.02%	0.003%
6	2.844	559	561	563	rVB2	318	130	0.01%	0.001%
7	2.970	598	600	602	rBV2	276	106	0.01%	0.001%
8	3.005	608	611	613	rBV3	308	211	0.01%	0.001%
9	3.044	621	623	629	rBV2	795	734	0.04%	0.005%
10	3.230	677	681	683	rBV	415	311	0.02%	0.002%
11	3.246	683	686	688	rVB3	223	126	0.01%	0.001%
12	3.275	693	695	700	rVB	233	114	0.01%	0.001%
13	3.314	702	707	709	rBV	287	238	0.01%	0.002%
14	3.339	713	715	717	rBV	243	120	0.01%	0.001%
15	3.429	740	743	745	rVB2	259	110	0.01%	0.001%
16	3.465	750	754	756	rBV2	286	169	0.01%	0.001%
17	3.484	758	760	763	rVB3	269	146	0.01%	0.001%
18	3.526	771	773	776	rBV	218	119	0.01%	0.001%
19	3.542	776	778	781	rVB3	422	224	0.01%	0.002%
20	3.754	842	844	845	rBV3	266	131	0.01%	0.001%
21	3.818	862	864	869	rVB2	270	176	0.01%	0.001%
22	3.851	869	874	875	rBV2	207	177	0.01%	0.001%
23	3.886	875	885	915	rBV	136183	383736	21.24%	2.689%
24	4.352	1015	1030	1064	rVB	284998	699706	38.73%	4.904%
25	4.635	1115	1118	1120	rBV2	456	249	0.01%	0.002%
26	4.754	1153	1155	1157	rBV	198	120	0.01%	0.001%
27	4.812	1168	1173	1175	rBV2	302	309	0.02%	0.002%
28	4.873	1187	1192	1194	rBV3	309	278	0.02%	0.002%
29	4.886	1194	1196	1198	rVB2	280	109	0.01%	0.001%
30	4.928	1207	1209	1212	rBV	262	167	0.01%	0.001%
31	4.950	1214	1216	1222	rVB2	379	320	0.02%	0.002%
32	4.982	1225	1226	1230	rVB	349	201	0.01%	0.001%
33	5.050	1230	1247	1280	rBV2	707615	1806678	100.00%	12.662%
34	5.484	1378	1382	1388	rBV3	469	522	0.03%	0.004%
35	5.523	1392	1394	1402	rVB3	645	606	0.03%	0.004%
36	5.558	1402	1405	1410	rVB	570	447	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021521.D
 Acq On : 07 Jun 2021 11:49
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK188

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	5.619	1410	1424	1466	rBV	531777	1071160	59.29%	7.507%
38	5.912	1506	1515	1530	rBV4	8556	18053	1.00%	0.127%
39	6.072	1552	1565	1589	rBV	383807	784681	43.43%	5.500%
40	6.297	1631	1635	1638	rBV2	485	408	0.02%	0.003%
41	6.339	1644	1648	1655	rVB3	503	671	0.04%	0.005%
42	6.416	1668	1672	1675	rBV2	332	273	0.02%	0.002%
43	6.445	1675	1681	1684	rBV3	405	430	0.02%	0.003%
44	6.593	1723	1727	1729	rVB2	230	141	0.01%	0.001%
45	6.629	1736	1738	1739	rBV	308	117	0.01%	0.001%
46	6.706	1758	1762	1764	rBV4	391	325	0.02%	0.002%
47	6.728	1767	1769	1772	rBV2	446	244	0.01%	0.002%
48	6.760	1776	1779	1780	rBV2	384	193	0.01%	0.001%
49	6.828	1796	1800	1802	rBV2	234	199	0.01%	0.001%
50	6.892	1817	1820	1825	rVB2	338	268	0.01%	0.002%
51	6.918	1825	1828	1829	rBV2	300	176	0.01%	0.001%
52	6.989	1838	1850	1887	rBV	250026	459953	25.46%	3.224%
53	7.320	1940	1953	1974	rBV	895219	1568198	86.80%	10.991%
54	7.625	2038	2048	2076	rBV	170845	302880	16.76%	2.123%
55	7.870	2121	2124	2125	rBV2	355	220	0.01%	0.002%
56	7.931	2141	2143	2148	rBV4	557	575	0.03%	0.004%
57	7.979	2152	2158	2169	rVB5	3063	5241	0.29%	0.037%
58	8.024	2169	2172	2177	rBV2	166	169	0.01%	0.001%
59	8.088	2181	2192	2226	rBV	487260	860118	47.61%	6.028%
60	8.551	2330	2336	2340	rBV4	338	401	0.02%	0.003%
61	8.661	2367	2370	2372	rBV2	208	140	0.01%	0.001%
62	8.674	2372	2374	2376	rVB	313	121	0.01%	0.001%
63	8.735	2385	2393	2397	rBV3	542	526	0.03%	0.004%
64	8.767	2401	2403	2406	rBV	250	144	0.01%	0.001%
65	8.854	2418	2430	2464	rBV	780924	1283821	71.06%	8.998%
66	9.018	2479	2481	2484	rBV4	577	333	0.02%	0.002%
67	9.191	2532	2535	2537	rVB4	444	205	0.01%	0.001%
68	9.207	2537	2540	2545	rBV3	547	409	0.02%	0.003%
69	9.227	2545	2546	2549	rVB	427	168	0.01%	0.001%
70	9.246	2550	2552	2557	rBV2	215	137	0.01%	0.001%
71	9.400	2593	2600	2606	rBV3	362	470	0.03%	0.003%
72	9.429	2607	2609	2612	rVV2	208	111	0.01%	0.001%
73	9.468	2619	2621	2624	rVB2	236	111	0.01%	0.001%
74	9.513	2632	2635	2637	rBV	270	169	0.01%	0.001%
75	9.545	2642	2645	2647	rBV2	403	294	0.02%	0.002%
76	9.583	2656	2657	2659	rBV2	220	105	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021521.D
 Acq On : 07 Jun 2021 11:49
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK188

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.677	2682	2686	2687	rBV2	348	263	0.01%	0.002%
78	9.776	2713	2717	2718	rBV	236	129	0.01%	0.001%
79	9.937	2762	2767	2768	rBV2	250	211	0.01%	0.001%
80	10.130	2821	2827	2835	rVB3	2260	3012	0.17%	0.021%
81	10.217	2841	2854	2878	rBV	575173	903569	50.01%	6.333%
82	10.365	2897	2900	2903	rBV5	650	580	0.03%	0.004%
83	10.419	2913	2917	2921	rBV2	422	338	0.02%	0.002%
84	10.542	2951	2955	2958	rBV2	864	665	0.04%	0.005%
85	10.664	2991	2993	2997	rVV2	489	269	0.01%	0.002%
86	10.693	2999	3002	3008	rVB2	420	305	0.02%	0.002%
87	10.879	3057	3060	3063	rVB3	276	195	0.01%	0.001%
88	10.921	3064	3073	3082	rVB7	2658	4066	0.23%	0.028%
89	10.963	3082	3086	3088	rBV	186	105	0.01%	0.001%
90	11.024	3102	3105	3108	rBV3	563	324	0.02%	0.002%
91	11.079	3120	3122	3124	rVB2	451	148	0.01%	0.001%
92	11.146	3136	3143	3153	rVB6	1379	2309	0.13%	0.016%
93	11.194	3153	3158	3161	rBV2	505	492	0.03%	0.003%
94	11.249	3163	3175	3204	rBV	924445	1443633	79.91%	10.118%
95	11.542	3263	3266	3267	rBV	488	203	0.01%	0.001%
96	11.625	3279	3292	3322	rBV	973289	1518037	84.02%	10.639%
97	12.120	3444	3446	3449	rBV2	388	181	0.01%	0.001%
98	12.169	3457	3461	3463	rBV2	409	344	0.02%	0.002%
99	12.590	3591	3592	3594	rBV	267	122	0.01%	0.001%
100	13.014	3721	3724	3727	rBV4	487	359	0.02%	0.003%




Sum of corrected areas: 14268067

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021521.D
Acq On : 07 Jun 2021 11:49
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK188

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

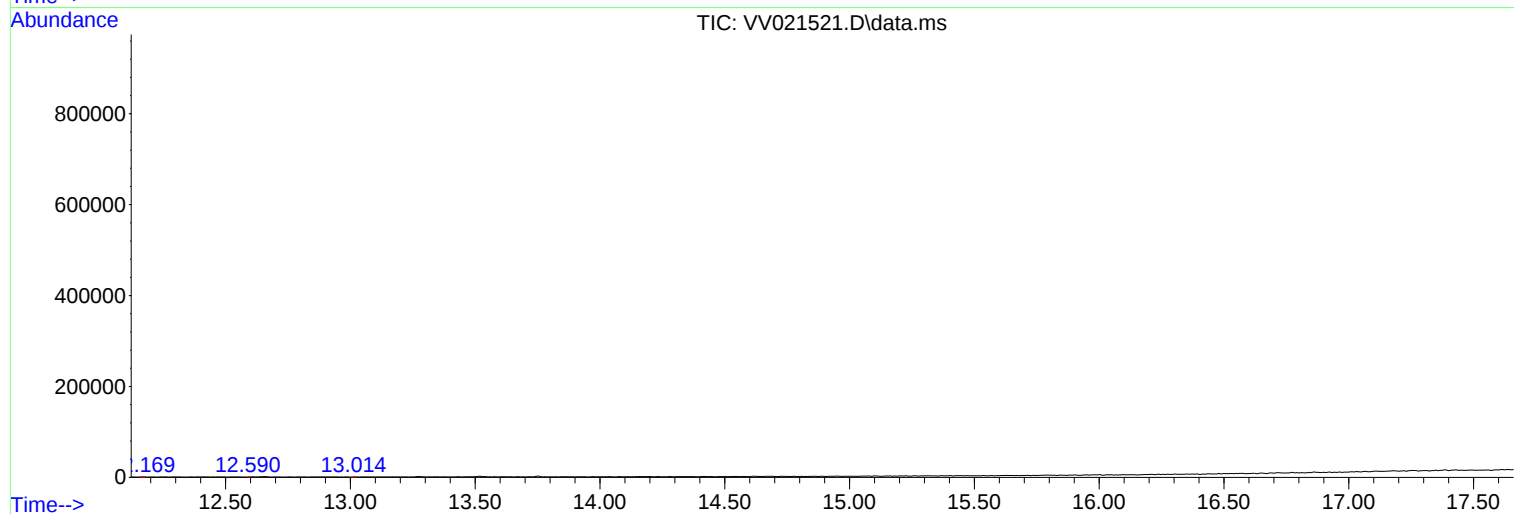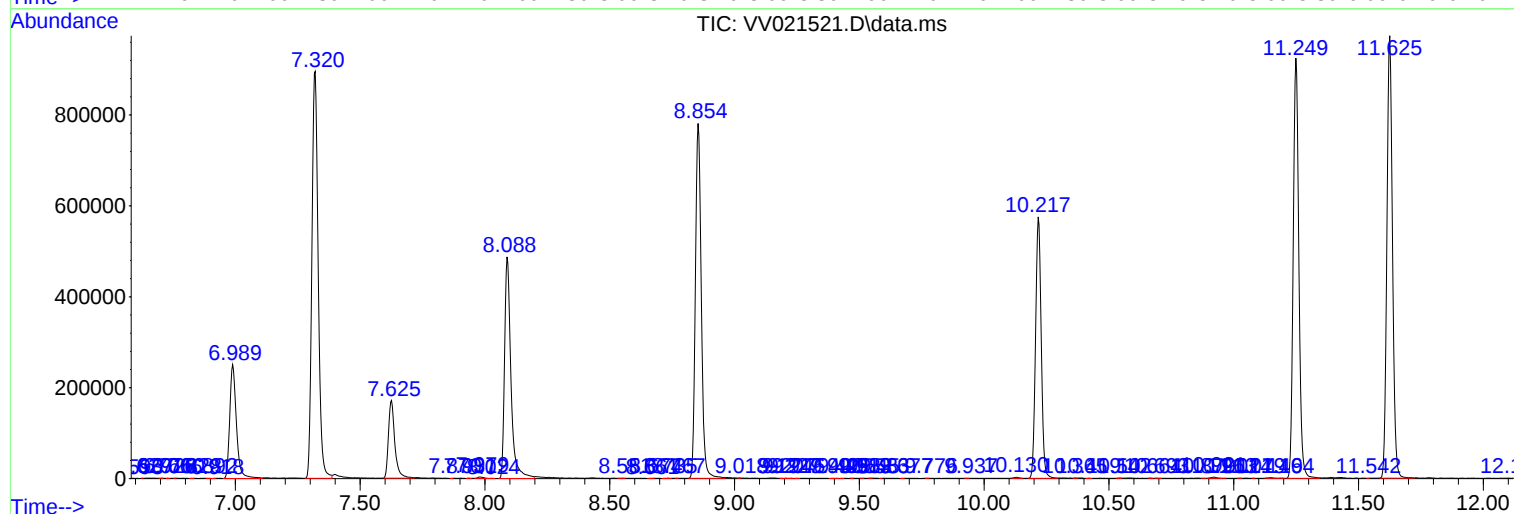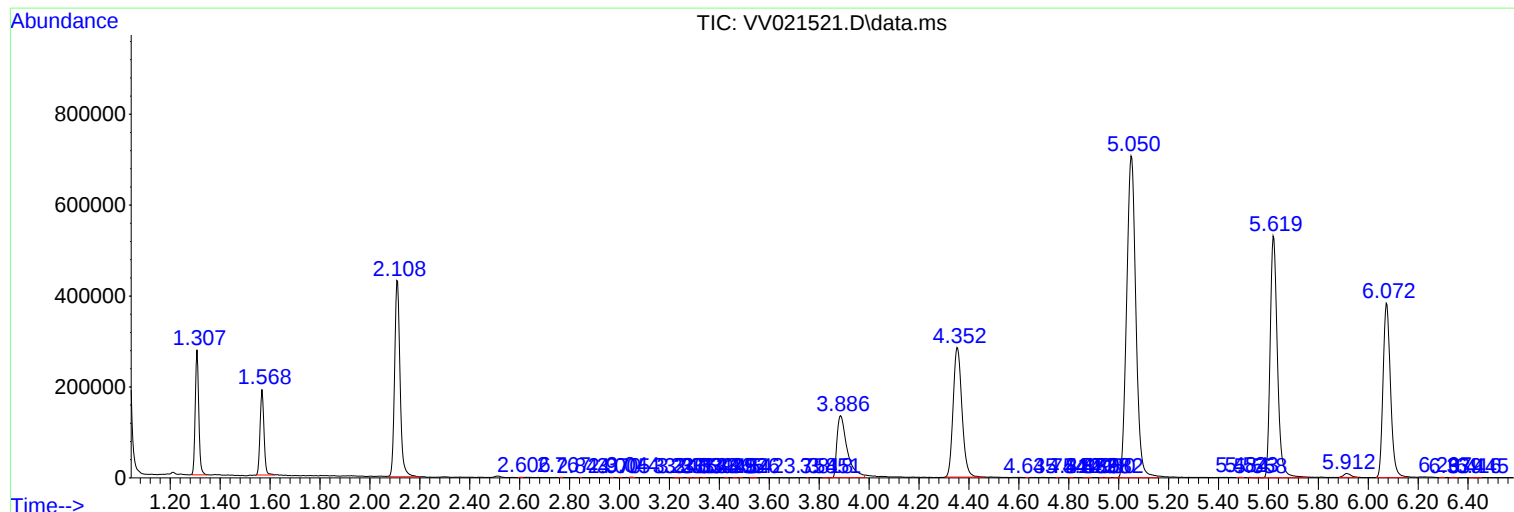

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021521.D
Acq On : 07 Jun 2021 11:49
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK188

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021521.D
Acq On : 07 Jun 2021 11:49
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK188

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
