

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021523.D
 Acq On : 07 Jun 2021 12:36
 Operator : SY/MD
 Sample : M2605-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021523.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	95	rVB	151822	153685	9.74%	1.005%
2	1.568	157	164	178	rVB	135464	148053	9.38%	0.968%
3	2.108	322	332	347	rBV	279422	414617	26.27%	2.711%
4	2.770	524	538	551	rBV4	4584	10411	0.66%	0.068%
5	2.854	562	564	567	rBV	231	121	0.01%	0.001%
6	2.873	567	570	573	rBV2	387	208	0.01%	0.001%
7	2.921	581	585	587	rBV2	386	209	0.01%	0.001%
8	2.957	594	596	603	rVB5	370	319	0.02%	0.002%
9	2.986	603	605	609	rBV3	236	164	0.01%	0.001%
10	3.044	615	623	638	rVB3	7107	14619	0.93%	0.096%
11	3.124	647	648	651	rBV2	325	189	0.01%	0.001%
12	3.172	661	663	665	rBV2	184	102	0.01%	0.001%
13	3.217	671	677	679	rBV3	382	342	0.02%	0.002%
14	3.233	679	682	684	rVV	246	135	0.01%	0.001%
15	3.278	693	696	698	rBV2	245	165	0.01%	0.001%
16	3.343	714	716	718	rBV2	235	138	0.01%	0.001%
17	3.423	738	741	744	rBV2	297	190	0.01%	0.001%
18	3.442	744	747	751	rVV2	181	173	0.01%	0.001%
19	3.519	769	771	774	rBV	162	95	0.01%	0.001%
20	3.536	774	776	780	rBV	194	132	0.01%	0.001%
21	3.629	801	805	807	rBV2	306	212	0.01%	0.001%
22	3.764	834	847	848	rBV6	3982	6279	0.40%	0.041%
23	3.889	870	886	904	rBV	143884	436565	27.66%	2.854%
24	4.352	1016	1030	1057	rBV	273283	665902	42.20%	4.354%
25	4.693	1132	1136	1137	rBV2	497	346	0.02%	0.002%
26	4.767	1156	1159	1160	rBV3	248	119	0.01%	0.001%
27	4.777	1160	1162	1165	rVB3	395	228	0.01%	0.001%
28	4.851	1181	1185	1190	rBV3	373	330	0.02%	0.002%
29	4.876	1190	1193	1196	rVV2	192	155	0.01%	0.001%
30	4.908	1200	1203	1205	rBV	179	131	0.01%	0.001%
31	4.928	1207	1209	1212	rVV2	311	183	0.01%	0.001%
32	5.050	1229	1247	1285	rBV2	587372	1533129	97.15%	10.024%
33	5.619	1411	1424	1457	rBV	513399	1034840	65.58%	6.766%
34	5.915	1502	1516	1552	rBV	506019	1002504	63.53%	6.555%
35	6.072	1552	1565	1593	rVV	334924	683109	43.29%	4.466%
36	6.269	1624	1626	1628	rVB	588	312	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021523.D
 Acq On : 07 Jun 2021 12:36
 Operator : SY/MD
 Sample : M2605-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.317	1639	1641	1643	rVB2	286	118	0.01%	0.001%
38	6.346	1646	1650	1653	rVB2	367	280	0.02%	0.002%
39	6.375	1653	1659	1660	rBV2	389	324	0.02%	0.002%
40	6.500	1694	1698	1700	rBV2	337	270	0.02%	0.002%
41	6.516	1700	1703	1707	rVV3	399	326	0.02%	0.002%
42	6.535	1707	1709	1714	rVV2	321	266	0.02%	0.002%
43	6.641	1733	1742	1760	rVV8	2008	5688	0.36%	0.037%
44	6.831	1797	1801	1803	rBV	191	106	0.01%	0.001%
45	6.867	1809	1812	1818	rVB3	445	319	0.02%	0.002%
46	6.934	1830	1833	1836	rBV2	249	211	0.01%	0.001%
47	6.989	1839	1850	1872	rBV	210259	384074	24.34%	2.511%
48	7.256	1930	1933	1940	rVB6	606	545	0.03%	0.004%
49	7.317	1940	1952	1972	rBV	711575	1236805	78.38%	8.087%
50	7.622	2038	2047	2076	rBV	147426	259927	16.47%	1.700%
51	7.857	2118	2120	2124	rVB2	583	417	0.03%	0.003%
52	7.883	2124	2128	2131	rBV2	281	274	0.02%	0.002%
53	7.976	2144	2157	2182	rVV	943449	1578045	100.00%	10.318%
54	8.088	2183	2192	2232	rVV	489664	850969	53.93%	5.564%
55	8.503	2319	2321	2323	rVB2	265	109	0.01%	0.001%
56	8.532	2328	2330	2332	rVV	504	289	0.02%	0.002%
57	8.555	2335	2337	2344	rVB3	601	471	0.03%	0.003%
58	8.587	2344	2347	2352	rBV3	387	320	0.02%	0.002%
59	8.612	2353	2355	2362	rVB3	385	301	0.02%	0.002%
60	8.703	2380	2383	2388	rBV3	443	308	0.02%	0.002%
61	8.725	2388	2390	2392	rBV	353	199	0.01%	0.001%
62	8.748	2395	2397	2399	rBV	305	196	0.01%	0.001%
63	8.780	2405	2407	2410	rBV3	150	117	0.01%	0.001%
64	8.854	2417	2430	2451	rBV	758279	1237435	78.42%	8.091%
65	9.243	2547	2551	2553	rBV2	259	186	0.01%	0.001%
66	9.297	2565	2568	2572	rBV4	437	285	0.02%	0.002%
67	9.384	2592	2595	2597	rBV	226	115	0.01%	0.001%
68	9.432	2608	2610	2612	rBV	266	144	0.01%	0.001%
69	9.555	2643	2648	2654	rVB3	686	821	0.05%	0.005%
70	9.609	2661	2665	2667	rBV	199	130	0.01%	0.001%
71	9.654	2676	2679	2683	rBV2	216	191	0.01%	0.001%
72	9.690	2687	2690	2697	rBV2	234	270	0.02%	0.002%
73	9.879	2744	2749	2756	rBV	427	555	0.04%	0.004%
74	10.027	2784	2795	2804	rBV5	3013	5748	0.36%	0.038%
75	10.130	2818	2827	2836	rVB3	1824	2746	0.17%	0.018%
76	10.217	2842	2854	2872	rBV	572338	882205	55.90%	5.768%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021523.D
 Acq On : 07 Jun 2021 12:36
 Operator : SY/MD
 Sample : M2605-10DL 50X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG7K2DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	10.548	2950	2957	2962	rBV4	704	1057	0.07%	0.007%
78	10.574	2962	2965	2966	rBV	482	235	0.01%	0.002%
79	10.783	3028	3030	3036	rVB3	295	256	0.02%	0.002%
80	10.818	3039	3041	3044	rVB2	418	164	0.01%	0.001%
81	10.834	3044	3046	3047	rBV2	248	115	0.01%	0.001%
82	10.844	3047	3049	3050	rVV2	343	128	0.01%	0.001%
83	10.857	3051	3053	3058	rVB3	659	348	0.02%	0.002%
84	10.899	3063	3066	3067	rBV	401	248	0.02%	0.002%
85	10.921	3067	3073	3083	rVB3	2865	3806	0.24%	0.025%
86	11.005	3097	3099	3102	rVB3	310	146	0.01%	0.001%
87	11.027	3103	3106	3109	rBV2	399	327	0.02%	0.002%
88	11.143	3137	3142	3143	rBV4	855	730	0.05%	0.005%
89	11.188	3154	3156	3161	rVB3	599	384	0.02%	0.003%
90	11.249	3163	3175	3198	rBV	910679	1397928	88.59%	9.140%
91	11.625	3279	3292	3314	rBV	835429	1325228	83.98%	8.665%
92	11.828	3353	3355	3357	rBV	306	99	0.01%	0.001%
93	11.854	3360	3363	3367	rVV4	571	458	0.03%	0.003%
94	12.136	3449	3451	3452	rBV4	251	94	0.01%	0.001%
95	12.191	3466	3468	3470	rBV2	312	150	0.01%	0.001%
96	12.490	3556	3561	3564	rBV2	386	281	0.02%	0.002%
97	12.571	3583	3586	3588	rBV	354	232	0.01%	0.002%
98	12.699	3623	3626	3629	rVB2	269	163	0.01%	0.001%
99	12.725	3630	3634	3637	rBV2	393	399	0.03%	0.003%
100	12.886	3680	3684	3686	rBV3	778	619	0.04%	0.004%




Sum of corrected areas: 15294111

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021523.D
Acq On : 07 Jun 2021 12:36
Operator : SY/MD
Sample : M2605-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampled :
BG7K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

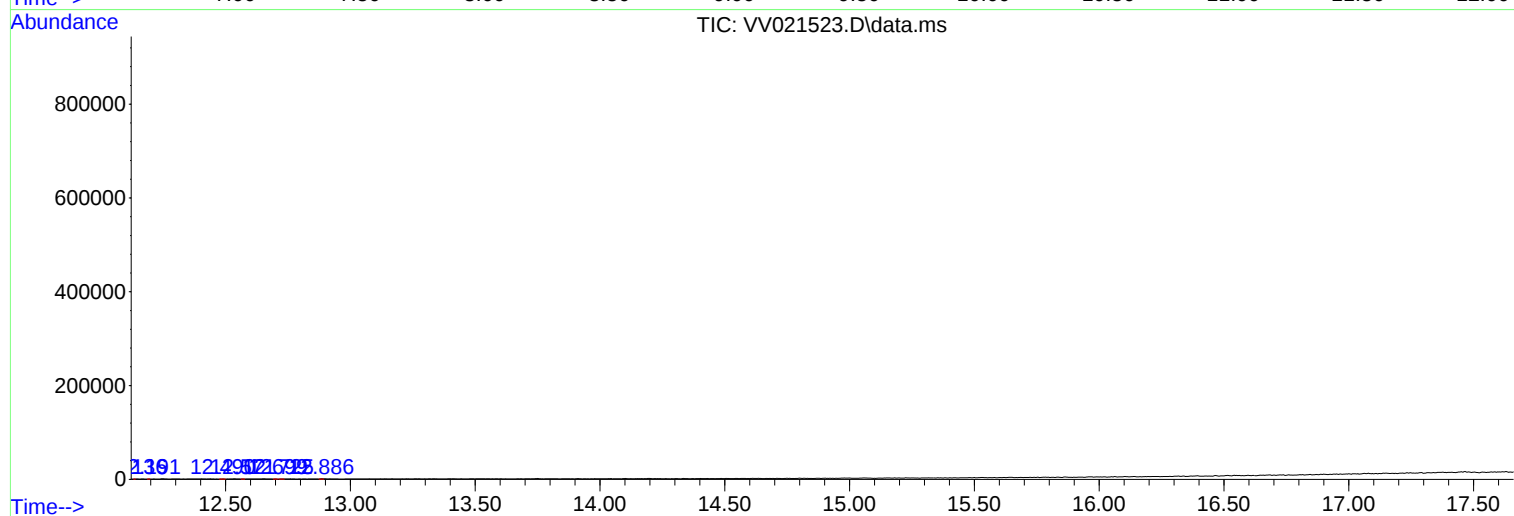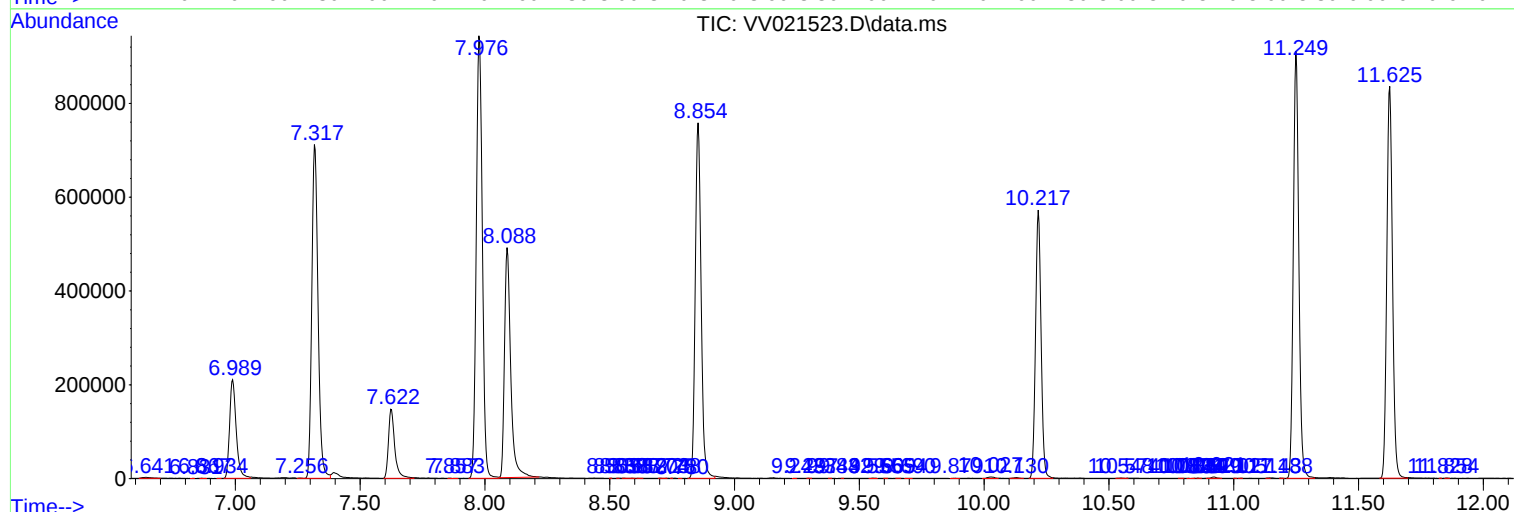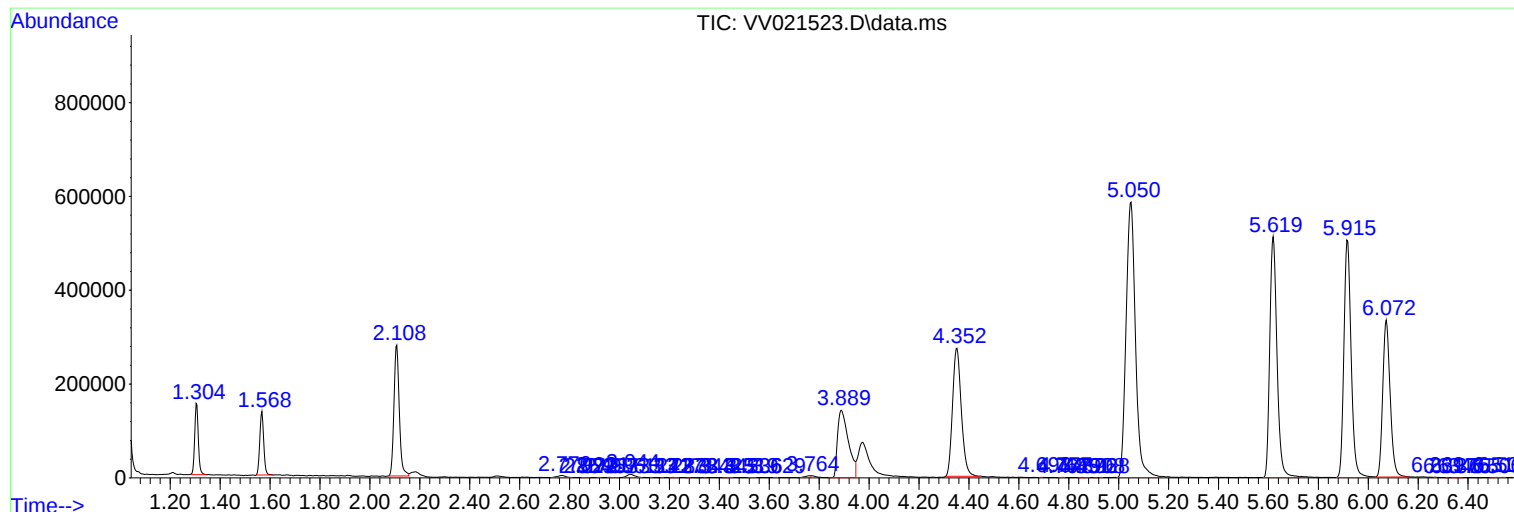

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021523.D
Acq On : 07 Jun 2021 12:36
Operator : SY/MD
Sample : M2605-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021523.D
Acq On : 07 Jun 2021 12:36
Operator : SY/MD
Sample : M2605-10DL 50X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG7K2DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
