

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021528.D
 Acq On : 07 Jun 2021 14:34
 Operator : SY/MD
 Sample : M2618-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021528.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	101	rVB	241493	249530	15.08%	1.903%
2	1.568	157	164	176	rVB	158184	177420	10.72%	1.353%
3	2.108	322	332	358	rVB	399614	599293	36.23%	4.571%
4	2.506	449	456	466	rBV4	3305	5638	0.34%	0.043%
5	2.664	502	505	508	rBV3	283	230	0.01%	0.002%
6	2.690	510	513	519	rVB2	249	195	0.01%	0.001%
7	2.748	528	531	532	rBV2	291	109	0.01%	0.001%
8	2.796	544	546	549	rVB3	304	176	0.01%	0.001%
9	2.969	598	600	603	rVB	230	129	0.01%	0.001%
10	2.989	603	606	608	rBV2	198	130	0.01%	0.001%
11	3.005	608	611	613	rBV	371	187	0.01%	0.001%
12	3.018	613	615	616	rBV2	393	159	0.01%	0.001%
13	3.043	621	623	629	rVB4	702	530	0.03%	0.004%
14	3.288	694	699	702	rBV2	294	228	0.01%	0.002%
15	3.394	730	732	736	rBV	260	174	0.01%	0.001%
16	3.497	761	764	767	rBV2	244	158	0.01%	0.001%
17	3.658	812	814	818	rVB2	237	126	0.01%	0.001%
18	3.696	824	826	829	rVB	299	154	0.01%	0.001%
19	3.760	844	846	847	rBV	250	112	0.01%	0.001%
20	3.883	874	884	925	rBV	125367	356433	21.55%	2.719%
21	4.352	1014	1030	1056	rBV2	264194	647620	39.15%	4.940%
22	4.648	1120	1122	1127	rVB2	452	243	0.01%	0.002%
23	4.680	1129	1132	1133	rBV	271	159	0.01%	0.001%
24	4.693	1134	1136	1140	rVB3	431	224	0.01%	0.002%
25	4.799	1166	1169	1170	rBV	249	132	0.01%	0.001%
26	4.812	1170	1173	1176	rVB	284	173	0.01%	0.001%
27	4.838	1180	1181	1184	rVB	247	121	0.01%	0.001%
28	4.857	1184	1187	1190	rBV2	178	134	0.01%	0.001%
29	5.050	1226	1247	1281	rBV2	641922	1654360	100.00%	12.619%
30	5.284	1318	1320	1323	rBV3	521	216	0.01%	0.002%
31	5.468	1375	1377	1379	rBV	343	143	0.01%	0.001%
32	5.490	1381	1384	1385	rVV2	413	204	0.01%	0.002%
33	5.519	1392	1393	1397	rVB2	277	114	0.01%	0.001%
34	5.619	1411	1424	1459	rBV	498510	999638	60.42%	7.625%
35	5.915	1505	1516	1533	rBV6	11235	26057	1.58%	0.199%
36	6.011	1544	1546	1550	rVB3	331	189	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060721\
 Data File : VW021528.D
 Acq On : 07 Jun 2021 14:34
 Operator : SY/MD
 Sample : M2618-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.072	1550	1565	1592	rBV	346911	716746	43.32%	5.467%
38	6.304	1635	1637	1639	rBV3	302	184	0.01%	0.001%
39	6.326	1643	1644	1647	rVB	300	120	0.01%	0.001%
40	6.371	1655	1658	1662	rVB3	346	251	0.02%	0.002%
41	6.397	1662	1666	1668	rBV	261	190	0.01%	0.001%
42	6.468	1686	1688	1691	rVB	245	135	0.01%	0.001%
43	6.519	1702	1704	1710	rVB2	245	180	0.01%	0.001%
44	6.587	1722	1725	1727	rBV2	290	212	0.01%	0.002%
45	6.606	1729	1731	1734	rVB	206	106	0.01%	0.001%
46	6.635	1734	1740	1742	rBV6	671	624	0.04%	0.005%
47	6.696	1757	1759	1762	rVB3	398	195	0.01%	0.001%
48	6.754	1773	1777	1779	rVB2	263	156	0.01%	0.001%
49	6.776	1779	1784	1787	rBV3	251	243	0.01%	0.002%
50	6.796	1787	1790	1793	rVV2	382	261	0.02%	0.002%
51	6.825	1796	1799	1804	rBV3	338	360	0.02%	0.003%
52	6.866	1810	1812	1815	rVB3	258	151	0.01%	0.001%
53	6.989	1833	1850	1878	rBV	226523	411240	24.86%	3.137%
54	7.317	1940	1952	1973	rBV	822016	1424508	86.11%	10.866%
55	7.625	2035	2048	2072	rBV	156073	273693	16.54%	2.088%
56	7.844	2110	2116	2120	rVB4	469	458	0.03%	0.003%
57	7.921	2138	2140	2141	rBV	387	145	0.01%	0.001%
58	7.944	2142	2147	2150	rVV3	1299	1269	0.08%	0.010%
59	7.982	2150	2159	2172	rVB3	11526	20422	1.23%	0.156%
60	8.050	2178	2180	2182	rBV	219	129	0.01%	0.001%
61	8.088	2182	2192	2218	rBV	435921	770524	46.58%	5.878%
62	8.410	2289	2292	2294	rBV3	856	590	0.04%	0.005%
63	8.461	2306	2308	2312	rVB3	480	245	0.01%	0.002%
64	8.561	2336	2339	2342	rBV3	253	153	0.01%	0.001%
65	8.680	2372	2376	2380	rBV3	245	213	0.01%	0.002%
66	8.709	2380	2385	2388	rBV2	559	447	0.03%	0.003%
67	8.805	2412	2415	2418	rBV3	586	369	0.02%	0.003%
68	8.853	2418	2430	2468	rBV	743058	1206395	72.92%	9.202%
69	9.104	2504	2508	2511	rVB2	405	273	0.02%	0.002%
70	9.130	2512	2516	2517	rBV	438	221	0.01%	0.002%
71	9.156	2521	2524	2530	rVB3	700	718	0.04%	0.005%
72	9.185	2530	2533	2536	rBV2	517	378	0.02%	0.003%
73	9.271	2558	2560	2564	rVB	237	141	0.01%	0.001%
74	9.349	2581	2584	2586	rBV	251	136	0.01%	0.001%
75	9.387	2592	2596	2597	rBV	308	172	0.01%	0.001%
76	9.410	2601	2603	2605	rVV	426	185	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021528.D
 Acq On : 07 Jun 2021 14:34
 Operator : SY/MD
 Sample : M2618-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.423	2605	2607	2611	rVV3	249	202	0.01%	0.002%
78	9.461	2616	2619	2621	rVV	237	148	0.01%	0.001%
79	9.558	2647	2649	2656	rVB3	430	329	0.02%	0.003%
80	9.718	2696	2699	2704	rVB	398	293	0.02%	0.002%
81	9.789	2718	2721	2724	rVB	346	193	0.01%	0.001%
82	9.918	2759	2761	2764	rBV	205	118	0.01%	0.001%
83	9.934	2764	2766	2768	rVV	304	133	0.01%	0.001%
84	9.992	2780	2784	2787	rBV2	258	212	0.01%	0.002%
85	10.037	2795	2798	2799	rBV	240	110	0.01%	0.001%
86	10.130	2819	2827	2835	rVB4	1957	2849	0.17%	0.022%
87	10.217	2841	2854	2876	rBV	524977	824699	49.85%	6.291%
88	10.384	2902	2906	2916	rVB2	2892	3553	0.21%	0.027%
89	10.545	2952	2956	2959	rBV2	435	336	0.02%	0.003%
90	10.702	3002	3005	3007	rBV	201	121	0.01%	0.001%
91	10.776	3025	3028	3030	rBV	204	126	0.01%	0.001%
92	10.857	3050	3053	3056	rVB3	496	305	0.02%	0.002%
93	10.914	3064	3071	3078	rBV5	1706	2707	0.16%	0.021%
94	11.249	3163	3175	3202	rBV	863761	1343728	81.22%	10.250%
95	11.561	3270	3272	3277	rBV3	485	470	0.03%	0.004%
96	11.625	3280	3292	3318	rVV	871180	1373985	83.05%	10.481%
97	12.233	3477	3481	3483	rBV2	366	256	0.02%	0.002%
98	12.249	3484	3486	3487	rBV2	464	201	0.01%	0.002%
99	12.352	3515	3518	3520	rBV	344	147	0.01%	0.001%
100	12.866	3675	3678	3681	rBV2	608	519	0.03%	0.004%




Sum of corrected areas: 13109716

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021528.D
Acq On : 07 Jun 2021 14:34
Operator : SY/MD
Sample : M2618-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

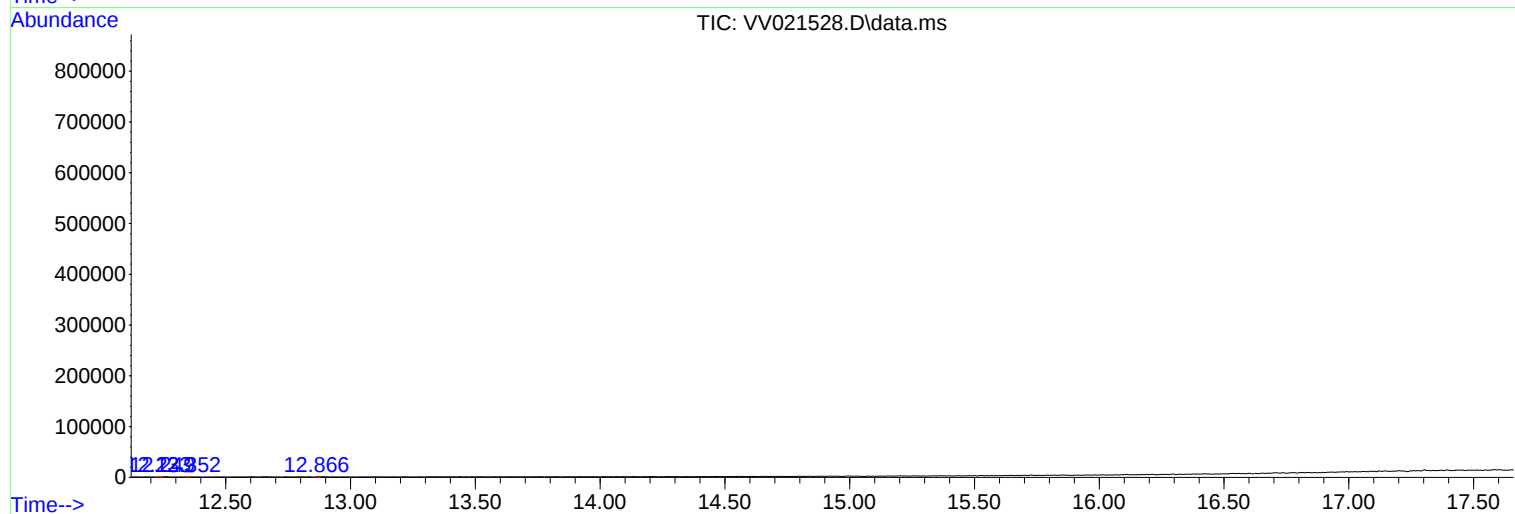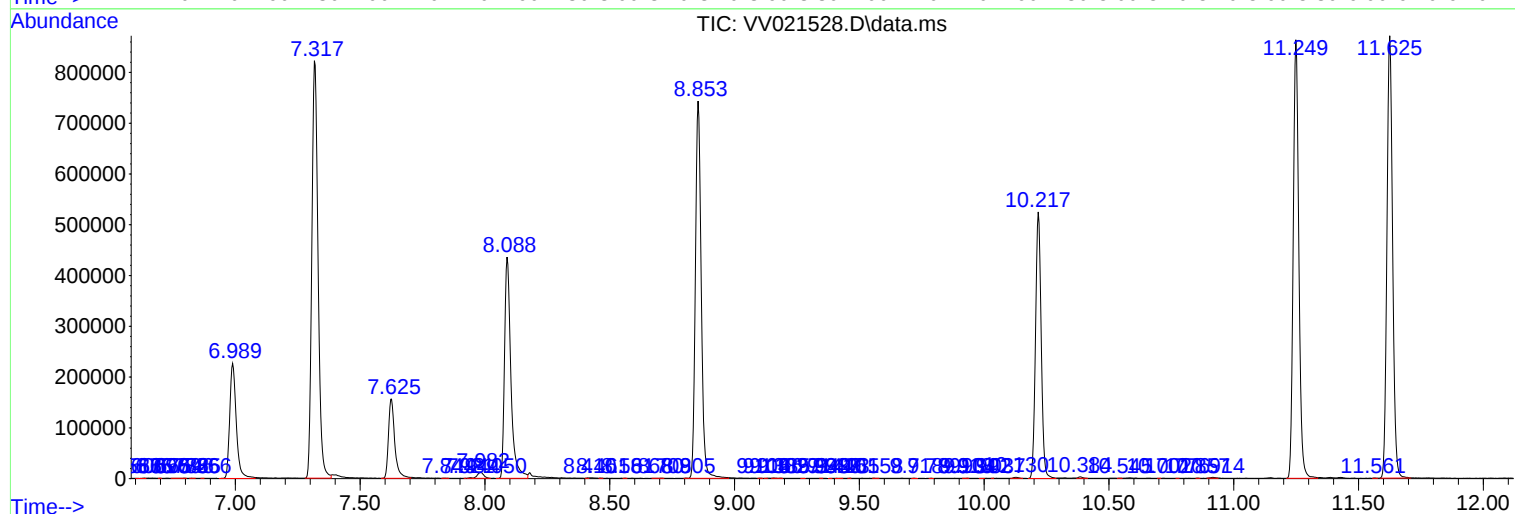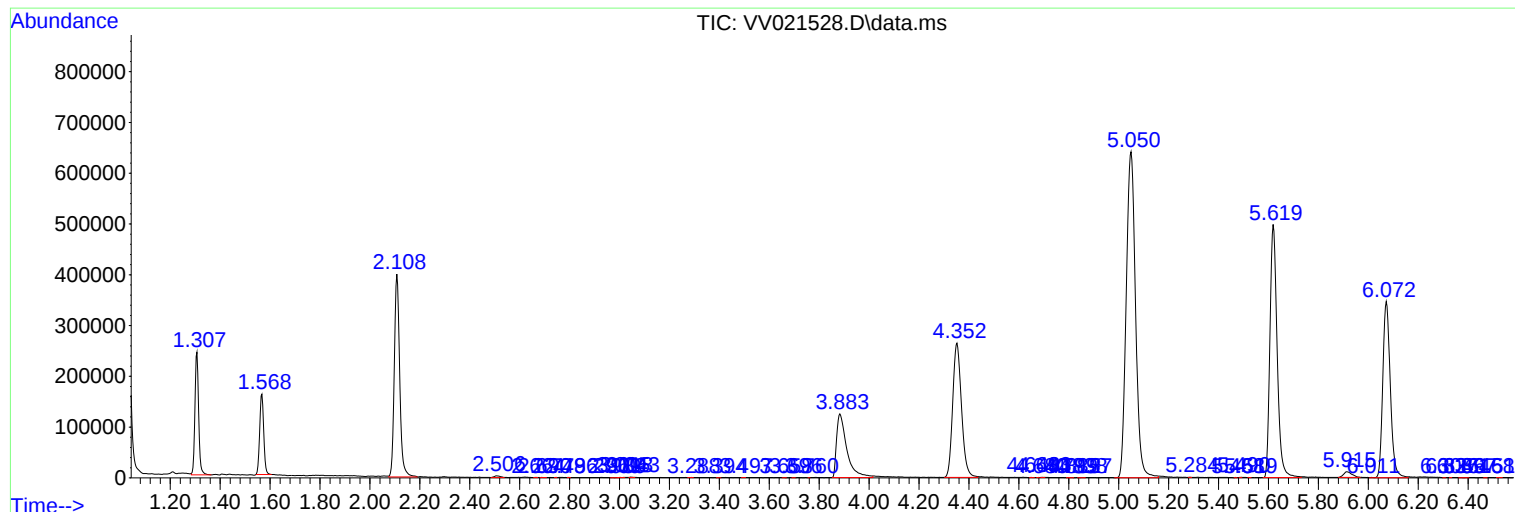

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021528.D
Acq On : 07 Jun 2021 14:34
Operator : SY/MD
Sample : M2618-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021528.D
Acq On : 07 Jun 2021 14:34
Operator : SY/MD
Sample : M2618-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
