

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021529.D
 Acq On : 07 Jun 2021 14:58
 Operator : SY/MD
 Sample : M2605-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M

Title : VOC Analysis

Signal : TIC: VV021529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	234375	242109	14.99%	1.885%
2	1.565	157	163	178	rVB	157411	172313	10.67%	1.342%
3	2.108	322	332	357	rVB	386119	573040	35.47%	4.462%
4	2.674	505	508	511	rBV2	426	233	0.01%	0.002%
5	2.712	518	520	521	rBV	280	155	0.01%	0.001%
6	2.851	560	563	565	rVB2	446	229	0.01%	0.002%
7	2.925	584	586	588	rBV3	197	126	0.01%	0.001%
8	3.073	630	632	637	rBV2	187	162	0.01%	0.001%
9	3.220	675	678	680	rBV2	272	135	0.01%	0.001%
10	3.301	701	703	705	rBV2	247	152	0.01%	0.001%
11	3.352	717	719	721	rVB	398	174	0.01%	0.001%
12	3.381	724	728	730	rBV4	400	290	0.02%	0.002%
13	3.417	736	739	742	rBV2	382	194	0.01%	0.002%
14	3.465	752	754	757	rBV2	172	124	0.01%	0.001%
15	3.481	757	759	763	rVB2	274	144	0.01%	0.001%
16	3.545	776	779	780	rBV	312	186	0.01%	0.001%
17	3.690	822	824	825	rBV	297	125	0.01%	0.001%
18	3.728	832	836	840	rVB	344	287	0.02%	0.002%
19	3.761	840	846	849	rBV	259	208	0.01%	0.002%
20	3.835	864	869	871	rBV2	231	173	0.01%	0.001%
21	3.883	874	884	919	rBV	128280	362020	22.41%	2.819%
22	4.352	1012	1030	1067	rBV	259252	637741	39.48%	4.965%
23	4.677	1126	1131	1135	rBV6	571	578	0.04%	0.005%
24	4.748	1150	1153	1157	rVB3	376	349	0.02%	0.003%
25	4.838	1178	1181	1185	rBB3	196	129	0.01%	0.001%
26	4.915	1203	1205	1210	rVB4	332	283	0.02%	0.002%
27	4.976	1220	1224	1228	rBV3	252	217	0.01%	0.002%
28	5.050	1229	1247	1276	rBV2	635007	1615370	100.00%	12.577%
29	5.288	1318	1321	1327	rVB3	536	354	0.02%	0.003%
30	5.397	1353	1355	1357	rBV	614	357	0.02%	0.003%
31	5.484	1378	1382	1385	rBV3	394	298	0.02%	0.002%
32	5.535	1395	1398	1401	rBV2	249	169	0.01%	0.001%
33	5.619	1411	1424	1452	rBV	480278	973261	60.25%	7.578%
34	5.915	1505	1516	1531	rBV5	9352	21467	1.33%	0.167%
35	6.072	1551	1565	1587	rBV	346158	702928	43.51%	5.473%
36	6.291	1631	1633	1636	rVB2	340	164	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021529.D
 Acq On : 07 Jun 2021 14:58
 Operator : SY/MD
 Sample : M2605-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

37	6.333	1643	1646	1649	rBV2	396	347	0.02%	0.003%
38	6.352	1649	1652	1653	rVV2	298	167	0.01%	0.001%
39	6.384	1660	1662	1663	rBV2	302	149	0.01%	0.001%
40	6.429	1672	1676	1679	rVB2	195	133	0.01%	0.001%
41	6.519	1699	1704	1705	rBV	253	173	0.01%	0.001%
42	6.545	1709	1712	1714	rBV	199	139	0.01%	0.001%
43	6.561	1714	1717	1722	rVB	296	195	0.01%	0.002%
44	6.600	1725	1729	1730	rBV	208	139	0.01%	0.001%
45	6.645	1738	1743	1745	rBV4	704	589	0.04%	0.005%
46	6.706	1758	1762	1766	rVB2	322	308	0.02%	0.002%
47	6.732	1767	1770	1772	rVB	504	209	0.01%	0.002%
48	6.748	1772	1775	1777	rBV2	343	232	0.01%	0.002%
49	6.809	1792	1794	1795	rBV	303	161	0.01%	0.001%
50	6.883	1815	1817	1822	rVB2	314	189	0.01%	0.001%
51	6.915	1825	1827	1832	rVV3	180	156	0.01%	0.001%
52	6.989	1838	1850	1879	rBV	218943	401778	24.87%	3.128%
53	7.317	1939	1952	1974	rBV	797430	1396082	86.42%	10.870%
54	7.622	2038	2047	2072	rBV	149303	263738	16.33%	2.053%
55	7.912	2133	2137	2139	rBV4	309	283	0.02%	0.002%
56	7.986	2151	2160	2170	rVB4	6256	10166	0.63%	0.079%
57	8.034	2173	2175	2176	rBV4	408	145	0.01%	0.001%
58	8.088	2182	2192	2227	rBV	439993	784024	48.54%	6.104%
59	8.420	2291	2295	2296	rBV3	924	633	0.04%	0.005%
60	8.529	2326	2329	2331	rVB2	420	223	0.01%	0.002%
61	8.551	2334	2336	2341	rVB4	612	403	0.02%	0.003%
62	8.584	2341	2346	2351	rBV	421	458	0.03%	0.004%
63	8.677	2371	2375	2381	rVB2	265	279	0.02%	0.002%
64	8.706	2381	2384	2387	rBV2	373	233	0.01%	0.002%
65	8.802	2410	2414	2416	rBV2	465	267	0.02%	0.002%
66	8.854	2417	2430	2454	rBV	729795	1170916	72.49%	9.117%
67	9.117	2510	2512	2514	rBV2	279	117	0.01%	0.001%
68	9.137	2514	2518	2520	rBV3	473	315	0.02%	0.002%
69	9.198	2534	2537	2540	rBV2	188	131	0.01%	0.001%
70	9.275	2559	2561	2563	rBV2	293	169	0.01%	0.001%
71	9.336	2576	2580	2582	rBV2	250	172	0.01%	0.001%
72	9.436	2605	2611	2616	rVB2	199	272	0.02%	0.002%
73	9.513	2631	2635	2638	rBV3	192	166	0.01%	0.001%
74	9.641	2673	2675	2679	rVB2	366	223	0.01%	0.002%
75	9.821	2727	2731	2734	rBV2	216	183	0.01%	0.001%
76	9.886	2748	2751	2753	rBV2	245	129	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021529.D
 Acq On : 07 Jun 2021 14:58
 Operator : SY/MD
 Sample : M2605-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis

77	9.937	2764	2767	2770	rBV2	323	199	0.01%	0.002%
78	9.992	2779	2784	2786	rBV	310	252	0.02%	0.002%
79	10.130	2822	2827	2838	rVB5	2259	2966	0.18%	0.023%
80	10.175	2838	2841	2842	rBV5	359	187	0.01%	0.001%
81	10.217	2842	2854	2878	rVV	516145	818809	50.69%	6.375%
82	10.378	2898	2904	2905	rBV3	932	860	0.05%	0.007%
83	10.532	2950	2952	2953	rBV	269	116	0.01%	0.001%
84	10.825	3040	3043	3048	rVB2	425	315	0.02%	0.002%
85	10.850	3048	3051	3058	rBV4	676	628	0.04%	0.005%
86	10.989	3091	3094	3097	rBV	294	208	0.01%	0.002%
87	11.027	3103	3106	3111	rBV3	497	546	0.03%	0.004%
88	11.075	3118	3121	3124	rBB	348	198	0.01%	0.002%
89	11.149	3138	3144	3153	rVB5	1219	1685	0.10%	0.013%
90	11.191	3153	3157	3158	rBV	361	249	0.02%	0.002%
91	11.249	3163	3175	3197	rBV	850515	1319237	81.67%	10.271%
92	11.551	3267	3269	3273	rVB3	376	240	0.01%	0.002%
93	11.574	3273	3276	3278	rBV2	217	158	0.01%	0.001%
94	11.625	3278	3292	3312	rBV	856778	1354133	83.83%	10.543%
95	11.850	3358	3362	3366	rBV4	415	375	0.02%	0.003%
96	11.879	3366	3371	3375	rBV5	675	704	0.04%	0.005%
97	11.995	3405	3407	3409	rBV	289	148	0.01%	0.001%
98	12.201	3469	3471	3474	rBV3	359	206	0.01%	0.002%
99	12.355	3516	3519	3522	rBV2	448	307	0.02%	0.002%
100	12.644	3606	3609	3612	rBV2	233	151	0.01%	0.001%




Sum of corrected areas: 12843912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021529.D
Acq On : 07 Jun 2021 14:58
Operator : SY/MD
Sample : M2605-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

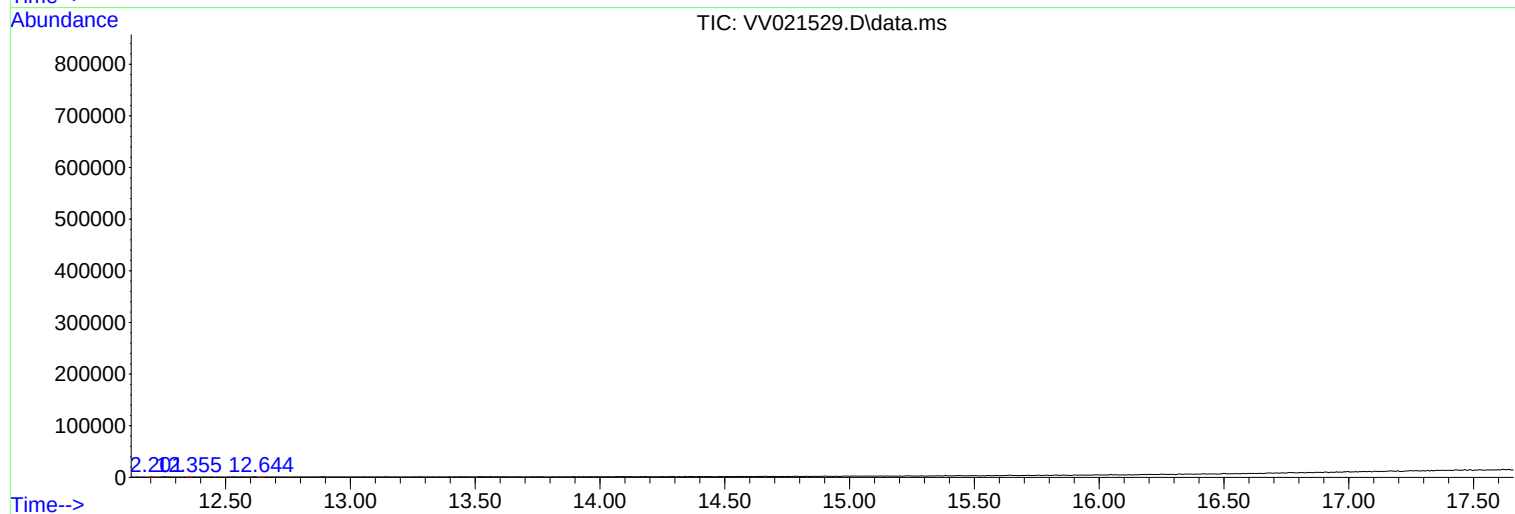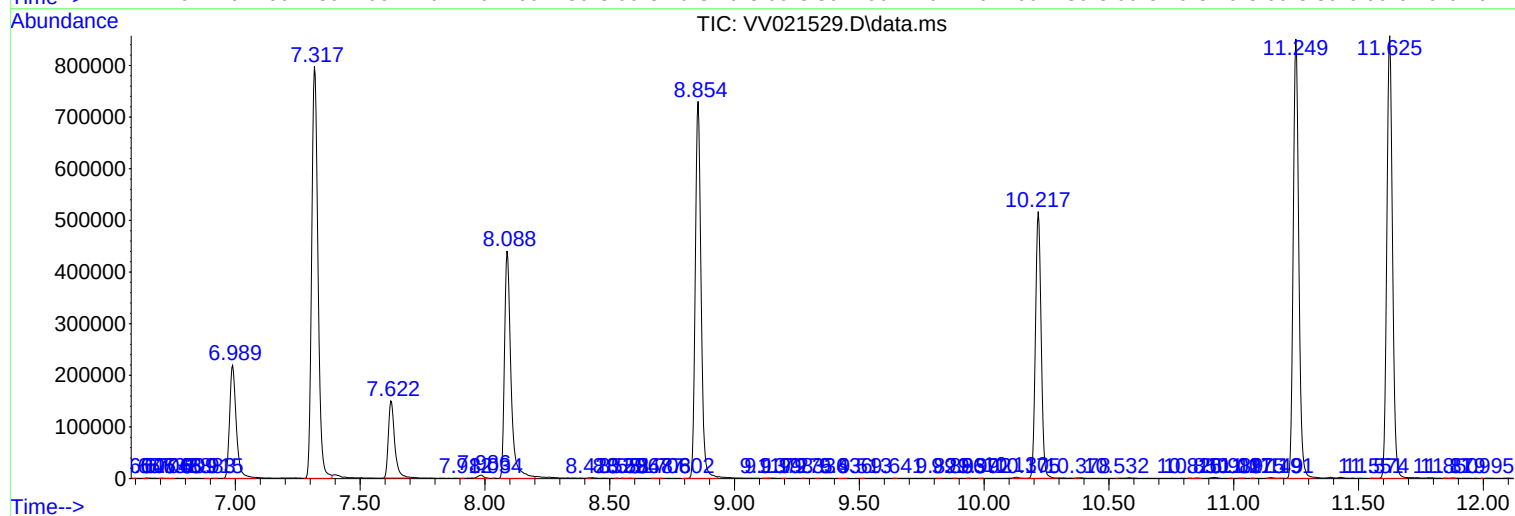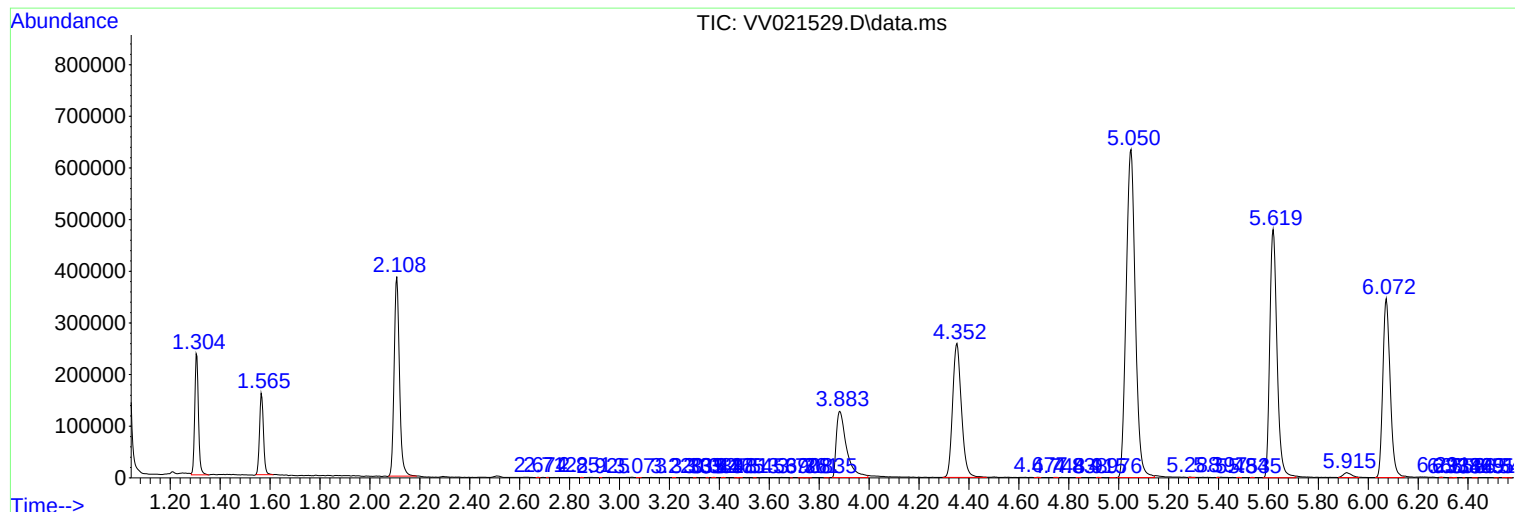

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021529.D
Acq On : 07 Jun 2021 14:58
Operator : SY/MD
Sample : M2605-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
Data File : VV021529.D
Acq On : 07 Jun 2021 14:58
Operator : SY/MD
Sample : M2605-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
Quant Title : VOC Analysis

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
