
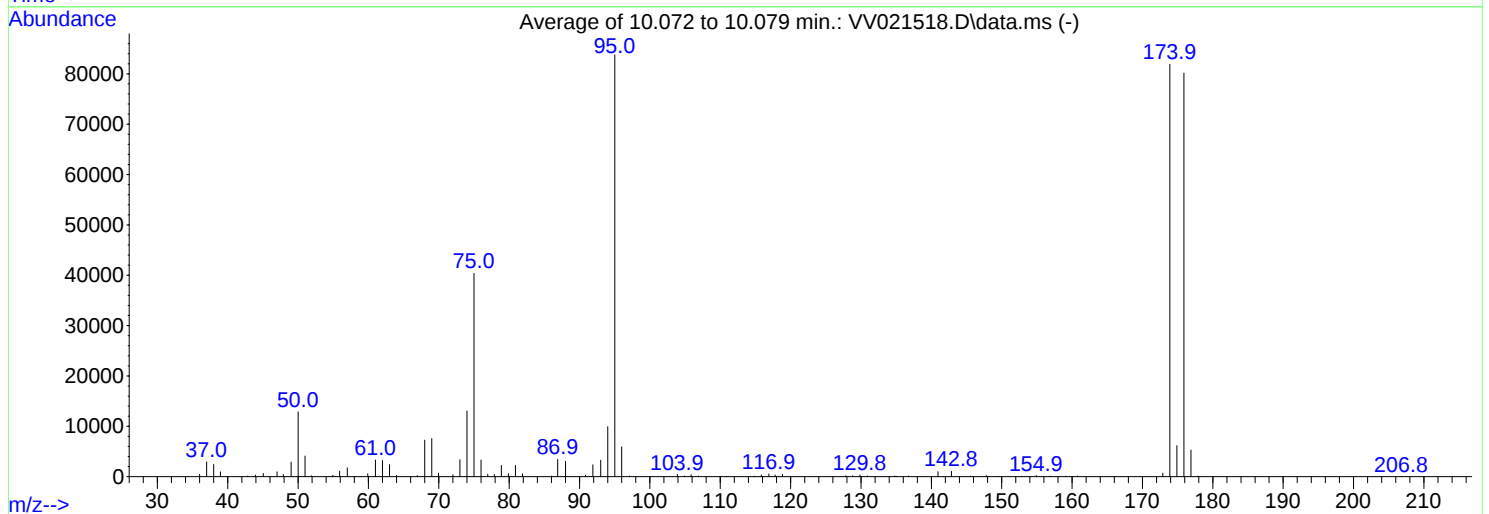


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060721\
 Data File : VV021518.D
 Acq On : 07 Jun 2021 10:13
 Operator : SY/MD
 Sample : BFB68
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB168

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM052721WMA.M
 Title : VOC Analysis
 Last Update : Tue Jun 08 03:17:01 2021

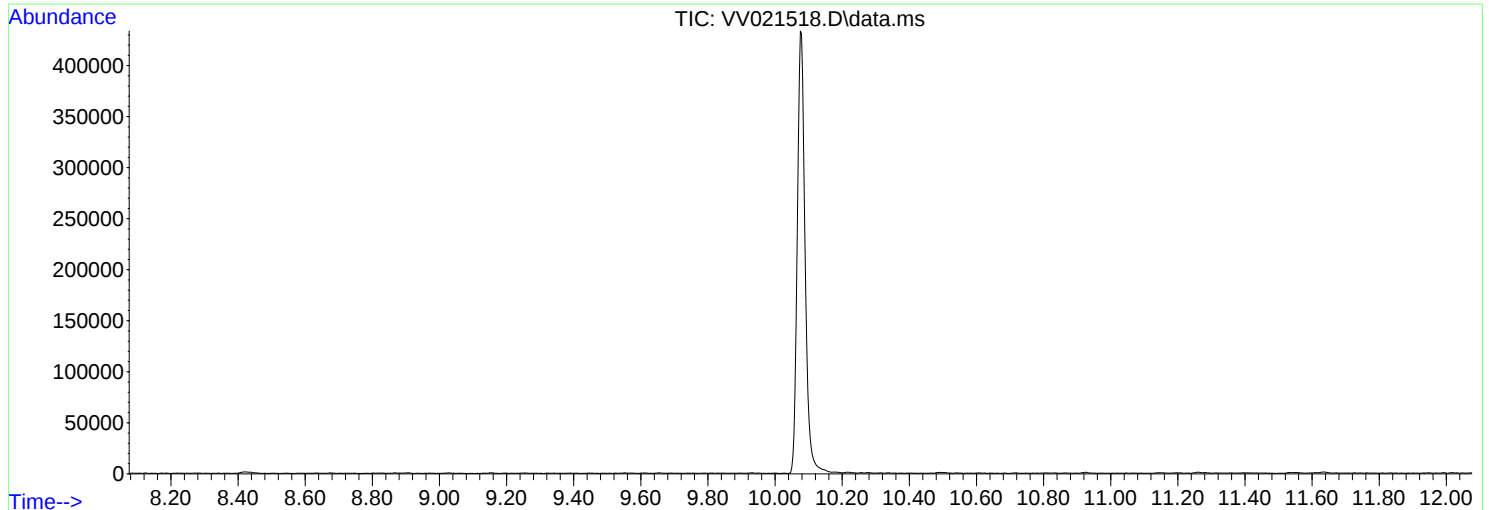

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.3	12856	PASS
75	95	30	80	48.2	40381	PASS
95	95	100	100	100.0	83771	PASS
96	95	5	9	7.0	5903	PASS
173	174	0.00	2	0.8	692	PASS
174	95	50	120	97.8	81904	PASS
175	174	5	9	7.5	6152	PASS
176	174	95	105	97.8	80128	PASS
177	176	5	10	6.6	5265	PASS

m/z	Abundance
36.00	468.0
37.00	2873.0
38.00	2482.0
38.90	936.0
39.90	190.0
42.80	104.0
44.00	727.0
45.10	643.0
47.00	998.0
47.90	460.0
49.00	2978.0
50.00	12810.0
51.00	4126.0
51.90	202.0
54.90	297.0
55.90	1061.0
57.00	1807.0
59.90	551.0
61.00	3393.0
62.00	3313.0
63.00	2436.0
64.00	294.0
66.90	215.0
68.00	7377.0
69.00	7720.0
70.00	669.0
72.00	374.0
73.00	3481.0
74.00	13126.0
75.00	40896.0
76.00	3259.0
77.00	525.0
77.90	351.0
78.90	2335.0
79.90	580.0
80.90	2167.0
81.90	583.0
86.10	129.0
86.90	3488.0
88.00	3126.0
90.90	342.0
91.90	2359.0
93.00	3198.0
94.00	10076.0
95.00	85480.0
96.00	5798.0
97.10	154.0
103.90	486.0
104.90	104.0
105.80	412.0
106.80	128.0
114.80	104.0
115.90	383.0
116.90	542.0
117.80	364.0
118.80	566.0
127.90	196.0
128.80	178.0
129.80	367.0
130.90	178.0
135.00	170.0
136.80	135.0
140.90	1023.0
142.80	1125.0
145.70	134.0
147.80	199.0
152.80	120.0
154.90	259.0
156.70	152.0
159.10	160.0
160.80	138.0
172.90	747.0
173.90	85720.0
174.90	6415.0
175.90	83888.0
176.90	5411.0
177.90	125.0

Instrument :
MSVOA_V
ClientSampleId :
BFB168

m/z	Abundance
36.00	457.0
37.00	3012.0
38.00	2513.0
39.00	966.0
39.90	210.0
42.80	132.0
44.00	735.0
45.00	683.0
47.00	1011.0
47.90	417.0
49.00	3013.0
50.00	13301.0
51.00	4209.0
51.90	180.0
54.90	289.0
55.90	1127.0
57.00	1830.0
58.10	117.0
59.90	606.0
61.00	3447.0
62.00	3302.0
63.00	2471.0
64.00	287.0
67.00	215.0
68.00	7516.0
69.00	7878.0
70.00	728.0
72.00	401.0
73.00	3523.0
74.00	13487.0
75.00	41944.0
76.00	3407.0
77.00	502.0
77.90	418.0
78.90	2302.0
79.90	606.0
80.90	2276.0
81.90	589.0
86.10	121.0
86.90	3542.0
88.00	3108.0
90.90	289.0
91.90	2473.0
93.00	3380.0
94.00	10240.0
95.00	86552.0
96.00	6147.0
97.10	154.0
103.90	450.0
104.90	124.0
105.90	378.0
106.90	137.0
110.80	120.0
114.80	110.0
115.90	385.0
116.90	553.0
117.80	316.0
118.80	488.0
127.90	187.0
128.80	202.0
129.90	397.0
130.90	158.0
134.80	191.0
136.70	133.0
140.90	1011.0
141.70	104.0
142.80	1092.0
145.60	123.0
147.80	212.0
149.60	106.0
152.80	121.0
154.90	248.0
157.00	145.0
159.10	150.0
160.80	128.0
172.90	709.0
173.90	84688.0
174.90	6325.0
175.90	82648.0
176.90	5432.0
177.90	138.0

Instrument :
MSVOA_V
ClientSampleId :
BFB168

m/z	Abundance
39.90	152.0
43.90	392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB168

m/z	Abundance
36.00	473.0
37.00	2851.0
38.00	2292.0
39.00	971.0
39.90	222.0
42.90	122.0
44.00	657.0
45.00	571.0
47.00	895.0
47.90	364.0
49.00	2703.0
50.00	12458.0
51.00	3945.0
51.90	167.0
55.00	265.0
55.90	1029.0
57.00	1625.0
58.10	111.0
59.90	564.0
61.00	3071.0
62.00	3013.0
63.00	2282.0
64.00	232.0
67.00	193.0
68.00	6857.0
69.00	7070.0
69.90	696.0
72.00	396.0
73.00	3082.0
74.00	12565.0
75.00	38304.0
76.00	3239.0
76.90	441.0
77.90	445.0
78.90	2047.0
79.90	596.0
80.90	2197.0
81.90	515.0
86.00	123.0
86.90	3305.0
88.00	2905.0
90.80	228.0
91.90	2208.0
93.00	3233.0
94.00	9383.0
95.00	79280.0
96.00	5764.0
97.10	121.0
103.90	374.0
104.90	124.0
105.90	332.0
107.00	131.0
110.90	129.0
114.90	106.0
115.80	316.0
116.90	527.0
117.80	290.0
118.90	363.0
127.80	205.0
128.80	175.0
129.80	336.0
130.90	137.0
134.80	170.0
136.70	140.0
141.00	889.0
142.90	946.0
145.50	110.0
147.80	214.0
154.90	207.0
156.90	133.0
160.80	109.0
172.90	620.0
173.90	75304.0
174.90	5717.0
175.90	73848.0
176.90	4953.0
177.90	163.0
206.80	102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB168