

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031412.D
 Acq On : 07 Jun 2023 21:09
 Operator : SY/MD
 Sample : VV0607WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Quant Time: Jun 08 05:17:28 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 08 05:16:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.542	114	252983	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	261010	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	124357	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	99972	44.914	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	89.820%
7) Chloroethane-d5	1.532	69	84206	46.728	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.460%
11) 1,1-Dichloroethene-d2	2.063	65	49657	47.072	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.140%
21) 2-Butanone-d5	3.796	46	142228	88.418	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	88.420%
24) Chloroform-d	4.256	84	196831	46.489	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	92.980%
26) 1,2-Dichloroethane-d4	4.950	65	137469	48.399	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.800%
32) Benzene-d6	4.966	84	351235	45.579	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.160%
36) 1,2-Dichloropropane-d6	5.995	67	125473	46.843	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	93.680%
41) Toluene-d8	7.249	98	305705	43.185	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.380%
43) trans-1,3-Dichloroprop...	7.558	79	55729	41.304	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	82.600%
47) 2-Hexanone-d5	8.030	63	75063	74.405	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.400%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	140389	41.531	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	83.060%
66) 1,2-Dichlorobenzene-d4	11.567	152	117129	50.774	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.540%
Target Compounds						
12) 1,1-Dichloroethene	2.063	96	1480	1.466	ug/L	Qvalue # 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031412.D
Acq On : 07 Jun 2023 21:09
Operator : SY/MD
Sample : VV0607WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Time: Jun 08 05:17:28 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 08 05:16:53 2023
Response via : Initial Calibration

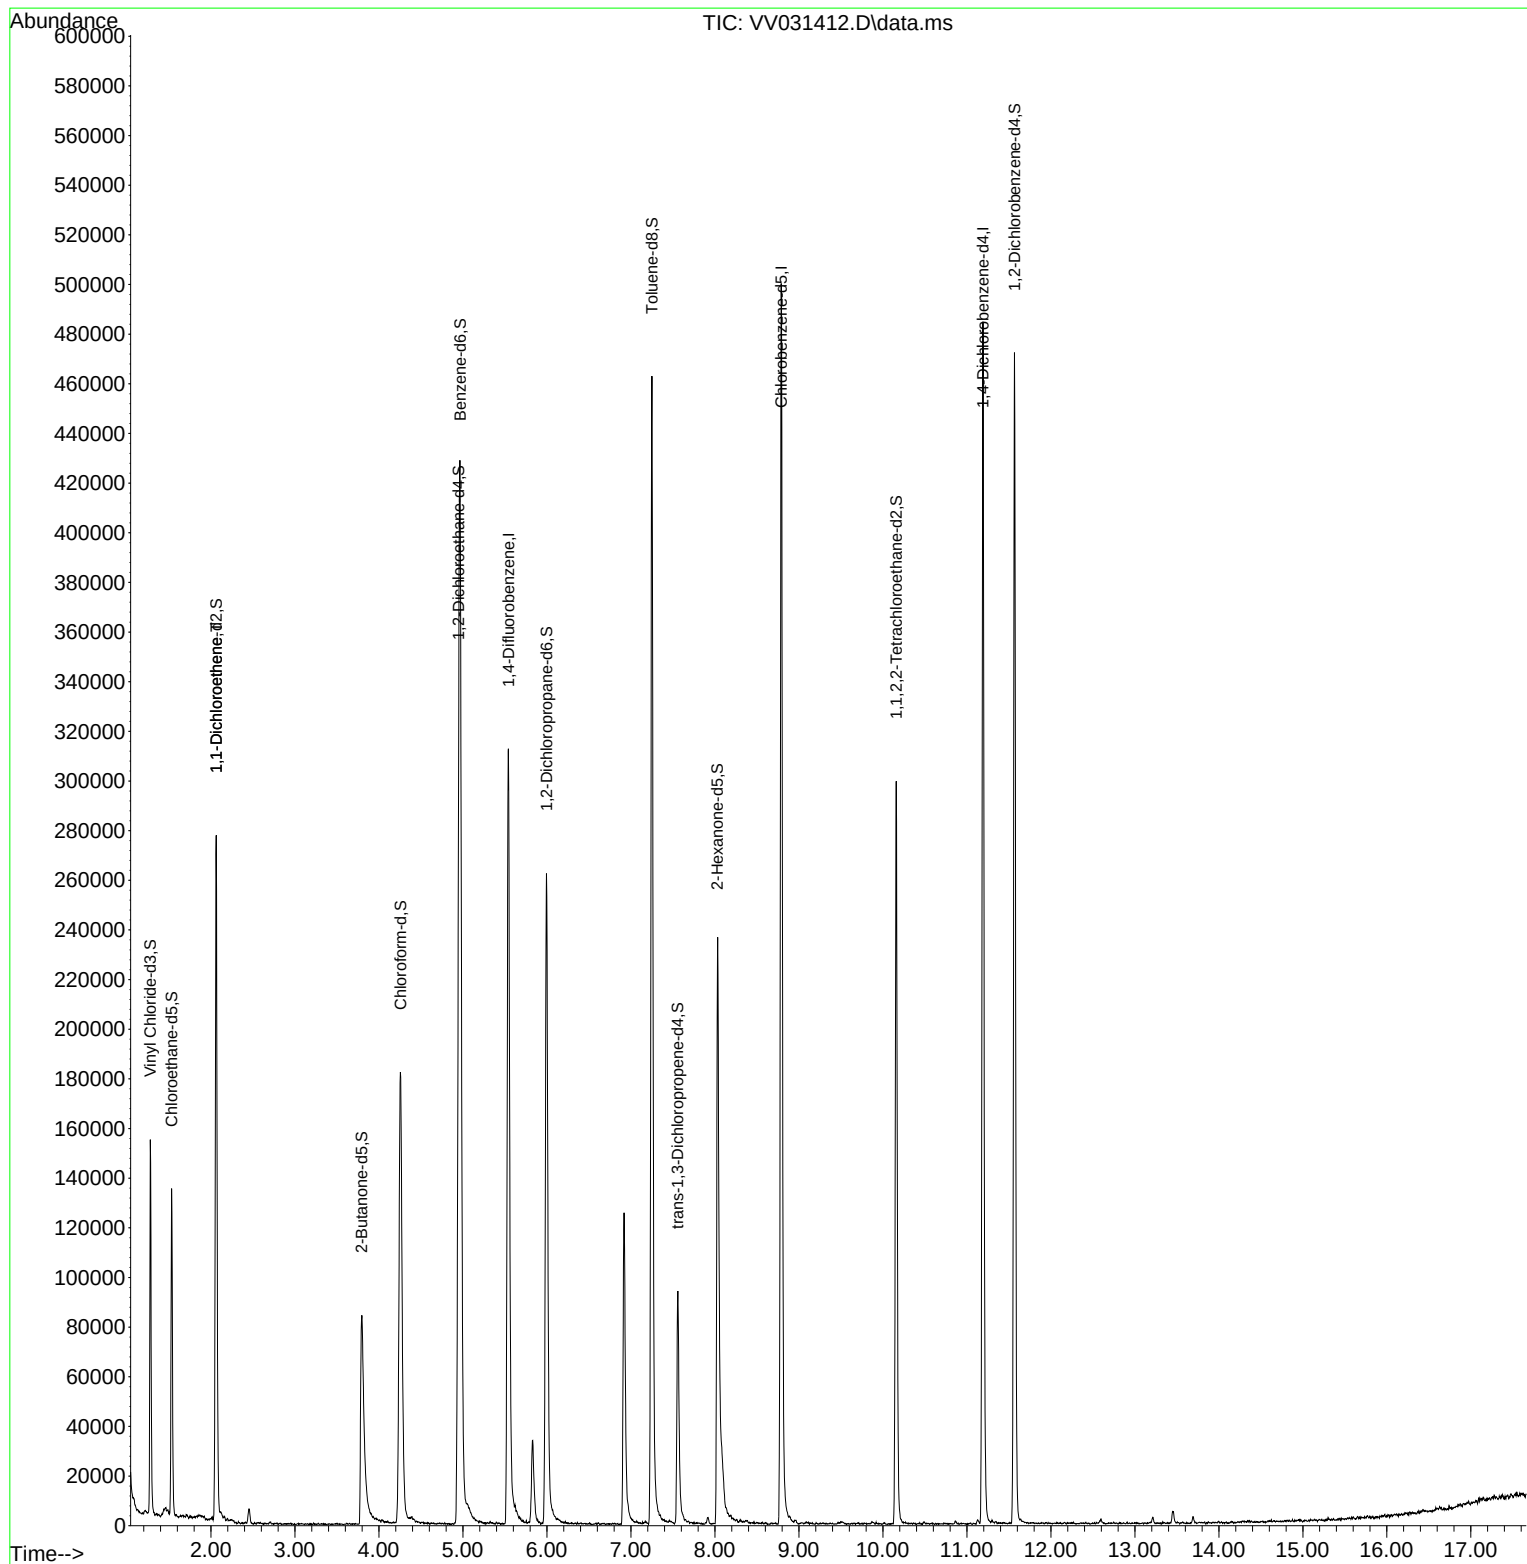

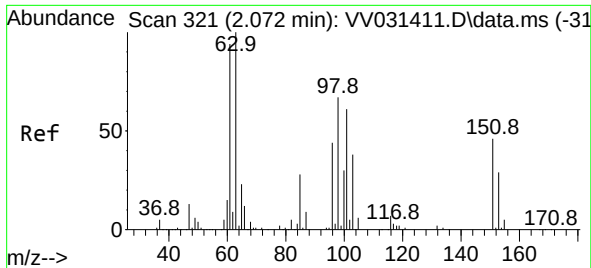

#12
 1,1-Dichloroethene
 Concen: 1.466 ug/L
 RT: 2.063 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV031412.D
 Acq: 07 Jun 2023 21:09

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Tgt Ion: 96 Resp: 1480
 Ion Ratio Lower Upper
 96 100
 61 1300.4 143.9 267.3#
 63 10452.4 158.3 293.9#

