

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031399.D
 Acq On : 07 Jun 2023 15:16
 Operator : SY/MD
 Sample : 03076-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F79

Quant Time: Jun 08 04:24:27 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 08 04:14:38 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	268891	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	273692	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	132238	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	106066	44.833	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	89.660%	
7) Chloroethane-d5	1.532	69	90717	47.363	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	94.720%	
11) 1,1-Dichloroethene-d2	2.063	65	50585	45.115	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	90.220%	
21) 2-Butanone-d5	3.796	46	159184	93.104	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	93.100%	
24) Chloroform-d	4.256	84	210617	46.802	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.600%	
26) 1,2-Dichloroethane-d4	4.947	65	144349	47.815	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	95.620%	
32) Benzene-d6	4.966	84	379281	46.938	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	93.880%	
36) 1,2-Dichloropropane-d6	5.992	67	135905	48.387	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	96.780%	
41) Toluene-d8	7.249	98	335046	45.137	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	90.280%	
43) trans-1,3-Dichloroprop...	7.558	79	62490	44.168	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	88.340%	
47) 2-Hexanone-d5	8.030	63	86843	82.093	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	82.090%	
56) 1,1,2,2-Tetrachloroeth...	10.159	84	156276	44.089	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.180%	
66) 1,2-Dichlorobenzene-d4	11.567	152	123269	50.251	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	100.500%	
Target Compounds						
13) Acetone	2.127	43	5755	3.763	ug/L	Qvalue 90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031399.D
Acq On : 07 Jun 2023 15:16
Operator : SY/MD
Sample : 03076-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F79

Quant Time: Jun 08 04:24:27 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 08 04:14:38 2023
Response via : Initial Calibration

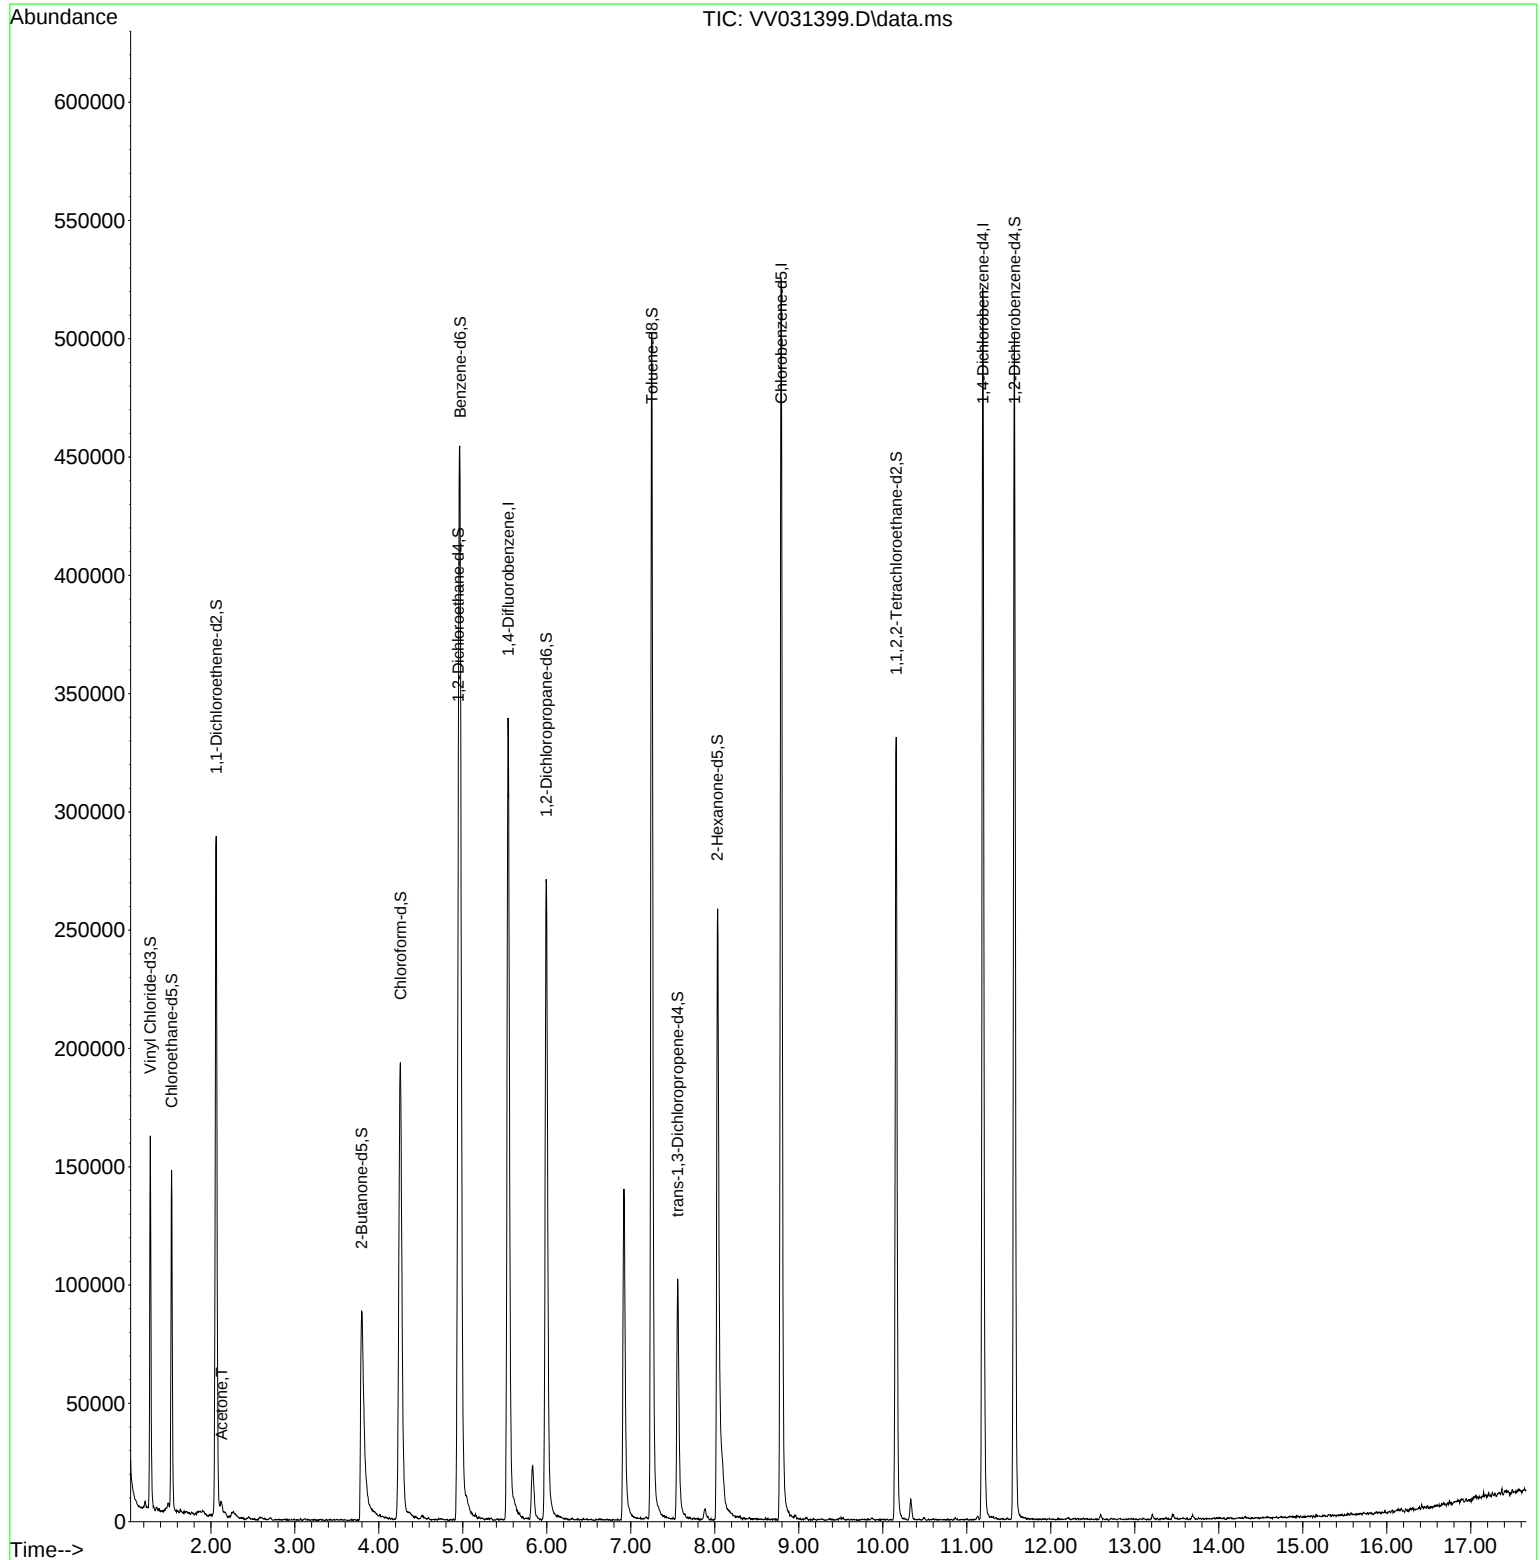

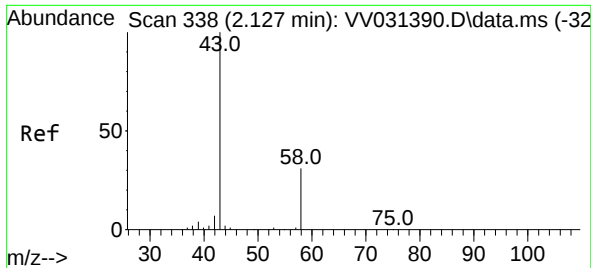

#13

Acetone

Concen: 3.763 ug/L

RT: 2.127 min Scan# 33

Delta R.T. -0.000 min

Lab File: VV031399.D


Acq: 07 Jun 2023 15:16

Instrument :

MSVOA_V

ClientSampleId :

C0F79

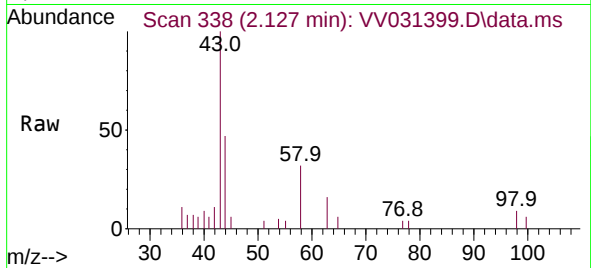

Tgt Ion: 43 Resp: 5755

Ion Ratio Lower Upper

43 100

58 25.1 0.0 61.0

