

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031417.D
 Acq On : 07 Jun 2023 23:07
 Operator : SY/MD
 Sample : 03076-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F94

Quant Time: Jun 08 05:45:29 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 08 05:16:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	244889	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	252160	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	120910	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	95351	44.254	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	88.500%
7) Chloroethane-d5	1.532	69	82594	47.348	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	94.700%
11) 1,1-Dichloroethene-d2	2.063	65	47070	46.095	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	92.180%
21) 2-Butanone-d5	3.796	46	141704	91.003	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	91.000%
24) Chloroform-d	4.256	84	197761	48.252	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.500%
26) 1,2-Dichloroethane-d4	4.947	65	137229	49.911	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.820%
32) Benzene-d6	4.966	84	351238	47.179	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	94.360%
36) 1,2-Dichloropropane-d6	5.995	67	127310	49.197	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	98.400%
41) Toluene-d8	7.249	98	303563	44.388	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	88.780%
43) trans-1,3-Dichloroprop...	7.558	79	56545	43.379	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.760%
47) 2-Hexanone-d5	8.034	63	72141	74.018	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	74.020%
56) 1,1,2,2-Tetrachloroeth...	10.159	84	145780	44.639	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	89.280%
66) 1,2-Dichlorobenzene-d4	11.567	152	116810	52.079	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	104.160%
Target Compounds					Qvalue	
13) Acetone	2.124	43	8432	6.053	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031417.D
Acq On : 07 Jun 2023 23:07
Operator : SY/MD
Sample : 03076-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F94

Quant Time: Jun 08 05:45:29 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 08 05:16:53 2023
Response via : Initial Calibration

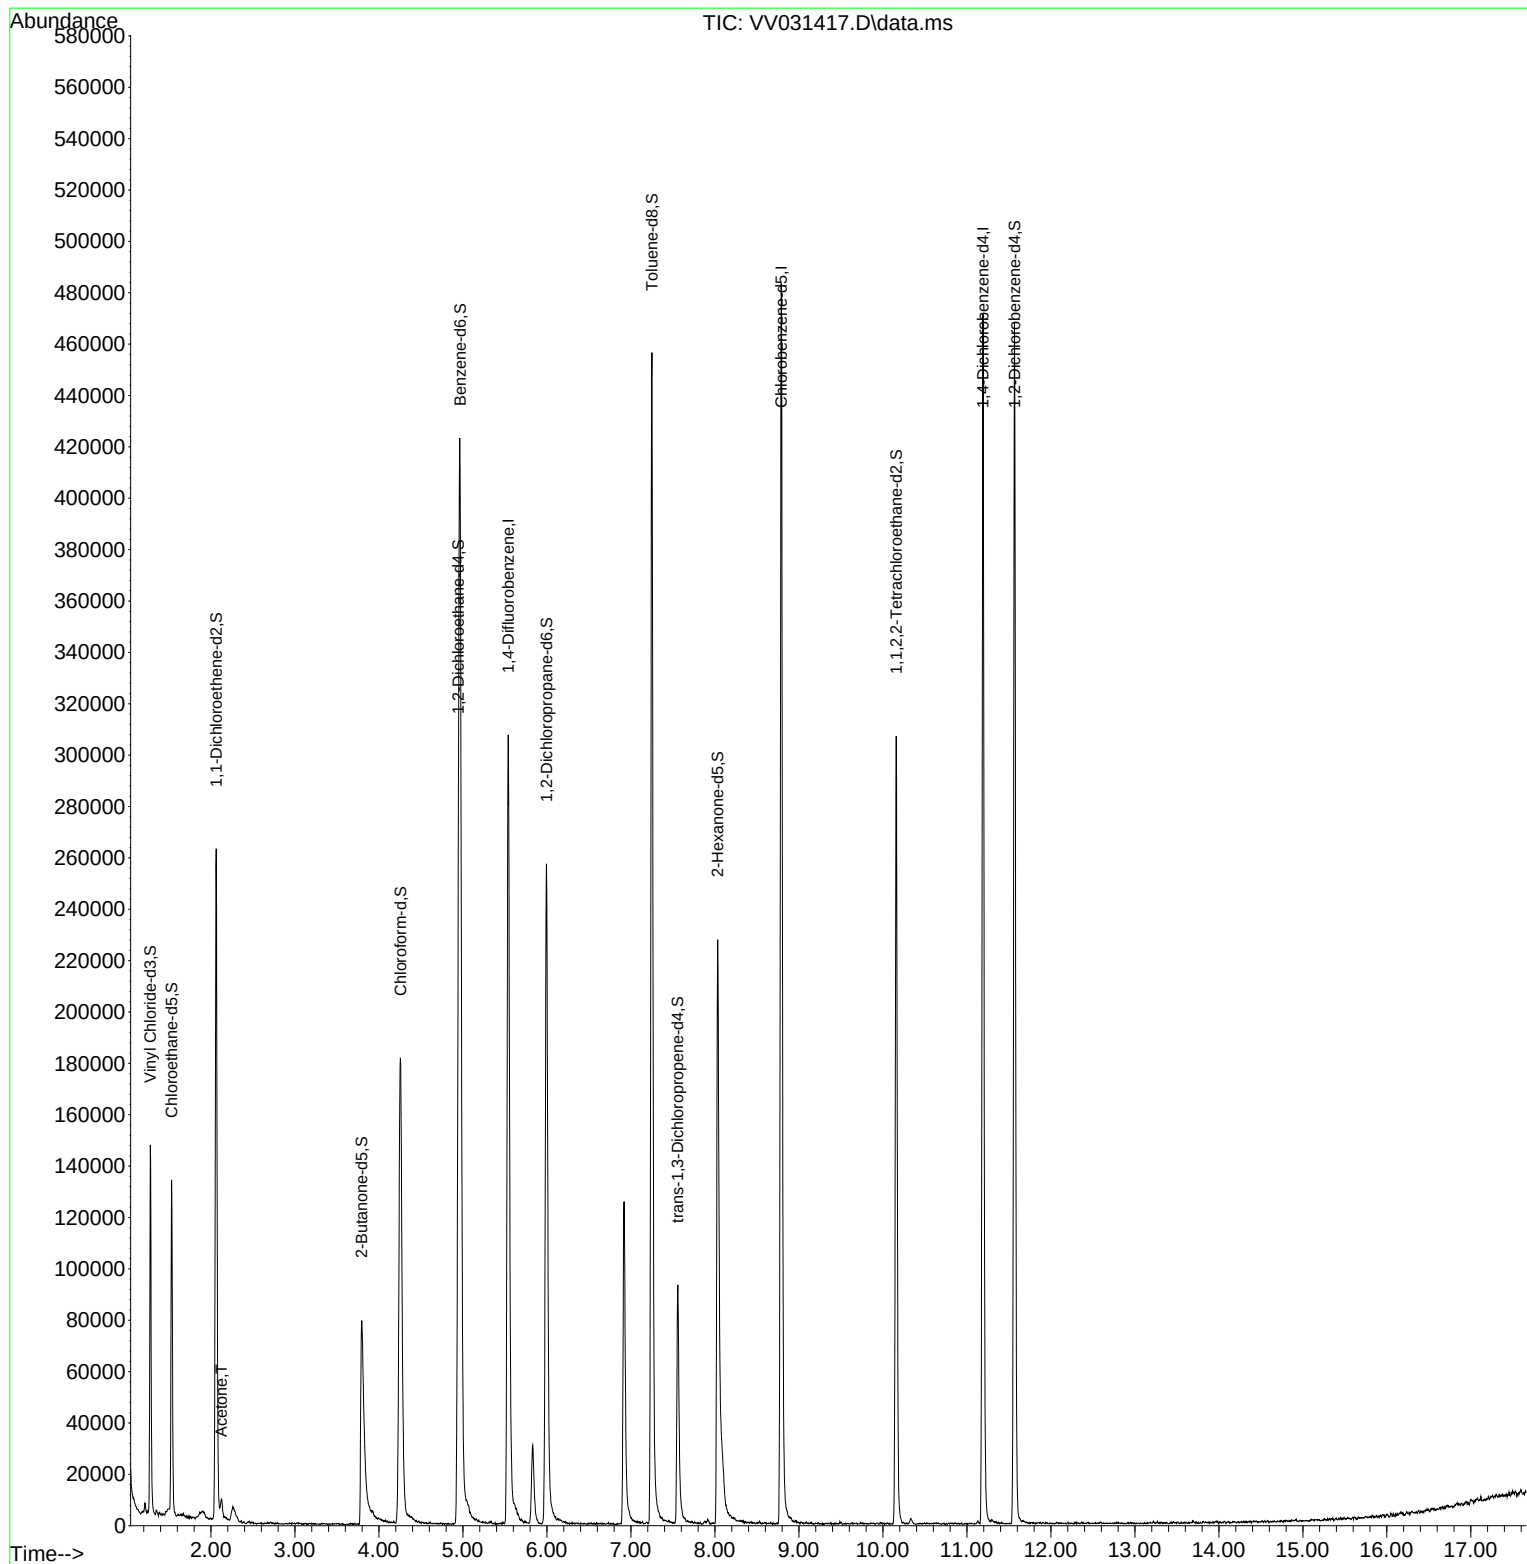

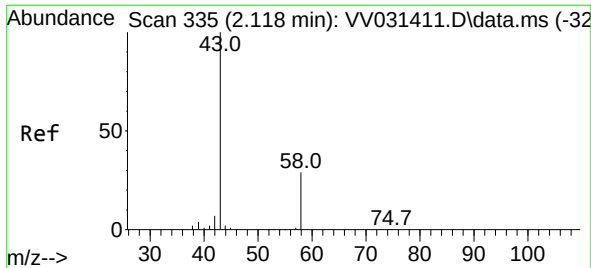

#13

Acetone

Concen: 6.053 ug/L

RT: 2.124 min Scan# 31

Delta R.T. 0.006 min

Lab File: VV031417.D

Acq: 07 Jun 2023 23:07

Instrument :

MSVOA_V

ClientSampleId :

C0F94

Tgt Ion: 43 Resp: 8432

Ion Ratio Lower Upper

43 100

58 27.8 0.0 61.0

