

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031419.D
 Acq On : 07 Jun 2023 23:55
 Operator : SY/MD
 Sample : 03076-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F97

Quant Time: Jun 08 05:45:55 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 08 05:16:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	237744	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	244786	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	117537	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	92664	44.300	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	88.600%		
7) Chloroethane-d5	1.532	69	78724	46.486	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	92.980%		
11) 1,1-Dichloroethene-d2	2.060	65	46693	47.100	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	94.200%		
21) 2-Butanone-d5	3.793	46	142243	94.095	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	94.090%		
24) Chloroform-d	4.256	84	193628	48.664	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.320%		
26) 1,2-Dichloroethane-d4	4.947	65	135783	50.870	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.740%		
32) Benzene-d6	4.966	84	343130	47.479	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.960%		
36) 1,2-Dichloropropane-d6	5.992	67	122806	48.886	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	97.780%		
41) Toluene-d8	7.249	98	294159	44.308	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	88.620%		
43) trans-1,3-Dichloroprop...	7.558	79	55178	43.606	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.220%		
47) 2-Hexanone-d5	8.030	63	74787	79.044	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	79.040%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	144544	45.594	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	91.180%		
66) 1,2-Dichlorobenzene-d4	11.567	152	117746	54.003	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.000%		
Target Compounds					Qvalue	
13) Acetone	2.117	43	5369	3.970	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031419.D
Acq On : 07 Jun 2023 23:55
Operator : SY/MD
Sample : 03076-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F97

Quant Time: Jun 08 05:45:55 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 08 05:16:53 2023
Response via : Initial Calibration

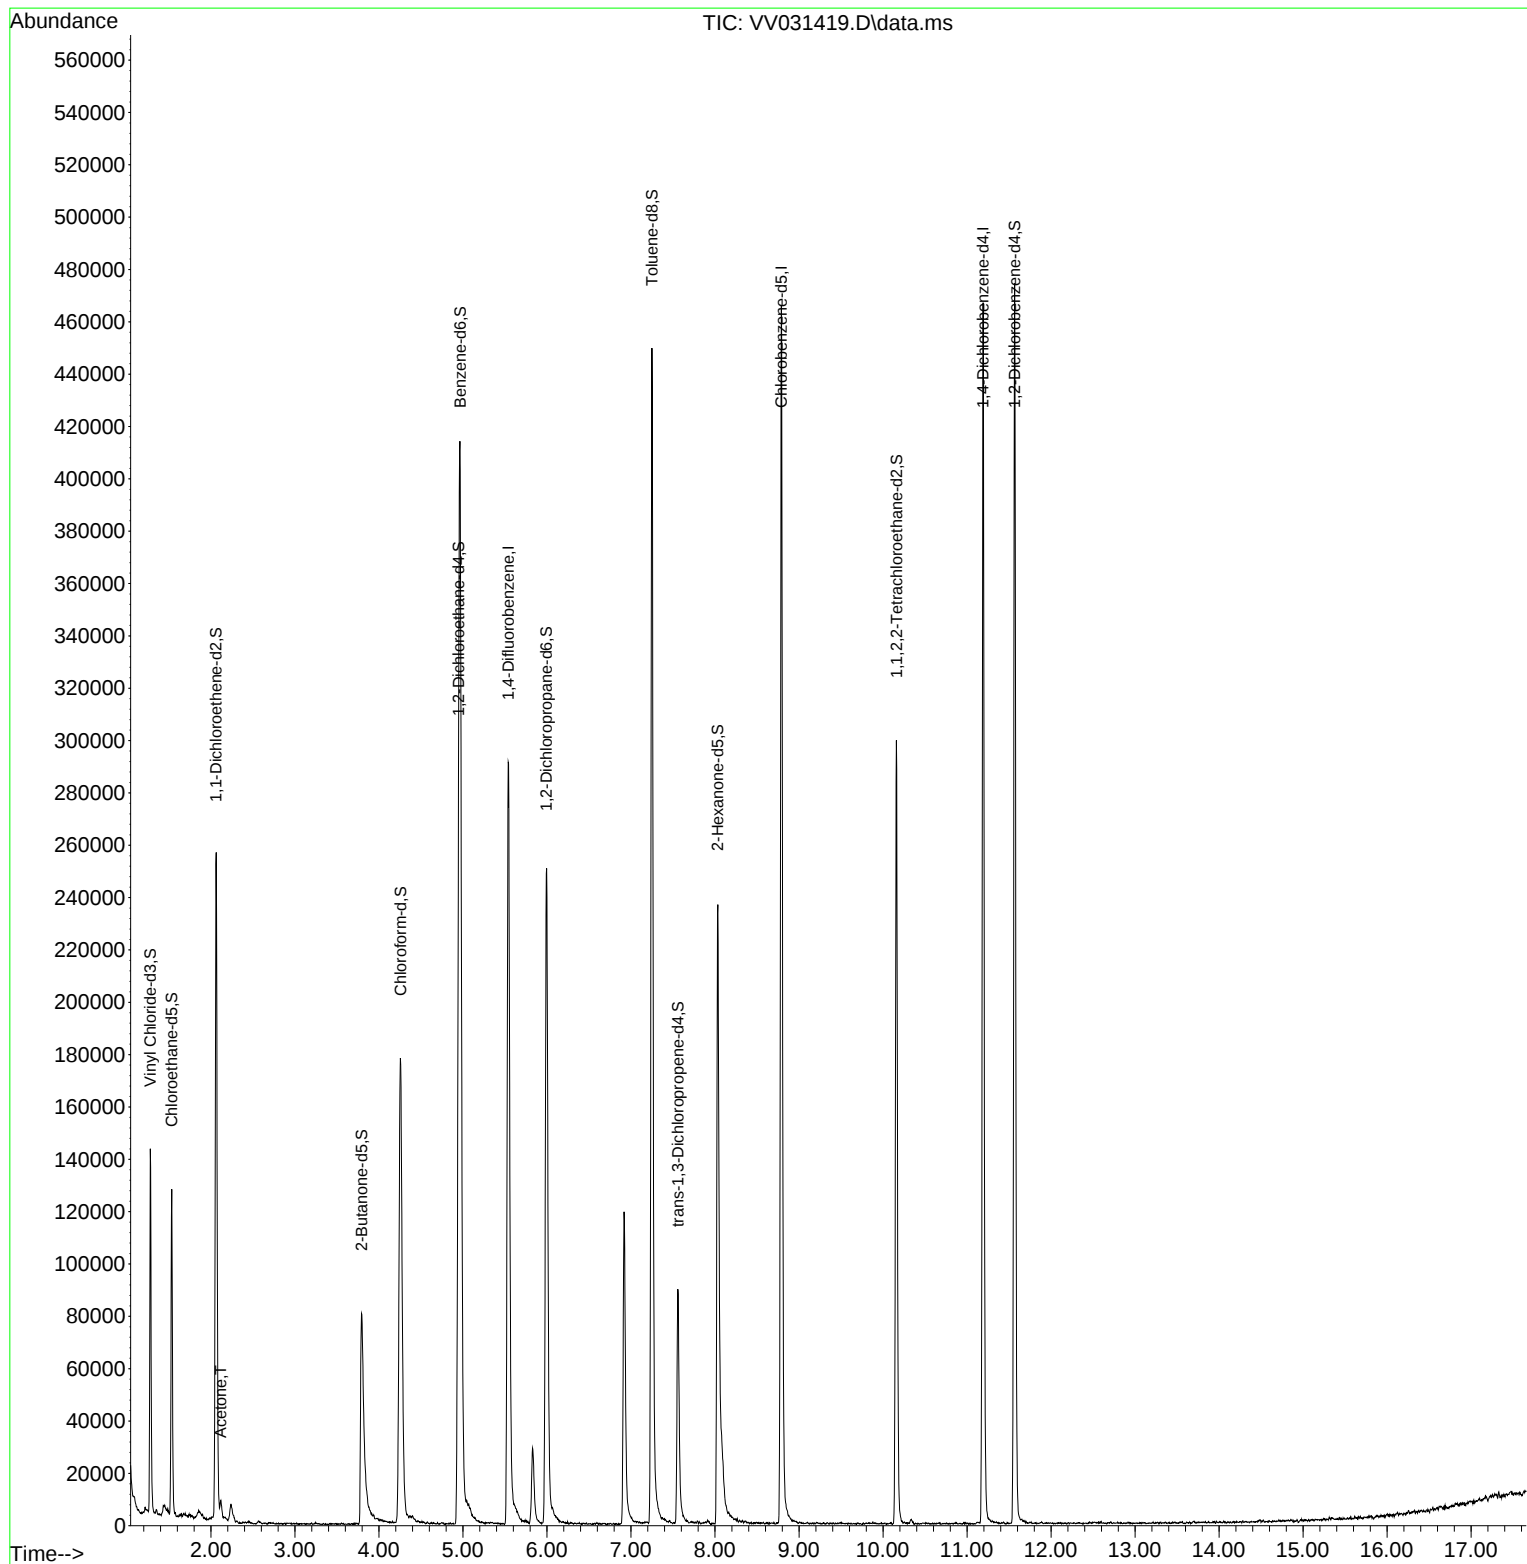

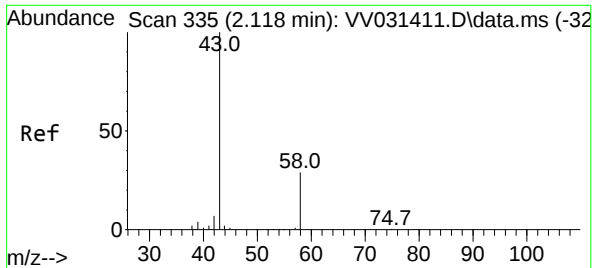

#13
 Acetone
 Concen: 3.970 ug/L
 RT: 2.117 min Scan# 31
 Delta R.T. -0.000 min
 Lab File: VV031419.D
 Acq: 07 Jun 2023 23:55

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F97

Tgt Ion: 43 Resp: 5369
 Ion Ratio Lower Upper
 43 100
 58 35.4 0.0 61.0

