

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031429.D
 Acq On : 08 Jun 2023 03:53
 Operator : SY/MD
 Sample : 03077-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB2

Quant Time: Jun 08 05:48:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 08 05:16:53 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.539	114	247801	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.789	117	253861	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.191	152	117176	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	88688	40.678	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	81.360%		
7) Chloroethane-d5	1.532	69	78296	44.357	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	88.720%		
11) 1,1-Dichloroethene-d2	2.063	65	43394	41.995	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	84.000%		
21) 2-Butanone-d5	3.793	46	143887	91.319	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	91.320%		
24) Chloroform-d	4.256	84	185527	44.735	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.480%		
26) 1,2-Dichloroethane-d4	4.947	65	131672	47.328	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.660%		
32) Benzene-d6	4.966	84	334143	44.582	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.160%		
36) 1,2-Dichloropropane-d6	5.995	67	120503	46.255	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.500%		
41) Toluene-d8	7.249	98	286610	41.628	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.260%		
43) trans-1,3-Dichloroprop...	7.558	79	52251	39.816	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.640%		
47) 2-Hexanone-d5	8.034	63	68999	70.320	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.320%		
56) 1,1,2,2-Tetrachloroeth...	10.159	84	123726	37.632	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	75.260%		
66) 1,2-Dichlorobenzene-d4	11.567	152	110470	50.822	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.640%		
Target Compounds					Qvalue	
13) Acetone	2.121	43	6365	4.516	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031429.D
Acq On : 08 Jun 2023 03:53
Operator : SY/MD
Sample : 03077-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB2

Quant Time: Jun 08 05:48:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 08 05:16:53 2023
Response via : Initial Calibration

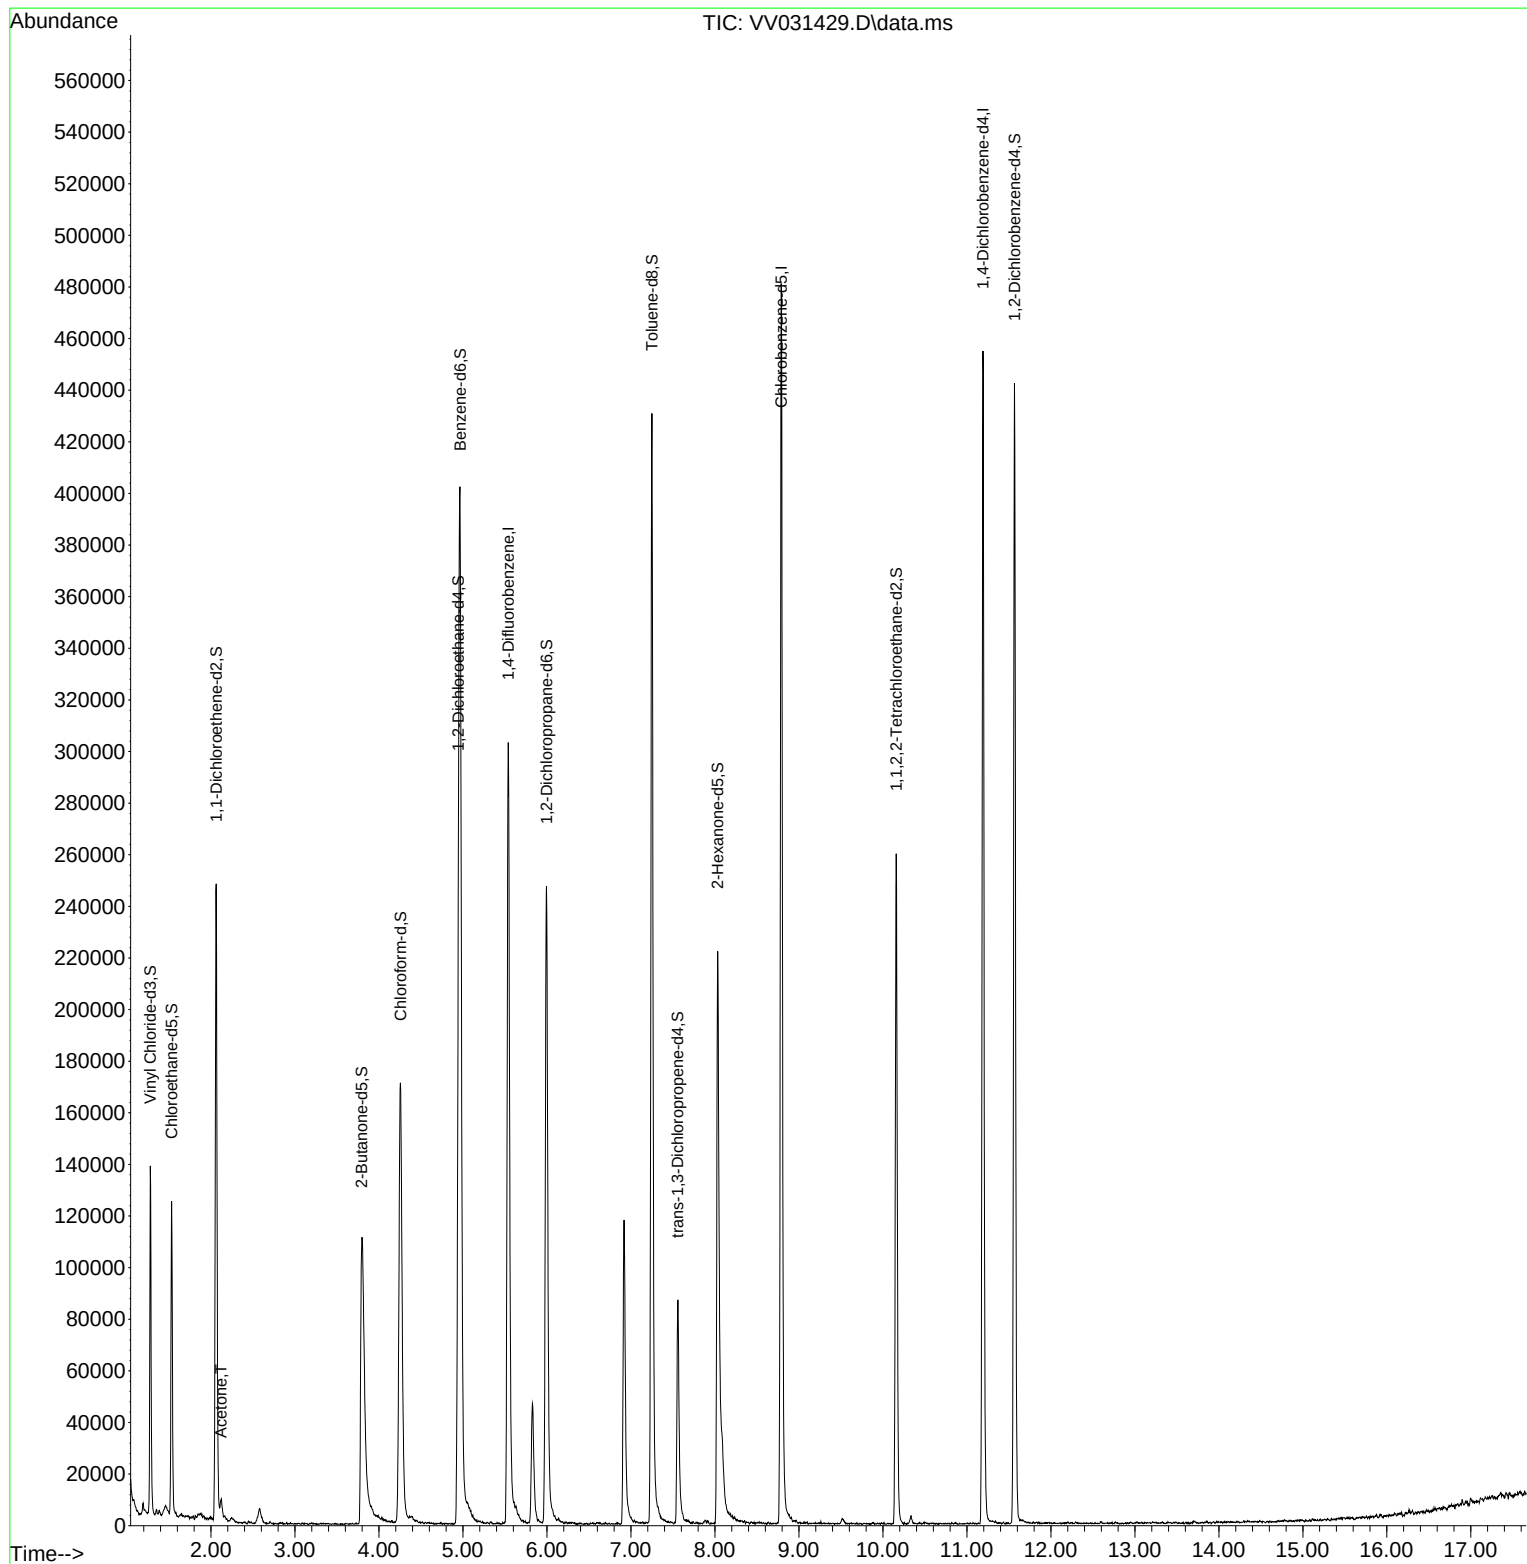

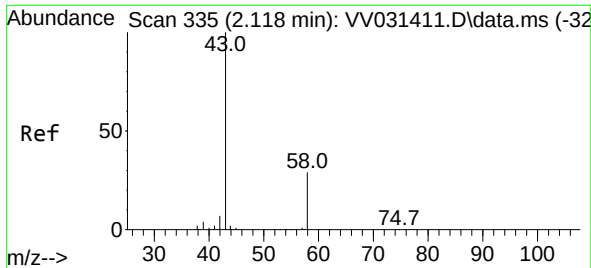

#13
 Acetone
 Concen: 4.516 ug/L
 RT: 2.121 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VV031429.D
 Acq: 08 Jun 2023 03:53

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB2

Tgt Ion: 43 Resp: 6365
 Ion Ratio Lower Upper
 43 100
 58 34.0 0.0 61.0

