

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031394.D
 Acq On : 07 Jun 2023 13:17
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031394.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	180259	192955	14.71%	1.965%
2	1.532	146	153	170	rVB	156381	184988	14.10%	1.884%
3	2.063	308	318	334	rBV	312800	463940	35.37%	4.726%
4	2.545	466	468	471	rVB2	739	363	0.03%	0.004%
5	2.774	537	539	542	rBB3	391	190	0.01%	0.002%
6	2.815	550	552	555	rVV2	373	190	0.01%	0.002%
7	2.831	555	557	561	rVB2	382	166	0.01%	0.002%
8	3.005	605	611	615	rBV4	611	635	0.05%	0.006%
9	3.082	632	635	636	rBV2	327	168	0.01%	0.002%
10	3.095	637	639	641	rVV	428	179	0.01%	0.002%
11	3.156	656	658	660	rVB2	520	192	0.01%	0.002%
12	3.175	662	664	667	rVV	374	231	0.02%	0.002%
13	3.262	688	691	693	rBV3	471	268	0.02%	0.003%
14	3.275	693	695	698	rBV	260	197	0.02%	0.002%
15	3.339	711	715	716	rBV2	510	313	0.02%	0.003%
16	3.384	724	729	731	rBV3	421	371	0.03%	0.004%
17	3.420	738	740	743	rBV2	573	340	0.03%	0.003%
18	3.462	748	753	754	rBV3	497	331	0.03%	0.003%
19	3.626	800	804	810	rVB3	306	293	0.02%	0.003%
20	3.651	810	812	814	rBV2	363	186	0.01%	0.002%
21	3.677	817	820	823	rVB2	542	315	0.02%	0.003%
22	3.799	848	858	893	rBV2	98015	288173	21.97%	2.935%
23	4.256	984	1000	1026	rBV	204353	527054	40.18%	5.369%
24	4.580	1098	1101	1106	rBV5	810	698	0.05%	0.007%
25	4.632	1114	1117	1118	rBV5	389	185	0.01%	0.002%
26	4.722	1143	1145	1147	rVB	397	158	0.01%	0.002%
27	4.735	1147	1149	1152	rBV	491	372	0.03%	0.004%
28	4.777	1160	1162	1164	rBV2	301	153	0.01%	0.002%
29	4.960	1202	1219	1244	rBV2	497547	1311610	100.00%	13.360%
30	5.269	1311	1315	1316	rBV3	648	373	0.03%	0.004%
31	5.359	1341	1343	1346	rVB3	604	222	0.02%	0.002%
32	5.436	1365	1367	1368	rBV	556	208	0.02%	0.002%
33	5.471	1376	1378	1379	rBV	718	341	0.03%	0.003%
34	5.539	1387	1399	1419	rBV	355043	731970	55.81%	7.456%
35	5.831	1478	1490	1507	rBV3	28159	61512	4.69%	0.627%
36	5.992	1527	1540	1568	rBV	295854	620401	47.30%	6.320%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031394.D
 Acq On : 07 Jun 2023 13:17
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.265	1621	1625	1629	rBV3	305	289	0.02%	0.003%
38	6.375	1656	1659	1661	rVB2	460	287	0.02%	0.003%
39	6.394	1662	1665	1670	rBV4	438	391	0.03%	0.004%
40	6.445	1678	1681	1686	rBV4	605	486	0.04%	0.005%
41	6.490	1692	1695	1697	rVB2	328	163	0.01%	0.002%
42	6.555	1713	1715	1717	rBV	441	187	0.01%	0.002%
43	6.661	1743	1748	1750	rBV2	519	401	0.03%	0.004%
44	6.683	1753	1755	1759	rVB2	683	394	0.03%	0.004%
45	6.703	1759	1761	1763	rBV	254	156	0.01%	0.002%
46	6.754	1773	1777	1781	rVV3	330	298	0.02%	0.003%
47	6.799	1787	1791	1792	rBV	730	428	0.03%	0.004%
48	6.831	1799	1801	1804	rVB3	309	175	0.01%	0.002%
49	6.918	1817	1828	1854	rBV	156405	297756	22.70%	3.033%
50	7.140	1894	1897	1900	rBV3	1265	583	0.04%	0.006%
51	7.191	1905	1913	1918	rVB7	1244	1923	0.15%	0.020%
52	7.249	1918	1931	1952	rBV	558076	989909	75.47%	10.083%
53	7.558	2017	2027	2048	rBV	113186	208531	15.90%	2.124%
54	7.860	2117	2121	2125	rBV3	728	726	0.06%	0.007%
55	7.957	2149	2151	2154	rBV2	397	240	0.02%	0.002%
56	8.034	2165	2175	2211	rBV	291442	616958	47.04%	6.285%
57	8.371	2277	2280	2283	rBV3	782	532	0.04%	0.005%
58	8.529	2326	2329	2332	rBV3	616	543	0.04%	0.006%
59	8.596	2349	2350	2354	rVB3	743	422	0.03%	0.004%
60	8.629	2357	2360	2362	rBV3	699	481	0.04%	0.005%
61	8.641	2362	2364	2369	rVB3	898	710	0.05%	0.007%
62	8.680	2373	2376	2379	rBV4	882	589	0.04%	0.006%
63	8.696	2379	2381	2383	rVV2	528	238	0.02%	0.002%
64	8.789	2398	2410	2435	rBV	552649	921126	70.23%	9.383%
65	9.047	2487	2490	2491	rBV	472	242	0.02%	0.002%
66	9.056	2491	2493	2494	rBV	397	170	0.01%	0.002%
67	9.124	2512	2514	2518	rVB4	676	459	0.03%	0.005%
68	9.143	2518	2520	2523	rBV3	542	293	0.02%	0.003%
69	9.330	2574	2578	2580	rBV2	624	521	0.04%	0.005%
70	9.484	2620	2626	2627	rBV3	1045	761	0.06%	0.008%
71	9.770	2708	2715	2716	rBV3	641	635	0.05%	0.006%
72	9.834	2729	2735	2738	rVB3	473	426	0.03%	0.004%
73	9.866	2741	2745	2747	rBV2	1222	962	0.07%	0.010%
74	9.963	2773	2775	2779	rVV3	256	186	0.01%	0.002%
75	10.159	2824	2836	2864	rBV	352550	558128	42.55%	5.685%
76	10.288	2874	2876	2879	rBV2	339	195	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031394.D
 Acq On : 07 Jun 2023 13:17
 Operator : SY/MD
 Sample : VV0607WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK349

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.313	2880	2884	2886	rVB2	378	251	0.02%	0.003%
78	10.333	2886	2890	2893	rBV3	425	239	0.02%	0.002%
79	10.378	2902	2904	2906	rVB	462	152	0.01%	0.002%
80	10.429	2918	2920	2923	rBV	437	295	0.02%	0.003%
81	10.487	2930	2938	2945	rBV6	1769	2556	0.19%	0.026%
82	10.587	2966	2969	2974	rBV3	623	616	0.05%	0.006%
83	10.728	3011	3013	3015	rBV	291	169	0.01%	0.002%
84	10.866	3046	3056	3060	rBV6	1541	2427	0.19%	0.025%
85	11.008	3098	3100	3102	rBV2	518	224	0.02%	0.002%
86	11.130	3131	3138	3146	rVB5	3045	5033	0.38%	0.051%
87	11.191	3146	3157	3183	rBV	563755	883942	67.39%	9.004%
88	11.352	3204	3207	3210	rBV2	411	330	0.03%	0.003%
89	11.397	3219	3221	3227	rVB4	826	641	0.05%	0.007%
90	11.442	3233	3235	3236	rBV	428	168	0.01%	0.002%
91	11.497	3249	3252	3255	rBV	467	382	0.03%	0.004%
92	11.567	3262	3274	3298	rBV	555661	882568	67.29%	8.990%
93	11.728	3322	3324	3327	rVB3	551	185	0.01%	0.002%
94	12.046	3421	3423	3425	rBV2	368	207	0.02%	0.002%
95	12.754	3640	3643	3647	rBV3	440	399	0.03%	0.004%
96	13.207	3777	3784	3799	rVB6	5832	9578	0.73%	0.098%
97	13.288	3807	3809	3812	rBV	422	237	0.02%	0.002%
98	13.323	3816	3820	3821	rBV2	519	375	0.03%	0.004%
99	13.452	3852	3860	3872	rBV2	11291	17625	1.34%	0.180%
100	13.686	3928	3933	3943	rVB6	6549	10378	0.79%	0.106%




Sum of corrected areas: 9817118

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031394.D
Acq On : 07 Jun 2023 13:17
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK349

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

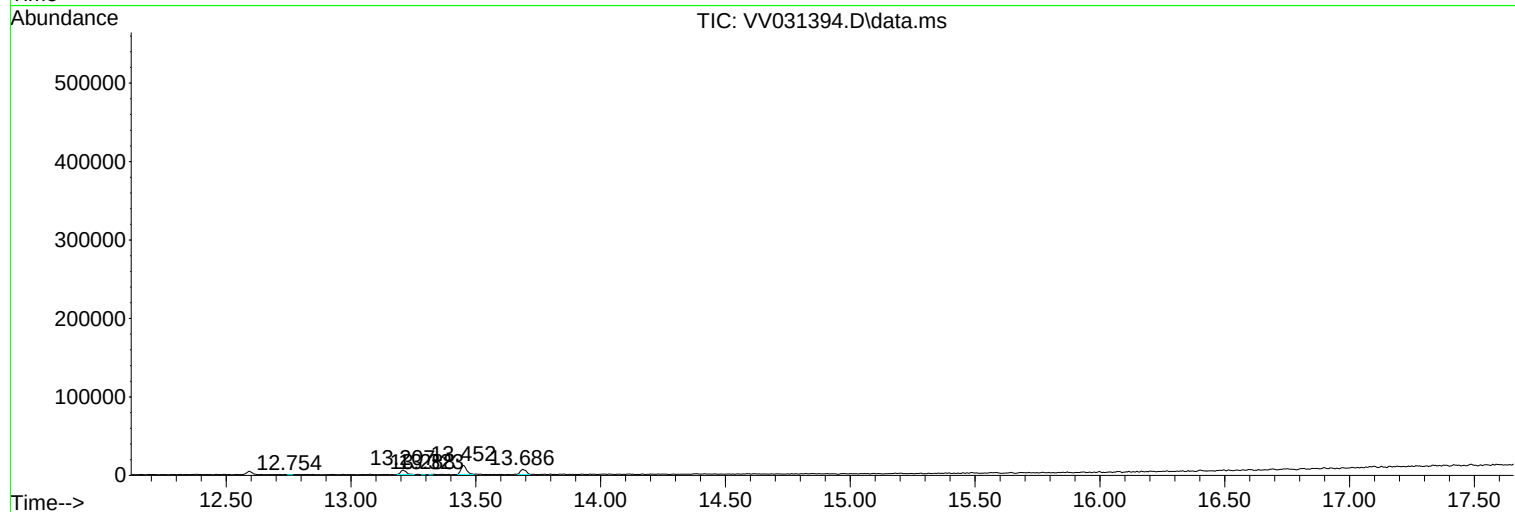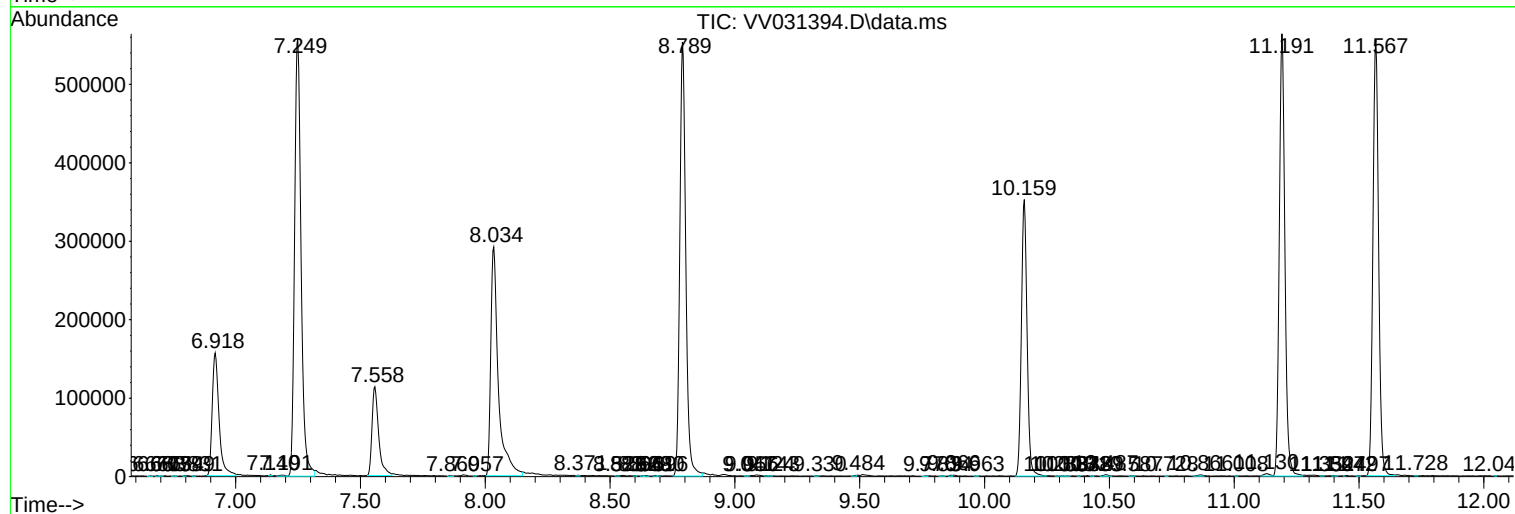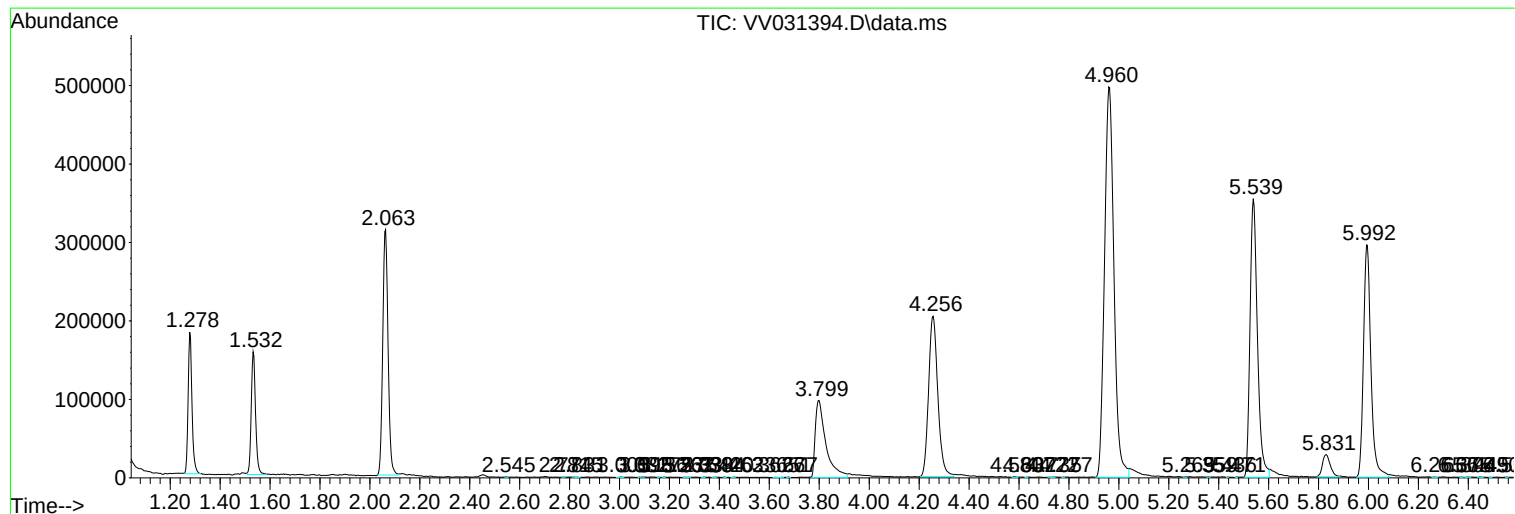

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031394.D
Acq On : 07 Jun 2023 13:17
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK349

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031394.D
Acq On : 07 Jun 2023 13:17
Operator : SY/MD
Sample : VV0607WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK349

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------