

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031395.D
 Acq On : 07 Jun 2023 13:41
 Operator : SY/MD
 Sample : 02951-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031395.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	175092	188179	14.44%	1.967%
2	1.532	146	153	171	rVB	153778	179727	13.79%	1.879%
3	2.063	308	318	334	rBV	298634	443300	34.01%	4.635%
4	2.391	418	420	422	rVB2	487	157	0.01%	0.002%
5	2.523	458	461	464	rVB3	609	362	0.03%	0.004%
6	2.545	465	468	470	rBV2	363	243	0.02%	0.003%
7	2.626	490	493	495	rBV2	532	256	0.02%	0.003%
8	2.674	506	508	510	rBV	491	276	0.02%	0.003%
9	2.735	524	527	532	rBV3	500	360	0.03%	0.004%
10	2.796	543	546	549	rBV2	502	300	0.02%	0.003%
11	2.886	572	574	576	rBV2	290	131	0.01%	0.001%
12	2.925	581	586	588	rBV2	499	480	0.04%	0.005%
13	3.031	616	619	620	rBV	405	157	0.01%	0.002%
14	3.079	633	634	637	rVB2	355	156	0.01%	0.002%
15	3.108	637	643	644	rBV2	525	418	0.03%	0.004%
16	3.153	654	657	659	rBV	384	202	0.02%	0.002%
17	3.169	659	662	663	rBV	326	141	0.01%	0.001%
18	3.201	668	672	676	rVV3	526	391	0.03%	0.004%
19	3.272	692	694	698	rBV2	338	206	0.02%	0.002%
20	3.526	770	773	774	rBV	290	136	0.01%	0.001%
21	3.587	790	792	795	rBV2	291	198	0.02%	0.002%
22	3.606	795	798	799	rBV2	216	150	0.01%	0.002%
23	3.745	838	841	845	rVB2	398	270	0.02%	0.003%
24	3.799	845	858	895	rBV	96165	288045	22.10%	3.011%
25	4.256	985	1000	1030	rBV2	200883	512077	39.29%	5.354%
26	4.587	1098	1103	1106	rBV5	780	811	0.06%	0.008%
27	4.674	1126	1130	1132	rVB2	429	268	0.02%	0.003%
28	4.825	1172	1177	1180	rBV5	516	492	0.04%	0.005%
29	4.963	1200	1220	1261	rBV2	481736	1303336	100.00%	13.626%
30	5.236	1302	1305	1308	rBV2	825	646	0.05%	0.007%
31	5.298	1322	1324	1327	rBV2	431	210	0.02%	0.002%
32	5.539	1387	1399	1433	rBV	339581	716875	55.00%	7.495%
33	5.828	1480	1489	1506	rVB2	28302	56843	4.36%	0.594%
34	5.944	1521	1525	1526	rBV2	406	272	0.02%	0.003%
35	5.995	1526	1541	1572	rVV	288918	607846	46.64%	6.355%
36	6.317	1638	1641	1643	rBV3	513	337	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031395.D
 Acq On : 07 Jun 2023 13:41
 Operator : SY/MD
 Sample : 02951-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.371	1656	1658	1663	rBV4	586	431	0.03%	0.005%
38	6.394	1663	1665	1669	rBV3	354	241	0.02%	0.003%
39	6.445	1678	1681	1683	rBV	482	329	0.03%	0.003%
40	6.516	1701	1703	1706	rBV4	287	124	0.01%	0.001%

41	6.590	1723	1726	1727	rBV	482	240	0.02%	0.003%
42	6.622	1733	1736	1737	rBV2	286	200	0.02%	0.002%
43	6.642	1740	1742	1746	rVV2	600	380	0.03%	0.004%
44	6.661	1746	1748	1752	rVB3	368	176	0.01%	0.002%
45	6.728	1765	1769	1772	rBV3	545	308	0.02%	0.003%

46	6.744	1772	1774	1778	rVB3	525	271	0.02%	0.003%
47	6.777	1781	1784	1787	rBV	442	269	0.02%	0.003%
48	6.873	1809	1814	1816	rBV3	471	260	0.02%	0.003%
49	6.918	1816	1828	1850	rBV	151579	291978	22.40%	3.053%
50	7.201	1914	1916	1918	rVB	826	341	0.03%	0.004%

51	7.249	1919	1931	1956	rBV	536768	960082	73.66%	10.037%
52	7.558	2017	2027	2054	rBV	108732	208658	16.01%	2.181%
53	7.860	2119	2121	2123	rVB3	671	295	0.02%	0.003%
54	7.876	2123	2126	2127	rBV	493	270	0.02%	0.003%
55	7.915	2135	2138	2146	rVB5	1166	1076	0.08%	0.011%

56	7.944	2146	2147	2151	rVB	735	445	0.03%	0.005%
57	7.969	2151	2155	2156	rBV2	540	372	0.03%	0.004%
58	8.034	2164	2175	2211	rBV	280574	601762	46.17%	6.291%
59	8.596	2347	2350	2354	rBV2	510	338	0.03%	0.004%
60	8.722	2387	2389	2392	rVB3	633	313	0.02%	0.003%

61	8.789	2398	2410	2438	rBV	538152	900164	69.07%	9.411%
62	9.047	2488	2490	2491	rBV	355	139	0.01%	0.001%
63	9.056	2491	2493	2494	rBV	662	200	0.02%	0.002%
64	9.223	2543	2545	2548	rVB2	669	333	0.03%	0.003%
65	9.243	2548	2551	2556	rBV3	671	476	0.04%	0.005%

66	9.339	2579	2581	2585	rVV3	414	237	0.02%	0.002%
67	9.481	2619	2625	2626	rBV	845	687	0.05%	0.007%
68	9.577	2652	2655	2657	rBV4	505	273	0.02%	0.003%
69	9.722	2698	2700	2703	rBV2	268	194	0.01%	0.002%
70	9.786	2717	2720	2722	rBV2	417	289	0.02%	0.003%

71	9.876	2736	2748	2753	rBV4	1408	2259	0.17%	0.024%
72	9.931	2763	2765	2768	rVB2	425	185	0.01%	0.002%
73	10.159	2824	2836	2854	rBV	344672	550534	42.24%	5.756%
74	10.336	2887	2891	2895	rBV3	643	502	0.04%	0.005%
75	10.355	2895	2897	2899	rBV	382	166	0.01%	0.002%

76	10.429	2915	2920	2923	rBV	547	625	0.05%	0.007%
----	--------	------	------	------	-----	-----	-----	-------	--------

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031395.D
 Acq On : 07 Jun 2023 13:41
 Operator : SY/MD
 Sample : 02951-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.455	2926	2928	2932	rBV	388	297	0.02%	0.003%
78	10.616	2973	2978	2980	rBV2	807	654	0.05%	0.007%
79	10.693	3000	3002	3004	rBV3	216	125	0.01%	0.001%
80	10.715	3006	3009	3014	rBV2	503	608	0.05%	0.006%
81	10.831	3042	3045	3047	rBV	290	164	0.01%	0.002%
82	10.863	3049	3055	3063	rVV5	1534	2159	0.17%	0.023%
83	10.895	3063	3065	3068	rVV2	483	303	0.02%	0.003%
84	10.924	3071	3074	3077	rVB4	590	373	0.03%	0.004%
85	11.030	3105	3107	3110	rBV2	464	256	0.02%	0.003%
86	11.063	3114	3117	3119	rBV2	248	212	0.02%	0.002%
87	11.127	3131	3137	3146	rBV7	2261	3399	0.26%	0.036%
88	11.191	3146	3157	3177	rBV	535948	846574	64.95%	8.851%
89	11.378	3214	3215	3218	rVB2	404	130	0.01%	0.001%
90	11.567	3262	3274	3297	rBV	532027	858102	65.84%	8.971%
91	12.214	3473	3475	3478	rBV	480	240	0.02%	0.003%
92	12.596	3585	3594	3603	rVB6	2985	4443	0.34%	0.046%
93	12.635	3603	3606	3610	rBV4	363	371	0.03%	0.004%
94	12.786	3651	3653	3654	rBV4	349	124	0.01%	0.001%
95	13.317	3816	3818	3821	rBV2	500	305	0.02%	0.003%
96	13.452	3854	3860	3869	rBV2	5940	8753	0.67%	0.092%
97	13.609	3907	3909	3913	rBV2	568	423	0.03%	0.004%
98	13.693	3928	3935	3944	rBV8	3921	5653	0.43%	0.059%
99	13.763	3955	3957	3959	rBV3	546	356	0.03%	0.004%
100	13.870	3988	3990	3992	rBV	596	269	0.02%	0.003%

Sum of corrected areas: 9564969




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031395.D
Acq On : 07 Jun 2023 13:41
Operator : SY/MD
Sample : 02951-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

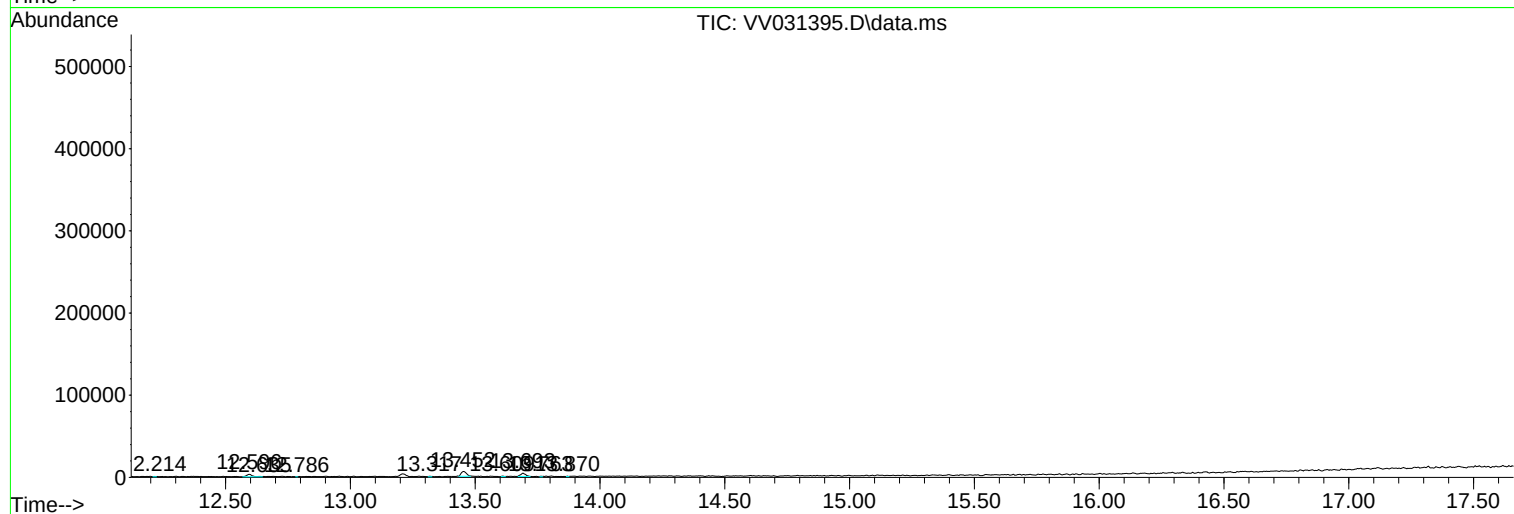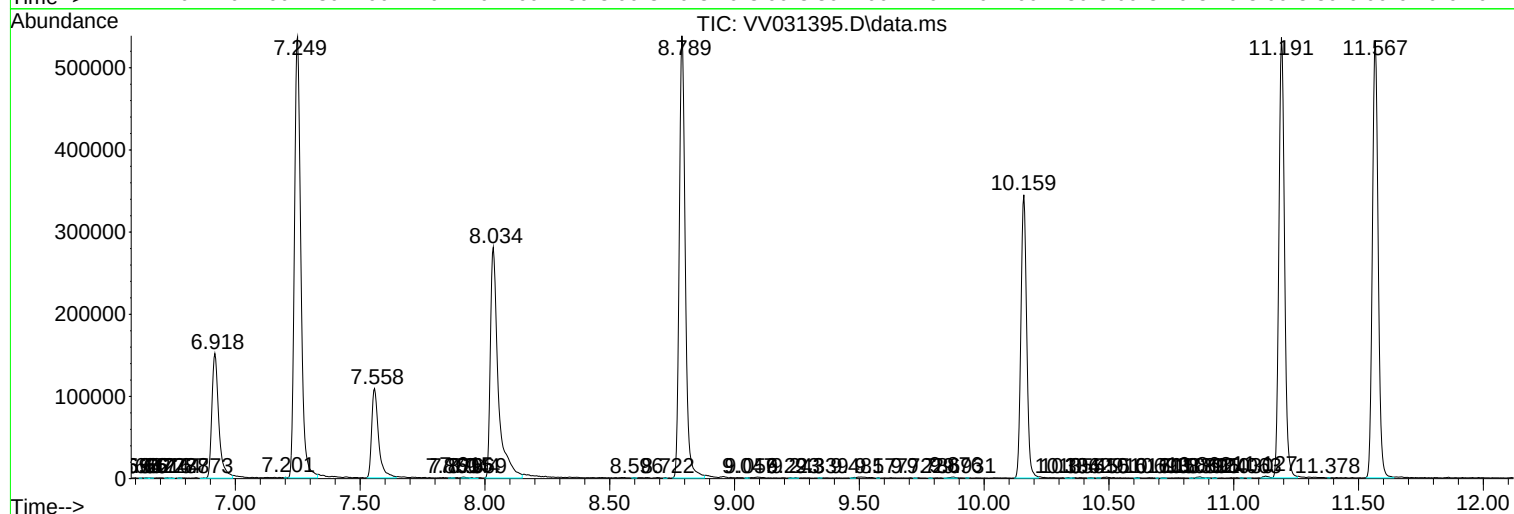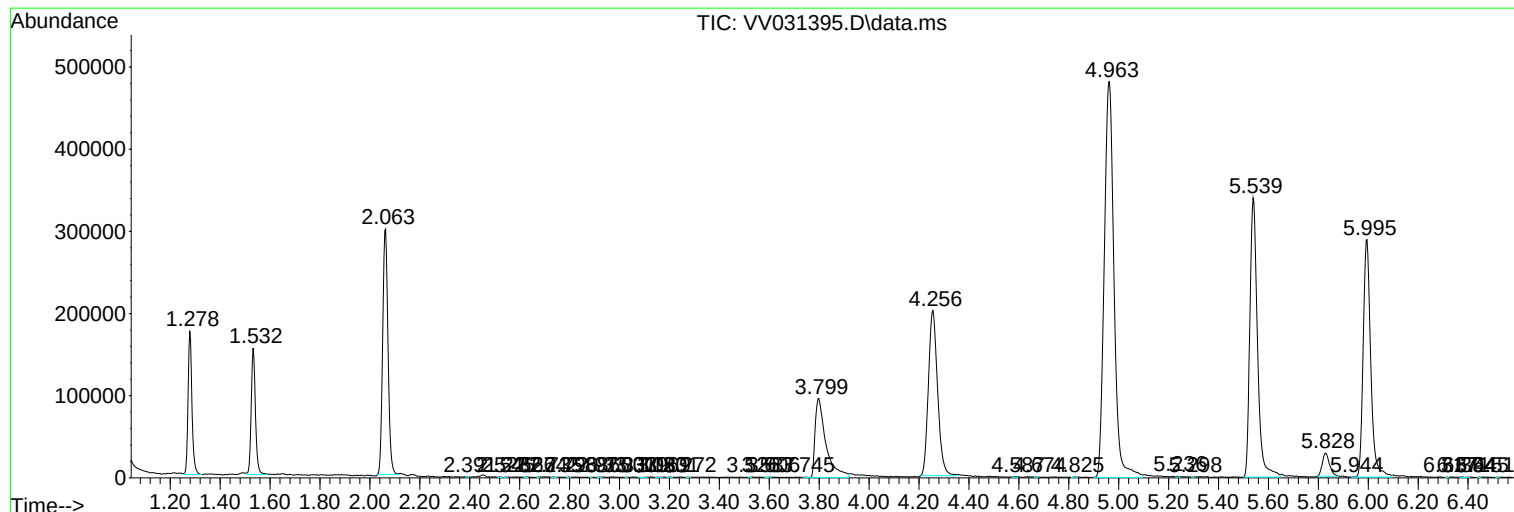

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031395.D
Acq On : 07 Jun 2023 13:41
Operator : SY/MD
Sample : 02951-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031395.D
Acq On : 07 Jun 2023 13:41
Operator : SY/MD
Sample : 02951-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------