

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031397.D
 Acq On : 07 Jun 2023 14:28
 Operator : SY/MD
 Sample : 03062-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZER2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031397.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	93	rVB	171294	184050	14.40%	1.936%
2	1.532	146	153	166	rVB	149047	173575	13.58%	1.826%
3	2.063	308	318	332	rBV	296561	440125	34.43%	4.629%
4	2.677	505	509	511	rBV2	625	497	0.04%	0.005%
5	2.703	514	517	521	rVV3	1275	873	0.07%	0.009%
6	2.754	529	533	536	rBV4	359	279	0.02%	0.003%
7	2.873	568	570	574	rVB3	593	309	0.02%	0.003%
8	2.918	582	584	586	rBV	408	232	0.02%	0.002%
9	2.941	589	591	599	rVB3	681	729	0.06%	0.008%
10	2.982	599	604	606	rBV4	577	573	0.04%	0.006%
11	3.076	631	633	638	rVB2	298	251	0.02%	0.003%
12	3.156	654	658	660	rBV2	245	216	0.02%	0.002%
13	3.178	663	665	668	rVV2	399	259	0.02%	0.003%
14	3.204	671	673	677	rVV3	506	295	0.02%	0.003%
15	3.252	685	688	691	rVB3	383	264	0.02%	0.003%
16	3.272	691	694	698	rVB	483	331	0.03%	0.003%
17	3.471	754	756	762	rVB3	348	271	0.02%	0.003%
18	3.548	774	780	782	rVB2	312	280	0.02%	0.003%
19	3.568	782	786	789	rBV	257	233	0.02%	0.002%
20	3.719	828	833	835	rVB3	384	322	0.03%	0.003%
21	3.799	847	858	900	rBV	92892	280452	21.94%	2.950%
22	4.256	985	1000	1027	rBV	196139	508763	39.80%	5.351%
23	4.603	1106	1108	1114	rBV3	406	404	0.03%	0.004%
24	4.757	1153	1156	1157	rVV	380	237	0.02%	0.002%
25	4.783	1161	1164	1167	rBV2	475	303	0.02%	0.003%
26	4.963	1203	1220	1255	rBV2	476682	1278188	100.00%	13.444%
27	5.278	1315	1318	1322	rBV2	747	448	0.04%	0.005%
28	5.384	1349	1351	1353	rBV3	449	218	0.02%	0.002%
29	5.474	1376	1379	1385	rBV3	387	466	0.04%	0.005%
30	5.539	1385	1399	1425	rBV	356735	742235	58.07%	7.807%
31	5.828	1477	1489	1508	rBV3	51455	110053	8.61%	1.158%
32	5.995	1528	1541	1578	rBV	284628	603460	47.21%	6.347%
33	6.275	1622	1628	1630	rBV3	563	495	0.04%	0.005%
34	6.387	1658	1663	1665	rBV3	386	417	0.03%	0.004%
35	6.429	1674	1676	1681	rVB3	285	231	0.02%	0.002%
36	6.452	1681	1683	1686	rBV2	513	239	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031397.D
 Acq On : 07 Jun 2023 14:28
 Operator : SY/MD
 Sample : 03062-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZER2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.571	1718	1720	1724	rBV2	353	277	0.02%	0.003%
38	6.731	1767	1770	1774	rBV2	447	234	0.02%	0.002%
39	6.792	1785	1789	1791	rBV2	418	308	0.02%	0.003%
40	6.876	1809	1815	1817	rBV3	393	353	0.03%	0.004%
41	6.918	1817	1828	1850	rBV	147452	281945	22.06%	2.966%
42	7.146	1896	1899	1902	rBV3	683	394	0.03%	0.004%
43	7.182	1908	1910	1912	rBV2	631	356	0.03%	0.004%
44	7.249	1918	1931	1953	rBV	529276	936292	73.25%	9.848%
45	7.558	2017	2027	2054	rBV	109339	200357	15.68%	2.107%
46	7.780	2093	2096	2098	rBV3	642	426	0.03%	0.004%
47	8.034	2165	2175	2217	rBV2	271045	597770	46.77%	6.288%
48	8.635	2359	2362	2363	rBV	359	221	0.02%	0.002%
49	8.709	2381	2385	2386	rBV	479	284	0.02%	0.003%
50	8.789	2398	2410	2438	rBV	551140	926081	72.45%	9.741%
51	8.953	2456	2461	2471	rBV7	1405	1948	0.15%	0.020%
52	9.056	2489	2493	2494	rBV3	452	352	0.03%	0.004%
53	9.072	2496	2498	2500	rBV2	1136	657	0.05%	0.007%
54	9.146	2519	2521	2526	rBV2	708	431	0.03%	0.005%
55	9.194	2534	2536	2541	rBV3	540	339	0.03%	0.004%
56	9.262	2553	2557	2559	rBV2	444	313	0.02%	0.003%
57	9.297	2563	2568	2570	rBV4	460	411	0.03%	0.004%
58	9.378	2588	2593	2598	rBV4	356	383	0.03%	0.004%
59	9.407	2600	2602	2604	rBV	634	277	0.02%	0.003%
60	9.474	2621	2623	2624	rBV2	461	233	0.02%	0.002%
61	9.493	2624	2629	2634	rVV4	1293	1731	0.14%	0.018%
62	9.522	2636	2638	2640	rVB2	1225	521	0.04%	0.005%
63	9.542	2640	2644	2648	rBV2	467	403	0.03%	0.004%
64	9.860	2739	2743	2744	rBV	512	293	0.02%	0.003%
65	9.873	2744	2747	2748	rBV2	836	463	0.04%	0.005%
66	9.905	2755	2757	2761	rBV3	458	358	0.03%	0.004%
67	10.062	2802	2806	2808	rBV	308	240	0.02%	0.003%
68	10.159	2825	2836	2856	rBV	294885	470240	36.79%	4.946%
69	10.265	2867	2869	2874	rVB3	561	439	0.03%	0.005%
70	10.294	2874	2878	2880	rBV2	632	473	0.04%	0.005%
71	10.352	2894	2896	2899	rVB2	734	302	0.02%	0.003%
72	10.381	2901	2905	2908	rVV3	714	517	0.04%	0.005%
73	10.480	2932	2936	2938	rBV3	827	646	0.05%	0.007%
74	10.934	3072	3077	3079	rBV2	407	322	0.03%	0.003%
75	11.008	3097	3100	3101	rBV2	504	248	0.02%	0.003%
76	11.082	3120	3123	3125	rBV2	567	290	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031397.D
 Acq On : 07 Jun 2023 14:28
 Operator : SY/MD
 Sample : 03062-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EZER2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	11.191	3146	3157	3176	rBV	555722	873881	68.37%	9.192%
78	11.471	3242	3244	3247	rBV2	428	239	0.02%	0.003%
79	11.513	3255	3257	3261	rBV2	355	253	0.02%	0.003%
80	11.567	3261	3274	3295	rBV	544720	858229	67.14%	9.027%
81	11.815	3349	3351	3354	rVB2	866	418	0.03%	0.004%
82	11.908	3376	3380	3385	rBV2	490	459	0.04%	0.005%
83	11.943	3388	3391	3398	rBV3	629	633	0.05%	0.007%
84	12.005	3406	3410	3415	rBV3	692	612	0.05%	0.006%
85	12.033	3418	3419	3422	rVV2	524	265	0.02%	0.003%
86	12.062	3426	3428	3431	rVB	592	284	0.02%	0.003%
87	12.210	3469	3474	3477	rBV4	882	691	0.05%	0.007%
88	12.278	3493	3495	3498	rVB3	662	340	0.03%	0.004%
89	12.374	3522	3525	3526	rBV2	503	331	0.03%	0.003%
90	12.590	3587	3592	3594	rBV4	2257	1874	0.15%	0.020%
91	12.760	3641	3645	3646	rBV2	346	242	0.02%	0.003%
92	12.857	3672	3675	3681	rVB2	697	359	0.03%	0.004%
93	12.963	3702	3708	3713	rBV3	476	536	0.04%	0.006%
94	12.988	3713	3716	3718	rBV4	552	432	0.03%	0.005%
95	13.175	3771	3774	3778	rBV2	434	316	0.02%	0.003%
96	13.210	3779	3785	3795	rVB6	1911	3343	0.26%	0.035%
97	13.358	3829	3831	3836	rVB2	605	466	0.04%	0.005%
98	13.387	3836	3840	3841	rBV	869	507	0.04%	0.005%
99	13.458	3854	3862	3863	rBV4	2541	3029	0.24%	0.032%
100	13.850	3981	3984	3989	rBV4	985	706	0.06%	0.007%




Sum of corrected areas: 9507146

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031397.D
Acq On : 07 Jun 2023 14:28
Operator : SY/MD
Sample : 03062-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZER2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

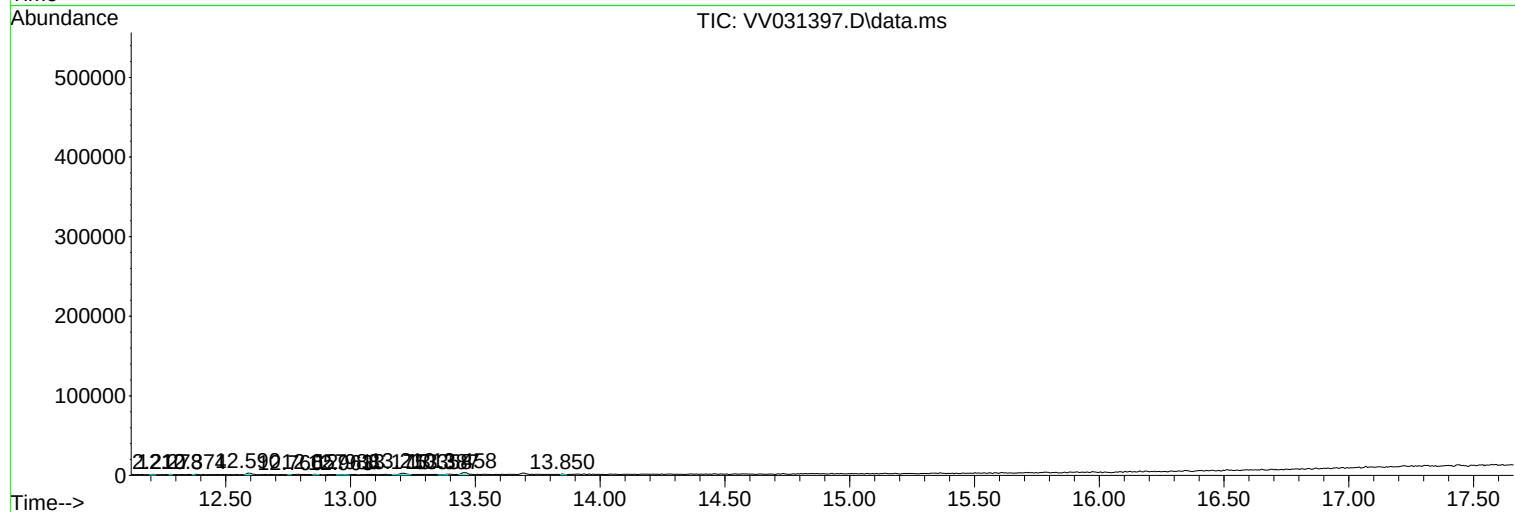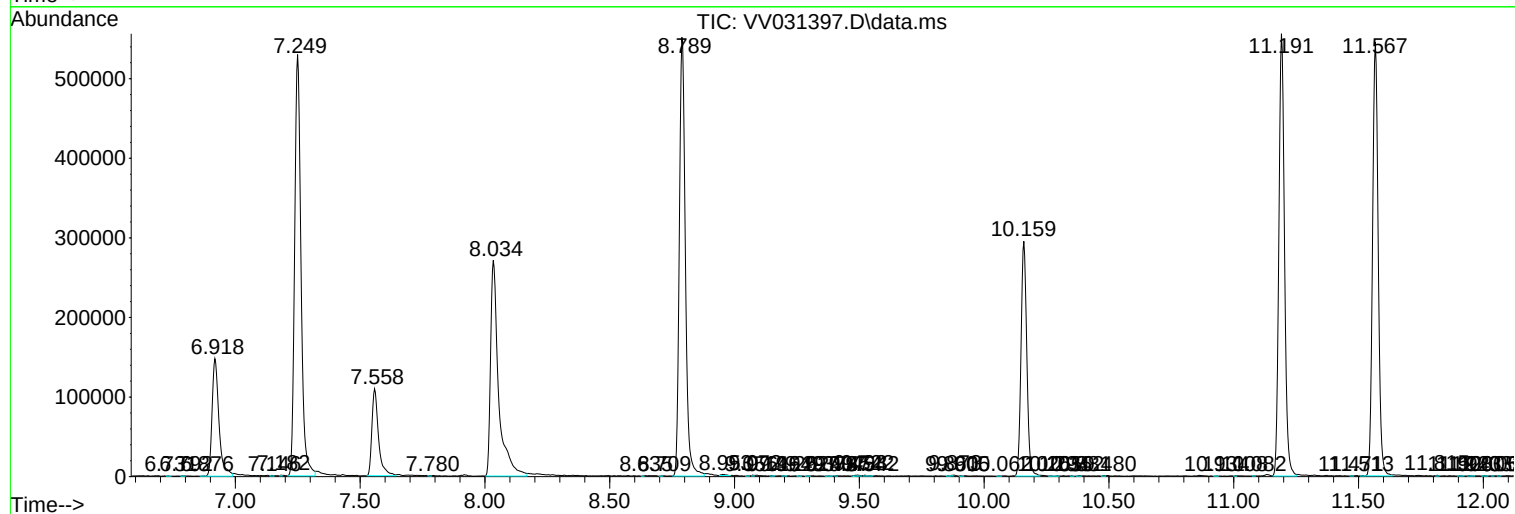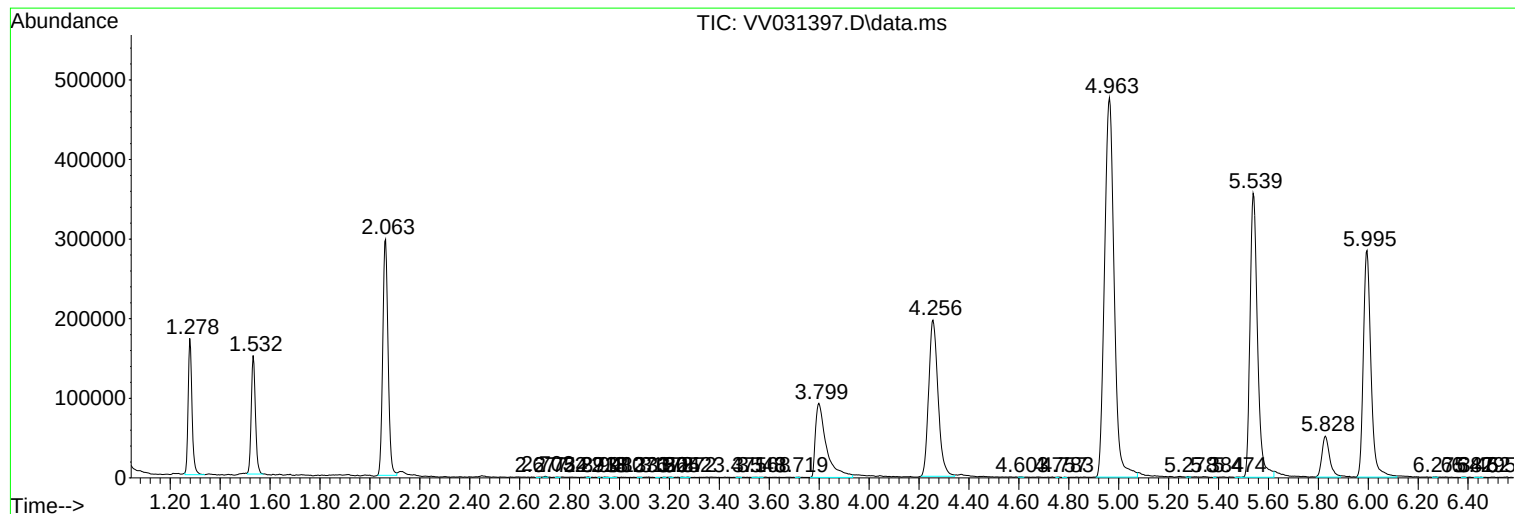

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031397.D
Acq On : 07 Jun 2023 14:28
Operator : SY/MD
Sample : 03062-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZER2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031397.D
Acq On : 07 Jun 2023 14:28
Operator : SY/MD
Sample : 03062-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EZER2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------