

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031398.D
 Acq On : 07 Jun 2023 14:52
 Operator : SY/MD
 Sample : 03062-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031398.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	144784	158557	13.78%	1.869%
2	1.532	146	153	173	rVB	129261	152864	13.29%	1.802%
3	2.063	307	318	331	rBV	256751	378718	32.91%	4.464%
4	2.384	416	418	419	rBV2	512	218	0.02%	0.003%
5	2.445	434	437	439	rBV2	1975	1540	0.13%	0.018%
6	2.770	536	538	540	rVB	673	237	0.02%	0.003%
7	2.815	550	552	553	rBV	382	158	0.01%	0.002%
8	2.880	570	572	575	rVB2	410	184	0.02%	0.002%
9	2.966	595	599	604	rBV4	456	426	0.04%	0.005%
10	3.179	661	665	669	rBV3	627	521	0.05%	0.006%
11	3.201	669	672	675	rVV	479	310	0.03%	0.004%
12	3.249	685	687	693	rBV	270	258	0.02%	0.003%
13	3.294	699	701	705	rBV	303	243	0.02%	0.003%
14	3.391	729	731	736	rVB3	574	385	0.03%	0.005%
15	3.420	736	740	741	rBV2	309	200	0.02%	0.002%
16	3.455	749	751	752	rBV	396	155	0.01%	0.002%
17	3.516	767	770	776	rBV2	428	417	0.04%	0.005%
18	3.574	784	788	789	rBV2	383	208	0.02%	0.002%
19	3.616	799	801	807	rBV3	350	284	0.02%	0.003%
20	3.680	819	821	825	rVB3	424	225	0.02%	0.003%
21	3.709	826	830	833	rBV2	519	325	0.03%	0.004%
22	3.722	833	834	839	rVB	340	173	0.02%	0.002%
23	3.799	848	858	898	rBV2	92440	291630	25.34%	3.438%
24	4.256	984	1000	1025	rBV	180086	467088	40.59%	5.506%
25	4.571	1096	1098	1101	rBV3	446	229	0.02%	0.003%
26	4.680	1128	1132	1134	rBV3	602	486	0.04%	0.006%
27	4.744	1148	1152	1154	rBV	578	417	0.04%	0.005%
28	4.963	1199	1220	1244	rBV2	431474	1150650	100.00%	13.564%
29	5.249	1305	1309	1312	rBV3	796	644	0.06%	0.008%
30	5.265	1312	1314	1317	rBV3	900	497	0.04%	0.006%
31	5.326	1328	1333	1334	rBV4	622	488	0.04%	0.006%
32	5.416	1360	1361	1363	rBV	573	206	0.02%	0.002%
33	5.477	1378	1380	1383	rVB2	519	219	0.02%	0.003%
34	5.497	1383	1386	1387	rBV2	325	228	0.02%	0.003%
35	5.539	1387	1399	1430	rBV	290014	614856	53.44%	7.248%
36	5.754	1464	1466	1470	rVB3	876	417	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031398.D
 Acq On : 07 Jun 2023 14:52
 Operator : SY/MD
 Sample : 03062-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.828	1478	1489	1507	rBV	28138	62117	5.40%	0.732%
38	5.995	1527	1541	1577	rBV	262726	556071	48.33%	6.555%
39	6.288	1630	1632	1634	rBV	370	203	0.02%	0.002%
40	6.387	1658	1663	1669	rVB3	551	485	0.04%	0.006%
41	6.445	1679	1681	1687	rVB3	578	436	0.04%	0.005%
42	6.474	1688	1690	1693	rBV	331	201	0.02%	0.002%
43	6.494	1693	1696	1701	rVB3	534	350	0.03%	0.004%
44	6.600	1727	1729	1732	rBV3	461	194	0.02%	0.002%
45	6.622	1732	1736	1739	rVB6	882	567	0.05%	0.007%
46	6.735	1768	1771	1774	rBV2	342	314	0.03%	0.004%
47	6.918	1816	1828	1861	rBV	132245	266479	23.16%	3.141%
48	7.153	1899	1901	1905	rVB4	803	368	0.03%	0.004%
49	7.249	1919	1931	1966	rBV	461217	824793	71.68%	9.723%
50	7.516	2013	2014	2016	rBV	530	199	0.02%	0.002%
51	7.558	2017	2027	2052	rVV	101351	189241	16.45%	2.231%
52	7.944	2144	2147	2149	rBV	332	172	0.01%	0.002%
53	7.956	2149	2151	2154	rBV	435	263	0.02%	0.003%
54	7.992	2160	2162	2164	rBV	409	196	0.02%	0.002%
55	8.034	2164	2175	2210	rBV2	265555	586679	50.99%	6.916%
56	8.696	2379	2381	2384	rVB	521	276	0.02%	0.003%
57	8.712	2384	2386	2387	rBV	535	234	0.02%	0.003%
58	8.789	2398	2410	2431	rBV	465733	779367	67.73%	9.187%
59	8.947	2457	2459	2461	rBV2	869	508	0.04%	0.006%
60	9.079	2498	2500	2502	rBV	564	240	0.02%	0.003%
61	9.133	2515	2517	2520	rVB	807	376	0.03%	0.004%
62	9.156	2520	2524	2526	rBV2	315	229	0.02%	0.003%
63	9.165	2526	2527	2530	rVB	452	173	0.02%	0.002%
64	9.243	2547	2551	2554	rVB2	658	527	0.05%	0.006%
65	9.268	2557	2559	2561	rBV2	455	196	0.02%	0.002%
66	9.358	2584	2587	2588	rBV2	333	206	0.02%	0.002%
67	9.413	2601	2604	2608	rVB2	559	351	0.03%	0.004%
68	9.432	2608	2610	2612	rBV2	505	255	0.02%	0.003%
69	9.538	2641	2643	2647	rBV2	483	331	0.03%	0.004%
70	9.580	2653	2656	2657	rBV	409	178	0.02%	0.002%
71	9.648	2674	2677	2681	rVB	354	196	0.02%	0.002%
72	9.680	2685	2687	2690	rVB	347	161	0.01%	0.002%
73	9.783	2717	2719	2722	rBV2	302	234	0.02%	0.003%
74	9.911	2757	2759	2762	rBV2	531	428	0.04%	0.005%
75	10.005	2786	2788	2792	rBV2	453	249	0.02%	0.003%
76	10.114	2818	2822	2823	rBV3	575	409	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031398.D
 Acq On : 07 Jun 2023 14:52
 Operator : SY/MD
 Sample : 03062-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.159	2824	2836	2856	rVV	331917	520175	45.21%	6.132%
78	10.323	2885	2887	2890	rBV2	774	510	0.04%	0.006%
79	10.374	2900	2903	2904	rVB2	384	183	0.02%	0.002%
80	10.461	2926	2930	2932	rBV2	488	303	0.03%	0.004%
81	10.567	2960	2963	2964	rBV2	543	235	0.02%	0.003%
82	10.661	2990	2992	2995	rVB	434	161	0.01%	0.002%
83	10.731	3012	3014	3018	rBV3	280	212	0.02%	0.002%
84	10.780	3027	3029	3033	rBV	374	289	0.03%	0.003%
85	10.976	3088	3090	3092	rBV2	368	157	0.01%	0.002%
86	11.034	3103	3108	3110	rBV4	383	348	0.03%	0.004%
87	11.072	3118	3120	3123	rVB3	414	198	0.02%	0.002%
88	11.130	3132	3138	3139	rBV	1463	1093	0.09%	0.013%
89	11.191	3146	3157	3186	rBV	451790	712473	61.92%	8.399%
90	11.567	3261	3274	3293	rBV	461960	743785	64.64%	8.768%
91	11.966	3396	3398	3400	rBV2	424	184	0.02%	0.002%
92	12.046	3421	3423	3424	rBV	452	201	0.02%	0.002%
93	12.432	3541	3543	3546	rBV	541	344	0.03%	0.004%
94	12.751	3640	3642	3646	rVB2	684	331	0.03%	0.004%
95	13.046	3732	3734	3741	rVB4	875	791	0.07%	0.009%
96	13.085	3742	3746	3749	rVV3	411	302	0.03%	0.004%
97	13.400	3841	3844	3845	rBV	656	342	0.03%	0.004%
98	13.876	3990	3992	3994	rBV2	500	263	0.02%	0.003%
99	13.892	3994	3997	3999	rBV4	524	353	0.03%	0.004%
100	14.162	4079	4081	4086	rBV4	700	675	0.06%	0.008%




Sum of corrected areas: 8483021

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031398.D
Acq On : 07 Jun 2023 14:52
Operator : SY/MD
Sample : 03062-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

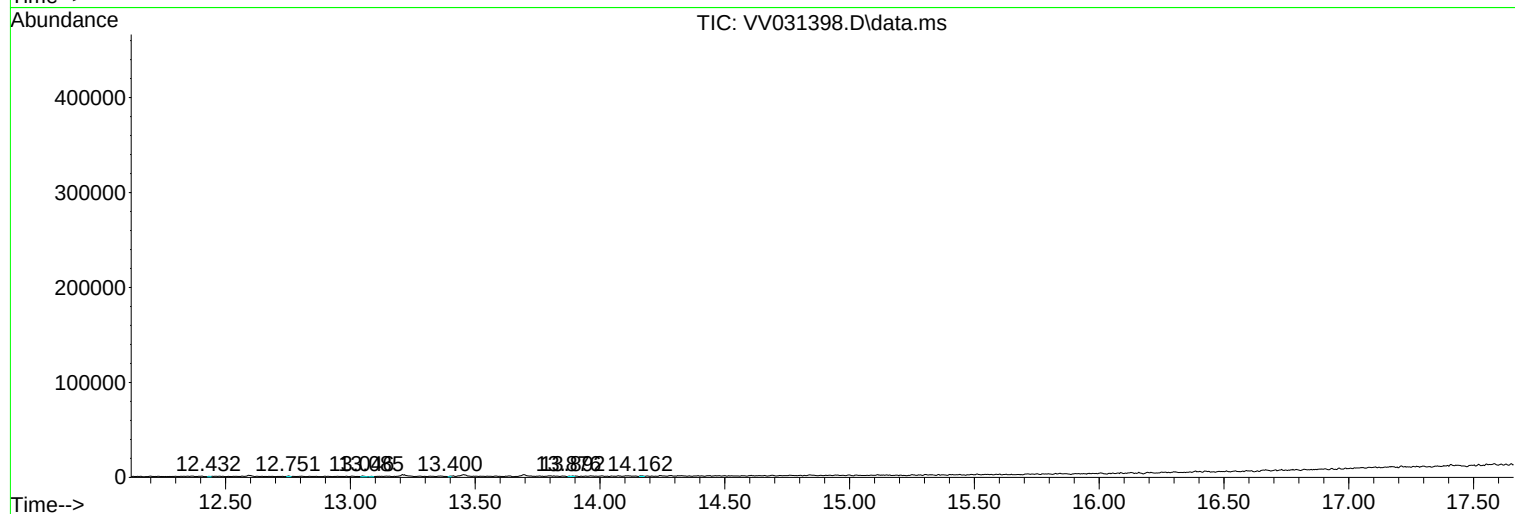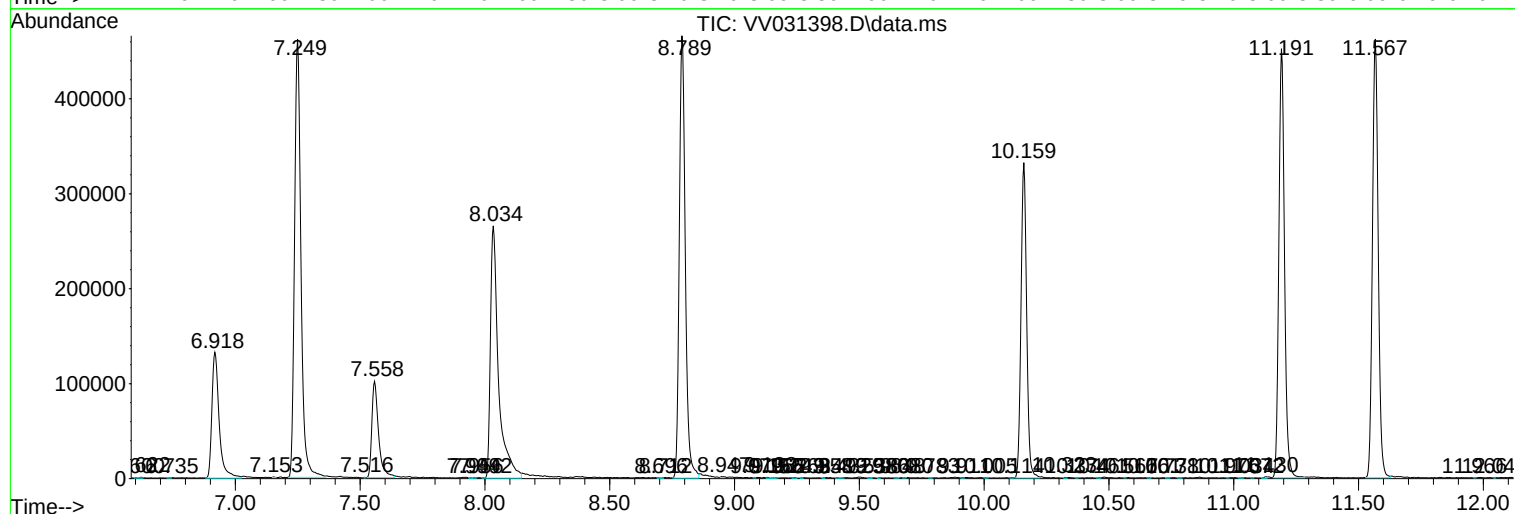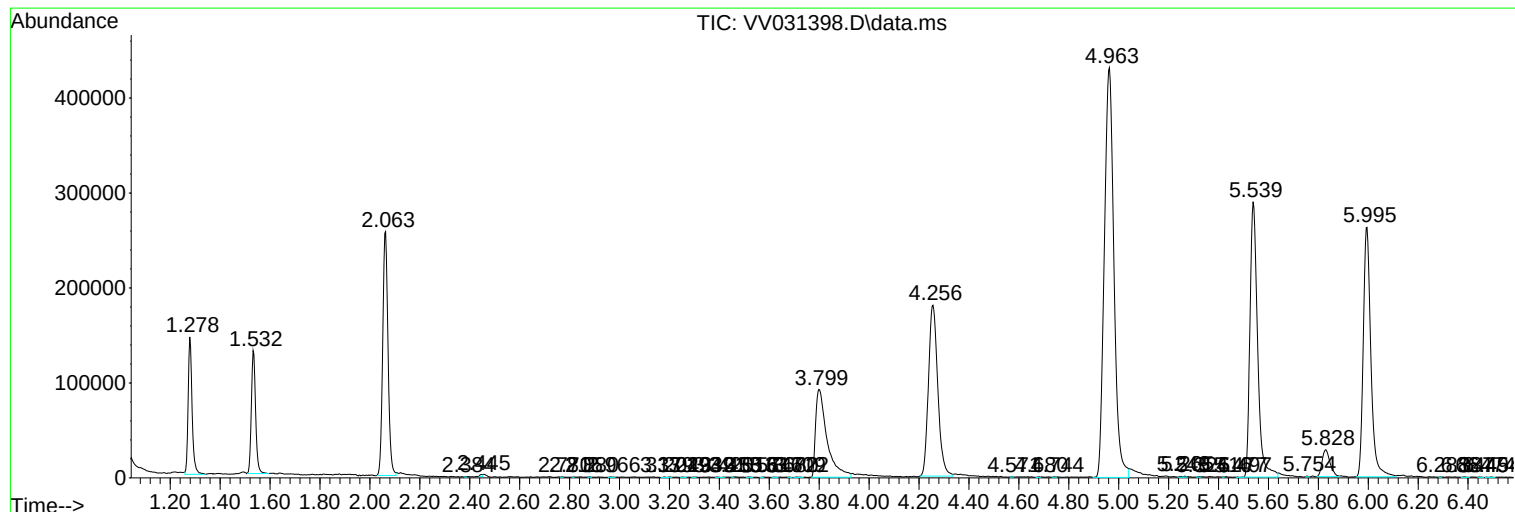

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031398.D
Acq On : 07 Jun 2023 14:52
Operator : SY/MD
Sample : 03062-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031398.D
Acq On : 07 Jun 2023 14:52
Operator : SY/MD
Sample : 03062-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------