

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031399.D
 Acq On : 07 Jun 2023 15:16
 Operator : SY/MD
 Sample : 03076-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031399.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	156935	166181	13.73%	1.830%
2	1.532	146	153	169	rVB	144076	167106	13.81%	1.840%
3	2.063	308	318	332	rBV	285581	421406	34.83%	4.641%
4	2.404	422	424	428	rVB2	440	245	0.02%	0.003%
5	2.426	428	431	434	rBV3	644	622	0.05%	0.007%
6	2.561	469	473	474	rBV2	494	324	0.03%	0.004%
7	2.577	474	478	481	rBV3	1067	991	0.08%	0.011%
8	2.767	532	537	540	rBV4	438	411	0.03%	0.005%
9	2.815	550	552	554	rVB	362	169	0.01%	0.002%
10	2.908	577	581	585	rVB3	587	395	0.03%	0.004%
11	2.931	585	588	593	rBV3	495	457	0.04%	0.005%
12	3.117	639	646	647	rBV4	665	686	0.06%	0.008%
13	3.230	677	681	684	rBV4	553	479	0.04%	0.005%
14	3.288	696	699	700	rBV	410	206	0.02%	0.002%
15	3.330	710	712	718	rVB2	515	411	0.03%	0.005%
16	3.371	723	725	726	rBV	434	191	0.02%	0.002%
17	3.423	739	741	743	rVV	470	225	0.02%	0.002%
18	3.642	804	809	812	rBV2	183	193	0.02%	0.002%
19	3.680	819	821	825	rVB2	495	231	0.02%	0.003%
20	3.699	825	827	828	rBV	380	185	0.02%	0.002%
21	3.796	847	857	892	rBV	88085	267332	22.09%	2.944%
22	4.256	983	1000	1027	rBV	192968	504431	41.69%	5.555%
23	4.648	1116	1122	1124	rBV2	376	427	0.04%	0.005%
24	4.680	1129	1132	1137	rVB4	486	406	0.03%	0.004%
25	4.838	1177	1181	1182	rBV2	247	178	0.01%	0.002%
26	4.889	1194	1197	1200	rBV3	534	337	0.03%	0.004%
27	4.963	1202	1220	1243	rBV3	454042	1209977	100.00%	13.325%
28	5.310	1325	1328	1331	rBV5	710	447	0.04%	0.005%
29	5.371	1345	1347	1348	rBV5	329	165	0.01%	0.002%
30	5.404	1353	1357	1360	rBV3	554	558	0.05%	0.006%
31	5.442	1367	1369	1371	rBV	464	214	0.02%	0.002%
32	5.539	1385	1399	1430	rBV	338973	710783	58.74%	7.827%
33	5.831	1478	1490	1504	rBV3	22759	50626	4.18%	0.558%
34	5.947	1524	1526	1527	rBV2	487	263	0.02%	0.003%
35	5.992	1527	1540	1569	rVV	270450	576197	47.62%	6.345%
36	6.291	1627	1633	1635	rBV5	755	737	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031399.D
 Acq On : 07 Jun 2023 15:16
 Operator : SY/MD
 Sample : 03076-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.371	1655	1658	1662	rVB2	648	406	0.03%	0.004%
38	6.432	1675	1677	1678	rBV	615	202	0.02%	0.002%
39	6.484	1691	1693	1697	rVB	568	263	0.02%	0.003%
40	6.584	1720	1724	1725	rBV3	640	379	0.03%	0.004%
41	6.715	1763	1765	1770	rVB2	516	356	0.03%	0.004%
42	6.789	1785	1788	1794	rBV2	489	489	0.04%	0.005%
43	6.821	1794	1798	1800	rBV3	319	189	0.02%	0.002%
44	6.841	1800	1804	1805	rBV2	430	185	0.02%	0.002%
45	6.873	1812	1814	1817	rBV2	340	238	0.02%	0.003%
46	6.918	1817	1828	1858	rBV	139928	274217	22.66%	3.020%
47	7.249	1919	1931	1968	rBV	501118	899280	74.32%	9.903%
48	7.558	2017	2027	2053	rBV	101575	191529	15.83%	2.109%
49	7.751	2082	2087	2090	rBV4	806	805	0.07%	0.009%
50	7.802	2101	2103	2106	rBV	695	382	0.03%	0.004%
51	7.834	2109	2113	2116	rBV4	754	536	0.04%	0.006%
52	7.953	2149	2150	2155	rVB	600	182	0.02%	0.002%
53	7.976	2155	2157	2160	rVB2	430	253	0.02%	0.003%
54	7.998	2160	2164	2165	rBV2	528	386	0.03%	0.004%
55	8.034	2165	2175	2213	rBV2	258044	557447	46.07%	6.139%
56	8.506	2320	2322	2323	rBV2	502	243	0.02%	0.003%
57	8.593	2346	2349	2351	rBV2	512	318	0.03%	0.004%
58	8.606	2351	2353	2356	rVB2	742	283	0.02%	0.003%
59	8.632	2356	2361	2363	rBV4	752	516	0.04%	0.006%
60	8.702	2379	2383	2388	rVB5	595	695	0.06%	0.008%
61	8.728	2388	2391	2394	rBV2	690	423	0.03%	0.005%
62	8.789	2398	2410	2438	rBV	524629	891836	73.71%	9.821%
63	9.117	2511	2512	2515	rBV2	335	214	0.02%	0.002%
64	9.136	2515	2518	2520	rVB3	515	265	0.02%	0.003%
65	9.149	2520	2522	2524	rBV2	314	186	0.02%	0.002%
66	9.172	2527	2529	2533	rBV2	666	480	0.04%	0.005%
67	9.217	2540	2543	2544	rBV	351	174	0.01%	0.002%
68	9.342	2578	2582	2583	rBV2	256	202	0.02%	0.002%
69	9.368	2588	2590	2593	rVV	680	449	0.04%	0.005%
70	9.394	2596	2598	2603	rVB3	476	278	0.02%	0.003%
71	9.503	2630	2632	2634	rVB2	722	222	0.02%	0.002%
72	9.564	2649	2651	2652	rBV	415	202	0.02%	0.002%
73	9.825	2729	2732	2734	rBV3	657	389	0.03%	0.004%
74	9.918	2759	2761	2762	rBV	364	167	0.01%	0.002%
75	9.963	2772	2775	2776	rBV2	419	206	0.02%	0.002%
76	9.989	2780	2783	2784	rBV2	297	182	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031399.D
 Acq On : 07 Jun 2023 15:16
 Operator : SY/MD
 Sample : 03076-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F79

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.088	2810	2814	2816	rBV2	444	287	0.02%	0.003%
78	10.159	2823	2836	2854	rBV	330974	526368	43.50%	5.797%
79	10.333	2879	2890	2900	rBV2	8843	14306	1.18%	0.158%
80	10.490	2935	2939	2947	rVB7	1239	1647	0.14%	0.018%
81	10.628	2980	2982	2987	rVB3	487	381	0.03%	0.004%
82	10.773	3025	3027	3029	rVB	613	244	0.02%	0.003%
83	10.786	3029	3031	3037	rVB2	229	176	0.01%	0.002%
84	10.844	3046	3049	3050	rBV2	508	221	0.02%	0.002%
85	10.863	3051	3055	3061	rVV4	1109	1251	0.10%	0.014%
86	10.889	3061	3063	3067	rVB	413	162	0.01%	0.002%
87	11.130	3132	3138	3143	rVB3	1536	2042	0.17%	0.022%
88	11.191	3145	3157	3182	rBV	520563	820504	67.81%	9.036%
89	11.567	3262	3274	3293	rBV	501107	795247	65.72%	8.757%
90	11.722	3320	3322	3324	rBV2	541	301	0.02%	0.003%
91	11.834	3355	3357	3360	rBV	404	242	0.02%	0.003%
92	11.963	3394	3397	3398	rBV2	465	221	0.02%	0.002%
93	12.069	3427	3430	3433	rBV2	368	303	0.03%	0.003%
94	12.085	3433	3435	3437	rVV	604	241	0.02%	0.003%
95	12.593	3586	3593	3600	rBV5	2140	2840	0.23%	0.031%
96	12.702	3623	3627	3628	rBV2	490	399	0.03%	0.004%
97	12.795	3653	3656	3657	rBV	424	216	0.02%	0.002%
98	12.924	3694	3696	3702	rBV3	478	396	0.03%	0.004%
99	13.210	3781	3785	3793	rBV7	2020	2171	0.18%	0.024%
100	13.445	3856	3858	3860	rBV2	1362	773	0.06%	0.009%

Sum of corrected areas: 9080785




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031399.D
Acq On : 07 Jun 2023 15:16
Operator : SY/MD
Sample : 03076-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

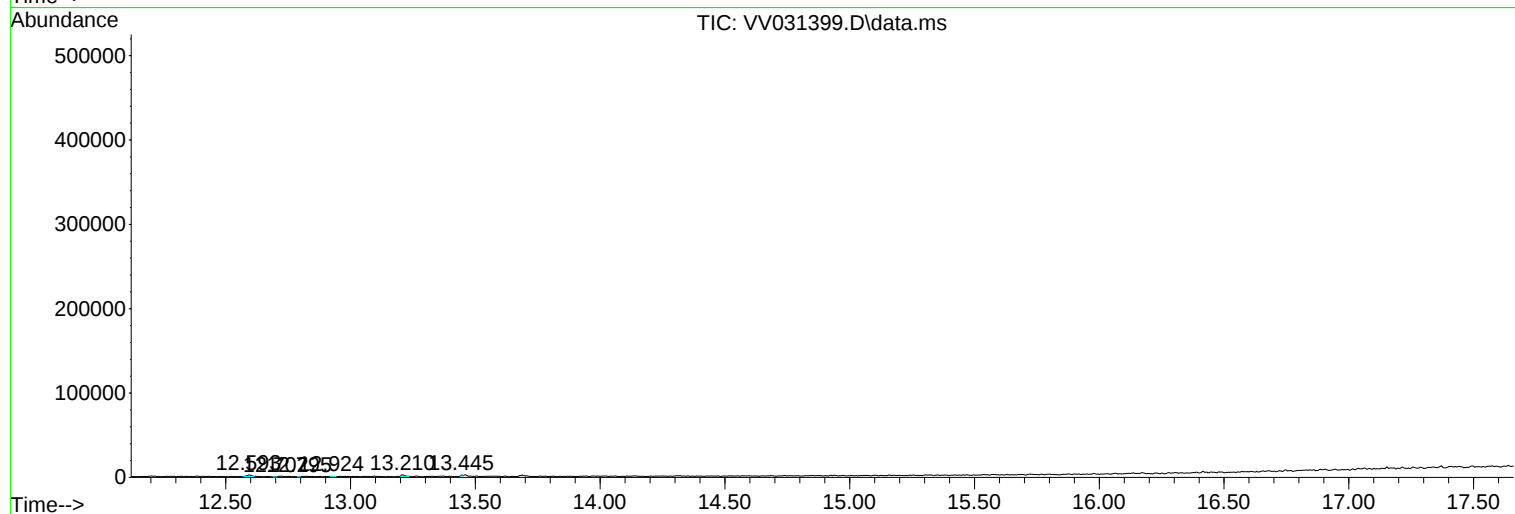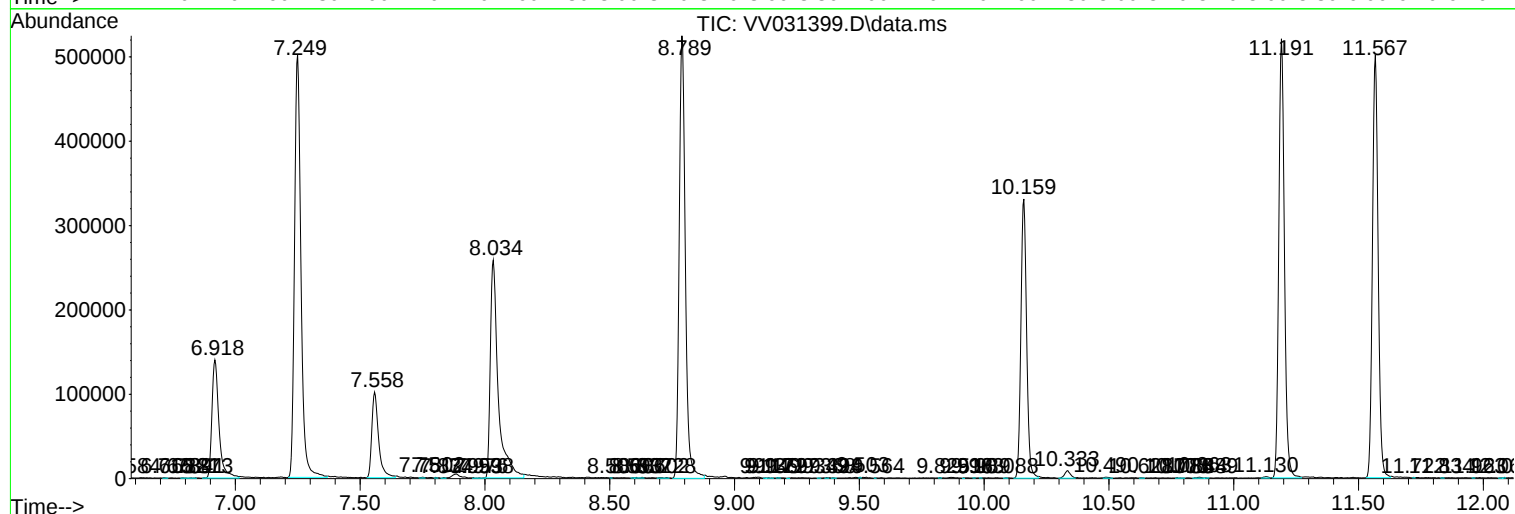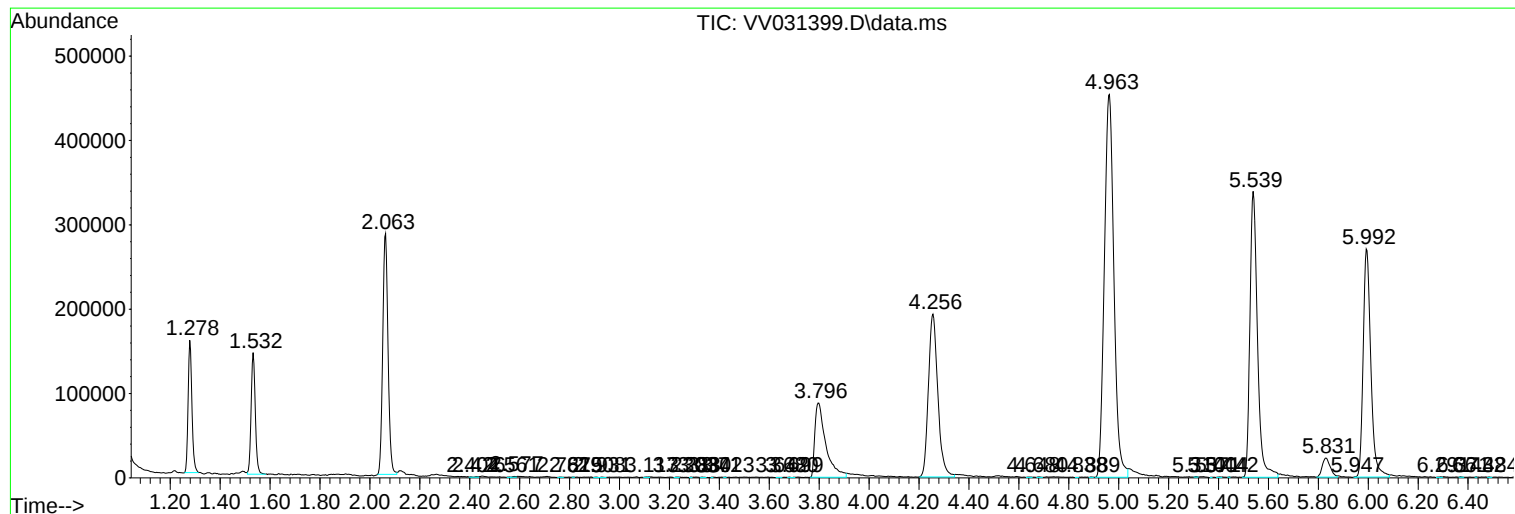

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031399.D
Acq On : 07 Jun 2023 15:16
Operator : SY/MD
Sample : 03076-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031399.D
Acq On : 07 Jun 2023 15:16
Operator : SY/MD
Sample : 03076-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F79

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------