

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031403.D
 Acq On : 07 Jun 2023 16:49
 Operator : SY/MD
 Sample : 03076-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031403.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	155483	167514	14.19%	1.920%
2	1.532	146	153	167	rVB	140244	162958	13.80%	1.868%
3	2.063	308	318	330	rBV	271064	405115	34.31%	4.643%
4	2.478	445	447	449	rBV	334	194	0.02%	0.002%
5	2.661	501	504	506	rBV2	332	176	0.01%	0.002%
6	2.709	518	519	521	rBV	488	259	0.02%	0.003%
7	2.738	527	528	531	rBV2	702	359	0.03%	0.004%
8	2.809	545	550	555	rBV5	725	611	0.05%	0.007%
9	2.970	598	600	602	rVB2	403	180	0.02%	0.002%
10	3.089	635	637	641	rVB	456	248	0.02%	0.003%
11	3.114	641	645	648	rBV2	584	549	0.05%	0.006%
12	3.163	657	660	663	rBV3	480	262	0.02%	0.003%
13	3.211	673	675	677	rBV	353	212	0.02%	0.002%
14	3.240	680	684	686	rBV2	358	290	0.02%	0.003%
15	3.355	717	720	721	rVV	443	208	0.02%	0.002%
16	3.375	725	726	730	rBV2	276	180	0.02%	0.002%
17	3.413	733	738	739	rBV2	339	240	0.02%	0.003%
18	3.487	758	761	764	rVB2	518	261	0.02%	0.003%
19	3.510	766	768	773	rVB3	680	412	0.03%	0.005%
20	3.532	773	775	779	rBV2	360	307	0.03%	0.004%
21	3.674	815	819	820	rBV	356	179	0.02%	0.002%
22	3.738	835	839	842	rBV	347	257	0.02%	0.003%
23	3.754	842	844	846	rBV	509	203	0.02%	0.002%
24	3.796	847	857	889	rBV	82936	250494	21.21%	2.871%
25	4.256	984	1000	1025	rBV	186743	489424	41.45%	5.609%
26	4.571	1095	1098	1100	rBV4	566	400	0.03%	0.005%
27	4.780	1160	1163	1165	rBV2	338	279	0.02%	0.003%
28	4.789	1165	1166	1171	rVB3	292	211	0.02%	0.002%
29	4.963	1201	1220	1246	rBV2	439933	1180788	100.00%	13.532%
30	5.429	1361	1365	1368	rBV3	984	667	0.06%	0.008%
31	5.478	1375	1380	1382	rBV3	592	508	0.04%	0.006%
32	5.539	1386	1399	1436	rBV	315919	674152	57.09%	7.726%
33	5.831	1478	1490	1509	rBV8	29475	68827	5.83%	0.789%
34	5.995	1523	1541	1567	rBV	266945	566207	47.95%	6.489%
35	6.294	1630	1634	1636	rBV3	891	627	0.05%	0.007%
36	6.378	1657	1660	1662	rBV2	595	234	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031403.D
 Acq On : 07 Jun 2023 16:49
 Operator : SY/MD
 Sample : 03076-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.442	1676	1680	1683	rBV2	609	443	0.04%	0.005%
38	6.478	1688	1691	1695	rBV2	706	557	0.05%	0.006%
39	6.513	1701	1702	1706	rVB2	473	290	0.02%	0.003%
40	6.535	1706	1709	1712	rBV3	456	242	0.02%	0.003%
41	6.568	1718	1719	1722	rVB2	387	185	0.02%	0.002%
42	6.645	1741	1743	1748	rVB2	650	494	0.04%	0.006%
43	6.670	1748	1751	1755	rBV3	384	387	0.03%	0.004%
44	6.715	1762	1765	1766	rBV	389	226	0.02%	0.003%
45	6.732	1768	1770	1772	rVB2	414	203	0.02%	0.002%
46	6.773	1780	1783	1785	rBV2	432	238	0.02%	0.003%
47	6.812	1792	1795	1799	rVB2	399	301	0.03%	0.003%
48	6.834	1799	1802	1803	rBV	382	231	0.02%	0.003%
49	6.918	1816	1828	1855	rBV	137399	265270	22.47%	3.040%
50	7.249	1918	1931	1953	rBV	490152	868030	73.51%	9.948%
51	7.445	1990	1992	1995	rVB3	905	439	0.04%	0.005%
52	7.558	2017	2027	2055	rBV	103528	187555	15.88%	2.149%
53	7.825	2108	2110	2114	rVB3	621	217	0.02%	0.002%
54	7.886	2119	2129	2136	rVV5	2031	3499	0.30%	0.040%
55	7.973	2151	2156	2158	rBV3	595	436	0.04%	0.005%
56	8.034	2163	2175	2211	rBV2	241416	524902	44.45%	6.015%
57	8.490	2314	2317	2319	rBV	623	336	0.03%	0.004%
58	8.619	2355	2357	2361	rVV2	395	262	0.02%	0.003%
59	8.651	2365	2367	2372	rVB3	563	404	0.03%	0.005%
60	8.789	2398	2410	2442	rBV	503079	842207	71.33%	9.652%
61	9.085	2499	2502	2504	rBV2	830	484	0.04%	0.006%
62	9.149	2519	2522	2525	rBV2	447	235	0.02%	0.003%
63	9.201	2534	2538	2540	rBV2	670	439	0.04%	0.005%
64	9.301	2566	2569	2572	rVB2	373	216	0.02%	0.002%
65	9.323	2572	2576	2577	rBV	411	243	0.02%	0.003%
66	9.413	2603	2604	2608	rBV3	372	228	0.02%	0.003%
67	9.583	2654	2657	2660	rVB3	559	339	0.03%	0.004%
68	9.664	2679	2682	2683	rBV	421	178	0.02%	0.002%
69	9.789	2718	2721	2722	rBV	439	199	0.02%	0.002%
70	9.821	2729	2731	2735	rBV3	382	360	0.03%	0.004%
71	9.866	2741	2745	2748	rBV6	707	512	0.04%	0.006%
72	9.911	2756	2759	2761	rBV2	300	231	0.02%	0.003%
73	10.018	2790	2792	2797	rVB3	641	468	0.04%	0.005%
74	10.040	2797	2799	2802	rBV2	517	313	0.03%	0.004%
75	10.075	2808	2810	2812	rBV2	291	177	0.01%	0.002%
76	10.159	2824	2836	2859	rBV	320300	511838	43.35%	5.866%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031403.D
 Acq On : 07 Jun 2023 16:49
 Operator : SY/MD
 Sample : 03076-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F85

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.336	2880	2891	2902	rVB2	5082	9582	0.81%	0.110%
78	10.381	2903	2905	2907	rBV2	375	233	0.02%	0.003%
79	10.532	2949	2952	2953	rBV2	391	241	0.02%	0.003%
80	10.680	2995	2998	3000	rBV	496	339	0.03%	0.004%
81	10.783	3028	3030	3033	rVV2	377	205	0.02%	0.002%
82	10.831	3043	3045	3048	rBV2	346	200	0.02%	0.002%
83	10.863	3052	3055	3057	rBV2	502	374	0.03%	0.004%
84	10.972	3085	3089	3095	rVB3	679	579	0.05%	0.007%
85	11.014	3100	3102	3105	rVB3	390	184	0.02%	0.002%
86	11.091	3123	3126	3128	rBV2	307	187	0.02%	0.002%
87	11.191	3145	3157	3176	rBV	482288	755852	64.01%	8.662%
88	11.442	3232	3235	3237	rBV3	429	225	0.02%	0.003%
89	11.567	3262	3274	3295	rBV	483056	765952	64.87%	8.778%
90	11.924	3382	3385	3386	rBV2	393	237	0.02%	0.003%
91	12.522	3570	3571	3574	rBV	417	190	0.02%	0.002%
92	12.664	3613	3615	3617	rBV	485	234	0.02%	0.003%
93	12.712	3626	3630	3634	rBV3	786	516	0.04%	0.006%
94	12.792	3652	3655	3657	rBV2	404	193	0.02%	0.002%
95	12.841	3668	3670	3672	rBV3	424	221	0.02%	0.003%
96	13.278	3803	3806	3808	rBV	481	343	0.03%	0.004%
97	13.670	3926	3928	3930	rBV3	772	469	0.04%	0.005%
98	13.943	4011	4013	4016	rBV2	466	289	0.02%	0.003%
99	14.149	4074	4077	4079	rBV2	1070	671	0.06%	0.008%
100	14.239	4103	4105	4109	rBV3	715	632	0.05%	0.007%




Sum of corrected areas: 8725954

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031403.D
Acq On : 07 Jun 2023 16:49
Operator : SY/MD
Sample : 03076-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

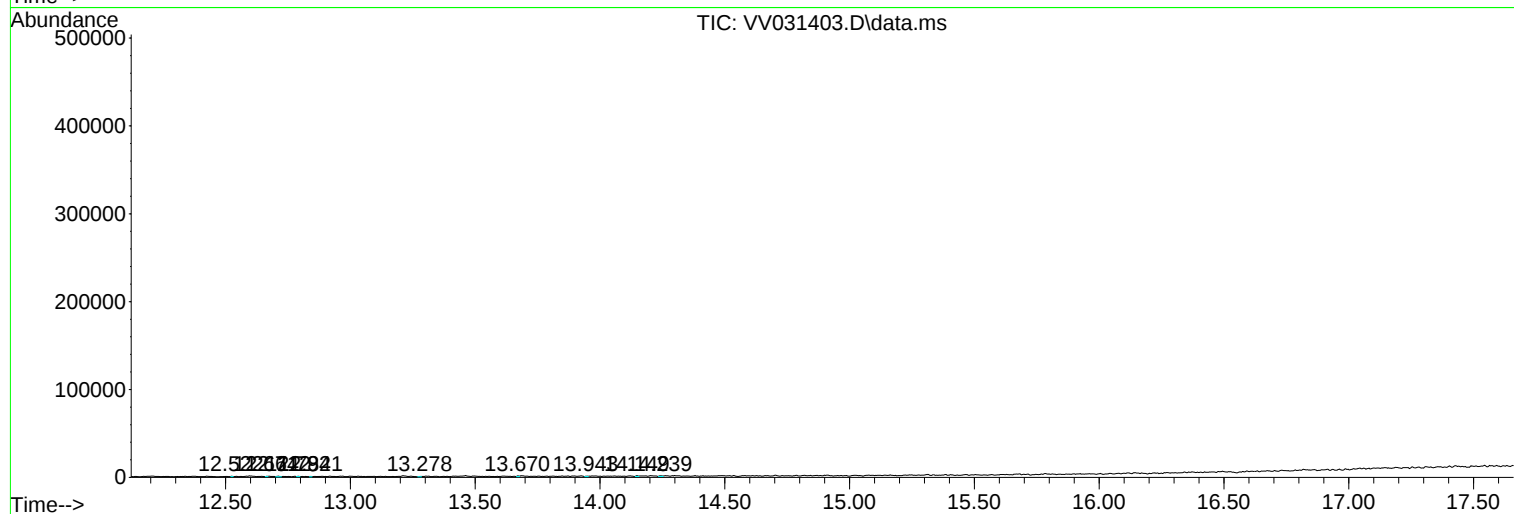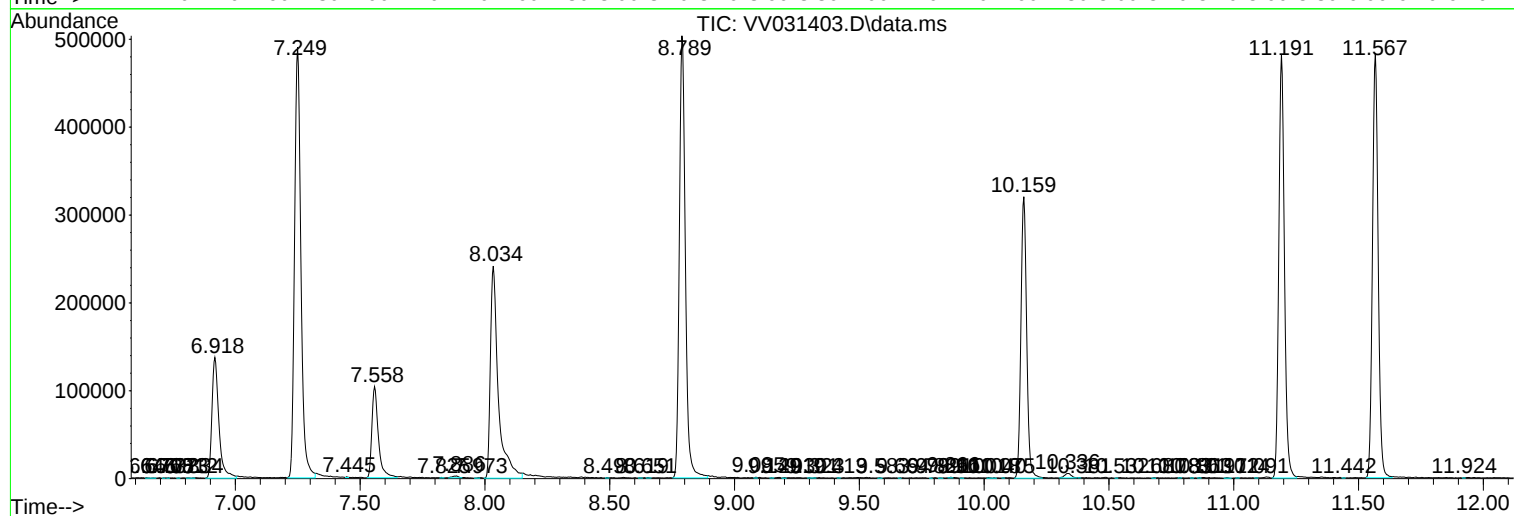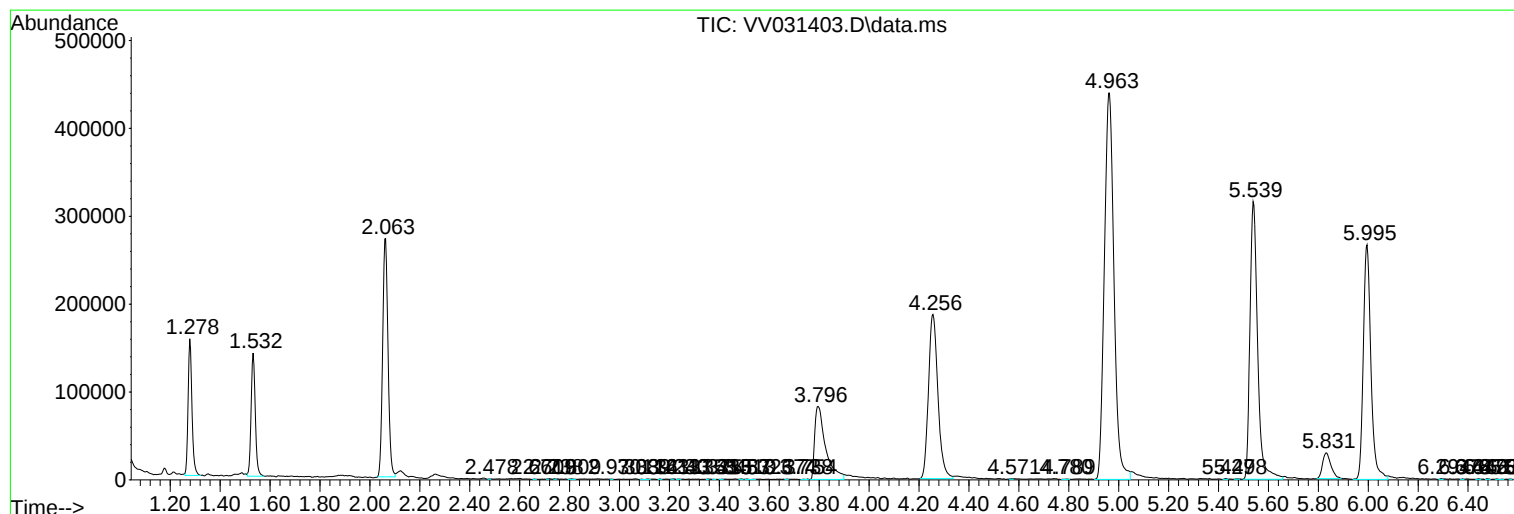

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031403.D
Acq On : 07 Jun 2023 16:49
Operator : SY/MD
Sample : 03076-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031403.D
Acq On : 07 Jun 2023 16:49
Operator : SY/MD
Sample : 03076-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F85

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc