

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031405.D
 Acq On : 07 Jun 2023 17:37
 Operator : SY/MD
 Sample : 02992-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031405.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	149070	160050	14.17%	2.054%
2	1.532	146	153	167	rVB	130725	152697	13.52%	1.960%
3	2.063	308	318	329	rBV	264027	385626	34.14%	4.950%
4	2.343	403	405	406	rBV2	520	168	0.01%	0.002%
5	2.445	434	437	443	rBV5	1053	1042	0.09%	0.013%
6	2.507	454	456	459	rVB2	475	272	0.02%	0.003%
7	2.535	462	465	466	rBV2	281	196	0.02%	0.003%
8	2.677	503	509	515	rBV3	1081	1344	0.12%	0.017%
9	2.957	592	596	597	rBV2	252	190	0.02%	0.002%
10	2.992	605	607	611	rVB2	600	318	0.03%	0.004%
11	3.069	630	631	636	rVB3	391	204	0.02%	0.003%
12	3.098	637	640	646	rVV2	345	319	0.03%	0.004%
13	3.130	648	650	654	rBV2	260	255	0.02%	0.003%
14	3.201	670	672	676	rVB2	460	237	0.02%	0.003%
15	3.281	694	697	702	rVB3	233	202	0.02%	0.003%
16	3.307	702	705	709	rVB3	473	293	0.03%	0.004%
17	3.330	709	712	715	rVB2	397	254	0.02%	0.003%
18	3.349	715	718	719	rBV2	348	212	0.02%	0.003%
19	3.368	721	724	728	rVB3	501	327	0.03%	0.004%
20	3.391	728	731	734	rBV2	340	269	0.02%	0.003%
21	3.439	744	746	752	rVB6	761	442	0.04%	0.006%
22	3.664	814	816	819	rVV2	365	204	0.02%	0.003%
23	3.696	822	826	829	rBV3	212	190	0.02%	0.002%
24	3.796	846	857	882	rBV2	76944	223424	19.78%	2.868%
25	4.256	982	1000	1024	rBV	176949	464904	41.16%	5.967%
26	4.757	1153	1156	1158	rBV	650	379	0.03%	0.005%
27	4.860	1182	1188	1192	rVB3	501	393	0.03%	0.005%
28	4.883	1192	1195	1196	rBV	264	167	0.01%	0.002%
29	4.963	1202	1220	1247	rBV2	426729	1129394	100.00%	14.496%
30	5.384	1346	1351	1353	rBV4	625	449	0.04%	0.006%
31	5.423	1360	1363	1366	rVB4	735	471	0.04%	0.006%
32	5.449	1366	1371	1373	rBV3	545	493	0.04%	0.006%
33	5.477	1376	1380	1382	rBV2	699	571	0.05%	0.007%
34	5.539	1387	1399	1422	rBV	236270	496949	44.00%	6.379%
35	5.828	1478	1489	1509	rBV2	35605	77866	6.89%	0.999%
36	5.995	1527	1541	1571	rBV	253976	538232	47.66%	6.909%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031405.D
 Acq On : 07 Jun 2023 17:37
 Operator : SY/MD
 Sample : 02992-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.442	1678	1680	1683	rVB2	588	296	0.03%	0.004%
38	6.468	1686	1688	1689	rBV	497	165	0.01%	0.002%
39	6.500	1696	1698	1700	rBV2	401	245	0.02%	0.003%
40	6.574	1717	1721	1723	rBV2	271	191	0.02%	0.002%
41	6.590	1723	1726	1729	rBV3	673	448	0.04%	0.006%
42	6.674	1750	1752	1754	rBV2	443	209	0.02%	0.003%
43	6.728	1767	1769	1773	rVB3	356	235	0.02%	0.003%
44	6.780	1779	1785	1789	rBV4	532	528	0.05%	0.007%
45	6.799	1789	1791	1797	rVB4	445	298	0.03%	0.004%
46	6.828	1798	1800	1802	rBV2	429	178	0.02%	0.002%
47	6.918	1817	1828	1849	rBV	128611	244175	21.62%	3.134%
48	7.249	1920	1931	1956	rBV	450098	813608	72.04%	10.443%
49	7.455	1993	1995	1996	rBV	710	292	0.03%	0.004%
50	7.558	2017	2027	2050	rBV	95181	174914	15.49%	2.245%
51	7.757	2085	2089	2090	rBV2	478	322	0.03%	0.004%
52	7.870	2118	2124	2125	rBV4	1062	950	0.08%	0.012%
53	7.956	2148	2151	2153	rBV3	511	361	0.03%	0.005%
54	8.034	2165	2175	2212	rBV2	221899	495737	43.89%	6.363%
55	8.329	2265	2267	2269	rBV3	617	335	0.03%	0.004%
56	8.538	2330	2332	2336	rBV3	506	350	0.03%	0.004%
57	8.661	2368	2370	2374	rBV4	483	282	0.02%	0.004%
58	8.789	2398	2410	2429	rBV	366760	626752	55.49%	8.045%
59	9.046	2487	2490	2495	rBV4	670	619	0.05%	0.008%
60	9.227	2544	2546	2548	rBV	445	223	0.02%	0.003%
61	9.275	2558	2561	2563	rBV3	674	323	0.03%	0.004%
62	9.288	2563	2565	2568	rVV3	571	375	0.03%	0.005%
63	9.403	2597	2601	2605	rVB5	824	583	0.05%	0.007%
64	9.477	2621	2624	2626	rBV2	671	346	0.03%	0.004%
65	9.593	2657	2660	2662	rBV	406	244	0.02%	0.003%
66	9.654	2674	2679	2683	rBV3	405	444	0.04%	0.006%
67	9.677	2683	2686	2690	rBV3	416	284	0.03%	0.004%
68	9.741	2703	2706	2707	rBV	408	259	0.02%	0.003%
69	9.767	2711	2714	2716	rVV2	549	251	0.02%	0.003%
70	9.854	2735	2741	2744	rBV4	578	567	0.05%	0.007%
71	9.915	2756	2760	2761	rBV	493	245	0.02%	0.003%
72	9.985	2780	2782	2788	rVB4	551	375	0.03%	0.005%
73	10.021	2791	2793	2796	rVB3	402	229	0.02%	0.003%
74	10.082	2808	2812	2814	rBV3	562	413	0.04%	0.005%
75	10.104	2816	2819	2823	rVB3	534	330	0.03%	0.004%
76	10.159	2823	2836	2852	rBV	274881	448155	39.68%	5.752%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031405.D
 Acq On : 07 Jun 2023 17:37
 Operator : SY/MD
 Sample : 02992-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.333	2881	2890	2900	rBV5	3801	6404	0.57%	0.082%
78	10.403	2910	2912	2916	rVB3	480	242	0.02%	0.003%
79	10.680	2996	2998	3001	rBV2	508	282	0.02%	0.004%
80	10.712	3003	3008	3012	rBV2	445	370	0.03%	0.005%
81	10.808	3034	3038	3040	rBV2	391	302	0.03%	0.004%
82	11.127	3132	3137	3141	rBV5	992	968	0.09%	0.012%
83	11.191	3145	3157	3177	rBV	369697	582032	51.53%	7.471%
84	11.378	3211	3215	3219	rBV2	396	332	0.03%	0.004%
85	11.477	3243	3246	3250	rBV3	745	557	0.05%	0.007%
86	11.567	3262	3274	3293	rBV	467852	739872	65.51%	9.497%
87	11.812	3347	3350	3352	rBV2	443	258	0.02%	0.003%
88	11.853	3361	3363	3365	rBV2	486	189	0.02%	0.002%
89	12.001	3408	3409	3413	rVB	598	193	0.02%	0.002%
90	12.197	3465	3470	3473	rBV2	661	790	0.07%	0.010%
91	12.326	3507	3510	3517	rVB3	843	852	0.08%	0.011%
92	12.355	3517	3519	3520	rBV	763	278	0.02%	0.004%
93	12.702	3625	3627	3630	rBV2	540	282	0.02%	0.004%
94	12.902	3687	3689	3690	rBV3	410	189	0.02%	0.002%
95	13.017	3723	3725	3727	rBV2	464	255	0.02%	0.003%
96	13.214	3781	3786	3787	rBV3	1087	966	0.09%	0.012%
97	13.287	3806	3809	3810	rBV2	516	283	0.03%	0.004%
98	13.323	3817	3820	3822	rBV2	385	222	0.02%	0.003%
99	13.786	3961	3964	3966	rBV3	595	413	0.04%	0.005%
100	14.056	4047	4048	4050	rVB	578	180	0.02%	0.002%




Sum of corrected areas: 7790850

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031405.D
Acq On : 07 Jun 2023 17:37
Operator : SY/MD
Sample : 02992-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

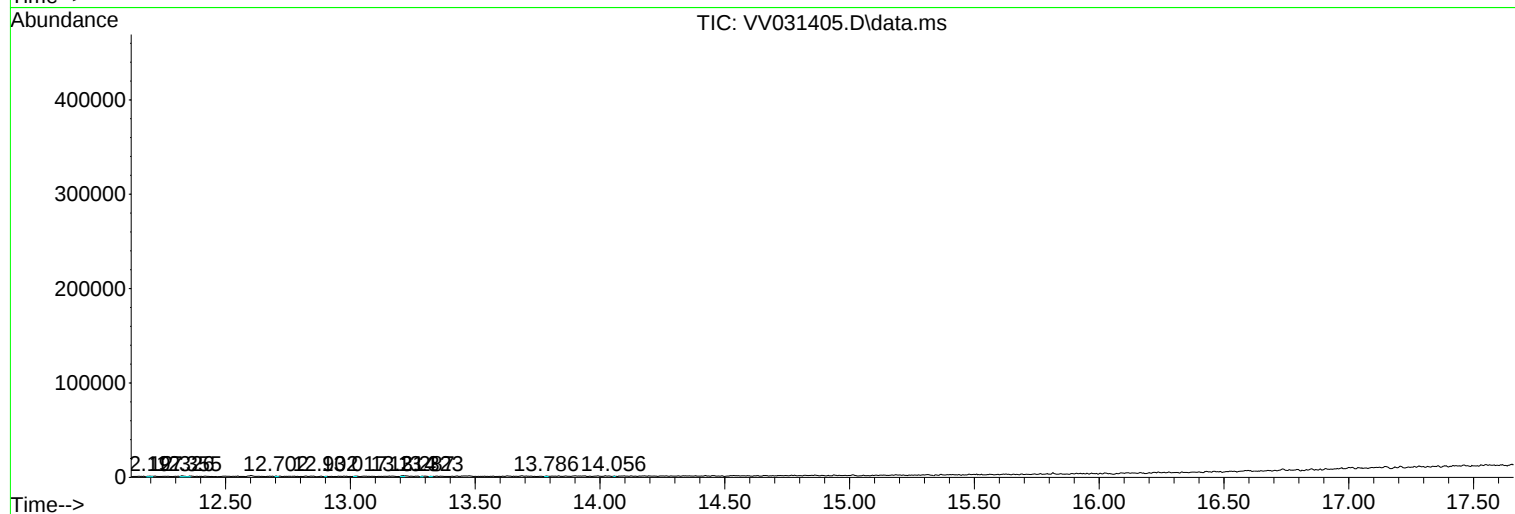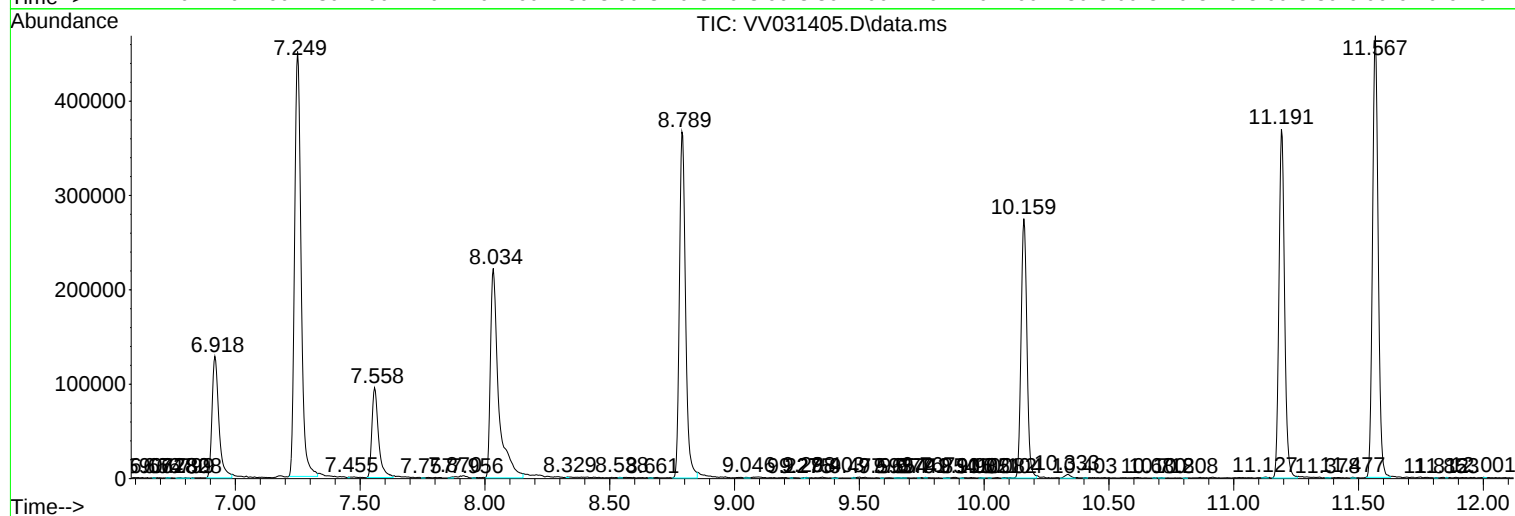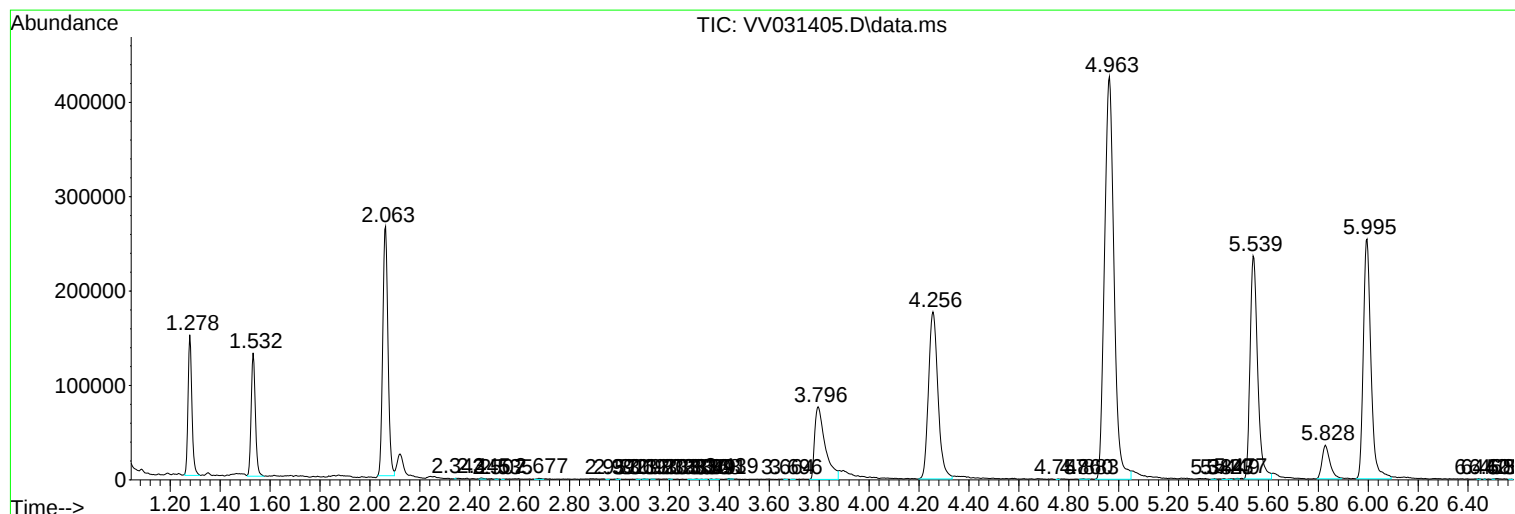

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031405.D
Acq On : 07 Jun 2023 17:37
Operator : SY/MD
Sample : 02992-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031405.D
Acq On : 07 Jun 2023 17:37
Operator : SY/MD
Sample : 02992-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------