

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031406.D
 Acq On : 07 Jun 2023 18:01
 Operator : SY/MD
 Sample : 02992-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031406.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	148128	158836	13.93%	1.886%
2	1.532	146	153	170	rVB	135530	160623	14.09%	1.907%
3	2.063	308	318	332	rBV	268045	394267	34.58%	4.681%
4	2.365	409	412	414	rBV2	451	359	0.03%	0.004%
5	2.410	424	426	428	rBV2	397	192	0.02%	0.002%
6	2.455	433	440	446	rVV3	1439	1792	0.16%	0.021%
7	2.539	464	466	469	rVB2	477	270	0.02%	0.003%
8	2.584	478	480	482	rBV2	627	337	0.03%	0.004%
9	2.761	533	535	539	rVB2	413	228	0.02%	0.003%
10	2.851	561	563	567	rVB3	487	256	0.02%	0.003%
11	2.876	569	571	574	rBV2	398	299	0.03%	0.004%
12	2.982	601	604	606	rBV2	534	332	0.03%	0.004%
13	3.118	641	646	647	rBV	286	219	0.02%	0.003%
14	3.156	656	658	662	rVB2	566	256	0.02%	0.003%
15	3.201	666	672	675	rVB3	514	544	0.05%	0.006%
16	3.236	679	683	686	rBV2	356	241	0.02%	0.003%
17	3.269	690	693	695	rVB2	509	320	0.03%	0.004%
18	3.285	695	698	700	rBV	535	332	0.03%	0.004%
19	3.394	730	732	737	rVB3	412	340	0.03%	0.004%
20	3.507	765	767	774	rVB3	479	408	0.04%	0.005%
21	3.535	774	776	779	rBV2	368	254	0.02%	0.003%
22	3.590	789	793	795	rBV3	344	259	0.02%	0.003%
23	3.738	836	839	841	rBV2	372	237	0.02%	0.003%
24	3.796	848	857	889	rBV	77235	225562	19.78%	2.678%
25	4.256	985	1000	1027	rBV	180833	464127	40.71%	5.511%
26	4.667	1125	1128	1131	rBV2	491	371	0.03%	0.004%
27	4.712	1139	1142	1144	rBV2	367	238	0.02%	0.003%
28	4.796	1165	1168	1169	rBV	512	276	0.02%	0.003%
29	4.860	1186	1188	1191	rVB3	409	194	0.02%	0.002%
30	4.879	1191	1194	1197	rVB2	342	213	0.02%	0.003%
31	4.963	1197	1220	1246	rBV3	424686	1140108	100.00%	13.537%
32	5.317	1328	1330	1333	rBV3	784	516	0.05%	0.006%
33	5.423	1358	1363	1366	rBV4	596	475	0.04%	0.006%
34	5.471	1376	1378	1384	rVB3	752	581	0.05%	0.007%
35	5.539	1384	1399	1421	rBV	307214	640509	56.18%	7.605%
36	5.828	1479	1489	1508	rVB2	47082	93989	8.24%	1.116%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031406.D
 Acq On : 07 Jun 2023 18:01
 Operator : SY/MD
 Sample : 02992-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.995	1527	1541	1576	rBV	255806	548102	48.07%	6.508%
38	6.452	1680	1683	1685	rBV2	539	394	0.03%	0.005%
39	6.490	1692	1695	1699	rBV3	320	281	0.02%	0.003%
40	6.513	1699	1702	1703	rBV3	583	358	0.03%	0.004%
41	6.574	1719	1721	1724	rVB2	573	342	0.03%	0.004%
42	6.609	1729	1732	1735	rBV2	395	289	0.03%	0.003%
43	6.754	1775	1777	1780	rBV2	350	234	0.02%	0.003%
44	6.828	1796	1800	1801	rBV	378	272	0.02%	0.003%
45	6.863	1807	1811	1814	rVB2	403	326	0.03%	0.004%
46	6.918	1814	1828	1860	rBV	126693	253843	22.26%	3.014%
47	7.133	1891	1895	1896	rBV3	689	453	0.04%	0.005%
48	7.249	1919	1931	1966	rBV	466182	845543	74.16%	10.039%
49	7.516	2012	2014	2017	rBV2	602	311	0.03%	0.004%
50	7.558	2017	2027	2053	rBV	95351	176980	15.52%	2.101%
51	7.821	2106	2109	2110	rBV2	806	345	0.03%	0.004%
52	7.873	2122	2125	2130	rBV2	859	1044	0.09%	0.012%
53	7.912	2134	2137	2140	rBV2	689	427	0.04%	0.005%
54	8.034	2165	2175	2217	rBV2	222152	509780	44.71%	6.053%
55	8.526	2325	2328	2330	rBV2	560	380	0.03%	0.005%
56	8.606	2349	2353	2354	rBV2	427	291	0.03%	0.003%
57	8.789	2397	2410	2433	rBV	483917	817417	71.70%	9.706%
58	9.011	2475	2479	2483	rVB3	795	744	0.07%	0.009%
59	9.156	2519	2524	2525	rBV2	411	366	0.03%	0.004%
60	9.233	2543	2548	2551	rBV3	462	348	0.03%	0.004%
61	9.291	2564	2566	2568	rBV	473	248	0.02%	0.003%
62	9.349	2582	2584	2587	rVB	493	245	0.02%	0.003%
63	9.378	2590	2593	2595	rBV2	489	291	0.03%	0.003%
64	9.622	2667	2669	2673	rBV2	373	343	0.03%	0.004%
65	9.670	2681	2684	2688	rBV2	601	463	0.04%	0.005%
66	9.712	2692	2697	2701	rBV4	461	402	0.04%	0.005%
67	9.754	2707	2710	2711	rBV2	440	273	0.02%	0.003%
68	9.879	2744	2749	2751	rBV2	603	604	0.05%	0.007%
69	9.969	2775	2777	2780	rBV2	355	256	0.02%	0.003%
70	10.072	2806	2809	2811	rBV2	379	209	0.02%	0.002%
71	10.159	2824	2836	2860	rBV	273614	431755	37.87%	5.126%
72	10.317	2883	2885	2887	rBV2	650	380	0.03%	0.005%
73	10.333	2887	2890	2901	rVB4	1993	2646	0.23%	0.031%
74	10.448	2924	2926	2930	rVB3	350	215	0.02%	0.003%
75	10.484	2930	2937	2941	rBV5	819	1061	0.09%	0.013%
76	10.583	2966	2968	2970	rBV	692	304	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031406.D
 Acq On : 07 Jun 2023 18:01
 Operator : SY/MD
 Sample : 02992-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C01

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.619	2974	2979	2982	rVB3	552	568	0.05%	0.007%
78	10.635	2982	2984	2988	rBV2	319	256	0.02%	0.003%
79	10.661	2988	2992	2994	rBV2	438	302	0.03%	0.004%
80	10.763	3020	3024	3025	rBV2	475	250	0.02%	0.003%
81	10.821	3039	3042	3044	rBV2	373	243	0.02%	0.003%
82	11.001	3095	3098	3102	rVB2	545	315	0.03%	0.004%
83	11.088	3123	3125	3128	rVB3	774	369	0.03%	0.004%
84	11.108	3128	3131	3133	rBV	534	264	0.02%	0.003%
85	11.120	3133	3135	3136	rBV	543	239	0.02%	0.003%
86	11.191	3143	3157	3179	rBV	487400	762983	66.92%	9.059%
87	11.326	3197	3199	3203	rVB3	666	345	0.03%	0.004%
88	11.567	3262	3274	3293	rBV	484984	765009	67.10%	9.083%
89	11.940	3387	3390	3393	rBV2	425	262	0.02%	0.003%
90	12.011	3410	3412	3417	rVB3	562	312	0.03%	0.004%
91	12.198	3467	3470	3473	rBV2	574	442	0.04%	0.005%
92	12.378	3522	3526	3528	rBV2	427	335	0.03%	0.004%
93	12.519	3567	3570	3573	rBV3	561	501	0.04%	0.006%
94	12.648	3607	3610	3614	rBV2	545	492	0.04%	0.006%
95	12.918	3691	3694	3696	rBV2	402	239	0.02%	0.003%
96	12.931	3696	3698	3700	rVV	674	265	0.02%	0.003%
97	13.204	3780	3783	3784	rBV2	653	381	0.03%	0.005%
98	13.413	3844	3848	3851	rBV3	518	480	0.04%	0.006%
99	13.516	3879	3880	3882	rBV	528	219	0.02%	0.003%
100	13.590	3901	3903	3904	rBV	589	207	0.02%	0.002%




Sum of corrected areas: 8422203

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031406.D
Acq On : 07 Jun 2023 18:01
Operator : SY/MD
Sample : 02992-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

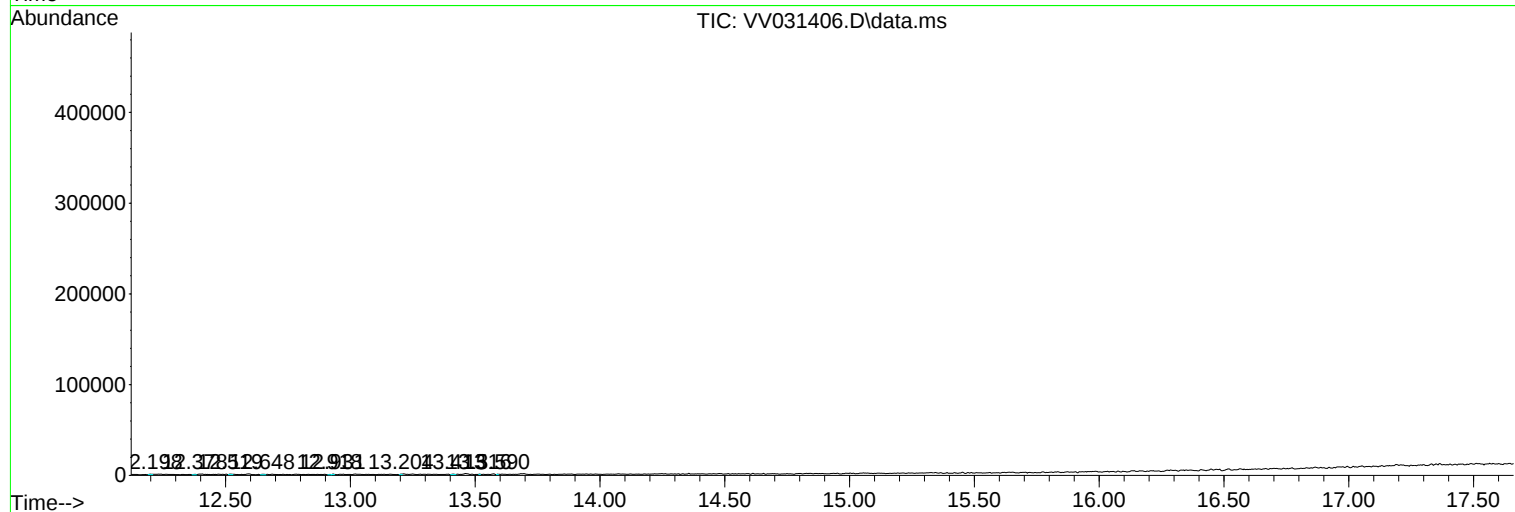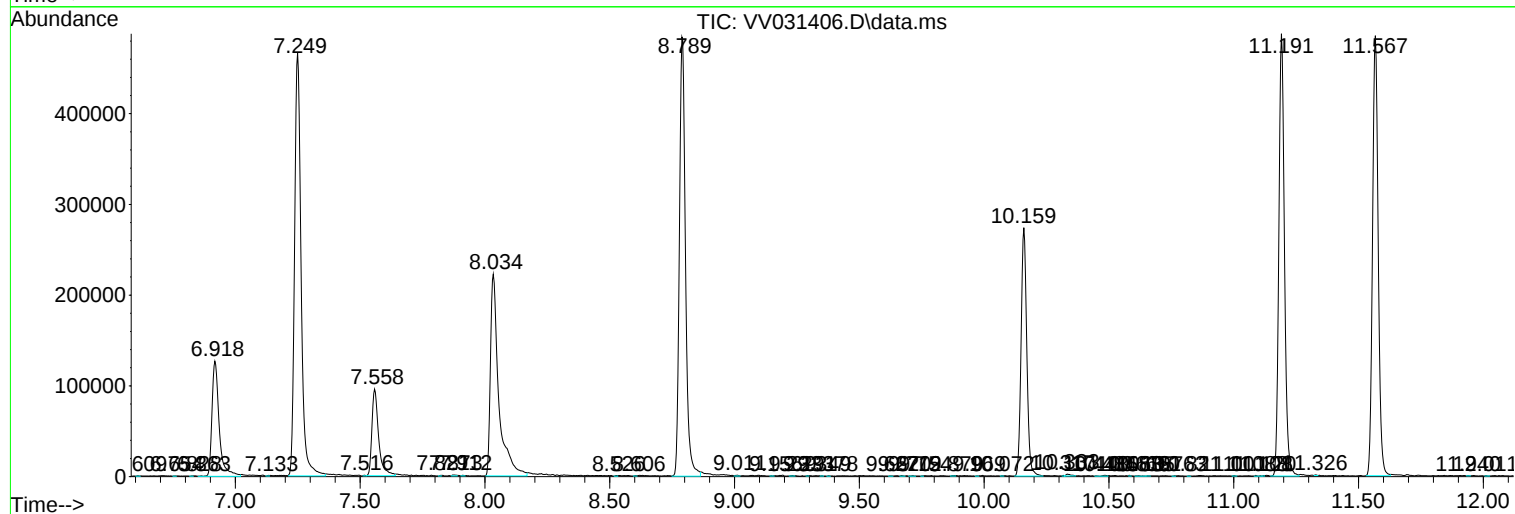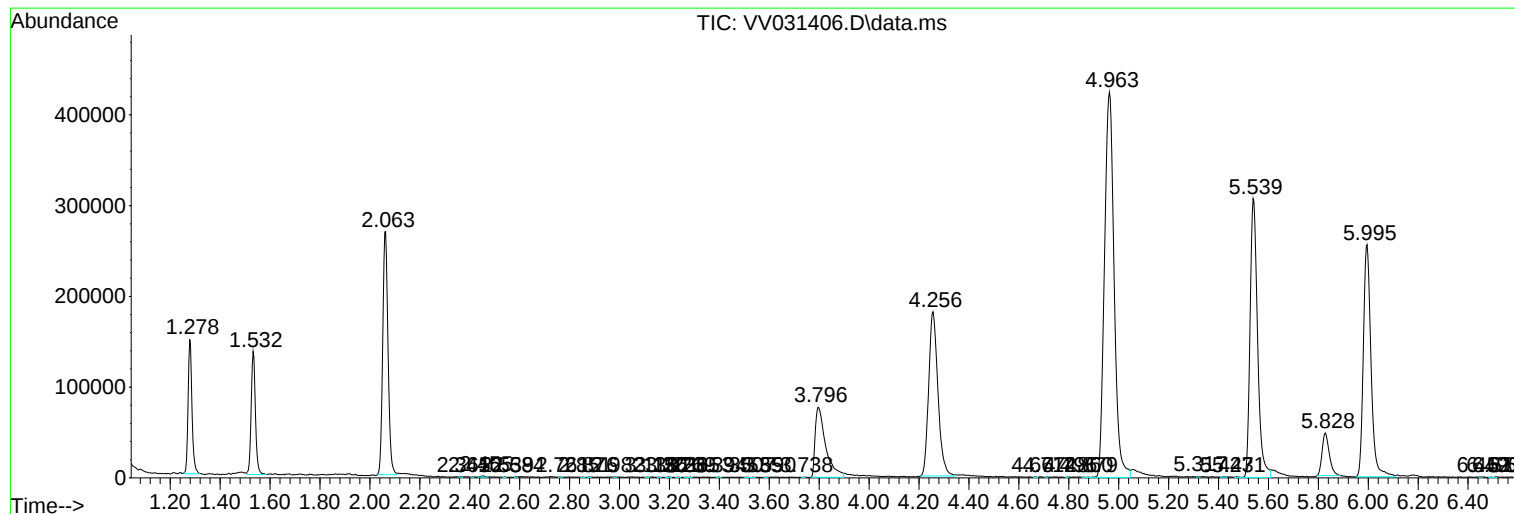

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031406.D
Acq On : 07 Jun 2023 18:01
Operator : SY/MD
Sample : 02992-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031406.D
Acq On : 07 Jun 2023 18:01
Operator : SY/MD
Sample : 02992-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc