

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031408.D
 Acq On : 07 Jun 2023 18:48
 Operator : SY/MD
 Sample : 02992-06 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031408.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	148283	162983	14.41%	1.760%
2	1.532	146	153	171	rVB	133243	160339	14.18%	1.731%
3	2.063	308	318	333	rBV	266826	391640	34.64%	4.229%
4	2.330	399	401	404	rVB2	734	278	0.02%	0.003%
5	2.404	422	424	426	rBV2	399	192	0.02%	0.002%
6	2.449	432	438	449	rVB8	2508	4424	0.39%	0.048%
7	2.651	496	501	506	rBV3	455	553	0.05%	0.006%
8	2.709	506	519	534	rVV2	8306	18253	1.61%	0.197%
9	2.809	547	550	554	rVB2	332	245	0.02%	0.003%
10	2.844	557	561	565	rBV2	524	531	0.05%	0.006%
11	2.986	601	605	606	rBV2	308	226	0.02%	0.002%
12	3.018	612	615	617	rBV	342	208	0.02%	0.002%
13	3.121	644	647	649	rBV	314	217	0.02%	0.002%
14	3.146	652	655	662	rBV3	303	346	0.03%	0.004%
15	3.208	671	674	677	rVV4	304	200	0.02%	0.002%
16	3.246	684	686	689	rVB2	556	319	0.03%	0.003%
17	3.272	692	694	699	rVV2	475	367	0.03%	0.004%
18	3.301	699	703	707	rVV2	185	162	0.01%	0.002%
19	3.333	711	713	715	rBV2	480	187	0.02%	0.002%
20	3.362	719	722	723	rBV	249	165	0.01%	0.002%
21	3.417	732	739	741	rBV2	494	487	0.04%	0.005%
22	3.478	756	758	762	rVB2	511	275	0.02%	0.003%
23	3.542	776	778	780	rVB	372	147	0.01%	0.002%
24	3.558	780	783	787	rBV2	308	212	0.02%	0.002%
25	3.613	797	800	803	rBV2	441	297	0.03%	0.003%
26	3.674	818	819	823	rVB	319	148	0.01%	0.002%
27	3.700	824	827	829	rBV2	265	153	0.01%	0.002%
28	3.806	848	860	892	rBV3	91072	324938	28.74%	3.508%
29	4.163	969	971	976	rVB5	573	459	0.04%	0.005%
30	4.256	984	1000	1024	rBV	182023	470195	41.58%	5.077%
31	4.590	1103	1104	1107	rVV2	468	245	0.02%	0.003%
32	4.619	1111	1113	1115	rVB	491	196	0.02%	0.002%
33	4.767	1157	1159	1162	rVB3	425	243	0.02%	0.003%
34	4.783	1162	1164	1166	rBV2	470	237	0.02%	0.003%
35	4.963	1203	1220	1242	rBV2	427053	1130756	100.00%	12.209%
36	5.240	1303	1306	1310	rBV4	813	642	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031408.D
 Acq On : 07 Jun 2023 18:48
 Operator : SY/MD
 Sample : 02992-06 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.394	1351	1354	1357	rBV4	704	519	0.05%	0.006%
38	5.462	1373	1375	1377	rBV2	451	197	0.02%	0.002%
39	5.539	1385	1399	1424	rBV	298607	627971	55.54%	6.780%
40	5.834	1477	1491	1513	rBV5	57916	141832	12.54%	1.531%
41	5.995	1527	1541	1570	rBV2	257739	547137	48.39%	5.908%
42	6.320	1640	1642	1643	rBV	292	152	0.01%	0.002%
43	6.375	1657	1659	1667	rVB6	545	409	0.04%	0.004%
44	6.410	1667	1670	1673	rBV3	395	233	0.02%	0.003%
45	6.609	1729	1732	1733	rBV2	501	301	0.03%	0.003%
46	6.638	1738	1741	1746	rVB3	615	454	0.04%	0.005%
47	6.661	1746	1748	1750	rBV2	379	184	0.02%	0.002%
48	6.754	1774	1777	1780	rVB2	419	299	0.03%	0.003%
49	6.796	1788	1790	1791	rBV2	307	158	0.01%	0.002%
50	6.844	1803	1805	1808	rBV3	241	157	0.01%	0.002%
51	6.918	1817	1828	1857	rBV2	128962	249915	22.10%	2.698%
52	7.121	1887	1891	1893	rBV3	543	332	0.03%	0.004%
53	7.249	1919	1931	1956	rBV	466977	833271	73.69%	8.997%
54	7.500	2006	2009	2010	rBV2	397	194	0.02%	0.002%
55	7.558	2014	2027	2050	rBV	95097	176251	15.59%	1.903%
56	7.825	2108	2110	2114	rBV2	379	301	0.03%	0.003%
57	7.908	2121	2136	2165	rBV	424881	740943	65.53%	8.000%
58	8.034	2165	2175	2212	rBV2	239905	516621	45.69%	5.578%
59	8.410	2290	2292	2294	rBV2	588	259	0.02%	0.003%
60	8.551	2333	2336	2339	rVB2	538	287	0.03%	0.003%
61	8.574	2339	2343	2345	rBV2	445	357	0.03%	0.004%
62	8.641	2362	2364	2367	rBV2	455	268	0.02%	0.003%
63	8.677	2372	2375	2378	rVB3	522	392	0.03%	0.004%
64	8.789	2398	2410	2433	rBV	473167	797052	70.49%	8.606%
65	8.995	2470	2474	2478	rBV4	871	744	0.07%	0.008%
66	9.050	2489	2491	2493	rBV	443	206	0.02%	0.002%
67	9.121	2510	2513	2516	rBV2	389	273	0.02%	0.003%
68	9.265	2555	2558	2562	rBV2	341	272	0.02%	0.003%
69	9.294	2564	2567	2570	rVV2	452	221	0.02%	0.002%
70	9.310	2570	2572	2576	rVV3	274	195	0.02%	0.002%
71	9.342	2580	2582	2585	rBV3	336	147	0.01%	0.002%
72	9.448	2611	2615	2616	rVV2	299	196	0.02%	0.002%
73	9.471	2620	2622	2624	rVV2	390	172	0.02%	0.002%
74	9.600	2659	2662	2663	rBV	351	180	0.02%	0.002%
75	9.699	2691	2693	2694	rBV	362	158	0.01%	0.002%
76	9.940	2762	2768	2770	rBV	516	397	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031408.D
 Acq On : 07 Jun 2023 18:48
 Operator : SY/MD
 Sample : 02992-06 20X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C07

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.014	2789	2791	2793	rVB	347	181	0.02%	0.002%
78	10.034	2795	2797	2803	rBV2	411	457	0.04%	0.005%
79	10.085	2809	2813	2814	rBV2	572	365	0.03%	0.004%
80	10.159	2824	2836	2865	rBV	306757	485531	42.94%	5.242%
81	10.487	2935	2938	2942	rBV2	634	460	0.04%	0.005%
82	10.567	2960	2963	2965	rBV2	296	190	0.02%	0.002%
83	10.780	3027	3029	3031	rBV4	366	163	0.01%	0.002%
84	10.976	3087	3090	3095	rVB2	414	346	0.03%	0.004%
85	10.998	3095	3097	3102	rBV3	334	264	0.02%	0.003%
86	11.104	3127	3130	3131	rBV2	315	169	0.01%	0.002%
87	11.137	3135	3140	3145	rVB4	647	760	0.07%	0.008%
88	11.191	3145	3157	3180	rBV	454076	716279	63.35%	7.734%
89	11.567	3262	3274	3296	rBV	470599	740672	65.50%	7.997%
90	11.889	3371	3374	3379	rBV5	604	642	0.06%	0.007%
91	11.989	3403	3405	3406	rBV	466	156	0.01%	0.002%
92	12.069	3427	3430	3432	rBV	443	320	0.03%	0.003%
93	12.233	3479	3481	3489	rVB3	506	469	0.04%	0.005%
94	12.866	3676	3678	3681	rBV	577	280	0.02%	0.003%
95	13.153	3764	3767	3769	rBV2	599	375	0.03%	0.004%
96	13.220	3781	3788	3791	rBV4	785	924	0.08%	0.010%
97	13.593	3900	3904	3908	rBV3	518	499	0.04%	0.005%
98	13.799	3966	3968	3971	rBV2	488	250	0.02%	0.003%
99	13.870	3987	3990	3991	rBV	734	327	0.03%	0.004%
100	13.966	4016	4020	4023	rBV3	598	529	0.05%	0.006%


Sum of corrected areas: 9261680

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031408.D
Acq On : 07 Jun 2023 18:48
Operator : SY/MD
Sample : 02992-06 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

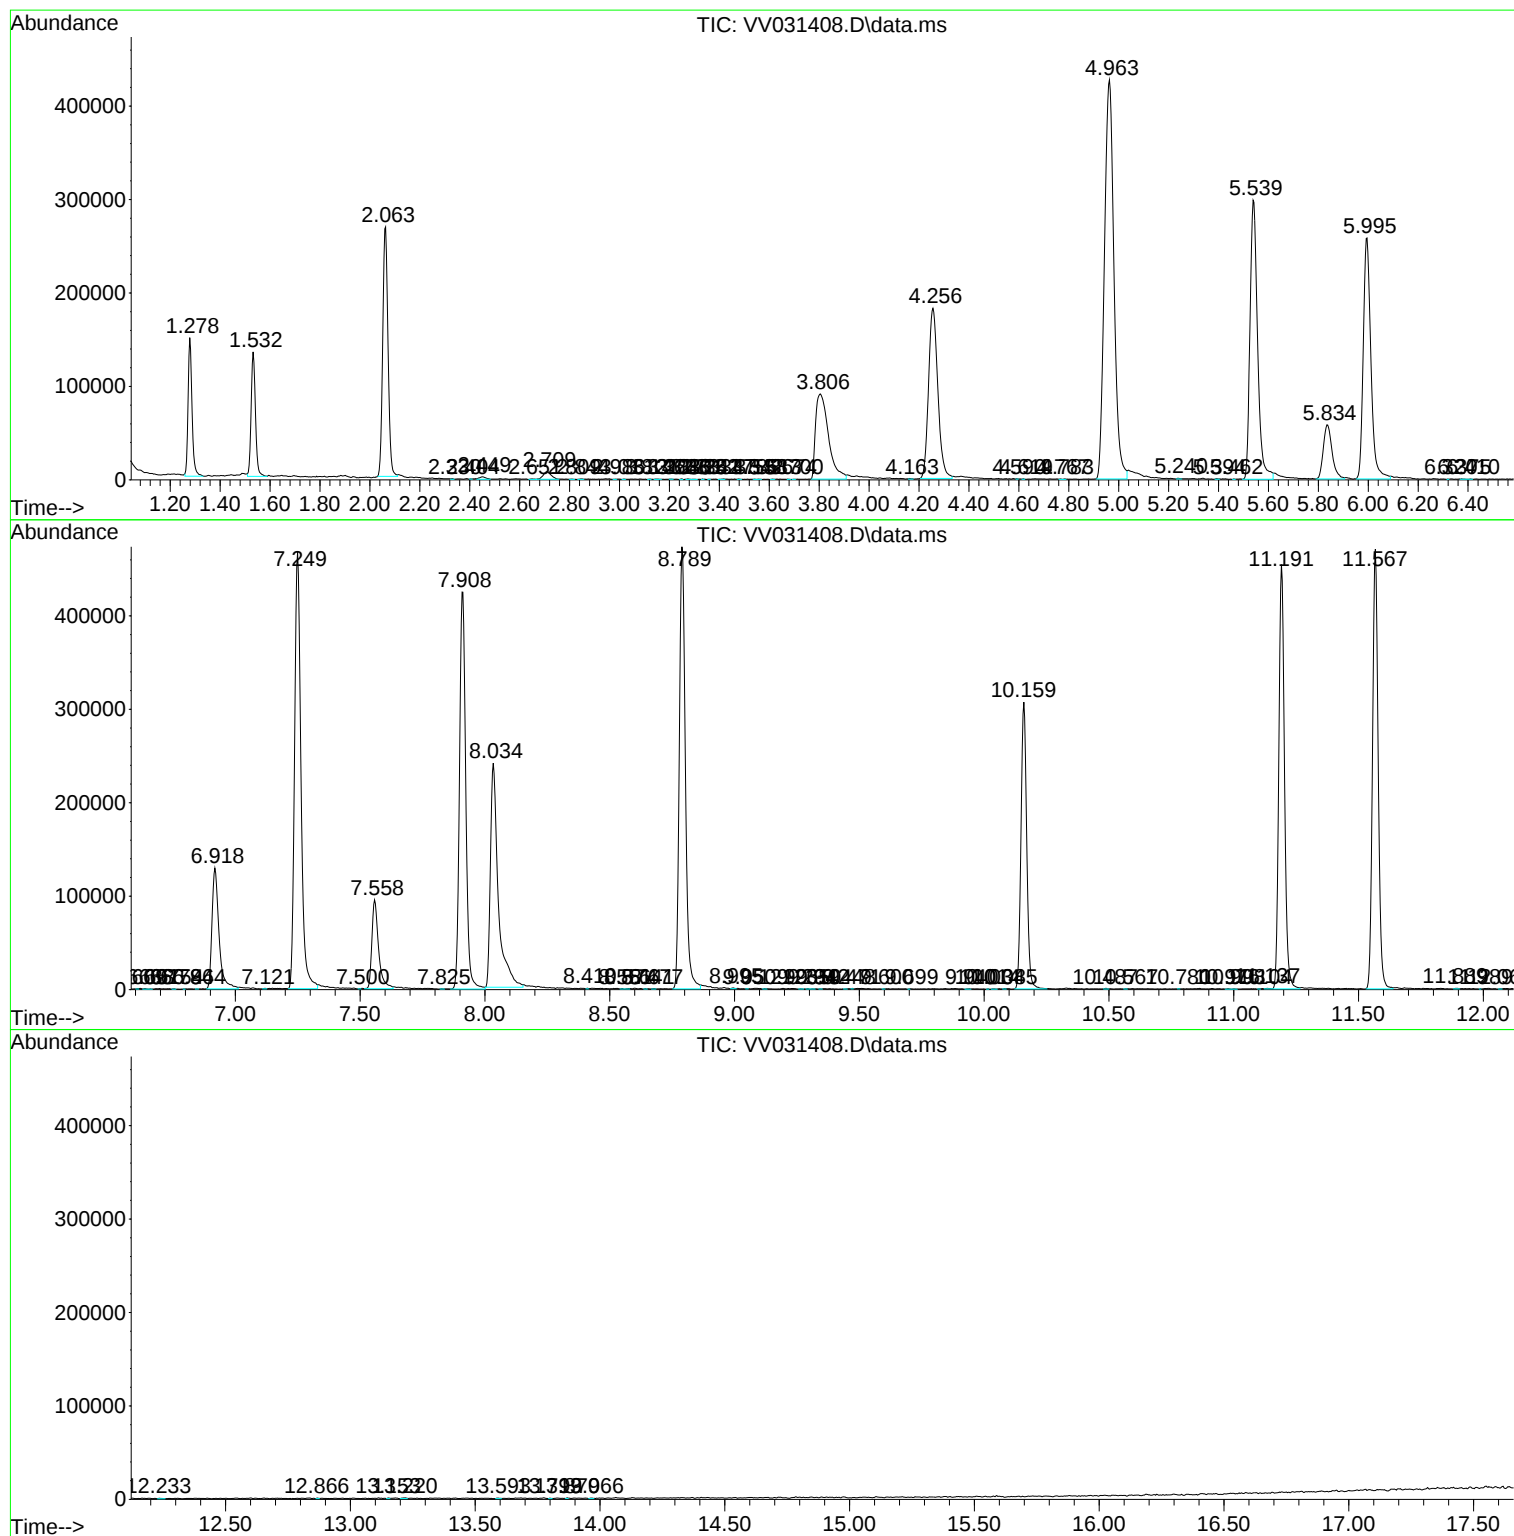

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031408.D
Acq On : 07 Jun 2023 18:48
Operator : SY/MD
Sample : 02992-06 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031408.D
Acq On : 07 Jun 2023 18:48
Operator : SY/MD
Sample : 02992-06 20X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C07

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------