

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031409.D
 Acq On : 07 Jun 2023 19:12
 Operator : SY/MD
 Sample : 02992-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031409.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	156949	171661	2.41%	0.978%
2	1.532	146	153	167	rVB	139783	163695	2.30%	0.933%
3	2.063	307	318	331	rBV	280875	413128	5.80%	2.354%
4	2.375	412	415	417	rBV3	707	449	0.01%	0.003%
5	2.474	444	446	447	rBV	334	132	0.00%	0.001%
6	2.555	469	471	473	rBV3	461	150	0.00%	0.001%
7	2.709	507	519	539	rVB2	26439	56287	0.79%	0.321%
8	2.998	608	609	610	rBV2	301	103	0.00%	0.001%
9	3.072	630	632	633	rBV	394	199	0.00%	0.001%
10	3.146	645	655	658	rBV3	541	665	0.01%	0.004%
11	3.169	660	662	663	rBV2	290	97	0.00%	0.001%
12	3.291	697	700	704	rVB3	482	291	0.00%	0.002%
13	3.314	704	707	709	rBV	563	272	0.00%	0.002%
14	3.326	709	711	718	rBV3	595	498	0.01%	0.003%
15	3.381	725	728	735	rBV2	453	584	0.01%	0.003%
16	3.429	740	743	745	rBV	354	219	0.00%	0.001%
17	3.523	768	772	774	rBV2	420	315	0.00%	0.002%
18	3.593	792	794	796	rVB	616	291	0.00%	0.002%
19	3.609	796	799	802	rBV2	463	280	0.00%	0.002%
20	3.629	802	805	807	rBV3	346	230	0.00%	0.001%
21	3.683	820	822	824	rBV3	390	123	0.00%	0.001%
22	3.732	834	837	839	rVB2	329	186	0.00%	0.001%
23	3.754	842	844	845	rBV	521	207	0.00%	0.001%
24	3.818	847	864	897	rBV2	156882	542048	7.61%	3.088%
25	4.256	982	1000	1024	rBV	192830	503507	7.07%	2.869%
26	4.516	1078	1081	1084	rBV3	797	639	0.01%	0.004%
27	4.667	1126	1128	1135	rVB4	566	568	0.01%	0.003%
28	4.751	1152	1154	1155	rBV	361	122	0.00%	0.001%
29	4.963	1203	1220	1278	rBV2	457199	1239871	17.41%	7.064%
30	5.330	1328	1334	1338	rBV5	1012	1050	0.01%	0.006%
31	5.420	1359	1362	1364	rBV3	553	413	0.01%	0.002%
32	5.445	1368	1370	1372	rBV2	322	184	0.00%	0.001%
33	5.539	1387	1399	1421	rBV	315760	648758	9.11%	3.696%
34	5.838	1477	1492	1526	rBV	620554	1275419	17.91%	7.266%
35	5.995	1530	1541	1573	rVB	274407	580247	8.15%	3.306%
36	6.339	1646	1648	1652	rBV2	703	445	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031409.D
 Acq On : 07 Jun 2023 19:12
 Operator : SY/MD
 Sample : 02992-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C11

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.519	1700	1704	1709	rBV4	677	715	0.01%	0.004%
38	6.542	1709	1711	1712	rBV	162	55	0.00%	0.000%
39	6.564	1712	1718	1723	rVV5	532	612	0.01%	0.003%
40	6.731	1768	1770	1773	rVB2	593	285	0.00%	0.002%
41	6.789	1787	1788	1789	rVB	269	52	0.00%	0.000%
42	6.879	1813	1816	1817	rBV2	703	430	0.01%	0.002%
43	6.918	1817	1828	1846	rVV	136470	259590	3.64%	1.479%
44	7.159	1899	1903	1904	rBV2	658	414	0.01%	0.002%
45	7.249	1919	1931	1963	rBV	502419	899484	12.63%	5.125%
46	7.558	2017	2027	2051	rBV	101006	188918	2.65%	1.076%
47	7.847	2115	2117	2120	rVB3	444	221	0.00%	0.001%
48	7.911	2120	2137	2165	rBV	4211861	7122319	100.00%	40.578%
49	8.034	2166	2175	2210	rVB	272261	559630	7.86%	3.188%
50	8.609	2352	2354	2356	rBV2	517	330	0.00%	0.002%
51	8.789	2398	2410	2435	rBV	495062	833627	11.70%	4.749%
52	9.146	2519	2521	2527	rBV4	603	503	0.01%	0.003%
53	9.198	2535	2537	2541	rBV2	391	278	0.00%	0.002%
54	9.243	2549	2551	2554	rBV3	407	216	0.00%	0.001%
55	9.310	2571	2572	2574	rBV	467	187	0.00%	0.001%
56	9.587	2656	2658	2660	rVB	307	88	0.00%	0.001%
57	10.159	2824	2836	2858	rBV	328209	519327	7.29%	2.959%
58	10.297	2877	2879	2883	rBV2	661	475	0.01%	0.003%
59	10.564	2960	2962	2966	rBV3	443	288	0.00%	0.002%
60	10.796	3031	3034	3037	rBV3	593	449	0.01%	0.003%
61	11.191	3146	3157	3176	rBV	480219	757218	10.63%	4.314%
62	11.567	3262	3274	3297	rBV	507521	802203	11.26%	4.570%
63	12.030	3416	3418	3421	rBV2	616	349	0.00%	0.002%
64	12.313	3503	3506	3508	rBV	674	403	0.01%	0.002%
65	13.027	3726	3728	3731	rBV	448	280	0.00%	0.002%




Sum of corrected areas: 17552279

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031409.D
Acq On : 07 Jun 2023 19:12
Operator : SY/MD
Sample : 02992-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

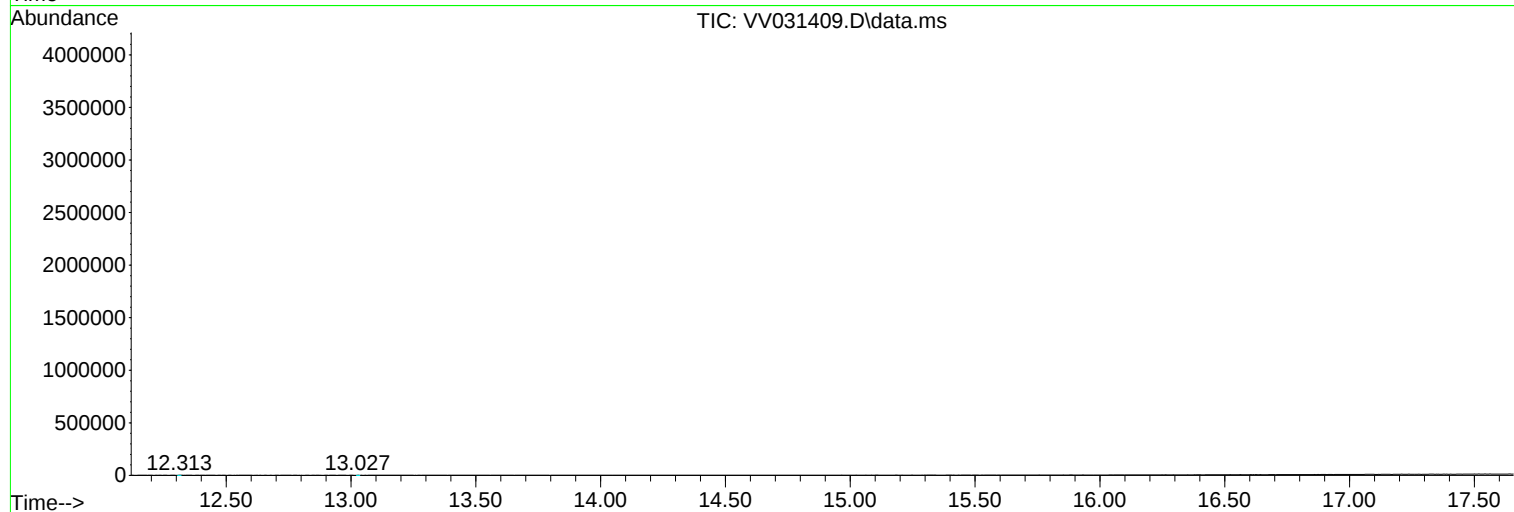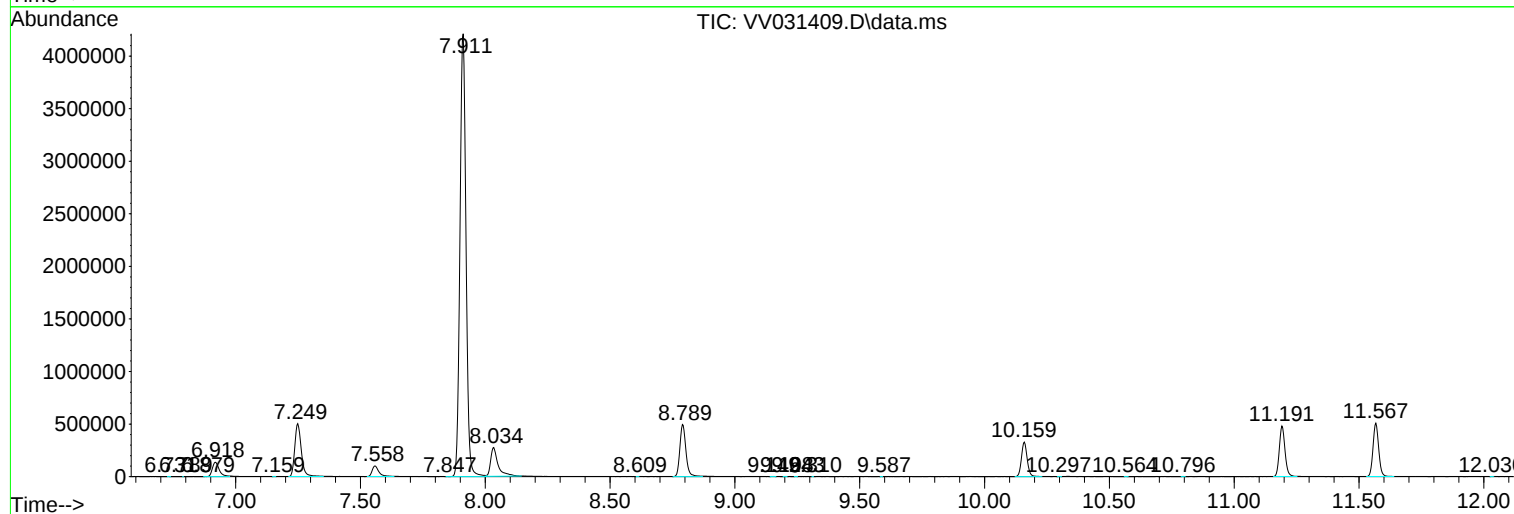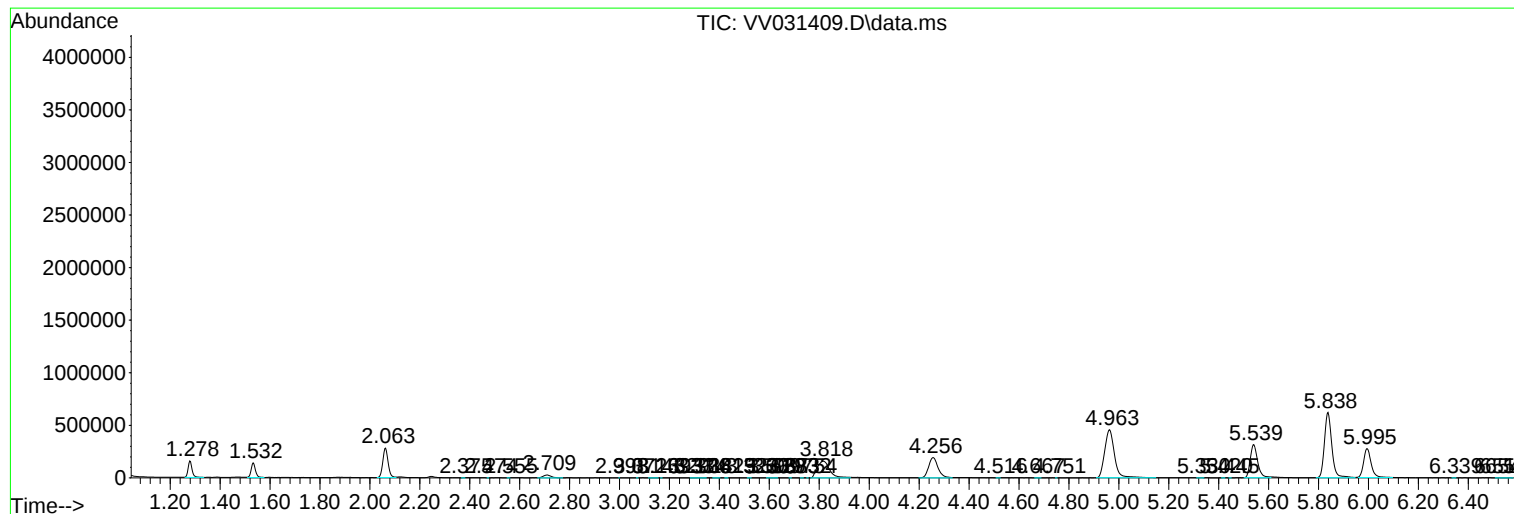

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031409.D
Acq On : 07 Jun 2023 19:12
Operator : SY/MD
Sample : 02992-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031409.D
Acq On : 07 Jun 2023 19:12
Operator : SY/MD
Sample : 02992-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C11

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc