

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031410.D
 Acq On : 07 Jun 2023 19:36
 Operator : SY/MD
 Sample : 02992-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	94	rVB	151064	163466	3.73%	1.185%
2	1.532	146	153	167	rVB	135841	159784	3.65%	1.158%
3	2.063	308	318	332	rBV	264187	392569	8.96%	2.846%
4	2.568	472	475	479	rBV4	609	495	0.01%	0.004%
5	2.709	504	519	543	rBV	176695	373438	8.52%	2.707%
6	2.989	601	606	611	rBV5	610	800	0.02%	0.006%
7	3.040	620	622	624	rBV	394	192	0.00%	0.001%
8	3.060	626	628	630	rVV	324	114	0.00%	0.001%
9	3.089	635	637	640	rVV2	318	145	0.00%	0.001%
10	3.143	652	654	657	rBV	241	169	0.00%	0.001%
11	3.204	672	673	677	rVB2	378	172	0.00%	0.001%
12	3.224	677	679	681	rBV	445	210	0.00%	0.002%
13	3.236	681	683	686	rVB2	238	100	0.00%	0.001%
14	3.272	690	694	700	rVB2	778	612	0.01%	0.004%
15	3.298	700	702	704	rBV	198	111	0.00%	0.001%
16	3.314	704	707	708	rBV2	335	172	0.00%	0.001%
17	3.362	717	722	724	rBV2	424	386	0.01%	0.003%
18	3.371	724	725	728	rBV2	429	210	0.00%	0.002%
19	3.416	738	739	743	rBV2	331	191	0.00%	0.001%
20	3.439	744	746	748	rBV2	355	188	0.00%	0.001%
21	3.481	757	759	761	rBV	220	91	0.00%	0.001%
22	3.587	788	792	794	rBV	422	312	0.01%	0.002%
23	3.609	794	799	800	rVV3	264	227	0.01%	0.002%
24	3.712	829	831	832	rBV2	339	165	0.00%	0.001%
25	3.751	840	843	844	rBV2	319	187	0.00%	0.001%
26	3.812	848	862	887	rBV3	110332	381962	8.71%	2.769%
27	4.256	986	1000	1028	rVB	178931	463464	10.57%	3.360%
28	4.513	1077	1080	1083	rVB3	805	445	0.01%	0.003%
29	4.535	1084	1087	1091	rVV4	736	404	0.01%	0.003%
30	4.670	1127	1129	1130	rBV	292	121	0.00%	0.001%
31	4.699	1135	1138	1140	rVV3	648	361	0.01%	0.003%
32	4.725	1144	1146	1148	rVV	581	267	0.01%	0.002%
33	4.751	1152	1154	1156	rVB	342	136	0.00%	0.001%
34	4.805	1168	1171	1174	rBV2	423	288	0.01%	0.002%
35	4.818	1174	1175	1179	rVB2	362	140	0.00%	0.001%
36	4.844	1179	1183	1187	rBV3	708	642	0.01%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031410.D
 Acq On : 07 Jun 2023 19:36
 Operator : SY/MD
 Sample : 02992-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	4.963	1202	1220	1263	rBV2	431891	1166896	26.62%	8.460%
38	5.317	1329	1330	1331	rBV	464	167	0.00%	0.001%
39	5.368	1343	1346	1347	rBV3	478	250	0.01%	0.002%
40	5.455	1371	1373	1376	rBV3	372	216	0.00%	0.002%
41	5.539	1387	1399	1419	rBV	317916	655379	14.95%	4.751%
42	5.838	1477	1492	1521	rBV3	143693	322603	7.36%	2.339%
43	5.995	1527	1541	1572	rBV	261360	548804	12.52%	3.979%
44	6.233	1609	1615	1617	rBV5	1201	1160	0.03%	0.008%
45	6.281	1627	1630	1632	rBV2	510	373	0.01%	0.003%
46	6.349	1649	1651	1653	rBV	566	288	0.01%	0.002%
47	6.391	1661	1664	1665	rBV	260	127	0.00%	0.001%
48	6.410	1668	1670	1672	rVV2	513	219	0.00%	0.002%
49	6.423	1672	1674	1677	rVV2	433	219	0.00%	0.002%
50	6.474	1687	1690	1691	rBV3	408	238	0.01%	0.002%
51	6.503	1696	1699	1700	rBV	213	102	0.00%	0.001%
52	6.564	1714	1718	1720	rBV2	792	577	0.01%	0.004%
53	6.580	1720	1723	1726	rVV3	1566	1191	0.03%	0.009%
54	6.651	1743	1745	1748	rVB2	429	240	0.01%	0.002%
55	6.670	1748	1751	1752	rBV	623	311	0.01%	0.002%
56	6.706	1752	1762	1772	rVV5	6510	13048	0.30%	0.095%
57	6.773	1781	1783	1789	rVB3	868	498	0.01%	0.004%
58	6.799	1789	1791	1792	rBV	536	227	0.01%	0.002%
59	6.825	1797	1799	1801	rVB	294	118	0.00%	0.001%
60	6.838	1801	1803	1804	rBV	200	112	0.00%	0.001%
61	6.918	1817	1828	1859	rBV2	129739	252363	5.76%	1.830%
62	7.133	1893	1895	1900	rBV4	626	596	0.01%	0.004%
63	7.172	1904	1907	1909	rBV3	631	425	0.01%	0.003%
64	7.249	1919	1931	1955	rBV	466596	836360	19.08%	6.063%
65	7.558	2017	2027	2055	rBV	98045	182985	4.17%	1.327%
66	7.818	2106	2108	2112	rVB3	410	251	0.01%	0.002%
67	7.841	2112	2115	2117	rBV2	681	391	0.01%	0.003%
68	7.911	2122	2137	2161	rBV	2603829	4383162	100.00%	31.776%
69	8.034	2166	2175	2214	rVB	261384	550980	12.57%	3.994%
70	8.529	2328	2329	2331	rBV	569	176	0.00%	0.001%
71	8.789	2399	2410	2439	rBV	508319	848732	19.36%	6.153%
72	9.040	2486	2488	2492	rVB4	1004	684	0.02%	0.005%
73	9.201	2535	2538	2545	rBV3	684	661	0.02%	0.005%
74	9.259	2554	2556	2560	rBV4	427	190	0.00%	0.001%
75	9.410	2600	2603	2605	rVB4	580	296	0.01%	0.002%
76	9.471	2620	2622	2624	rBV	591	210	0.00%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031410.D
 Acq On : 07 Jun 2023 19:36
 Operator : SY/MD
 Sample : 02992-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F6C02

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.580	2653	2656	2661	rBV3	660	684	0.02%	0.005%
78	9.625	2667	2670	2672	rVB2	550	267	0.01%	0.002%
79	9.722	2697	2700	2701	rBV2	536	240	0.01%	0.002%
80	9.767	2712	2714	2716	rBV	415	256	0.01%	0.002%
81	9.889	2750	2752	2755	rVB2	661	249	0.01%	0.002%
82	10.021	2791	2793	2794	rBV	343	133	0.00%	0.001%
83	10.159	2824	2836	2862	rBV	323383	505339	11.53%	3.663%
84	10.333	2881	2890	2897	rBV4	3041	4779	0.11%	0.035%
85	10.580	2965	2967	2971	rBV2	452	353	0.01%	0.003%
86	11.001	3095	3098	3099	rBV	425	234	0.01%	0.002%
87	11.050	3111	3113	3119	rVB2	397	336	0.01%	0.002%
88	11.075	3119	3121	3124	rBV	388	210	0.00%	0.002%
89	11.191	3146	3157	3176	rBV	502793	784370	17.90%	5.686%
90	11.419	3226	3228	3231	rBV3	651	297	0.01%	0.002%
91	11.567	3263	3274	3295	rBV	480150	767373	17.51%	5.563%
92	11.911	3379	3381	3387	rVB2	624	528	0.01%	0.004%
93	11.985	3397	3404	3413	rVB7	1723	2524	0.06%	0.018%
94	12.146	3453	3454	3458	rBV2	389	262	0.01%	0.002%
95	12.487	3559	3560	3563	rVB2	348	146	0.00%	0.001%
96	12.503	3563	3565	3567	rBV2	296	146	0.00%	0.001%
97	12.770	3642	3648	3661	rVB6	6842	9647	0.22%	0.070%
98	13.040	3730	3732	3736	rVB3	740	428	0.01%	0.003%
99	13.387	3837	3840	3841	rBV	325	172	0.00%	0.001%
100	13.963	4015	4019	4021	rBV	419	359	0.01%	0.003%



Sum of corrected areas: 13793893

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031410.D
Acq On : 07 Jun 2023 19:36
Operator : SY/MD
Sample : 02992-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

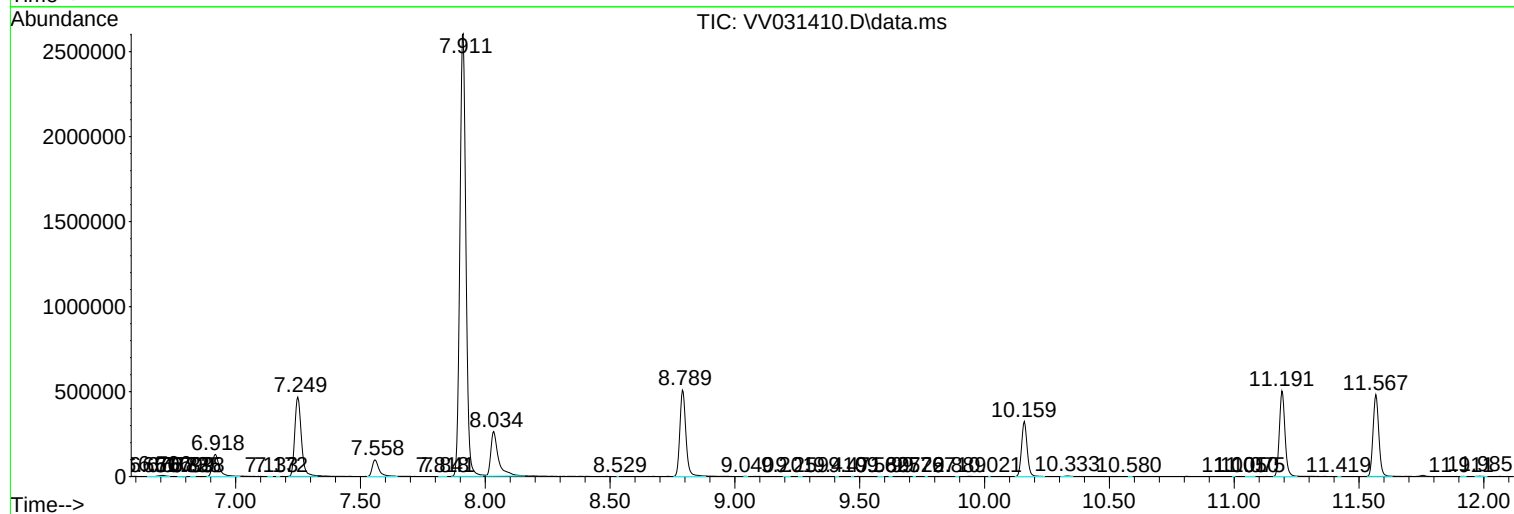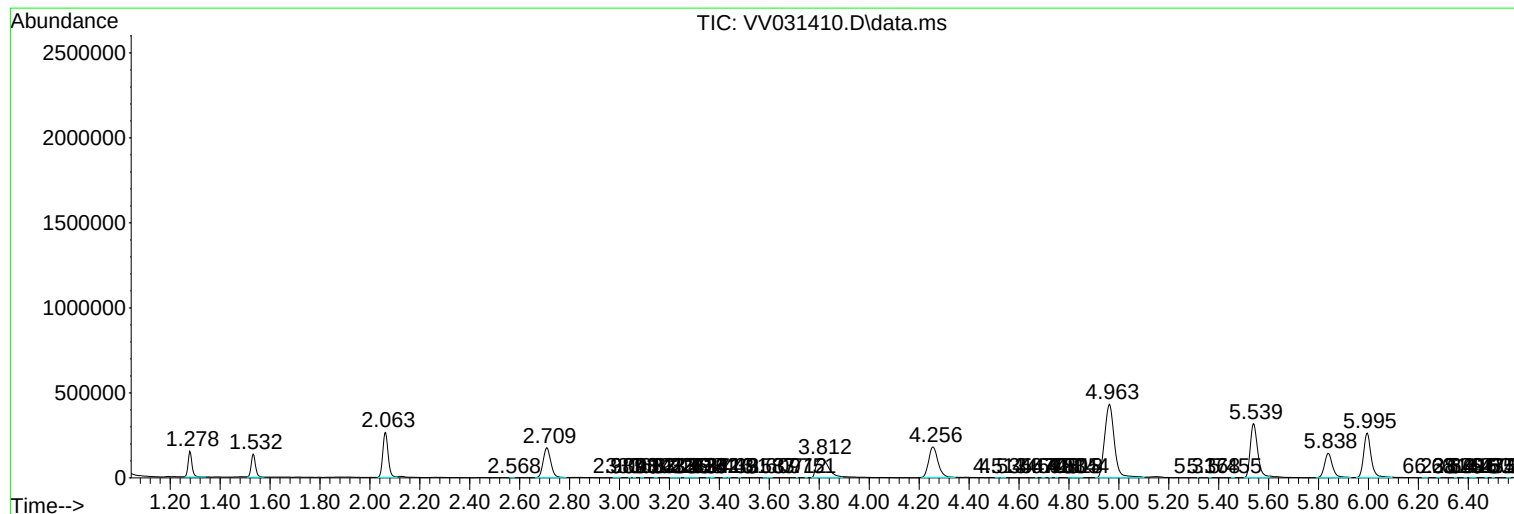

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031410.D
Acq On : 07 Jun 2023 19:36
Operator : SY/MD
Sample : 02992-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031410.D
Acq On : 07 Jun 2023 19:36
Operator : SY/MD
Sample : 02992-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F6C02

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------