

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031412.D
 Acq On : 07 Jun 2023 21:09
 Operator : SY/MD
 Sample : VV0607WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031412.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	151430	164983	14.56%	1.946%
2	1.532	146	153	166	rVB	131759	152595	13.47%	1.800%
3	2.063	308	318	332	rBV	274900	400765	35.37%	4.726%
4	2.400	420	423	424	rBV2	473	266	0.02%	0.003%
5	2.455	431	440	452	rVB3	5930	9541	0.84%	0.113%
6	2.519	458	460	465	rVB4	633	310	0.03%	0.004%
7	2.642	496	498	501	rVV2	411	260	0.02%	0.003%
8	2.696	512	515	516	rBV2	722	383	0.03%	0.005%
9	2.754	530	533	535	rBV2	524	336	0.03%	0.004%
10	2.815	550	552	555	rBV2	308	207	0.02%	0.002%
11	2.969	598	600	605	rVB3	381	237	0.02%	0.003%
12	2.995	605	608	611	rBV2	373	207	0.02%	0.002%
13	3.040	614	622	623	rBV4	508	440	0.04%	0.005%
14	3.121	645	647	653	rBV4	429	461	0.04%	0.005%
15	3.178	662	665	667	rBV2	506	278	0.02%	0.003%
16	3.223	676	679	682	rVB	593	322	0.03%	0.004%
17	3.278	690	696	699	rBV2	579	446	0.04%	0.005%
18	3.317	706	708	713	rVB2	375	310	0.03%	0.004%
19	3.461	750	753	756	rBV2	206	220	0.02%	0.003%
20	3.590	790	793	796	rBV2	230	218	0.02%	0.003%
21	3.722	830	834	840	rBV2	358	360	0.03%	0.004%
22	3.796	847	857	890	rBV	84028	250430	22.10%	2.953%
23	4.256	984	1000	1030	rBV	181408	472583	41.71%	5.573%
24	4.558	1090	1094	1098	rBV3	407	367	0.03%	0.004%
25	4.577	1098	1100	1102	rVB3	495	227	0.02%	0.003%
26	4.754	1151	1155	1159	rBV3	390	332	0.03%	0.004%
27	4.899	1197	1200	1202	rBV	651	397	0.04%	0.005%
28	4.963	1203	1220	1246	rBV2	428119	1133000	100.00%	13.362%
29	5.194	1290	1292	1295	rBV3	879	519	0.05%	0.006%
30	5.323	1328	1332	1337	rBV5	807	786	0.07%	0.009%
31	5.400	1351	1356	1360	rBV4	799	804	0.07%	0.009%
32	5.542	1383	1400	1423	rBV	312415	653896	57.71%	7.712%
33	5.831	1478	1490	1507	rBV	33104	69141	6.10%	0.815%
34	5.944	1521	1525	1527	rBV	480	261	0.02%	0.003%
35	5.995	1527	1541	1562	rBV	261849	540413	47.70%	6.373%
36	6.294	1632	1634	1638	rBV2	510	347	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031412.D
 Acq On : 07 Jun 2023 21:09
 Operator : SY/MD
 Sample : VV0607WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.333	1642	1646	1649	rBV3	456	453	0.04%	0.005%
38	6.362	1653	1655	1659	rBV2	641	380	0.03%	0.004%
39	6.506	1698	1700	1702	rVB2	596	269	0.02%	0.003%
40	6.606	1729	1731	1733	rBV2	396	251	0.02%	0.003%
41	6.657	1743	1747	1750	rVV3	363	314	0.03%	0.004%
42	6.715	1762	1765	1769	rVV3	395	285	0.03%	0.003%
43	6.741	1769	1773	1775	rVB2	363	230	0.02%	0.003%
44	6.783	1781	1786	1791	rBV3	483	507	0.04%	0.006%
45	6.873	1810	1814	1817	rBV2	389	279	0.02%	0.003%
46	6.918	1817	1828	1853	rBV	125559	244233	21.56%	2.880%
47	7.249	1919	1931	1960	rBV	462496	831766	73.41%	9.810%
48	7.558	2015	2027	2053	rBV	93867	176209	15.55%	2.078%
49	7.751	2085	2087	2090	rVB3	692	334	0.03%	0.004%
50	7.841	2111	2115	2117	rVB3	451	265	0.02%	0.003%
51	7.886	2126	2129	2132	rBV3	611	500	0.04%	0.006%
52	8.034	2165	2175	2204	rBV2	236215	501374	44.25%	5.913%
53	8.468	2308	2310	2312	rVB	721	289	0.03%	0.003%
54	8.619	2355	2357	2360	rVB3	545	284	0.03%	0.003%
55	8.664	2368	2371	2372	rBV	516	254	0.02%	0.003%
56	8.789	2399	2410	2438	rBV	499807	841455	74.27%	9.924%
57	9.008	2476	2478	2481	rBV2	319	229	0.02%	0.003%
58	9.066	2493	2496	2497	rBV	400	208	0.02%	0.002%
59	9.088	2498	2503	2506	rVV3	741	660	0.06%	0.008%
60	9.133	2514	2517	2519	rBV4	578	411	0.04%	0.005%
61	9.204	2537	2539	2545	rBV2	565	509	0.04%	0.006%
62	9.400	2598	2600	2604	rVB3	391	212	0.02%	0.003%
63	9.587	2653	2658	2660	rBV3	374	341	0.03%	0.004%
64	9.728	2699	2702	2705	rVB2	312	222	0.02%	0.003%
65	9.751	2705	2709	2712	rVB2	528	339	0.03%	0.004%
66	9.870	2740	2746	2750	rBV5	924	1048	0.09%	0.012%
67	9.918	2759	2761	2767	rBV5	715	473	0.04%	0.006%
68	10.008	2787	2789	2791	rBV2	453	251	0.02%	0.003%
69	10.062	2802	2806	2809	rBV2	396	320	0.03%	0.004%
70	10.159	2824	2836	2859	rBV	299181	472224	41.68%	5.569%
71	10.365	2896	2900	2902	rBV3	525	336	0.03%	0.004%
72	10.410	2911	2914	2916	rBV2	335	248	0.02%	0.003%
73	10.439	2921	2923	2928	rVB4	584	239	0.02%	0.003%
74	10.487	2933	2938	2939	rBV2	921	773	0.07%	0.009%
75	10.570	2960	2964	2965	rBV	307	216	0.02%	0.003%
76	10.593	2969	2971	2973	rBV2	500	243	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031412.D
 Acq On : 07 Jun 2023 21:09
 Operator : SY/MD
 Sample : VV0607WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK350

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.625	2978	2981	2986	rBV	404	342	0.03%	0.004%
78	10.657	2987	2991	2993	rVB2	492	395	0.03%	0.005%
79	10.677	2993	2997	3000	rBV4	471	394	0.03%	0.005%
80	10.863	3051	3055	3058	rBV3	1079	942	0.08%	0.011%
81	11.024	3102	3105	3106	rBV2	368	226	0.02%	0.003%
82	11.075	3118	3121	3124	rBV2	551	438	0.04%	0.005%
83	11.127	3131	3137	3146	rBV8	1825	3010	0.27%	0.035%
84	11.191	3146	3157	3177	rBV	484077	768906	67.86%	9.068%
85	11.300	3189	3191	3195	rVB3	941	447	0.04%	0.005%
86	11.525	3257	3261	3262	rBV	432	294	0.03%	0.003%
87	11.567	3262	3274	3294	rBV	471565	751555	66.33%	8.864%
88	11.937	3384	3389	3390	rBV2	462	395	0.03%	0.005%
89	11.966	3396	3398	3402	rBV2	408	240	0.02%	0.003%
90	12.197	3468	3470	3472	rVV	495	241	0.02%	0.003%
91	12.747	3639	3641	3645	rVB2	547	310	0.03%	0.004%
92	12.815	3659	3662	3664	rBV2	570	343	0.03%	0.004%
93	13.024	3724	3727	3732	rBV4	615	431	0.04%	0.005%
94	13.111	3752	3754	3758	rBV2	508	461	0.04%	0.005%
95	13.149	3764	3766	3769	rBV	542	296	0.03%	0.003%
96	13.213	3780	3786	3794	rVB6	2496	3349	0.30%	0.039%
97	13.332	3819	3823	3826	rBV2	967	727	0.06%	0.009%
98	13.451	3853	3860	3872	rVB2	4760	8195	0.72%	0.097%
99	13.853	3982	3985	3989	rBV3	612	602	0.05%	0.007%
100	13.873	3989	3991	3995	rBV3	702	531	0.05%	0.006%


Sum of corrected areas: 8479151

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031412.D
Acq On : 07 Jun 2023 21:09
Operator : SY/MD
Sample : VV0607WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

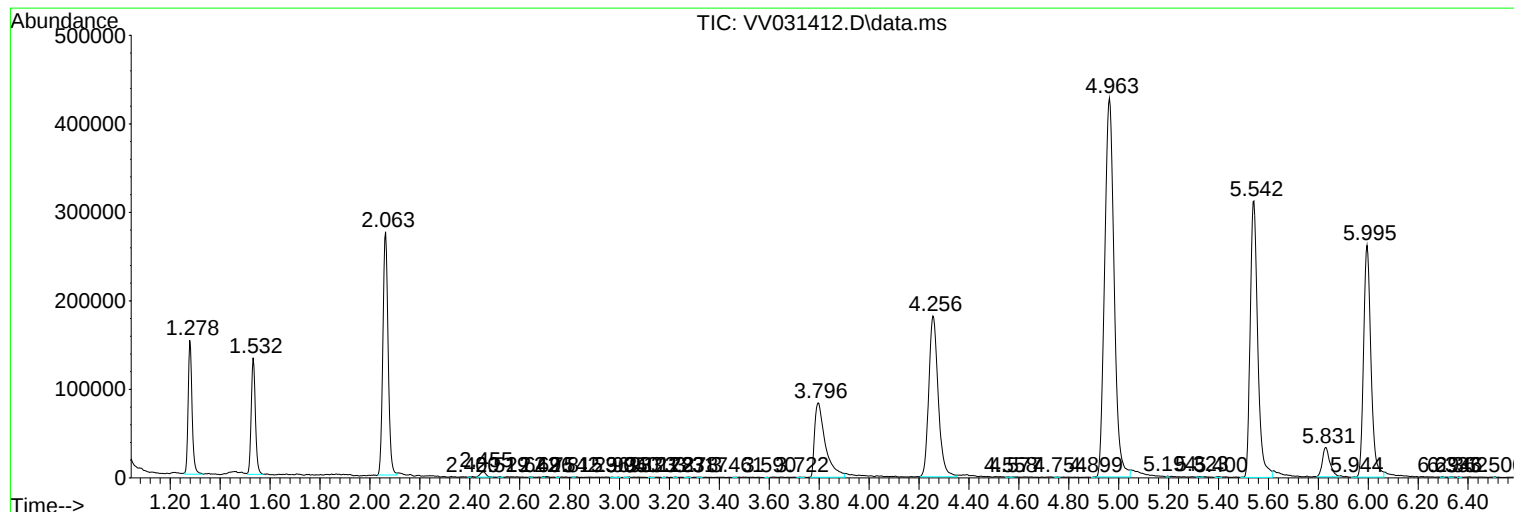

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031412.D
Acq On : 07 Jun 2023 21:09
Operator : SY/MD
Sample : VV0607WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031412.D
Acq On : 07 Jun 2023 21:09
Operator : SY/MD
Sample : VV0607WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK350

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------