

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031414.D
 Acq On : 07 Jun 2023 21:56
 Operator : SY/MD
 Sample : 03076-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M

Title : VOC Analysis

Signal : TIC: VV031414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	152569	164017	13.36%	1.830%
2	1.532	146	153	169	rVB	143978	168249	13.70%	1.877%
3	2.063	308	318	332	rBV	275655	405551	33.03%	4.525%
4	2.587	477	481	485	rBV4	755	837	0.07%	0.009%
5	2.715	519	521	525	rBV3	491	296	0.02%	0.003%
6	2.786	541	543	546	rBV2	324	191	0.02%	0.002%
7	2.857	561	565	569	rBV2	266	246	0.02%	0.003%
8	3.021	615	616	620	rVB	348	136	0.01%	0.002%
9	3.066	628	630	635	rVB3	516	316	0.03%	0.004%
10	3.092	635	638	640	rBV	286	191	0.02%	0.002%
11	3.159	657	659	662	rVB	478	210	0.02%	0.002%
12	3.217	672	677	680	rBV2	440	403	0.03%	0.004%
13	3.246	683	686	691	rVV5	415	364	0.03%	0.004%
14	3.278	694	696	697	rBV	339	163	0.01%	0.002%
15	3.503	763	766	771	rVB	371	260	0.02%	0.003%
16	3.545	776	779	781	rVV3	293	206	0.02%	0.002%
17	3.661	813	815	818	rVB2	383	194	0.02%	0.002%
18	3.680	818	821	822	rBV2	293	165	0.01%	0.002%
19	3.796	847	857	900	rBV2	84127	266569	21.71%	2.974%
20	4.256	984	1000	1029	rBV	194232	507539	41.33%	5.663%
21	4.683	1131	1133	1135	rBV	377	177	0.01%	0.002%
22	4.731	1146	1148	1153	rBV3	501	483	0.04%	0.005%
23	4.786	1163	1165	1167	rBV3	364	139	0.01%	0.002%
24	4.825	1174	1177	1180	rBV3	356	314	0.03%	0.004%
25	4.863	1185	1189	1194	rBV2	459	453	0.04%	0.005%
26	4.963	1202	1220	1251	rBV2	456438	1227906	100.00%	13.700%
27	5.416	1359	1361	1365	rVB4	686	354	0.03%	0.004%
28	5.448	1369	1371	1374	rVB2	608	280	0.02%	0.003%
29	5.468	1374	1377	1378	rBV2	320	160	0.01%	0.002%
30	5.477	1378	1380	1381	rBV	398	149	0.01%	0.002%
31	5.538	1387	1399	1425	rBV	315307	675958	55.05%	7.542%
32	5.831	1480	1490	1511	rVB5	39915	94905	7.73%	1.059%
33	5.995	1527	1541	1578	rBV	276819	587760	47.87%	6.558%
34	6.326	1642	1644	1645	rBV	518	202	0.02%	0.002%
35	6.381	1657	1661	1666	rBV4	654	586	0.05%	0.007%
36	6.516	1701	1703	1707	rBV4	323	246	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031414.D
 Acq On : 07 Jun 2023 21:56
 Operator : SY/MD
 Sample : 03076-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.574	1719	1721	1723	rBV3	291	184	0.01%	0.002%
38	6.599	1724	1729	1731	rVV3	887	858	0.07%	0.010%
39	6.622	1734	1736	1741	rVB2	941	578	0.05%	0.006%
40	6.651	1741	1745	1746	rBV2	599	333	0.03%	0.004%
41	6.670	1749	1751	1753	rBV2	325	170	0.01%	0.002%
42	6.738	1769	1772	1776	rBV3	649	584	0.05%	0.007%
43	6.821	1796	1798	1802	rBV2	217	188	0.02%	0.002%
44	6.918	1816	1828	1862	rBV	135273	262580	21.38%	2.930%
45	7.111	1884	1888	1890	rBB2	562	320	0.03%	0.004%
46	7.249	1919	1931	1964	rBV	488082	879928	71.66%	9.818%
47	7.558	2017	2027	2052	rBV2	100934	186425	15.18%	2.080%
48	7.821	2107	2109	2115	rVB2	663	479	0.04%	0.005%
49	7.866	2119	2123	2124	rBV3	889	680	0.06%	0.008%
50	7.956	2150	2151	2153	rBV	512	207	0.02%	0.002%
51	7.969	2153	2155	2157	rVB3	424	178	0.01%	0.002%
52	7.998	2162	2164	2165	rBV2	472	231	0.02%	0.003%
53	8.034	2165	2175	2212	rBV2	252699	558990	45.52%	6.237%
54	8.442	2299	2302	2304	rBV3	745	483	0.04%	0.005%
55	8.455	2304	2306	2307	rVV	435	136	0.01%	0.002%
56	8.506	2319	2322	2325	rBV3	648	484	0.04%	0.005%
57	8.567	2338	2341	2346	rBV4	769	781	0.06%	0.009%
58	8.612	2354	2355	2359	rVB2	474	204	0.02%	0.002%
59	8.654	2365	2368	2369	rBV	398	217	0.02%	0.002%
60	8.722	2386	2389	2391	rBV	447	233	0.02%	0.003%
61	8.789	2398	2410	2432	rBV	520795	856987	69.79%	9.562%
62	9.091	2503	2504	2507	rBV	747	289	0.02%	0.003%
63	9.304	2562	2570	2572	rBV3	609	641	0.05%	0.007%
64	9.361	2585	2588	2594	rBV5	464	568	0.05%	0.006%
65	9.561	2643	2650	2653	rBV3	688	771	0.06%	0.009%
66	9.583	2655	2657	2661	rVV	398	240	0.02%	0.003%
67	9.693	2689	2691	2695	rVB2	565	300	0.02%	0.003%
68	9.718	2695	2699	2704	rBV3	396	426	0.03%	0.005%
69	9.786	2719	2720	2723	rBV2	361	197	0.02%	0.002%
70	9.818	2727	2730	2735	rVB2	698	431	0.04%	0.005%
71	9.847	2735	2739	2740	rBV	422	322	0.03%	0.004%
72	9.873	2744	2747	2749	rBV2	566	353	0.03%	0.004%
73	10.046	2798	2801	2806	rBV2	451	383	0.03%	0.004%
74	10.159	2823	2836	2859	rBV	329153	529458	43.12%	5.907%
75	10.445	2922	2925	2927	rBV2	643	389	0.03%	0.004%
76	10.638	2981	2985	2987	rVB2	533	283	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031414.D
 Acq On : 07 Jun 2023 21:56
 Operator : SY/MD
 Sample : 03076-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F89

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.709	3004	3007	3010	rVB2	490	264	0.02%	0.003%
78	10.747	3016	3019	3021	rBV2	352	234	0.02%	0.003%
79	10.799	3033	3035	3039	rBV3	455	274	0.02%	0.003%
80	10.850	3047	3051	3052	rBV2	323	185	0.02%	0.002%
81	10.863	3052	3055	3059	rVB3	845	741	0.06%	0.008%
82	10.889	3059	3063	3064	rBV	553	321	0.03%	0.004%
83	10.956	3082	3084	3086	rBV3	389	180	0.01%	0.002%
84	11.053	3112	3114	3115	rBV	574	247	0.02%	0.003%
85	11.111	3129	3132	3134	rBV2	522	292	0.02%	0.003%
86	11.136	3136	3140	3144	rVV4	926	820	0.07%	0.009%
87	11.191	3146	3157	3179	rVV	486388	764905	62.29%	8.534%
88	11.567	3262	3274	3299	rBV	498107	796019	64.83%	8.882%
89	11.905	3374	3379	3382	rBV4	484	429	0.03%	0.005%
90	11.969	3395	3399	3402	rVB4	677	387	0.03%	0.004%
91	12.149	3452	3455	3458	rBV2	502	397	0.03%	0.004%
92	12.342	3512	3515	3517	rVB	452	209	0.02%	0.002%
93	12.358	3517	3520	3521	rBV2	448	223	0.02%	0.002%
94	12.741	3636	3639	3644	rBV3	376	274	0.02%	0.003%
95	13.201	3781	3782	3785	rBV2	765	451	0.04%	0.005%
96	13.400	3842	3844	3845	rBV2	548	267	0.02%	0.003%
97	13.638	3915	3918	3919	rBV	518	288	0.02%	0.003%
98	13.750	3951	3953	3955	rBV2	591	271	0.02%	0.003%
99	14.017	4034	4036	4040	rBV3	735	617	0.05%	0.007%
100	14.699	4245	4248	4251	rBV3	923	667	0.05%	0.007%




Sum of corrected areas: 8962626

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031414.D
Acq On : 07 Jun 2023 21:56
Operator : SY/MD
Sample : 03076-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

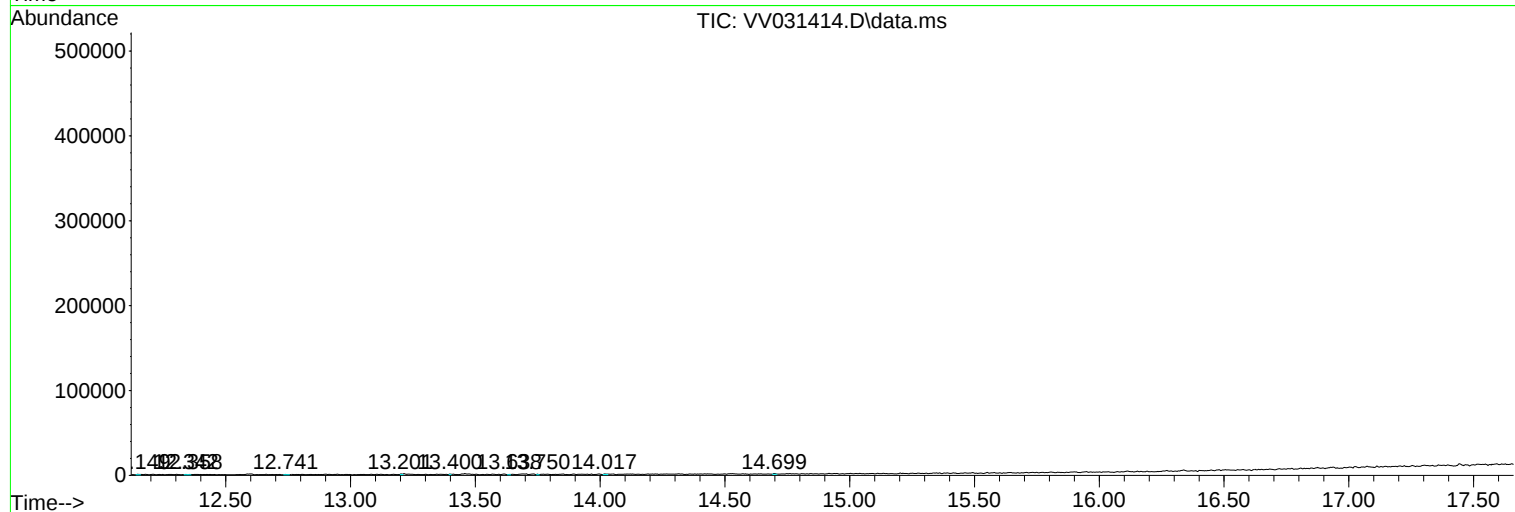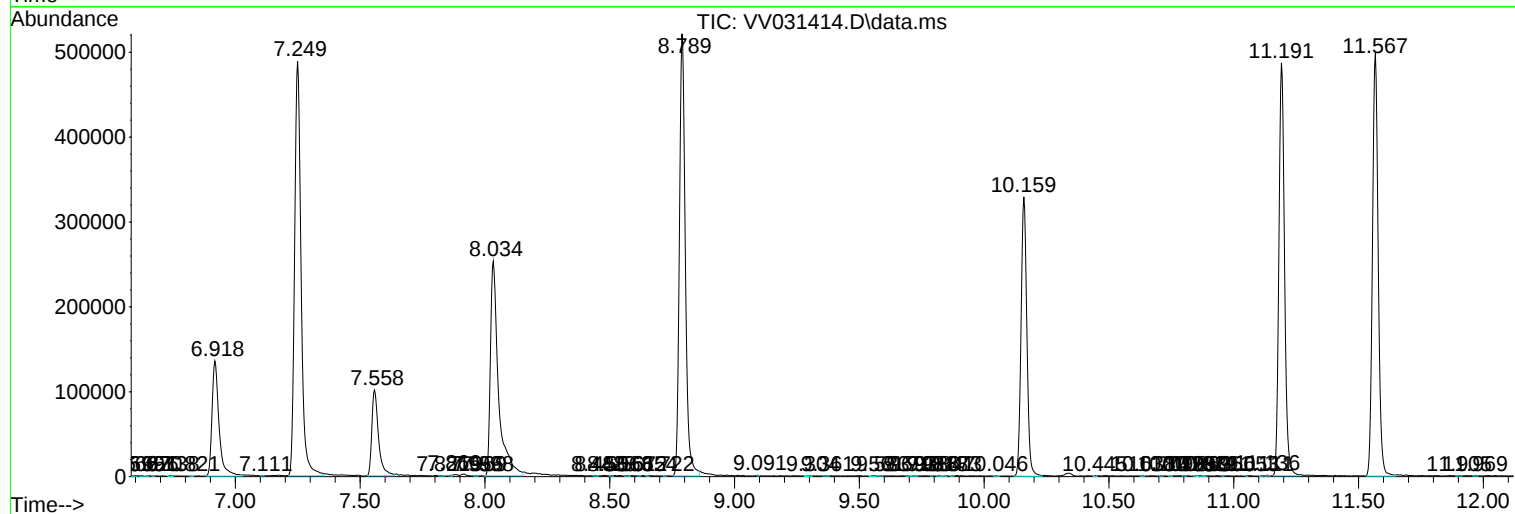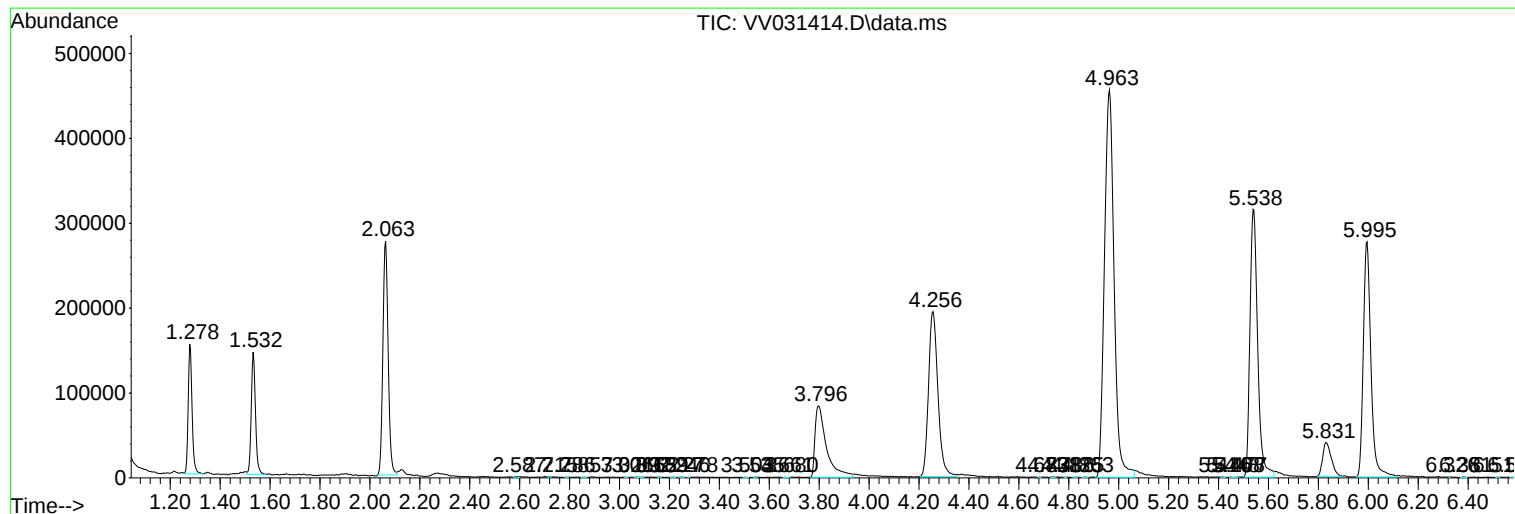

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031414.D
Acq On : 07 Jun 2023 21:56
Operator : SY/MD
Sample : 03076-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031414.D
Acq On : 07 Jun 2023 21:56
Operator : SY/MD
Sample : 03076-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F89

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc