

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031415.D
 Acq On : 07 Jun 2023 22:20
 Operator : SY/MD
 Sample : 03076-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	147815	160319	13.97%	1.860%
2	1.532	146	153	167	rVB	135029	157372	13.71%	1.826%
3	2.063	308	318	331	rBV2	285797	442054	38.51%	5.129%
4	2.960	595	597	598	rBV	317	94	0.01%	0.001%
5	3.024	614	617	620	rBV2	612	293	0.03%	0.003%
6	3.056	624	627	628	rBV2	313	146	0.01%	0.002%
7	3.079	632	634	636	rBV	224	88	0.01%	0.001%
8	3.121	636	647	651	rBV5	930	1918	0.17%	0.022%
9	3.211	672	675	685	rVB4	478	767	0.07%	0.009%
10	3.256	685	689	690	rBV	337	218	0.02%	0.003%
11	3.288	697	699	702	rBV2	262	140	0.01%	0.002%
12	3.323	707	710	713	rBV3	316	221	0.02%	0.003%
13	3.346	715	717	720	rBV	329	132	0.01%	0.002%
14	3.410	735	737	738	rVB2	230	53	0.00%	0.001%
15	3.458	750	752	754	rBV	522	238	0.02%	0.003%
16	3.500	763	765	769	rVB	510	196	0.02%	0.002%
17	3.529	773	774	777	rVB2	175	52	0.00%	0.001%
18	3.561	781	784	786	rBV2	173	124	0.01%	0.001%
19	3.635	804	807	810	rBV2	222	126	0.01%	0.001%
20	3.654	810	813	814	rVB	280	112	0.01%	0.001%
21	3.664	814	816	817	rBV	297	119	0.01%	0.001%
22	3.706	827	829	831	rBV2	334	128	0.01%	0.001%
23	3.764	843	847	848	rBV	483	317	0.03%	0.004%
24	3.802	848	859	896	rBV	87185	295295	25.73%	3.426%
25	4.256	983	1000	1026	rBV	185932	484300	42.19%	5.619%
26	4.654	1120	1124	1126	rBV4	726	460	0.04%	0.005%
27	4.744	1144	1152	1154	rBV3	893	1103	0.10%	0.013%
28	4.799	1165	1169	1172	rBV4	415	375	0.03%	0.004%
29	4.831	1178	1179	1183	rBV3	353	217	0.02%	0.003%
30	4.873	1190	1192	1195	rBV	347	168	0.01%	0.002%
31	4.963	1203	1220	1251	rBV3	425927	1147794	100.00%	13.317%
32	5.384	1347	1351	1353	rBV3	625	463	0.04%	0.005%
33	5.439	1366	1368	1371	rBV2	332	176	0.02%	0.002%
34	5.484	1380	1382	1385	rBV3	560	307	0.03%	0.004%
35	5.539	1387	1399	1438	rVV	306151	651079	56.72%	7.554%
36	5.831	1480	1490	1511	rVB6	32911	75379	6.57%	0.875%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031415.D
 Acq On : 07 Jun 2023 22:20
 Operator : SY/MD
 Sample : 03076-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.995	1527	1541	1568	rBV	257289	550552	47.97%	6.388%
38	6.413	1670	1671	1674	rBV	299	109	0.01%	0.001%
39	6.445	1676	1681	1684	rVV4	749	771	0.07%	0.009%
40	6.567	1717	1719	1721	rBV2	460	217	0.02%	0.003%
41	6.658	1745	1747	1749	rBV	316	113	0.01%	0.001%
42	6.812	1791	1795	1798	rBV	478	406	0.04%	0.005%
43	6.838	1799	1803	1806	rVB2	531	350	0.03%	0.004%
44	6.857	1807	1809	1810	rBV2	491	160	0.01%	0.002%
45	6.918	1817	1828	1859	rBV	124606	248401	21.64%	2.882%
46	7.124	1889	1892	1893	rBV2	714	406	0.04%	0.005%
47	7.249	1919	1931	1956	rBV	461841	832034	72.49%	9.653%
48	7.558	2015	2027	2055	rBV	93457	182903	15.94%	2.122%
49	7.783	2093	2097	2105	rVB6	1461	1959	0.17%	0.023%
50	7.866	2119	2123	2124	rBV3	609	436	0.04%	0.005%
51	8.034	2165	2175	2212	rBV2	233343	524962	45.74%	6.091%
52	8.590	2345	2348	2352	rBV3	489	353	0.03%	0.004%
53	8.609	2352	2354	2356	rVV2	387	215	0.02%	0.002%
54	8.638	2360	2363	2369	rVB5	777	639	0.06%	0.007%
55	8.664	2369	2371	2373	rBV2	396	211	0.02%	0.002%
56	8.680	2374	2376	2377	rVB	380	92	0.01%	0.001%
57	8.789	2398	2410	2440	rBV	485728	825645	71.93%	9.579%
58	9.043	2486	2489	2493	rBV4	829	649	0.06%	0.008%
59	9.063	2493	2495	2496	rBV	654	250	0.02%	0.003%
60	9.185	2530	2533	2535	rBV2	366	284	0.02%	0.003%
61	9.239	2548	2550	2554	rBV2	492	304	0.03%	0.004%
62	9.461	2617	2619	2620	rBV	254	76	0.01%	0.001%
63	9.571	2650	2653	2658	rBV2	444	378	0.03%	0.004%
64	9.593	2658	2660	2664	rBV2	351	234	0.02%	0.003%
65	9.648	2675	2677	2679	rVB3	343	101	0.01%	0.001%
66	9.670	2681	2684	2688	rBV4	880	662	0.06%	0.008%
67	9.725	2699	2701	2705	rBV2	573	305	0.03%	0.004%
68	9.802	2721	2725	2728	rBV2	395	393	0.03%	0.005%
69	9.818	2728	2730	2731	rVV	289	76	0.01%	0.001%
70	9.937	2765	2767	2771	rBV3	469	299	0.03%	0.003%
71	9.953	2771	2772	2776	rVB2	683	249	0.02%	0.003%
72	10.050	2800	2802	2803	rBV	281	95	0.01%	0.001%
73	10.159	2824	2836	2865	rBV	304693	499949	43.56%	5.801%
74	10.310	2881	2883	2884	rBV2	527	218	0.02%	0.003%
75	10.329	2886	2889	2900	rVB4	1845	2859	0.25%	0.033%
76	10.429	2916	2920	2921	rBV	411	289	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031415.D
 Acq On : 07 Jun 2023 22:20
 Operator : SY/MD
 Sample : 03076-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F91

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.442	2922	2924	2927	rVB	530	245	0.02%	0.003%
78	10.522	2947	2949	2951	rBV2	429	178	0.02%	0.002%
79	10.571	2961	2964	2969	rVB3	473	380	0.03%	0.004%
80	10.593	2969	2971	2972	rVB	299	75	0.01%	0.001%
81	10.603	2972	2974	2975	rBV	271	135	0.01%	0.002%
82	10.641	2984	2986	2989	rBV2	417	215	0.02%	0.002%
83	10.744	3013	3018	3019	rBV	360	234	0.02%	0.003%
84	10.866	3048	3056	3065	rBV5	2141	2615	0.23%	0.030%
85	10.982	3091	3092	3094	rVB	213	49	0.00%	0.001%
86	11.050	3109	3113	3118	rBV3	386	445	0.04%	0.005%
87	11.079	3120	3122	3124	rBV2	277	116	0.01%	0.001%
88	11.095	3124	3127	3131	rVV3	539	419	0.04%	0.005%
89	11.191	3145	3157	3180	rBV	478134	747711	65.14%	8.675%
90	11.567	3262	3274	3294	rBV	486212	760185	66.23%	8.820%
91	11.799	3344	3346	3352	rVB4	746	564	0.05%	0.007%
92	11.895	3374	3376	3381	rVB3	534	319	0.03%	0.004%
93	11.972	3397	3400	3402	rBV2	385	263	0.02%	0.003%
94	12.529	3571	3573	3575	rVB2	418	162	0.01%	0.002%
95	12.593	3589	3593	3601	rVB5	1867	2358	0.21%	0.027%
96	12.931	3695	3698	3700	rBV2	621	407	0.04%	0.005%
97	12.982	3712	3714	3718	rBV3	485	227	0.02%	0.003%
98	13.162	3769	3770	3772	rBV	384	189	0.02%	0.002%
99	13.841	3980	3981	3982	rBV	372	87	0.01%	0.001%
100	13.886	3991	3995	3998	rBV2	638	506	0.04%	0.006%




Sum of corrected areas: 8619031

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031415.D
Acq On : 07 Jun 2023 22:20
Operator : SY/MD
Sample : 03076-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

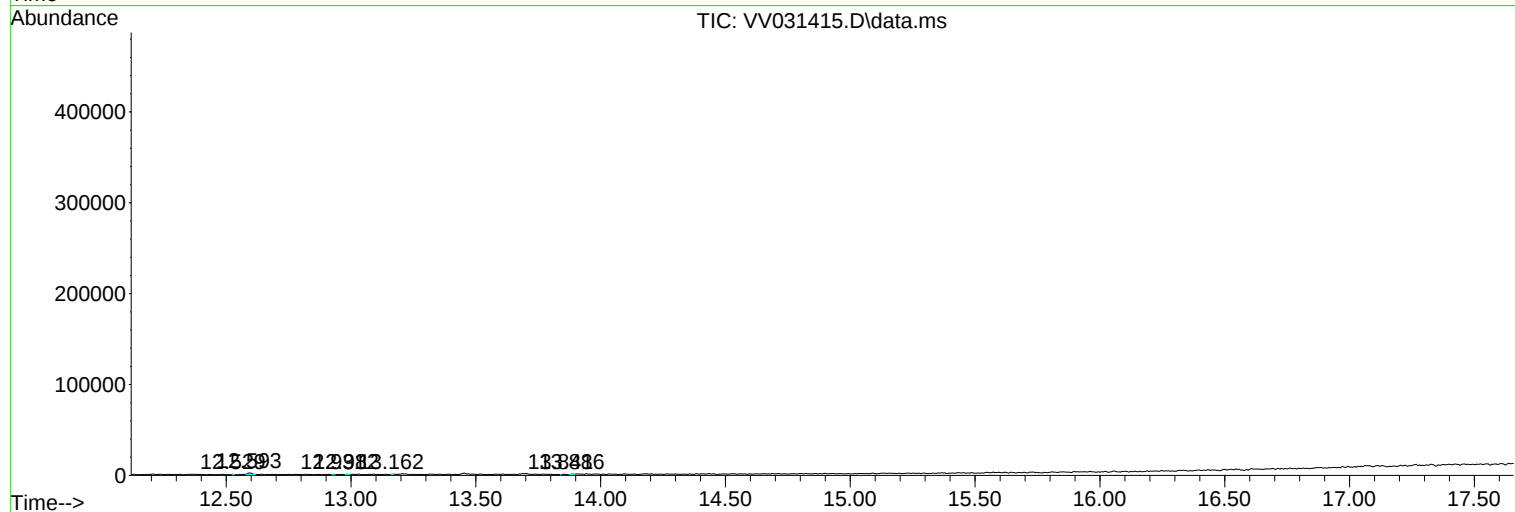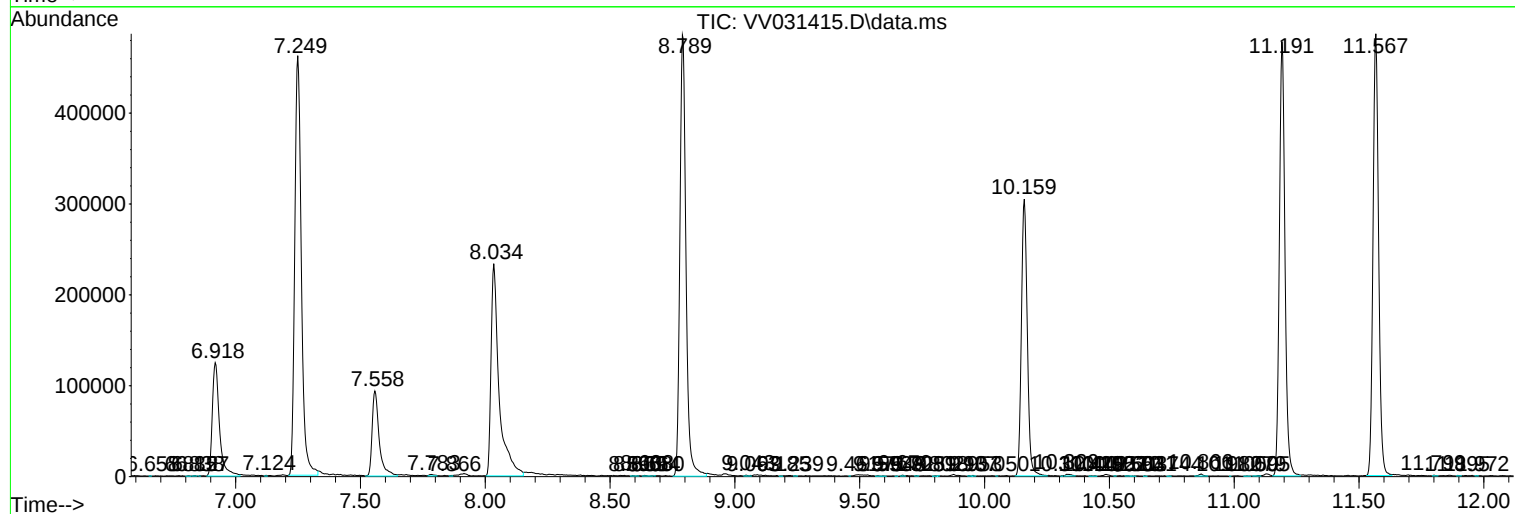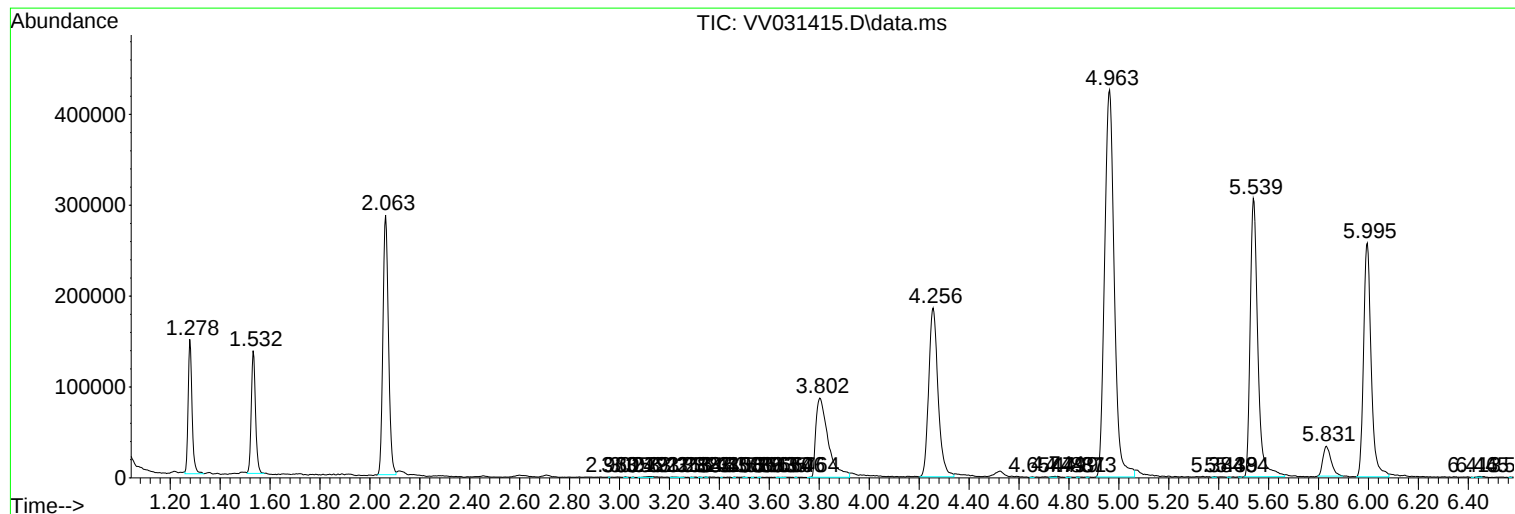

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031415.D
Acq On : 07 Jun 2023 22:20
Operator : SY/MD
Sample : 03076-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031415.D
Acq On : 07 Jun 2023 22:20
Operator : SY/MD
Sample : 03076-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------