

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031418.D
 Acq On : 07 Jun 2023 23:31
 Operator : SY/MD
 Sample : 03076-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031418.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	148862	158292	13.62%	1.858%
2	1.532	146	153	165	rVB	132072	154490	13.30%	1.813%
3	2.063	308	318	331	rBV	266005	392376	33.77%	4.605%
4	2.690	510	513	515	rBV2	637	356	0.03%	0.004%
5	2.796	543	546	548	rVB2	440	223	0.02%	0.003%
6	2.838	554	559	561	rBV3	480	392	0.03%	0.005%
7	3.002	604	610	614	rBV3	609	679	0.06%	0.008%
8	3.031	616	619	623	rVB	857	672	0.06%	0.008%
9	3.188	666	668	671	rVB2	453	271	0.02%	0.003%
10	3.220	674	678	682	rBV3	625	514	0.04%	0.006%
11	3.259	686	690	691	rBV	420	252	0.02%	0.003%
12	3.294	699	701	706	rBV	527	379	0.03%	0.004%
13	3.355	715	720	724	rBV3	689	622	0.05%	0.007%
14	3.416	736	739	741	rBV	347	208	0.02%	0.002%
15	3.474	755	757	759	rVV2	513	253	0.02%	0.003%
16	3.500	759	765	767	rVV4	446	437	0.04%	0.005%
17	3.516	767	770	772	rVV	494	331	0.03%	0.004%
18	3.613	797	800	803	rVB2	495	224	0.02%	0.003%
19	3.661	811	815	823	rBV4	278	382	0.03%	0.004%
20	3.699	823	827	828	rBV2	421	271	0.02%	0.003%
21	3.735	835	838	843	rBV2	533	323	0.03%	0.004%
22	3.796	847	857	885	rBV	82077	238651	20.54%	2.801%
23	4.256	983	1000	1024	rBV2	187716	481700	41.46%	5.653%
24	4.619	1111	1113	1116	rBV3	391	202	0.02%	0.002%
25	4.686	1130	1134	1138	rBV2	716	728	0.06%	0.009%
26	4.751	1152	1154	1159	rVB3	557	321	0.03%	0.004%
27	4.883	1193	1195	1199	rVB3	360	237	0.02%	0.003%
28	4.963	1199	1220	1248	rBV2	431504	1161915	100.00%	13.637%
29	5.297	1322	1324	1329	rBV3	645	636	0.05%	0.007%
30	5.320	1329	1331	1333	rBV	616	315	0.03%	0.004%
31	5.432	1363	1366	1368	rBV2	626	517	0.04%	0.006%
32	5.539	1387	1399	1423	rBV	301923	642137	55.27%	7.536%
33	5.831	1477	1490	1508	rBV5	32457	72200	6.21%	0.847%
34	5.995	1527	1541	1561	rBV	261829	550348	47.37%	6.459%
35	6.281	1627	1630	1631	rBV2	805	380	0.03%	0.004%
36	6.307	1637	1638	1640	rBV	635	203	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031418.D
 Acq On : 07 Jun 2023 23:31
 Operator : SY/MD
 Sample : 03076-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.416	1667	1672	1673	rBV2	643	396	0.03%	0.005%
38	6.442	1676	1680	1682	rBV4	378	309	0.03%	0.004%
39	6.506	1696	1700	1705	rVB2	644	505	0.04%	0.006%
40	6.587	1722	1725	1728	rVB3	617	369	0.03%	0.004%
41	6.612	1728	1733	1735	rBV3	591	591	0.05%	0.007%
42	6.786	1783	1787	1789	rBV2	443	353	0.03%	0.004%
43	6.837	1800	1803	1804	rBV2	408	229	0.02%	0.003%
44	6.918	1816	1828	1850	rBV	127335	244246	21.02%	2.867%
45	7.091	1879	1882	1887	rVB3	739	483	0.04%	0.006%
46	7.143	1896	1898	1901	rVB3	611	291	0.03%	0.003%
47	7.249	1919	1931	1961	rBV	468313	842374	72.50%	9.887%
48	7.558	2017	2027	2054	rBV	95316	179882	15.48%	2.111%
49	7.950	2147	2149	2151	rBV3	509	238	0.02%	0.003%
50	8.034	2164	2175	2218	rBV2	242361	541850	46.63%	6.359%
51	8.477	2310	2313	2314	rBV2	1034	618	0.05%	0.007%
52	8.558	2336	2338	2341	rBV	370	238	0.02%	0.003%
53	8.651	2362	2367	2369	rBV3	688	591	0.05%	0.007%
54	8.673	2372	2374	2377	rVB4	609	332	0.03%	0.004%
55	8.735	2389	2393	2395	rBV3	696	547	0.05%	0.006%
56	8.789	2399	2410	2433	rBV	480116	813543	70.02%	9.548%
57	9.114	2509	2511	2512	rBV2	635	231	0.02%	0.003%
58	9.201	2536	2538	2540	rBV	604	249	0.02%	0.003%
59	9.268	2555	2559	2562	rBV2	371	207	0.02%	0.002%
60	9.426	2605	2608	2610	rBV4	427	279	0.02%	0.003%
61	9.477	2622	2624	2627	rBV3	399	311	0.03%	0.004%
62	9.532	2639	2641	2646	rVB2	388	280	0.02%	0.003%
63	9.577	2651	2655	2658	rVB4	474	363	0.03%	0.004%
64	9.596	2658	2661	2665	rBV3	298	208	0.02%	0.002%
65	9.625	2667	2670	2672	rBV2	303	233	0.02%	0.003%
66	9.670	2681	2684	2687	rVB	338	214	0.02%	0.003%
67	9.812	2725	2728	2731	rBV3	431	306	0.03%	0.004%
68	9.825	2731	2732	2737	rVB	559	237	0.02%	0.003%
69	9.866	2743	2745	2746	rBV	549	244	0.02%	0.003%
70	9.943	2765	2769	2770	rBV2	295	233	0.02%	0.003%
71	9.982	2780	2781	2786	rBV2	378	295	0.03%	0.003%
72	10.159	2822	2836	2857	rVV	309880	503732	43.35%	5.912%
73	10.336	2880	2891	2905	rBV4	2592	4714	0.41%	0.055%
74	10.406	2910	2913	2915	rBV	520	313	0.03%	0.004%
75	10.419	2915	2917	2920	rVB	597	271	0.02%	0.003%
76	10.445	2923	2925	2931	rBV3	298	268	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031418.D
 Acq On : 07 Jun 2023 23:31
 Operator : SY/MD
 Sample : 03076-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.525	2949	2950	2954	rVB2	397	272	0.02%	0.003%
78	10.574	2958	2965	2967	rBV3	402	446	0.04%	0.005%
79	10.638	2982	2985	2991	rBV4	476	491	0.04%	0.006%
80	10.712	3006	3008	3012	rBV2	316	229	0.02%	0.003%
81	10.763	3022	3024	3028	rBV	340	240	0.02%	0.003%
82	10.808	3035	3038	3041	rBV2	546	461	0.04%	0.005%
83	10.927	3070	3075	3076	rBV2	338	253	0.02%	0.003%
84	11.191	3145	3157	3180	rBV	466486	742977	63.94%	8.720%
85	11.374	3212	3214	3216	rVB2	574	206	0.02%	0.002%
86	11.567	3260	3274	3292	rBV	482514	766026	65.93%	8.990%
87	11.738	3325	3327	3329	rBV2	659	349	0.03%	0.004%
88	11.895	3374	3376	3385	rVB4	538	560	0.05%	0.007%
89	11.950	3390	3393	3394	rBV2	529	280	0.02%	0.003%
90	12.008	3408	3411	3412	rBV3	644	290	0.02%	0.003%
91	12.088	3435	3436	3440	rBV3	321	265	0.02%	0.003%
92	12.535	3573	3575	3578	rBV2	361	257	0.02%	0.003%
93	12.644	3607	3609	3611	rBV2	474	234	0.02%	0.003%
94	12.657	3611	3613	3616	rVV	373	255	0.02%	0.003%
95	12.773	3646	3649	3651	rBV2	356	209	0.02%	0.002%
96	13.371	3834	3835	3838	rBV2	360	207	0.02%	0.002%
97	13.522	3877	3882	3884	rBV3	732	660	0.06%	0.008%
98	13.609	3907	3909	3913	rBV3	505	356	0.03%	0.004%
99	14.111	4063	4065	4068	rBV3	817	520	0.04%	0.006%
100	14.226	4099	4101	4106	rBV4	938	763	0.07%	0.009%




Sum of corrected areas: 8520416

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031418.D
Acq On : 07 Jun 2023 23:31
Operator : SY/MD
Sample : 03076-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

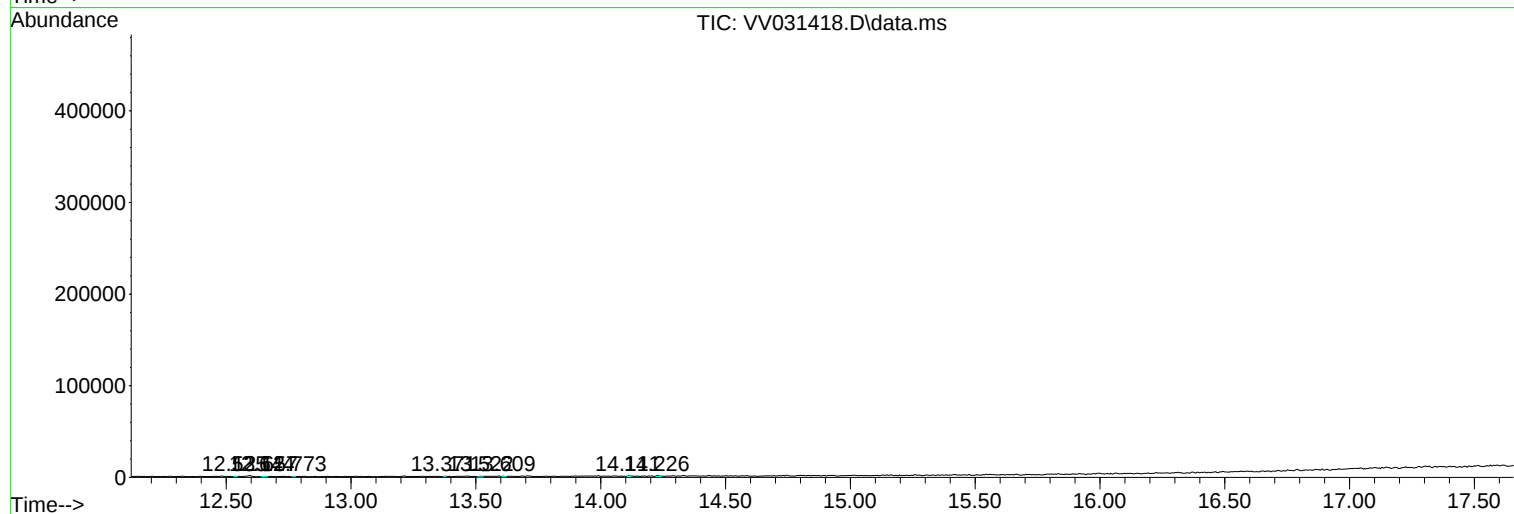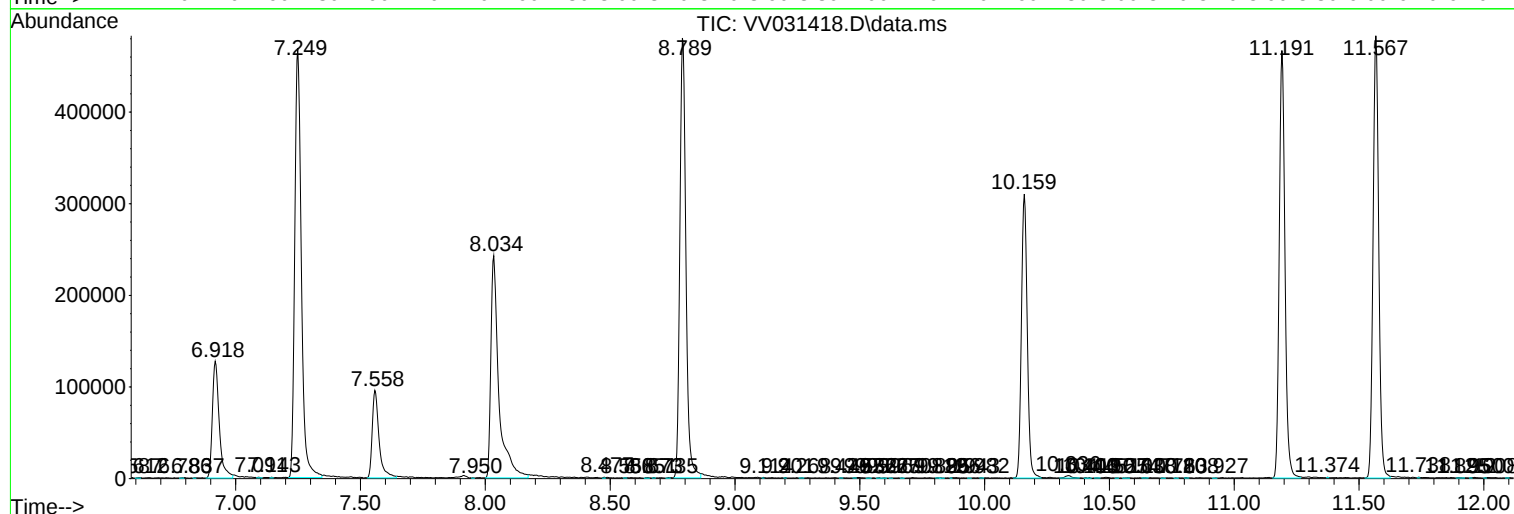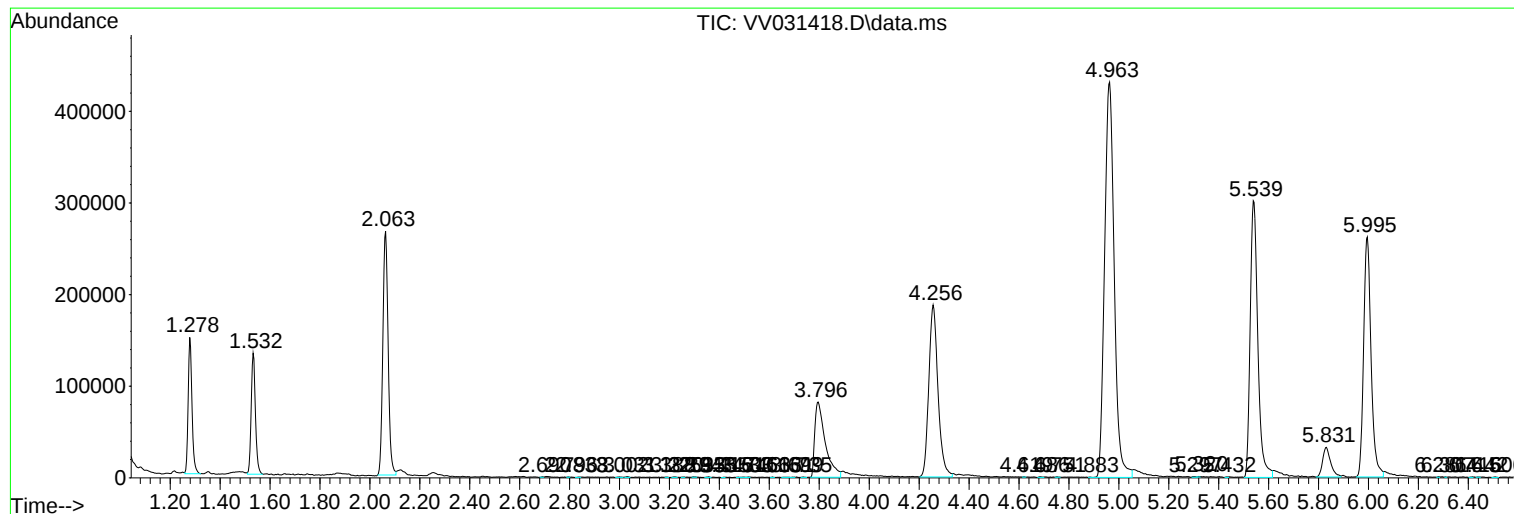

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031418.D
Acq On : 07 Jun 2023 23:31
Operator : SY/MD
Sample : 03076-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031418.D
Acq On : 07 Jun 2023 23:31
Operator : SY/MD
Sample : 03076-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
