

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031419.D
 Acq On : 07 Jun 2023 23:55
 Operator : SY/MD
 Sample : 03076-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	139095	148061	13.46%	1.814%
2	1.532	146	153	164	rVB	123730	141949	12.91%	1.739%
3	2.063	308	318	330	rBV	253271	374930	34.09%	4.592%
4	2.336	401	403	405	rBV2	536	219	0.02%	0.003%
5	2.683	509	511	512	rBV2	515	255	0.02%	0.003%
6	2.806	547	549	552	rBV2	403	182	0.02%	0.002%
7	2.873	568	570	573	rBV2	305	191	0.02%	0.002%
8	2.960	595	597	599	rBV2	421	161	0.01%	0.002%
9	3.021	614	616	618	rVV3	439	164	0.01%	0.002%
10	3.137	649	652	653	rBV2	332	182	0.02%	0.002%
11	3.198	668	671	676	rVB4	640	466	0.04%	0.006%
12	3.230	676	681	683	rBV	414	342	0.03%	0.004%
13	3.243	683	685	688	rBV2	525	229	0.02%	0.003%
14	3.336	711	714	717	rBV	371	286	0.03%	0.004%
15	3.416	732	739	740	rBV3	505	440	0.04%	0.005%
16	3.519	769	771	773	rBV2	328	193	0.02%	0.002%
17	3.552	777	781	785	rBV3	514	374	0.03%	0.005%
18	3.674	815	819	823	rVB3	357	253	0.02%	0.003%
19	3.732	833	837	839	rBV2	389	274	0.02%	0.003%
20	3.793	845	856	892	rBV	80653	240214	21.84%	2.942%
21	4.256	986	1000	1023	rBV	176075	453756	41.26%	5.558%
22	4.629	1114	1116	1118	rVB	552	225	0.02%	0.003%
23	4.651	1120	1123	1129	rVB5	533	382	0.03%	0.005%
24	4.696	1135	1137	1142	rVB4	707	397	0.04%	0.005%
25	4.796	1166	1168	1169	rBV	368	171	0.02%	0.002%
26	4.834	1178	1180	1183	rBV2	346	174	0.02%	0.002%
27	4.963	1202	1220	1243	rBV2	413748	1099674	100.00%	13.470%
28	5.268	1313	1315	1318	rBV3	649	444	0.04%	0.005%
29	5.442	1368	1369	1371	rVB	428	154	0.01%	0.002%
30	5.458	1371	1374	1377	rBV2	305	203	0.02%	0.002%
31	5.477	1377	1380	1385	rVB3	483	455	0.04%	0.006%
32	5.539	1385	1399	1419	rBV	291265	611401	55.60%	7.489%
33	5.828	1478	1489	1519	rVB2	28667	64786	5.89%	0.794%
34	5.995	1523	1541	1571	rBV	250497	538114	48.93%	6.591%
35	6.259	1622	1623	1626	rBV2	378	208	0.02%	0.003%
36	6.330	1640	1645	1646	rBV2	437	307	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031419.D
 Acq On : 07 Jun 2023 23:55
 Operator : SY/MD
 Sample : 03076-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.384	1660	1662	1665	rVB	474	174	0.02%	0.002%
38	6.429	1672	1676	1679	rBV2	636	573	0.05%	0.007%
39	6.471	1687	1689	1693	rVB2	482	203	0.02%	0.002%
40	6.545	1711	1712	1716	rVV2	342	184	0.02%	0.002%
41	6.571	1716	1720	1722	rVV3	414	316	0.03%	0.004%
42	6.587	1722	1725	1726	rBV2	414	252	0.02%	0.003%
43	6.596	1726	1728	1732	rVV4	538	280	0.03%	0.003%
44	6.629	1734	1738	1740	rBV2	526	322	0.03%	0.004%
45	6.725	1765	1768	1773	rBV4	481	499	0.05%	0.006%
46	6.789	1785	1788	1791	rBV3	389	207	0.02%	0.003%
47	6.825	1796	1799	1804	rVB3	377	291	0.03%	0.004%
48	6.854	1806	1808	1811	rBV	453	234	0.02%	0.003%
49	6.918	1817	1828	1855	rBV2	119108	232531	21.15%	2.848%
50	7.140	1895	1897	1900	rBV3	405	276	0.03%	0.003%
51	7.249	1919	1931	1955	rBV	448848	800112	72.76%	9.800%
52	7.558	2016	2027	2056	rBV3	89467	171843	15.63%	2.105%
53	7.789	2097	2099	2104	rVB5	1013	908	0.08%	0.011%
54	7.841	2112	2115	2117	rBV2	347	263	0.02%	0.003%
55	7.969	2153	2155	2157	rBV2	316	167	0.02%	0.002%
56	8.034	2164	2175	2212	rBV2	236676	521032	47.38%	6.382%
57	8.616	2353	2356	2358	rVV2	595	332	0.03%	0.004%
58	8.648	2362	2366	2369	rBV4	465	303	0.03%	0.004%
59	8.702	2382	2383	2388	rVB	619	258	0.02%	0.003%
60	8.735	2390	2393	2394	rBV3	461	218	0.02%	0.003%
61	8.744	2394	2396	2398	rBV2	370	165	0.02%	0.002%
62	8.789	2399	2410	2436	rBV	465177	779195	70.86%	9.544%
63	9.130	2514	2516	2520	rBV3	398	307	0.03%	0.004%
64	9.339	2576	2581	2584	rBV3	524	485	0.04%	0.006%
65	9.432	2608	2610	2614	rBV	390	277	0.03%	0.003%
66	9.461	2616	2619	2623	rVV3	423	314	0.03%	0.004%
67	9.506	2631	2633	2635	rBV	495	227	0.02%	0.003%
68	9.590	2657	2659	2665	rVV3	416	363	0.03%	0.004%
69	9.616	2665	2667	2671	rVB2	403	301	0.03%	0.004%
70	9.699	2688	2693	2694	rBV2	594	487	0.04%	0.006%
71	9.767	2710	2714	2717	rBV2	603	428	0.04%	0.005%
72	9.879	2746	2749	2752	rBV	686	427	0.04%	0.005%
73	9.979	2778	2780	2782	rVB	435	168	0.02%	0.002%
74	10.053	2800	2803	2805	rBV	354	212	0.02%	0.003%
75	10.088	2813	2814	2816	rBV2	390	154	0.01%	0.002%
76	10.159	2820	2836	2860	rBV	299654	486666	44.26%	5.961%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031419.D
 Acq On : 07 Jun 2023 23:55
 Operator : SY/MD
 Sample : 03076-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0F97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.294	2876	2878	2882	rBV2	526	346	0.03%	0.004%
78	10.445	2921	2925	2929	rBV4	238	233	0.02%	0.003%
79	10.509	2943	2945	2948	rBV2	485	250	0.02%	0.003%
80	10.590	2968	2970	2975	rBV2	411	291	0.03%	0.004%
81	10.773	3024	3027	3029	rVB2	388	253	0.02%	0.003%
82	10.963	3080	3086	3089	rBV3	719	602	0.05%	0.007%
83	10.979	3089	3091	3094	rBV2	662	388	0.04%	0.005%
84	10.998	3094	3097	3098	rBV	358	156	0.01%	0.002%
85	11.027	3104	3106	3109	rBV2	458	280	0.03%	0.003%
86	11.191	3146	3157	3177	rBV	466345	725017	65.93%	8.881%
87	11.477	3244	3246	3247	rBV	490	169	0.02%	0.002%
88	11.567	3262	3274	3296	rBV	473675	750096	68.21%	9.188%
89	11.702	3314	3316	3321	rVB4	770	408	0.04%	0.005%
90	12.040	3418	3421	3424	rBV2	325	248	0.02%	0.003%
91	12.136	3449	3451	3455	rVB3	298	185	0.02%	0.002%
92	12.223	3476	3478	3479	rBV3	350	167	0.02%	0.002%
93	12.451	3545	3549	3550	rBV3	624	356	0.03%	0.004%
94	12.461	3550	3552	3556	rVB2	477	276	0.03%	0.003%
95	12.677	3615	3619	3620	rBV2	455	356	0.03%	0.004%
96	12.741	3637	3639	3644	rBV4	408	384	0.03%	0.005%
97	13.056	3735	3737	3741	rBV3	462	344	0.03%	0.004%
98	13.297	3808	3812	3813	rBV2	569	330	0.03%	0.004%
99	13.966	4017	4020	4021	rBV2	860	393	0.04%	0.005%
100	14.191	4088	4090	4094	rBV2	520	357	0.03%	0.004%




Sum of corrected areas: 8164055

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031419.D
Acq On : 07 Jun 2023 23:55
Operator : SY/MD
Sample : 03076-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

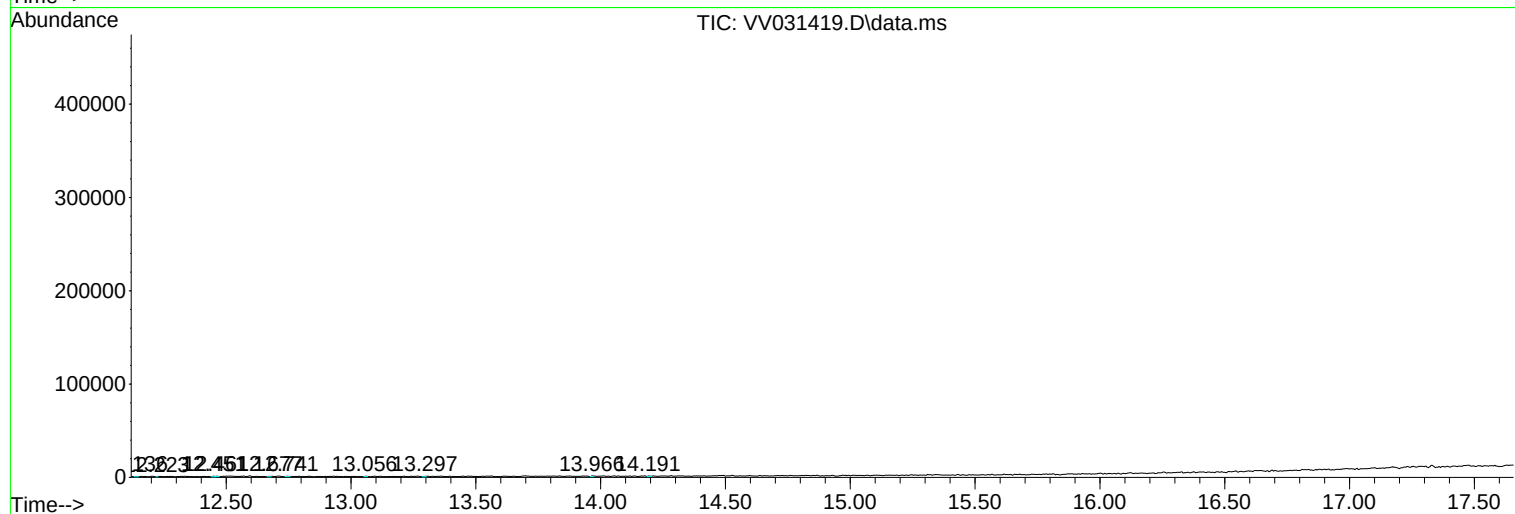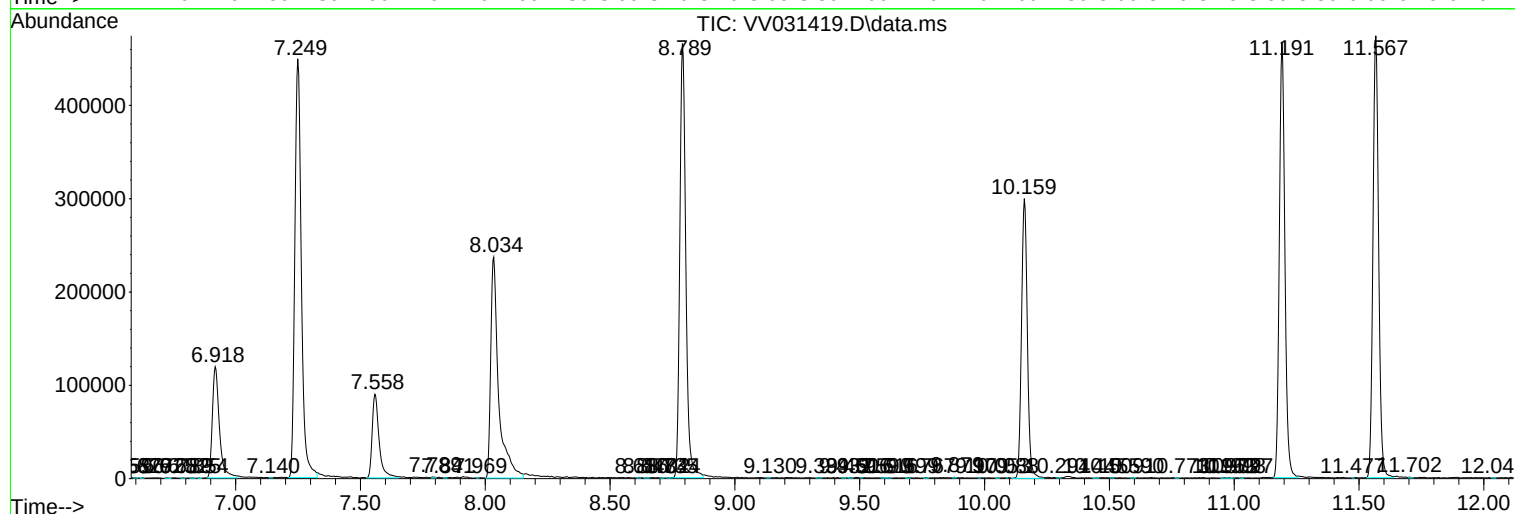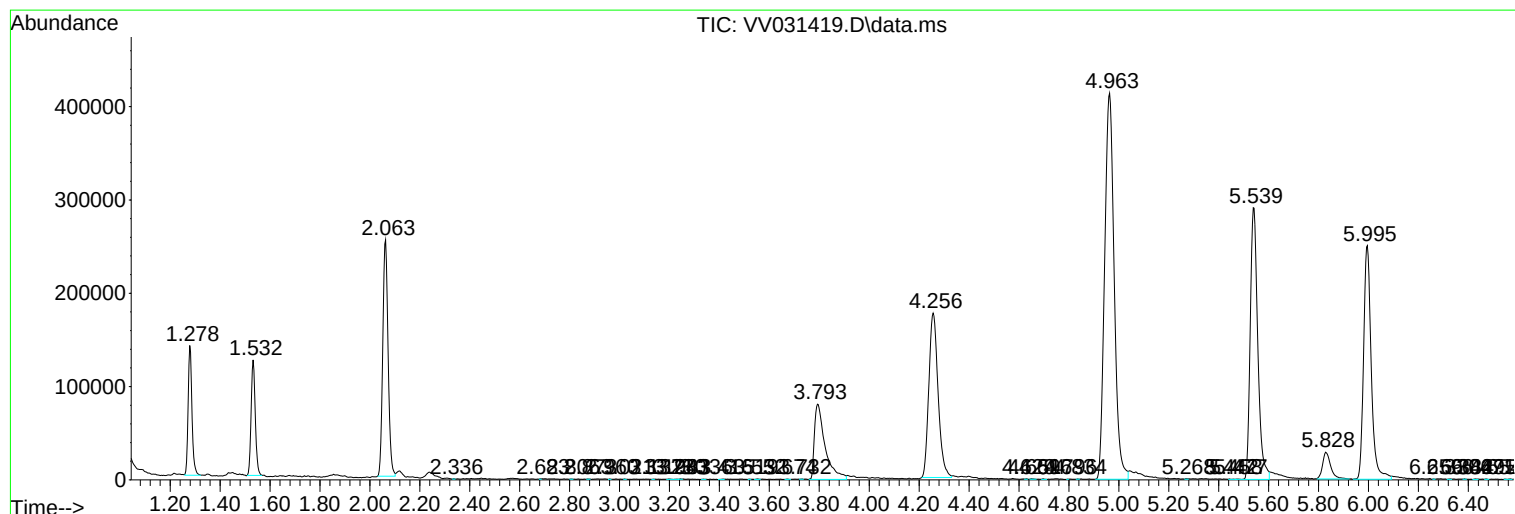

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031419.D
Acq On : 07 Jun 2023 23:55
Operator : SY/MD
Sample : 03076-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031419.D
Acq On : 07 Jun 2023 23:55
Operator : SY/MD
Sample : 03076-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0F97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------