

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031422.D
 Acq On : 08 Jun 2023 01:06
 Operator : SY/MD
 Sample : 03076-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	134166	142227	13.40%	1.814%
2	1.532	146	153	165	rVB	119262	140847	13.27%	1.797%
3	2.063	307	318	330	rBV	238044	351576	33.13%	4.485%
4	2.423	426	430	432	rBV2	616	488	0.05%	0.006%
5	2.555	469	471	473	rVB2	529	266	0.03%	0.003%
6	2.638	492	497	501	rVB2	475	420	0.04%	0.005%
7	2.658	501	503	505	rBV	610	291	0.03%	0.004%
8	2.674	505	508	510	rVV2	511	275	0.03%	0.004%
9	2.786	541	543	545	rBV	448	245	0.02%	0.003%
10	2.979	600	603	606	rBV3	359	263	0.02%	0.003%
11	3.005	608	611	614	rVB2	374	224	0.02%	0.003%
12	3.191	663	669	671	rBV	540	506	0.05%	0.006%
13	3.256	684	689	691	rBV4	348	378	0.04%	0.005%
14	3.294	697	701	703	rBV2	433	285	0.03%	0.004%
15	3.365	721	723	726	rBV	360	250	0.02%	0.003%
16	3.449	746	749	754	rVB3	513	478	0.05%	0.006%
17	3.613	795	800	802	rBV3	508	375	0.04%	0.005%
18	3.693	822	825	827	rBV2	435	282	0.03%	0.004%
19	3.744	838	841	843	rBV	323	202	0.02%	0.003%
20	3.796	847	857	887	rBV	79056	227947	21.48%	2.908%
21	4.256	985	1000	1027	rBV	171613	445908	42.02%	5.688%
22	4.510	1077	1079	1082	rBV2	489	302	0.03%	0.004%
23	4.526	1082	1084	1086	rVV3	564	221	0.02%	0.003%
24	4.616	1109	1112	1114	rBV	685	366	0.03%	0.005%
25	4.802	1166	1170	1173	rBV3	449	377	0.04%	0.005%
26	4.821	1175	1176	1181	rVV2	235	179	0.02%	0.002%
27	4.963	1202	1220	1244	rBV2	394558	1061120	100.00%	13.536%
28	5.352	1339	1341	1346	rVB3	526	309	0.03%	0.004%
29	5.477	1375	1380	1381	rBV2	373	295	0.03%	0.004%
30	5.542	1387	1400	1421	rBV	279365	591182	55.71%	7.542%
31	5.831	1478	1490	1509	rBV5	34802	83439	7.86%	1.064%
32	5.924	1517	1519	1522	rVB2	742	366	0.03%	0.005%
33	5.944	1522	1525	1527	rBV2	481	219	0.02%	0.003%
34	5.995	1527	1541	1559	rBV	249030	511216	48.18%	6.521%
35	6.227	1609	1613	1618	rBV3	602	604	0.06%	0.008%
36	6.272	1623	1627	1631	rBV4	502	532	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031422.D
 Acq On : 08 Jun 2023 01:06
 Operator : SY/MD
 Sample : 03076-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.362	1653	1655	1658	rBV2	579	290	0.03%	0.004%
38	6.381	1658	1661	1664	rVB2	462	306	0.03%	0.004%
39	6.419	1670	1673	1678	rBV	424	344	0.03%	0.004%
40	6.445	1678	1681	1686	rBV3	578	371	0.03%	0.005%
41	6.497	1694	1697	1698	rBV2	357	182	0.02%	0.002%
42	6.535	1707	1709	1712	rVB2	391	175	0.02%	0.002%
43	6.555	1712	1715	1719	rBV4	381	231	0.02%	0.003%
44	6.625	1736	1737	1740	rBV	433	197	0.02%	0.003%
45	6.673	1748	1752	1755	rVB4	377	244	0.02%	0.003%
46	6.744	1767	1774	1775	rBV2	290	262	0.02%	0.003%
47	6.796	1785	1790	1792	rBV4	500	409	0.04%	0.005%
48	6.837	1801	1803	1807	rVB2	367	262	0.02%	0.003%
49	6.918	1817	1828	1854	rBV2	115667	224705	21.18%	2.867%
50	7.172	1905	1907	1910	rBV2	426	310	0.03%	0.004%
51	7.249	1919	1931	1961	rBV	420885	755616	71.21%	9.639%
52	7.490	2005	2006	2009	rBV3	418	254	0.02%	0.003%
53	7.558	2018	2027	2050	rBV	89364	162549	15.32%	2.074%
54	7.725	2076	2079	2081	rBV2	732	451	0.04%	0.006%
55	7.815	2105	2107	2111	rVB2	498	266	0.03%	0.003%
56	7.944	2144	2147	2150	rVB3	665	389	0.04%	0.005%
57	7.963	2150	2153	2155	rBV2	461	297	0.03%	0.004%
58	8.034	2164	2175	2213	rBV2	224908	509867	48.05%	6.504%
59	8.278	2248	2251	2256	rBV5	958	1025	0.10%	0.013%
60	8.426	2295	2297	2298	rBV	597	272	0.03%	0.003%
61	8.596	2348	2350	2353	rVB4	594	330	0.03%	0.004%
62	8.648	2363	2366	2368	rBV4	522	336	0.03%	0.004%
63	8.789	2399	2410	2432	rBV	453321	750630	70.74%	9.576%
64	9.027	2482	2484	2486	rBV2	517	300	0.03%	0.004%
65	9.082	2495	2501	2503	rBV3	970	917	0.09%	0.012%
66	9.275	2558	2561	2562	rBV	351	178	0.02%	0.002%
67	9.288	2562	2565	2569	rBV3	466	261	0.02%	0.003%
68	9.548	2643	2646	2650	rBV	410	268	0.03%	0.003%
69	9.696	2688	2692	2693	rBV2	617	332	0.03%	0.004%
70	9.747	2705	2708	2713	rBV3	683	583	0.05%	0.007%
71	9.776	2713	2717	2720	rVV3	523	406	0.04%	0.005%
72	9.873	2744	2747	2748	rBV3	466	295	0.03%	0.004%
73	9.924	2757	2763	2768	rBV3	467	632	0.06%	0.008%
74	10.024	2790	2794	2798	rBV2	365	323	0.03%	0.004%
75	10.159	2824	2836	2852	rBV	289384	461843	43.52%	5.892%
76	10.332	2884	2890	2899	rVB6	2131	3218	0.30%	0.041%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031422.D
 Acq On : 08 Jun 2023 01:06
 Operator : SY/MD
 Sample : 03076-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.371	2899	2902	2905	rBB2	291	181	0.02%	0.002%
78	10.384	2905	2906	2909	rBV2	336	179	0.02%	0.002%
79	10.468	2928	2932	2935	rBV3	513	471	0.04%	0.006%
80	10.580	2962	2967	2970	rBV3	601	549	0.05%	0.007%
81	10.657	2985	2991	2994	rBV3	636	498	0.05%	0.006%
82	10.705	3003	3006	3007	rBV2	362	211	0.02%	0.003%
83	10.734	3012	3015	3018	rBV3	461	449	0.04%	0.006%
84	10.837	3044	3047	3050	rBV2	373	270	0.03%	0.003%
85	10.869	3054	3057	3061	rVV2	471	343	0.03%	0.004%
86	11.030	3104	3107	3109	rBV3	544	345	0.03%	0.004%
87	11.111	3129	3132	3134	rBV2	302	197	0.02%	0.003%
88	11.191	3146	3157	3180	rBV	438876	687838	64.82%	8.775%
89	11.358	3208	3209	3212	rVB3	588	259	0.02%	0.003%
90	11.506	3251	3255	3259	rBV2	542	569	0.05%	0.007%
91	11.567	3262	3274	3292	rBV	438891	697907	65.77%	8.903%
92	11.789	3341	3343	3348	rVB3	798	551	0.05%	0.007%
93	11.924	3383	3385	3389	rVV3	453	400	0.04%	0.005%
94	12.094	3436	3438	3442	rBV2	405	267	0.03%	0.003%
95	12.127	3446	3448	3450	rBV2	469	251	0.02%	0.003%
96	12.641	3601	3608	3611	rBV3	649	808	0.08%	0.010%
97	13.223	3785	3789	3790	rBV3	701	440	0.04%	0.006%
98	13.252	3796	3798	3802	rBV2	450	327	0.03%	0.004%
99	13.400	3841	3844	3845	rBV	304	172	0.02%	0.002%
100	14.127	4065	4070	4074	rBV4	833	889	0.08%	0.011%

Sum of corrected areas: 7838957




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031422.D
Acq On : 08 Jun 2023 01:06
Operator : SY/MD
Sample : 03076-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

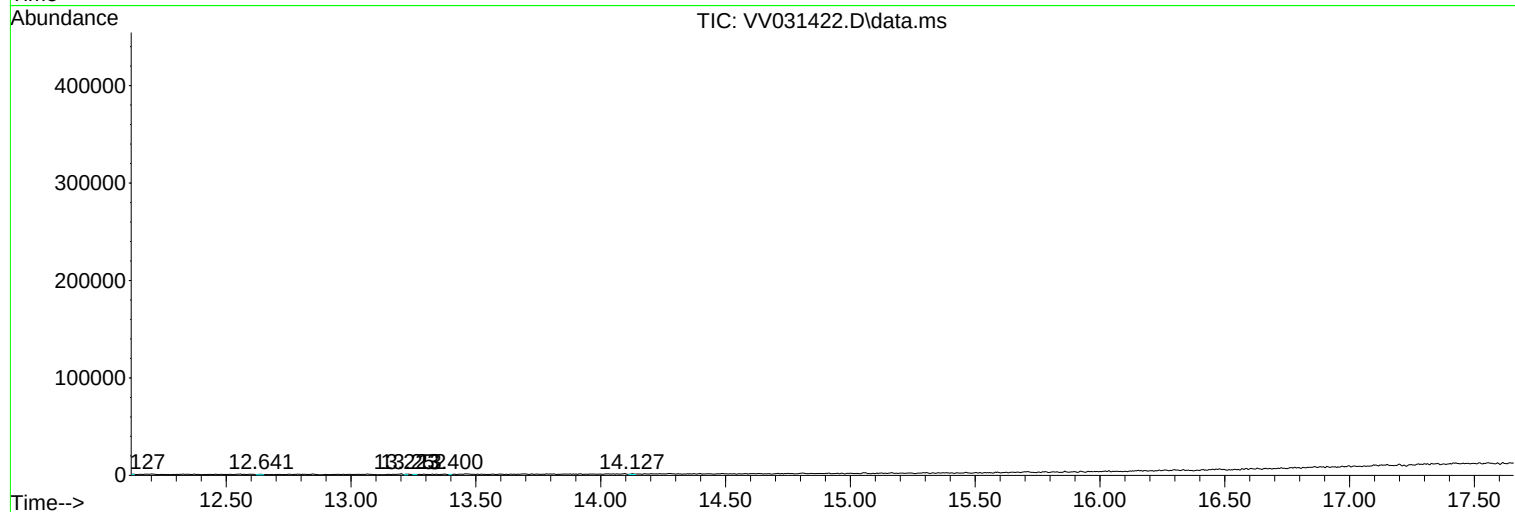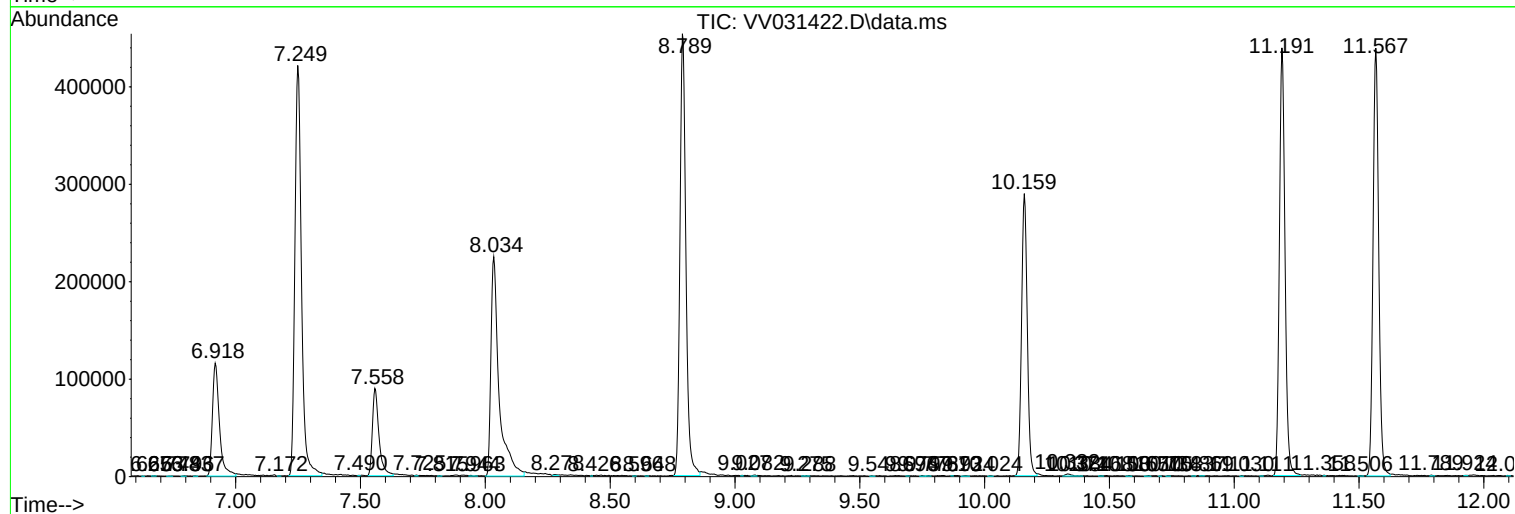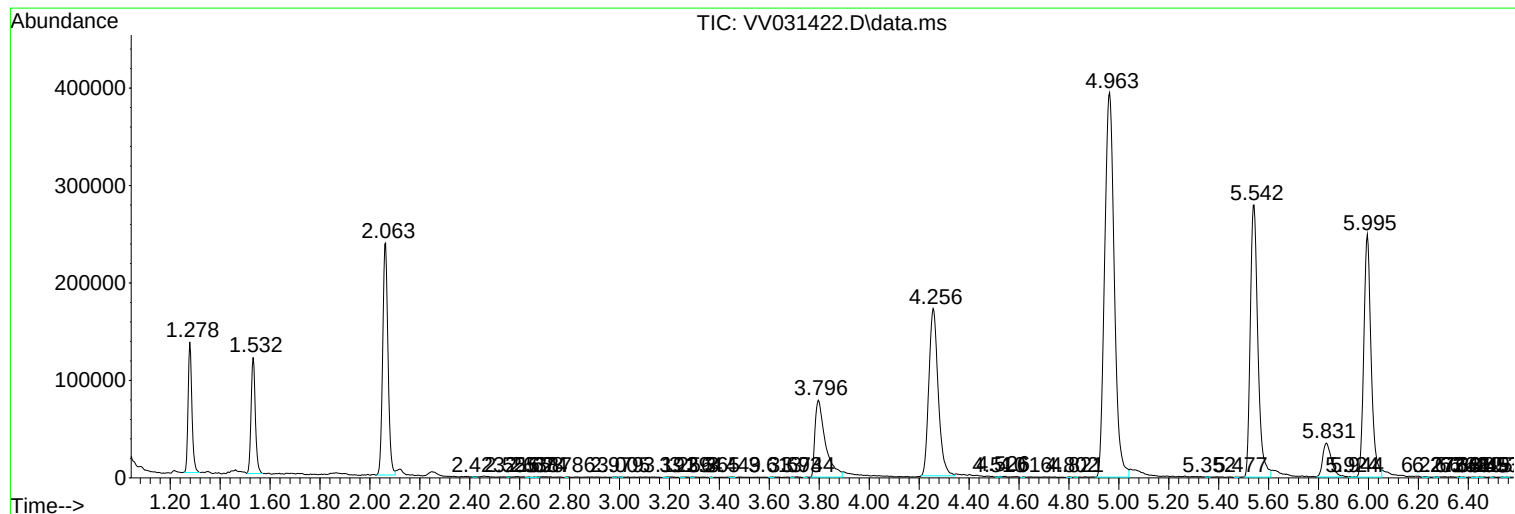

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031422.D
Acq On : 08 Jun 2023 01:06
Operator : SY/MD
Sample : 03076-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031422.D
Acq On : 08 Jun 2023 01:06
Operator : SY/MD
Sample : 03076-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------