

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031423.D
 Acq On : 08 Jun 2023 01:30
 Operator : SY/MD
 Sample : 03076-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031423.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	86	rVB	135016	143320	13.25%	1.761%
2	1.532	146	153	167	rVB	123065	143541	13.27%	1.763%
3	2.063	308	318	330	rBV	249417	368476	34.05%	4.527%
4	2.445	435	437	440	rBV4	1130	806	0.07%	0.010%
5	2.551	468	470	473	rBV	336	246	0.02%	0.003%
6	2.677	506	509	512	rBV2	412	251	0.02%	0.003%
7	2.696	512	515	516	rBV	525	252	0.02%	0.003%
8	2.712	516	520	524	rBV3	769	714	0.07%	0.009%
9	2.793	542	545	548	rBV3	411	234	0.02%	0.003%
10	2.937	588	590	594	rVB2	470	282	0.03%	0.003%
11	3.117	638	646	660	rBV4	3119	6314	0.58%	0.078%
12	3.188	666	668	670	rBV	421	253	0.02%	0.003%
13	3.220	674	678	681	rBV3	391	287	0.03%	0.004%
14	3.256	687	689	691	rBV2	317	207	0.02%	0.003%
15	3.307	703	705	709	rVV3	385	340	0.03%	0.004%
16	3.432	738	744	746	rBV2	396	232	0.02%	0.003%
17	3.490	760	762	765	rBV2	341	233	0.02%	0.003%
18	3.561	780	784	786	rBV2	425	260	0.02%	0.003%
19	3.638	804	808	811	rBV2	437	289	0.03%	0.004%
20	3.719	831	833	836	rBV2	389	213	0.02%	0.003%
21	3.735	836	838	844	rVB3	348	309	0.03%	0.004%
22	3.796	844	857	887	rBV2	82593	254698	23.54%	3.129%
23	4.256	983	1000	1026	rBV	176409	462065	42.70%	5.676%
24	4.593	1102	1105	1111	rBV3	964	941	0.09%	0.012%
25	4.654	1121	1124	1125	rBV2	384	219	0.02%	0.003%
26	4.731	1144	1148	1152	rBV4	456	392	0.04%	0.005%
27	4.748	1152	1153	1157	rVV3	523	363	0.03%	0.004%
28	4.770	1157	1160	1162	rVV2	510	329	0.03%	0.004%
29	4.799	1166	1169	1173	rVB3	618	371	0.03%	0.005%
30	4.883	1192	1195	1201	rVB3	487	372	0.03%	0.005%
31	4.963	1201	1220	1245	rBV2	408448	1082058	100.00%	13.293%
32	5.416	1359	1361	1363	rBV	602	302	0.03%	0.004%
33	5.448	1368	1371	1374	rBV3	388	298	0.03%	0.004%
34	5.474	1376	1379	1380	rBV2	364	212	0.02%	0.003%
35	5.542	1387	1400	1421	rBV	303827	628282	58.06%	7.718%
36	5.831	1478	1490	1510	rBV3	26394	59572	5.51%	0.732%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031423.D
 Acq On : 08 Jun 2023 01:30
 Operator : SY/MD
 Sample : 03076-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	5.944	1523	1525	1527	rBV2	656	422	0.04%	0.005%
38	5.995	1527	1541	1581	rVV	247067	529581	48.94%	6.506%
39	6.294	1630	1634	1635	rBV2	322	197	0.02%	0.002%
40	6.336	1644	1647	1649	rBV2	844	518	0.05%	0.006%
41	6.371	1655	1658	1660	rBV2	409	329	0.03%	0.004%
42	6.429	1674	1676	1680	rVB3	548	336	0.03%	0.004%
43	6.590	1724	1726	1729	rVB	399	237	0.02%	0.003%
44	6.625	1733	1737	1739	rBV2	653	456	0.04%	0.006%
45	6.661	1744	1748	1750	rBV	406	290	0.03%	0.004%
46	6.767	1774	1781	1783	rBV3	594	631	0.06%	0.008%
47	6.821	1797	1798	1801	rBV2	373	205	0.02%	0.003%
48	6.918	1818	1828	1853	rBV	117311	227987	21.07%	2.801%
49	7.143	1894	1898	1900	rBV2	822	653	0.06%	0.008%
50	7.249	1919	1931	1960	rBV	433915	779754	72.06%	9.579%
51	7.558	2017	2027	2051	rVV	87847	164638	15.22%	2.023%
52	7.818	2106	2108	2111	rBV	398	231	0.02%	0.003%
53	7.908	2133	2136	2138	rBV4	696	485	0.04%	0.006%
54	7.976	2154	2157	2161	rVB3	402	347	0.03%	0.004%
55	8.034	2165	2175	2210	rBV2	232828	509998	47.13%	6.265%
56	8.381	2280	2283	2286	rBV2	576	369	0.03%	0.005%
57	8.400	2286	2289	2290	rBV2	535	352	0.03%	0.004%
58	8.506	2319	2322	2324	rBV2	444	299	0.03%	0.004%
59	8.529	2327	2329	2332	rBV3	525	371	0.03%	0.005%
60	8.574	2339	2343	2346	rVB3	980	684	0.06%	0.008%
61	8.789	2396	2410	2433	rBV	483452	807276	74.61%	9.917%
62	9.159	2523	2525	2527	rVB	572	236	0.02%	0.003%
63	9.181	2527	2532	2533	rBV2	512	432	0.04%	0.005%
64	9.197	2534	2537	2538	rBV	493	222	0.02%	0.003%
65	9.252	2551	2554	2558	rVB2	488	316	0.03%	0.004%
66	9.336	2579	2580	2585	rBV3	353	289	0.03%	0.004%
67	9.484	2624	2626	2628	rBV3	489	280	0.03%	0.003%
68	9.529	2638	2640	2642	rVB2	728	228	0.02%	0.003%
69	9.609	2663	2665	2668	rBV2	696	380	0.04%	0.005%
70	9.632	2668	2672	2674	rVV2	432	217	0.02%	0.003%
71	9.660	2679	2681	2686	rVB4	697	567	0.05%	0.007%
72	9.837	2732	2736	2739	rBV3	510	455	0.04%	0.006%
73	9.860	2739	2743	2745	rBV3	426	300	0.03%	0.004%
74	9.921	2758	2762	2764	rBV2	307	265	0.02%	0.003%
75	9.966	2774	2776	2778	rBV	533	220	0.02%	0.003%
76	9.982	2778	2781	2787	rVB3	507	423	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031423.D
 Acq On : 08 Jun 2023 01:30
 Operator : SY/MD
 Sample : 03076-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.011	2787	2790	2791	rBV	450	265	0.02%	0.003%
78	10.037	2795	2798	2803	rVB5	688	578	0.05%	0.007%
79	10.159	2825	2836	2854	rVV	300397	475723	43.96%	5.844%
80	10.451	2923	2927	2932	rBV2	302	291	0.03%	0.004%
81	10.956	3082	3084	3092	rVB2	605	348	0.03%	0.004%
82	11.053	3108	3114	3118	rBV3	379	408	0.04%	0.005%
83	11.075	3118	3121	3125	rVB3	709	596	0.06%	0.007%
84	11.101	3125	3129	3133	rBV2	414	447	0.04%	0.005%
85	11.191	3146	3157	3179	rBV	469316	741769	68.55%	9.113%
86	11.484	3245	3248	3251	rBV2	522	448	0.04%	0.006%
87	11.567	3262	3274	3293	rBV	454194	724456	66.95%	8.900%
88	11.847	3358	3361	3365	rBV2	643	493	0.05%	0.006%
89	11.998	3406	3408	3412	rVB3	459	326	0.03%	0.004%
90	12.088	3433	3436	3438	rBV	544	445	0.04%	0.005%
91	12.278	3493	3495	3500	rBV2	358	267	0.02%	0.003%
92	13.017	3722	3725	3728	rBV3	657	397	0.04%	0.005%
93	13.033	3728	3730	3733	rVV2	369	203	0.02%	0.002%
94	13.101	3746	3751	3754	rBV4	655	636	0.06%	0.008%
95	13.844	3978	3982	3985	rBV3	617	490	0.05%	0.006%
96	13.914	4002	4004	4006	rBV2	747	375	0.03%	0.005%
97	14.056	4046	4048	4052	rBV2	640	367	0.03%	0.005%
98	14.094	4057	4060	4062	rBV	523	317	0.03%	0.004%
99	14.300	4118	4124	4128	rBV4	816	805	0.07%	0.010%
100	15.011	4342	4345	4346	rBV2	924	573	0.05%	0.007%




Sum of corrected areas: 8140032

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031423.D
Acq On : 08 Jun 2023 01:30
Operator : SY/MD
Sample : 03076-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

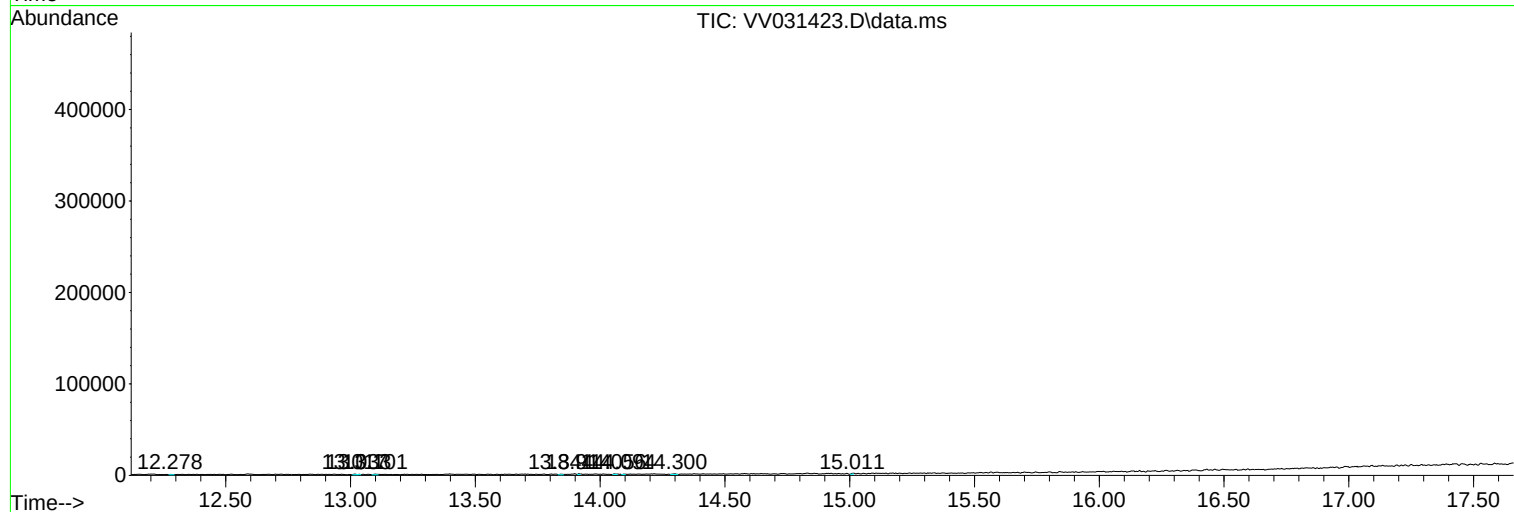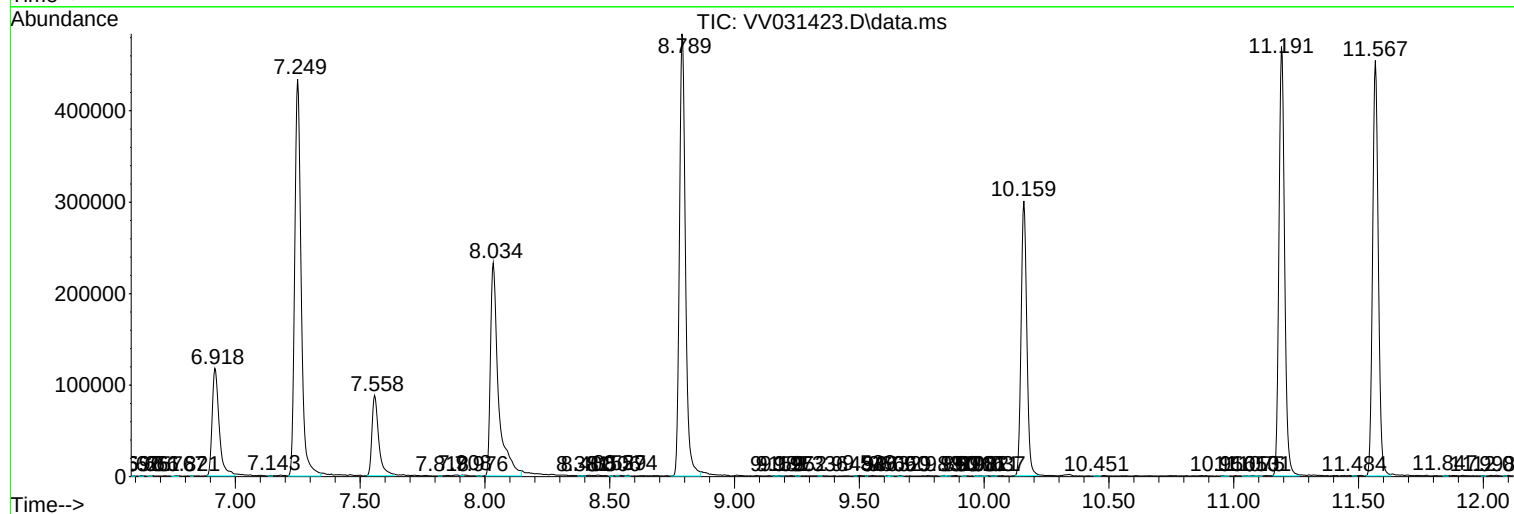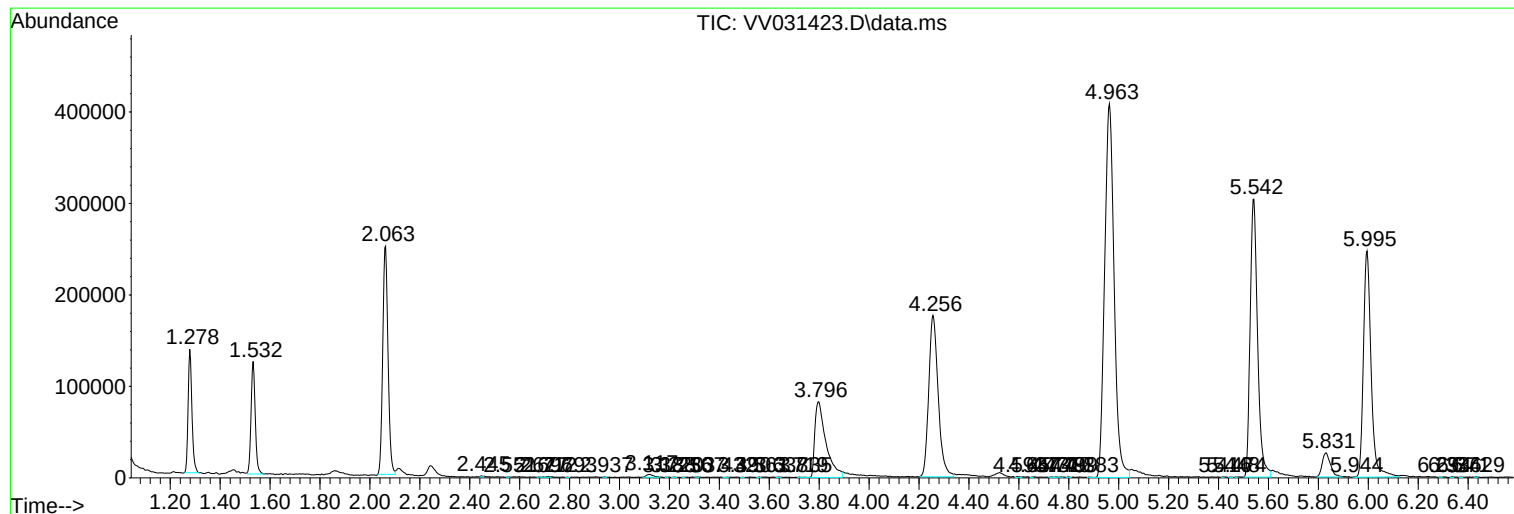

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031423.D
Acq On : 08 Jun 2023 01:30
Operator : SY/MD
Sample : 03076-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031423.D
Acq On : 08 Jun 2023 01:30
Operator : SY/MD
Sample : 03076-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------