

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031424.D
 Acq On : 08 Jun 2023 01:54
 Operator : SY/MD
 Sample : 03077-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	137370	147078	13.77%	1.713%
2	1.532	146	153	166	rVB	120511	142032	13.30%	1.655%
3	2.063	308	318	330	rBV	244583	360186	33.73%	4.196%
4	2.452	430	439	447	rBV10	1610	3111	0.29%	0.036%
5	2.500	452	454	458	rBV3	388	270	0.03%	0.003%
6	2.568	468	475	476	rBV2	779	817	0.08%	0.010%
7	2.699	510	516	531	rVB7	2779	5390	0.50%	0.063%
8	3.076	631	633	636	rVV3	312	177	0.02%	0.002%
9	3.114	642	645	649	rBV2	745	598	0.06%	0.007%
10	3.195	667	670	675	rVV3	331	272	0.03%	0.003%
11	3.375	723	726	727	rBV2	351	211	0.02%	0.002%
12	3.497	762	764	767	rVV	387	225	0.02%	0.003%
13	3.513	767	769	772	rVB	423	222	0.02%	0.003%
14	3.645	806	810	813	rBV2	539	461	0.04%	0.005%
15	3.667	815	817	821	rVB	478	315	0.03%	0.004%
16	3.722	831	834	837	rBV2	281	177	0.02%	0.002%
17	3.796	847	857	887	rBV	77503	250525	23.46%	2.918%
18	4.256	986	1000	1030	rBV	174265	446232	41.79%	5.198%
19	4.661	1122	1126	1127	rBV2	380	281	0.03%	0.003%
20	4.686	1132	1134	1136	rVV2	439	230	0.02%	0.003%
21	4.696	1136	1137	1139	rVV	602	238	0.02%	0.003%
22	4.728	1143	1147	1150	rBV2	382	308	0.03%	0.004%
23	4.963	1202	1220	1245	rBV2	399437	1067878	100.00%	12.440%
24	5.355	1338	1342	1345	rBV3	604	467	0.04%	0.005%
25	5.465	1374	1376	1379	rVB	498	200	0.02%	0.002%
26	5.539	1387	1399	1421	rBV	294300	626682	58.68%	7.300%
27	5.838	1479	1492	1527	rBV3	261312	554895	51.96%	6.464%
28	5.995	1529	1541	1561	rBV	247289	506941	47.47%	5.906%
29	6.336	1645	1647	1649	rBV3	627	293	0.03%	0.003%
30	6.471	1687	1689	1695	rVB3	675	609	0.06%	0.007%
31	6.503	1695	1699	1701	rVV3	334	270	0.03%	0.003%
32	6.529	1704	1707	1710	rBV2	572	373	0.03%	0.004%
33	6.551	1710	1714	1715	rVV2	328	202	0.02%	0.002%
34	6.561	1715	1717	1719	rVV	508	268	0.03%	0.003%
35	6.580	1721	1723	1726	rVV2	374	225	0.02%	0.003%
36	6.600	1726	1729	1731	rVV2	530	304	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031424.D
 Acq On : 08 Jun 2023 01:54
 Operator : SY/MD
 Sample : 03077-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.632	1735	1739	1745	rVB5	527	555	0.05%	0.006%
38	6.744	1771	1774	1776	rBV2	508	306	0.03%	0.004%
39	6.854	1805	1808	1810	rBV	682	313	0.03%	0.004%
40	6.918	1817	1828	1847	rBV	116542	227611	21.31%	2.652%
41	7.108	1881	1887	1892	rBV7	694	1159	0.11%	0.014%
42	7.178	1907	1909	1911	rBV2	368	185	0.02%	0.002%
43	7.207	1915	1918	1919	rBV2	619	335	0.03%	0.004%
44	7.249	1919	1931	1956	rBV	434411	775819	72.65%	9.038%
45	7.558	2017	2027	2053	rBV	89191	165076	15.46%	1.923%
46	7.760	2087	2090	2093	rBV4	557	417	0.04%	0.005%
47	7.818	2106	2108	2111	rVB2	483	197	0.02%	0.002%
48	7.841	2113	2115	2117	rBV3	407	252	0.02%	0.003%
49	8.034	2165	2175	2210	rBV2	229007	506078	47.39%	5.895%
50	8.500	2317	2320	2322	rBV3	635	478	0.04%	0.006%
51	8.561	2337	2339	2342	rBV2	933	371	0.03%	0.004%
52	8.590	2346	2348	2352	rVV4	436	314	0.03%	0.004%
53	8.622	2355	2358	2360	rBV	380	217	0.02%	0.003%
54	8.661	2368	2370	2375	rBV2	513	370	0.03%	0.004%
55	8.683	2375	2377	2380	rBV3	466	274	0.03%	0.003%
56	8.789	2399	2410	2443	rBV	466713	804954	75.38%	9.377%
57	8.960	2460	2463	2468	rVB6	1057	865	0.08%	0.010%
58	9.091	2502	2504	2506	rBV2	512	249	0.02%	0.003%
59	9.159	2522	2525	2529	rBV5	759	447	0.04%	0.005%
60	9.239	2548	2550	2553	rBV2	320	232	0.02%	0.003%
61	9.300	2566	2569	2571	rBV2	398	207	0.02%	0.002%
62	9.329	2576	2578	2580	rBV	359	212	0.02%	0.002%
63	9.403	2599	2601	2604	rBV2	438	234	0.02%	0.003%
64	9.577	2653	2655	2659	rVB3	427	187	0.02%	0.002%
65	9.603	2659	2663	2668	rVB3	711	648	0.06%	0.008%
66	9.638	2671	2674	2675	rBV	429	208	0.02%	0.002%
67	9.667	2680	2683	2684	rBV	510	293	0.03%	0.003%
68	9.734	2700	2704	2707	rBV	367	272	0.03%	0.003%
69	9.763	2707	2713	2717	rBV6	3580	4338	0.41%	0.051%
70	9.956	2770	2773	2776	rBV2	533	436	0.04%	0.005%
71	10.079	2807	2811	2814	rBV3	543	485	0.05%	0.006%
72	10.159	2824	2836	2858	rBV	298747	476964	44.66%	5.556%
73	10.336	2882	2891	2901	rVB3	3149	5278	0.49%	0.061%
74	10.416	2913	2916	2917	rVB2	450	188	0.02%	0.002%
75	10.435	2917	2922	2923	rBV2	286	250	0.02%	0.003%
76	10.686	2996	3000	3004	rVB2	344	240	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031424.D
 Acq On : 08 Jun 2023 01:54
 Operator : SY/MD
 Sample : 03077-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.751	3017	3020	3022	rBV2	410	255	0.02%	0.003%
78	10.902	3062	3067	3069	rBV3	882	821	0.08%	0.010%
79	10.969	3084	3088	3089	rBV2	674	463	0.04%	0.005%
80	11.107	3125	3131	3146	rVB2	3073	5382	0.50%	0.063%
81	11.191	3146	3157	3183	rBV	473297	740742	69.37%	8.629%
82	11.403	3221	3223	3228	rBV4	638	489	0.05%	0.006%
83	11.445	3231	3236	3237	rBV2	346	231	0.02%	0.003%
84	11.477	3244	3246	3250	rBV2	602	370	0.03%	0.004%
85	11.567	3262	3274	3293	rBV	460823	731918	68.54%	8.526%
86	11.921	3381	3384	3385	rBV3	614	360	0.03%	0.004%
87	12.114	3443	3444	3448	rBV2	413	233	0.02%	0.003%
88	12.130	3448	3449	3451	rBV2	280	149	0.01%	0.002%
89	12.329	3509	3511	3517	rBV4	728	797	0.07%	0.009%
90	12.461	3547	3552	3556	rBV2	764	725	0.07%	0.008%
91	12.513	3564	3568	3572	rBV3	790	753	0.07%	0.009%
92	12.596	3589	3594	3598	rBV4	583	588	0.06%	0.007%
93	12.914	3688	3693	3695	rBV3	583	546	0.05%	0.006%
94	13.249	3795	3797	3799	rBV	686	295	0.03%	0.003%
95	13.352	3828	3829	3831	rBV	307	162	0.02%	0.002%
96	13.361	3831	3832	3837	rVB3	595	389	0.04%	0.005%
97	13.644	3917	3920	3923	rVB3	762	431	0.04%	0.005%
98	13.660	3923	3925	3926	rBV	345	185	0.02%	0.002%
99	13.853	3980	3985	3986	rBV3	652	574	0.05%	0.007%
100	14.088	4054	4058	4061	rBV3	731	831	0.08%	0.010%




Sum of corrected areas: 8584166

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031424.D
Acq On : 08 Jun 2023 01:54
Operator : SY/MD
Sample : 03077-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

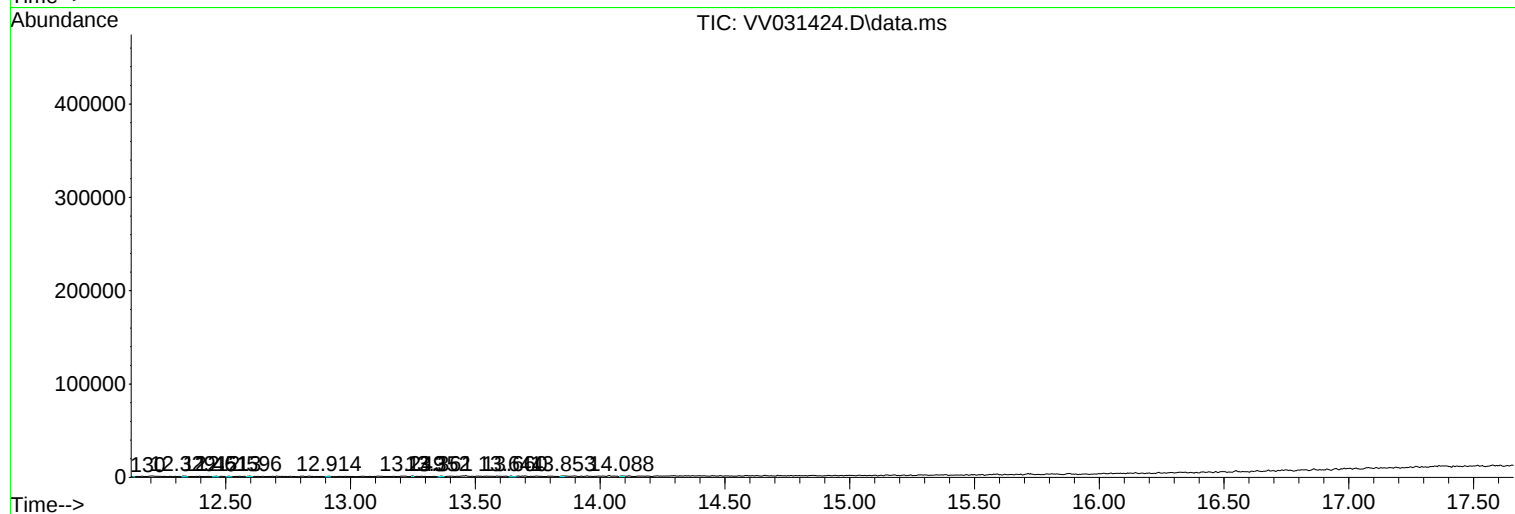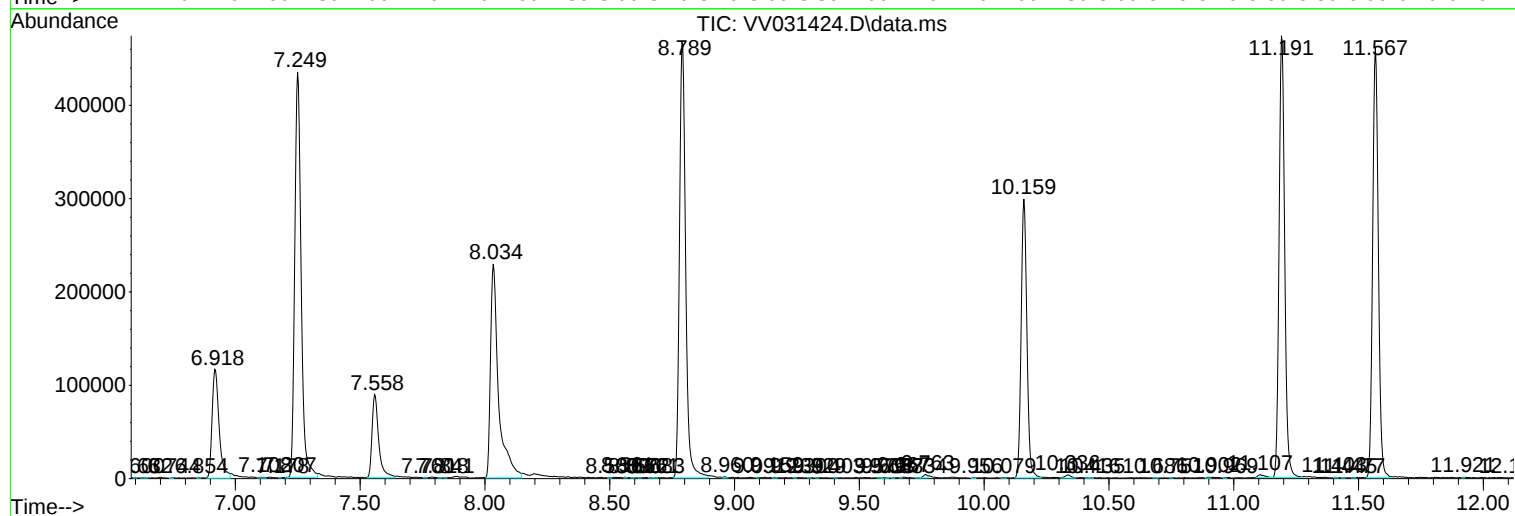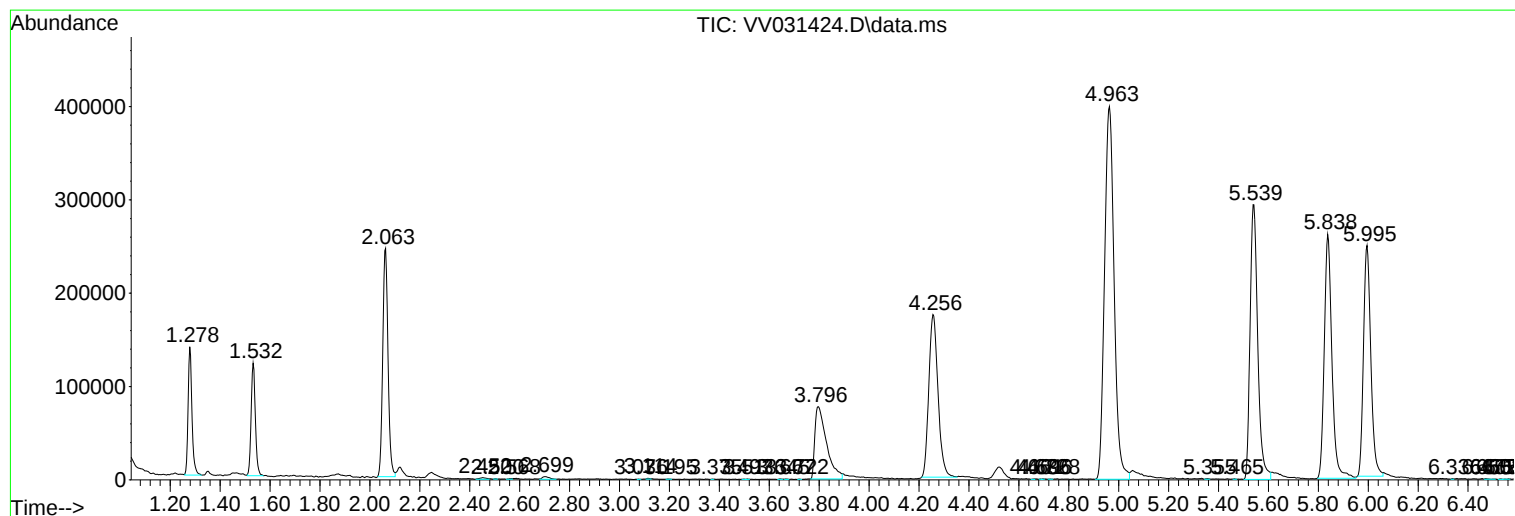

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031424.D
Acq On : 08 Jun 2023 01:54
Operator : SY/MD
Sample : 03077-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031424.D
Acq On : 08 Jun 2023 01:54
Operator : SY/MD
Sample : 03077-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------