

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031426.D
 Acq On : 08 Jun 2023 02:41
 Operator : SY/MD
 Sample : 03077-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031426.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	92	rVB	130647	142170	13.80%	1.807%
2	1.532	146	153	168	rVB	116590	138972	13.49%	1.766%
3	2.063	308	318	331	rBV	239851	350690	34.04%	4.457%
4	2.568	472	475	483	rBV6	929	1429	0.14%	0.018%
5	2.677	505	509	511	rBV4	621	452	0.04%	0.006%
6	2.786	539	543	545	rBV2	416	276	0.03%	0.004%
7	2.908	579	581	584	rVB2	401	188	0.02%	0.002%
8	3.011	609	613	614	rVV2	267	191	0.02%	0.002%
9	3.153	655	657	660	rBV2	421	208	0.02%	0.003%
10	3.230	677	681	684	rBV2	565	500	0.05%	0.006%
11	3.252	684	688	692	rVV6	506	510	0.05%	0.006%
12	3.275	692	695	698	rVV2	441	378	0.04%	0.005%
13	3.481	754	759	762	rBV4	442	489	0.05%	0.006%
14	3.542	776	778	782	rVB2	264	185	0.02%	0.002%
15	3.593	788	794	797	rBV2	309	281	0.03%	0.004%
16	3.613	797	800	803	rBV3	252	197	0.02%	0.003%
17	3.651	807	812	813	rBV	395	258	0.03%	0.003%
18	3.796	847	857	892	rBV	78607	230732	22.40%	2.933%
19	4.256	983	1000	1025	rBV	167857	441503	42.85%	5.612%
20	4.635	1115	1118	1119	rBV	423	269	0.03%	0.003%
21	4.735	1147	1149	1151	rBV	422	203	0.02%	0.003%
22	4.748	1151	1153	1156	rVB3	582	266	0.03%	0.003%
23	4.847	1180	1184	1185	rBV	369	240	0.02%	0.003%
24	4.963	1202	1220	1242	rBV2	386781	1030265	100.00%	13.095%
25	5.352	1339	1341	1343	rBV2	424	217	0.02%	0.003%
26	5.378	1346	1349	1350	rBV2	410	260	0.03%	0.003%
27	5.436	1365	1367	1370	rVB3	712	282	0.03%	0.004%
28	5.538	1384	1399	1424	rBV	291057	612656	59.47%	7.787%
29	5.834	1479	1491	1519	rBV4	40566	97198	9.43%	1.235%
30	5.995	1526	1541	1565	rBV	236708	505859	49.10%	6.429%
31	6.198	1600	1604	1608	rVB4	1145	1071	0.10%	0.014%
32	6.301	1632	1636	1637	rBV3	590	410	0.04%	0.005%
33	6.439	1676	1679	1681	rBV	422	227	0.02%	0.003%
34	6.455	1681	1684	1686	rBV2	352	223	0.02%	0.003%
35	6.513	1698	1702	1707	rVB4	805	618	0.06%	0.008%
36	6.535	1707	1709	1710	rBV	526	199	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031426.D
 Acq On : 08 Jun 2023 02:41
 Operator : SY/MD
 Sample : 03077-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.571	1717	1720	1724	rBV3	542	402	0.04%	0.005%
38	6.657	1740	1747	1750	rBV3	585	633	0.06%	0.008%
39	6.857	1805	1809	1817	rVB3	377	442	0.04%	0.006%
40	6.918	1817	1828	1851	rBV	114530	218205	21.18%	2.773%
41	7.159	1900	1903	1908	rBV5	496	554	0.05%	0.007%
42	7.249	1918	1931	1965	rBV	411992	750978	72.89%	9.545%
43	7.487	2003	2005	2007	rBV2	473	294	0.03%	0.004%
44	7.516	2012	2014	2017	rVB3	476	197	0.02%	0.003%
45	7.558	2017	2027	2047	rBV	82820	156410	15.18%	1.988%
46	7.828	2109	2111	2114	rBV3	650	451	0.04%	0.006%
47	7.866	2119	2123	2126	rBV3	705	546	0.05%	0.007%
48	7.966	2151	2154	2155	rBV	495	223	0.02%	0.003%
49	8.034	2164	2175	2213	rBV2	225206	501928	48.72%	6.380%
50	8.487	2313	2316	2319	rBV3	446	346	0.03%	0.004%
51	8.522	2324	2327	2329	rBV4	483	330	0.03%	0.004%
52	8.644	2362	2365	2367	rBV3	480	331	0.03%	0.004%
53	8.680	2374	2376	2379	rBV3	576	379	0.04%	0.005%
54	8.789	2398	2410	2438	rBV	466736	783002	76.00%	9.952%
55	9.333	2577	2579	2581	rBV2	401	192	0.02%	0.002%
56	9.368	2588	2590	2593	rBV2	343	209	0.02%	0.003%
57	9.403	2599	2601	2606	rVB2	511	212	0.02%	0.003%
58	9.474	2621	2623	2626	rBV	455	214	0.02%	0.003%
59	9.574	2651	2654	2655	rBV	626	328	0.03%	0.004%
60	9.683	2687	2688	2690	rBV	683	256	0.02%	0.003%
61	9.789	2719	2721	2724	rBV	474	310	0.03%	0.004%
62	9.821	2729	2731	2733	rBV	369	193	0.02%	0.002%
63	9.876	2744	2748	2752	rVB3	801	635	0.06%	0.008%
64	9.898	2752	2755	2757	rBV2	522	313	0.03%	0.004%
65	10.091	2813	2815	2817	rBV2	474	224	0.02%	0.003%
66	10.159	2824	2836	2854	rBV	282224	453338	44.00%	5.762%
67	10.333	2883	2890	2896	rBV4	2286	3099	0.30%	0.039%
68	10.435	2920	2922	2926	rVB	478	266	0.03%	0.003%
69	10.480	2934	2936	2937	rBV	540	291	0.03%	0.004%
70	10.541	2953	2955	2957	rBV2	475	261	0.03%	0.003%
71	10.577	2963	2966	2970	rBV2	468	252	0.02%	0.003%
72	10.596	2970	2972	2974	rBV3	412	219	0.02%	0.003%
73	10.648	2986	2988	2991	rBV	396	290	0.03%	0.004%
74	10.763	3022	3024	3028	rVB2	470	272	0.03%	0.003%
75	10.789	3028	3032	3038	rBV3	360	438	0.04%	0.006%
76	10.972	3085	3089	3094	rBV3	395	431	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031426.D
 Acq On : 08 Jun 2023 02:41
 Operator : SY/MD
 Sample : 03077-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	11.046	3110	3112	3116	rVB2	426	289	0.03%	0.004%
78	11.066	3116	3118	3123	rBV	347	299	0.03%	0.004%
79	11.130	3136	3138	3140	rBV2	721	389	0.04%	0.005%
80	11.191	3145	3157	3181	rBV	451357	720572	69.94%	9.158%
81	11.480	3245	3247	3252	rVB2	386	248	0.02%	0.003%
82	11.567	3260	3274	3294	rBV	441435	700404	67.98%	8.902%
83	11.718	3319	3321	3326	rVB3	937	794	0.08%	0.010%
84	11.831	3353	3356	3360	rVB3	676	518	0.05%	0.007%
85	11.963	3395	3397	3400	rBV	512	251	0.02%	0.003%
86	12.133	3448	3450	3454	rVV3	487	239	0.02%	0.003%
87	12.152	3454	3456	3459	rVB	478	233	0.02%	0.003%
88	12.339	3510	3514	3517	rBV2	459	364	0.04%	0.005%
89	12.410	3530	3536	3538	rBV4	409	462	0.04%	0.006%
90	12.564	3582	3584	3585	rBV4	537	215	0.02%	0.003%
91	12.635	3602	3606	3607	rBV	453	253	0.02%	0.003%
92	12.680	3618	3620	3624	rVV3	547	343	0.03%	0.004%
93	12.885	3681	3684	3688	rVB3	698	412	0.04%	0.005%
94	13.381	3835	3838	3840	rBV2	609	369	0.04%	0.005%
95	13.512	3878	3879	3885	rBV5	605	453	0.04%	0.006%
96	13.564	3892	3895	3898	rVB3	618	347	0.03%	0.004%
97	13.686	3930	3933	3935	rBV	935	521	0.05%	0.007%
98	13.866	3987	3989	3993	rVB2	615	302	0.03%	0.004%
99	13.892	3993	3997	4000	rBV4	640	573	0.06%	0.007%
100	14.281	4113	4118	4122	rBV4	809	1007	0.10%	0.013%




Sum of corrected areas: 7867823

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031426.D
Acq On : 08 Jun 2023 02:41
Operator : SY/MD
Sample : 03077-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

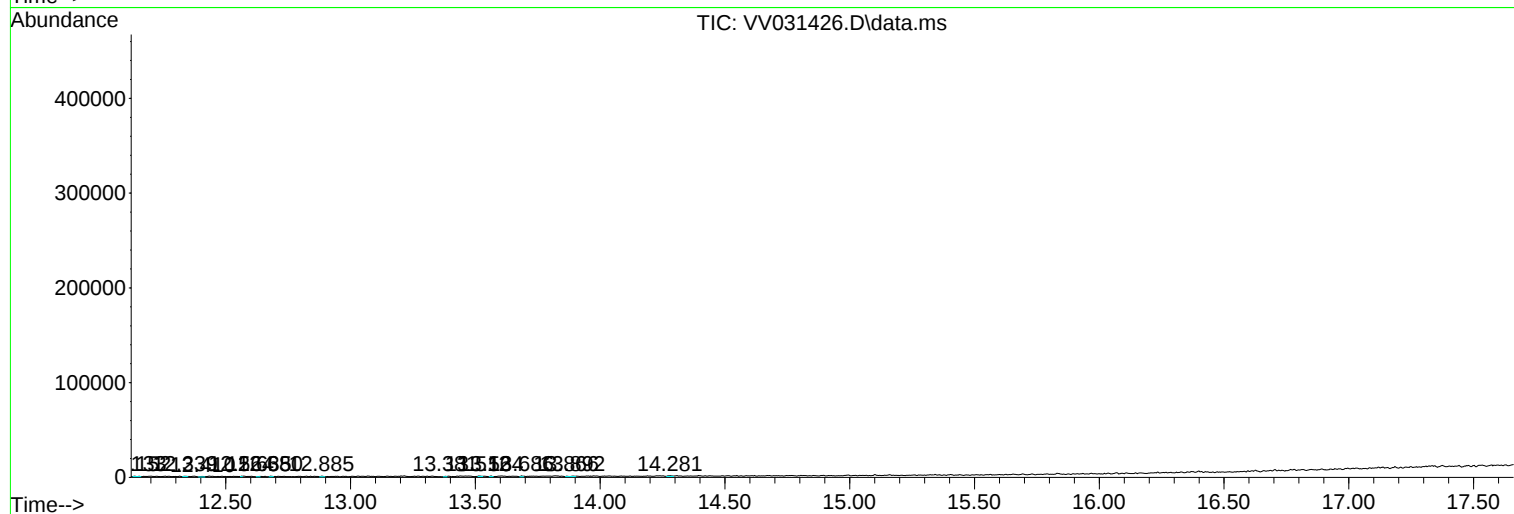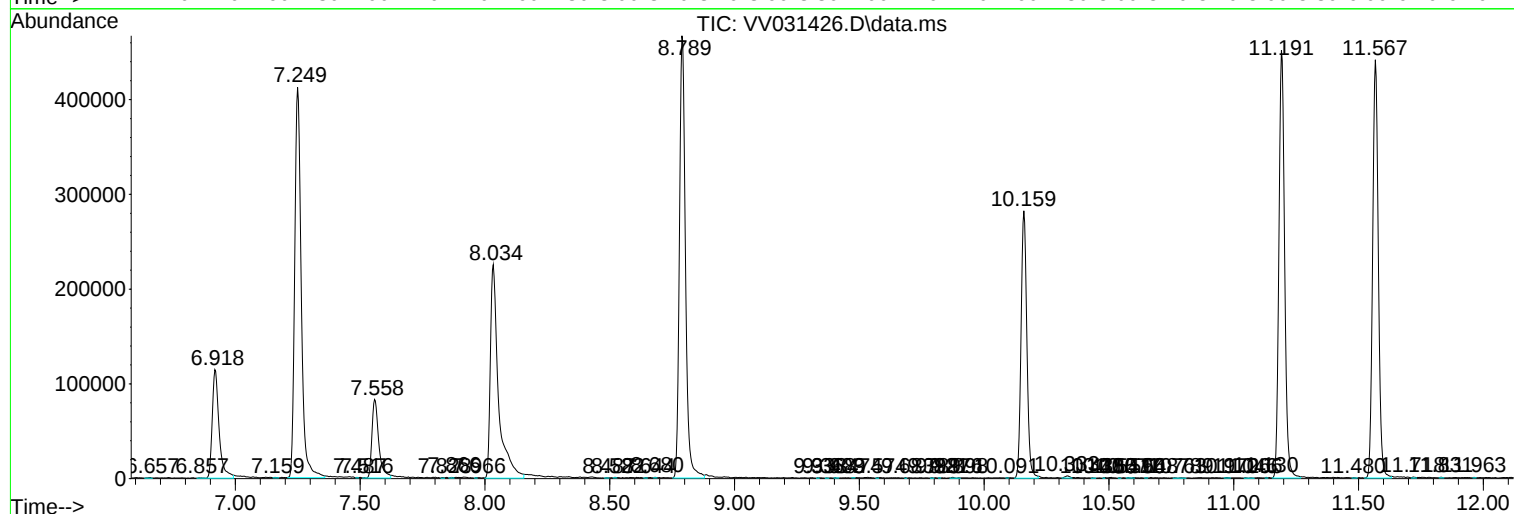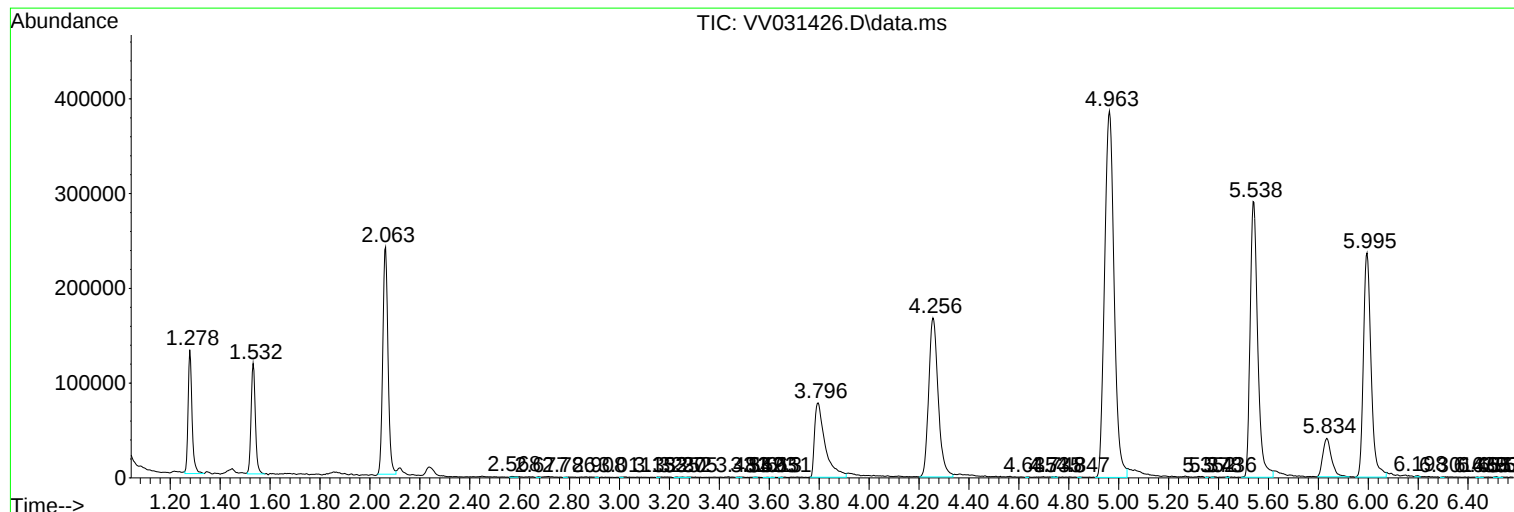

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031426.D
Acq On : 08 Jun 2023 02:41
Operator : SY/MD
Sample : 03077-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031426.D
Acq On : 08 Jun 2023 02:41
Operator : SY/MD
Sample : 03077-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------