

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031427.D
 Acq On : 08 Jun 2023 03:05
 Operator : SY/MD
 Sample : 03077-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031427.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	90	rVB	131574	142276	13.68%	1.838%
2	1.532	146	153	169	rVB	117072	139249	13.39%	1.799%
3	2.063	308	318	329	rBV	232884	338375	32.54%	4.371%
4	2.362	409	411	416	rVB4	725	448	0.04%	0.006%
5	2.577	470	478	483	rBV6	1699	3038	0.29%	0.039%
6	2.642	497	498	502	rBV3	329	211	0.02%	0.003%
7	2.690	510	513	517	rVB3	698	556	0.05%	0.007%
8	2.712	517	520	521	rBV	550	363	0.03%	0.005%
9	2.892	572	576	577	rBV	455	267	0.03%	0.003%
10	3.124	645	648	651	rBV4	554	471	0.05%	0.006%
11	3.211	670	675	677	rBV2	527	427	0.04%	0.006%
12	3.252	684	688	691	rBV2	479	414	0.04%	0.005%
13	3.301	699	703	705	rBV2	455	305	0.03%	0.004%
14	3.359	718	721	722	rBV	391	181	0.02%	0.002%
15	3.439	744	746	754	rVB2	377	405	0.04%	0.005%
16	3.490	759	762	764	rBV	370	239	0.02%	0.003%
17	3.552	778	781	784	rVB	740	406	0.04%	0.005%
18	3.577	784	789	791	rBV	416	317	0.03%	0.004%
19	3.793	847	856	882	rBV	79263	224504	21.59%	2.900%
20	4.256	983	1000	1025	rBV2	167656	440140	42.32%	5.685%
21	4.609	1107	1110	1111	rBV	467	244	0.02%	0.003%
22	4.818	1172	1175	1177	rBV2	335	228	0.02%	0.003%
23	4.963	1203	1220	1251	rBV2	385978	1040021	100.00%	13.434%
24	5.449	1369	1371	1377	rVB4	491	347	0.03%	0.004%
25	5.539	1387	1399	1422	rBV	279283	590153	56.74%	7.623%
26	5.770	1468	1471	1473	rBV4	501	382	0.04%	0.005%
27	5.828	1479	1489	1505	rBV2	27890	58599	5.63%	0.757%
28	5.995	1527	1541	1566	rBV	235257	504280	48.49%	6.514%
29	6.310	1637	1639	1642	rVB2	420	198	0.02%	0.003%
30	6.442	1678	1680	1684	rVB3	434	222	0.02%	0.003%
31	6.468	1684	1688	1691	rBV2	453	318	0.03%	0.004%
32	6.632	1736	1739	1747	rVB4	798	934	0.09%	0.012%
33	6.664	1747	1749	1753	rVB2	415	254	0.02%	0.003%
34	6.686	1753	1756	1758	rBV2	252	187	0.02%	0.002%
35	6.731	1768	1770	1771	rBV	447	200	0.02%	0.003%
36	6.744	1772	1774	1779	rVB4	539	427	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031427.D
 Acq On : 08 Jun 2023 03:05
 Operator : SY/MD
 Sample : 03077-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.764	1779	1780	1786	rBV3	277	228	0.02%	0.003%
38	6.870	1810	1813	1815	rVB2	420	188	0.02%	0.002%
39	6.918	1815	1828	1854	rBV	111819	219945	21.15%	2.841%
40	7.249	1919	1931	1963	rBV	408303	731742	70.36%	9.452%
41	7.558	2017	2027	2045	rBV	84355	154017	14.81%	1.989%
42	7.744	2083	2085	2087	rBV	508	232	0.02%	0.003%
43	7.828	2107	2111	2117	rVB3	313	378	0.04%	0.005%
44	7.889	2124	2130	2134	rBV5	713	835	0.08%	0.011%
45	7.956	2149	2151	2153	rVB2	398	181	0.02%	0.002%
46	7.969	2153	2155	2159	rBV2	484	355	0.03%	0.005%
47	8.034	2164	2175	2221	rBV2	233365	520923	50.09%	6.729%
48	8.442	2300	2302	2303	rBV	511	222	0.02%	0.003%
49	8.593	2345	2349	2350	rBV	699	496	0.05%	0.006%
50	8.651	2365	2367	2368	rVB2	598	230	0.02%	0.003%
51	8.661	2368	2370	2372	rBV2	399	200	0.02%	0.003%
52	8.690	2375	2379	2382	rBV4	463	306	0.03%	0.004%
53	8.722	2385	2389	2390	rBV2	429	275	0.03%	0.004%
54	8.789	2399	2410	2439	rBV	440906	754471	72.54%	9.745%
55	9.072	2497	2498	2503	rBV2	377	254	0.02%	0.003%
56	9.146	2518	2521	2524	rBV3	357	258	0.02%	0.003%
57	9.178	2527	2531	2533	rBV2	854	565	0.05%	0.007%
58	9.207	2538	2540	2542	rBV	542	254	0.02%	0.003%
59	9.391	2595	2597	2600	rBV	451	181	0.02%	0.002%
60	9.436	2607	2611	2613	rBV2	289	277	0.03%	0.004%
61	9.468	2618	2621	2623	rBV3	469	269	0.03%	0.003%
62	9.529	2633	2640	2644	rBV4	691	949	0.09%	0.012%
63	9.638	2671	2674	2676	rBV2	374	235	0.02%	0.003%
64	9.715	2694	2698	2702	rVB3	750	501	0.05%	0.006%
65	9.818	2726	2730	2735	rBV2	354	377	0.04%	0.005%
66	9.844	2735	2738	2742	rVB3	405	312	0.03%	0.004%
67	9.873	2745	2747	2749	rBV2	440	269	0.03%	0.003%
68	9.944	2766	2769	2772	rBV4	472	364	0.03%	0.005%
69	9.972	2776	2778	2783	rVB3	413	212	0.02%	0.003%
70	10.159	2825	2836	2862	rBV	291966	466767	44.88%	6.029%
71	10.278	2871	2873	2878	rVB2	684	386	0.04%	0.005%
72	10.304	2878	2881	2884	rBV3	670	509	0.05%	0.007%
73	10.410	2912	2914	2915	rBV3	391	186	0.02%	0.002%
74	10.458	2926	2929	2932	rBV2	371	267	0.03%	0.003%
75	10.477	2933	2935	2936	rVV	477	211	0.02%	0.003%
76	10.487	2936	2938	2945	rVB4	868	701	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031427.D
 Acq On : 08 Jun 2023 03:05
 Operator : SY/MD
 Sample : 03077-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FA9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.577	2964	2966	2971	rBV2	295	224	0.02%	0.003%
78	10.632	2980	2983	2986	rBV2	569	388	0.04%	0.005%
79	10.757	3019	3022	3024	rBV2	428	279	0.03%	0.004%
80	10.825	3039	3043	3045	rBV	522	340	0.03%	0.004%
81	10.950	3079	3082	3084	rBV3	520	243	0.02%	0.003%
82	11.082	3119	3123	3125	rBV3	408	327	0.03%	0.004%
83	11.127	3133	3137	3138	rBV3	486	334	0.03%	0.004%
84	11.191	3145	3157	3177	rBV	432454	694057	66.73%	8.965%
85	11.567	3261	3274	3294	rBV	435554	689979	66.34%	8.912%
86	11.815	3347	3351	3354	rBV4	462	357	0.03%	0.005%
87	12.114	3440	3444	3447	rBV3	561	400	0.04%	0.005%
88	12.252	3482	3487	3489	rBV2	583	485	0.05%	0.006%
89	12.474	3554	3556	3561	rBV2	485	450	0.04%	0.006%
90	12.538	3573	3576	3578	rBV	614	421	0.04%	0.005%
91	12.853	3671	3674	3675	rBV2	670	357	0.03%	0.005%
92	13.027	3725	3728	3730	rBV3	724	413	0.04%	0.005%
93	13.098	3748	3750	3752	rVB	414	190	0.02%	0.002%
94	13.423	3849	3851	3855	rBV4	602	475	0.05%	0.006%
95	13.455	3855	3861	3863	rBV5	814	780	0.07%	0.010%
96	13.558	3891	3893	3895	rBV	367	239	0.02%	0.003%
97	13.622	3911	3913	3915	rBV	644	290	0.03%	0.004%
98	13.786	3961	3964	3966	rBV3	499	348	0.03%	0.004%
99	13.821	3970	3975	3976	rBV2	646	495	0.05%	0.006%
100	13.908	3995	4002	4003	rBV5	864	912	0.09%	0.012%




Sum of corrected areas: 7741897

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031427.D
Acq On : 08 Jun 2023 03:05
Operator : SY/MD
Sample : 03077-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

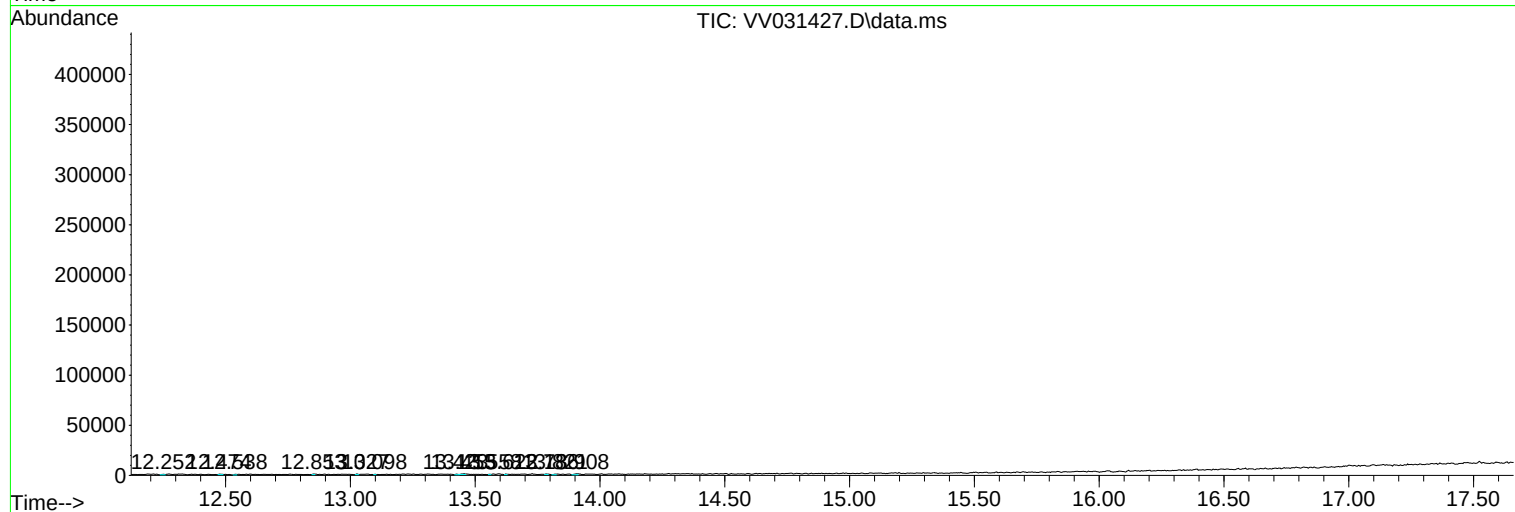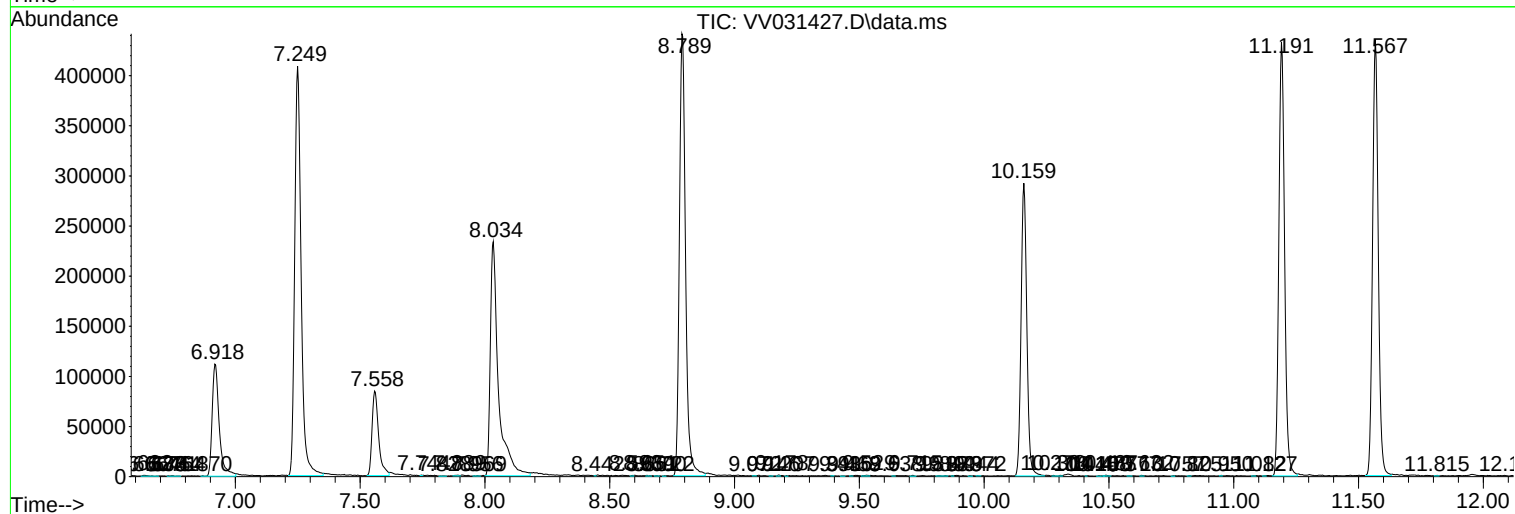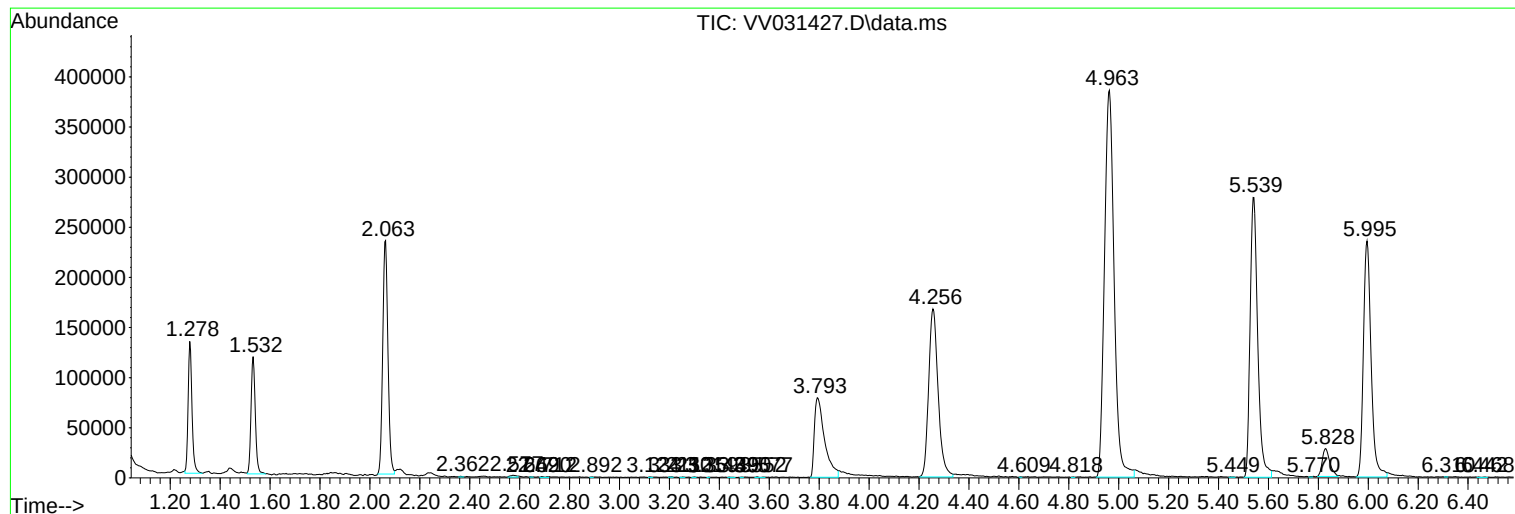

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031427.D
Acq On : 08 Jun 2023 03:05
Operator : SY/MD
Sample : 03077-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031427.D
Acq On : 08 Jun 2023 03:05
Operator : SY/MD
Sample : 03077-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FA9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc