

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031429.D
 Acq On : 08 Jun 2023 03:53
 Operator : SY/MD
 Sample : 03077-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	135326	146682	13.66%	1.804%
2	1.532	146	153	167	rVB	120944	139553	12.99%	1.716%
3	2.063	307	318	331	rBV	246426	365448	34.03%	4.495%
4	2.445	434	437	440	rBV3	928	662	0.06%	0.008%
5	2.661	503	504	507	rBV2	461	231	0.02%	0.003%
6	2.735	525	527	530	rVB2	409	200	0.02%	0.002%
7	2.806	548	549	551	rBV2	424	184	0.02%	0.002%
8	2.825	551	555	557	rVV4	506	353	0.03%	0.004%
9	2.902	576	579	581	rVB2	626	347	0.03%	0.004%
10	2.998	605	609	612	rBV2	382	290	0.03%	0.004%
11	3.089	633	637	640	rBV4	534	367	0.03%	0.005%
12	3.175	659	664	666	rBV2	539	404	0.04%	0.005%
13	3.301	701	703	708	rVB3	372	258	0.02%	0.003%
14	3.445	746	748	752	rBV2	269	256	0.02%	0.003%
15	3.561	780	784	786	rVB2	410	280	0.03%	0.003%
16	3.580	786	790	792	rBV	292	203	0.02%	0.002%
17	3.606	795	798	802	rBV2	369	288	0.03%	0.004%
18	3.651	810	812	815	rBV3	357	265	0.02%	0.003%
19	3.728	831	836	838	rBV3	559	361	0.03%	0.004%
20	3.799	843	858	889	rBV3	111166	363096	33.81%	4.466%
21	4.256	986	1000	1026	rBV	168535	437448	40.73%	5.380%
22	4.648	1120	1122	1125	rVB	650	323	0.03%	0.004%
23	4.670	1125	1129	1132	rBV2	431	377	0.04%	0.005%
24	4.738	1147	1150	1152	rBV2	674	357	0.03%	0.004%
25	4.786	1163	1165	1168	rBV2	362	239	0.02%	0.003%
26	4.863	1187	1189	1192	rBV2	363	203	0.02%	0.002%
27	4.879	1192	1194	1198	rVB2	447	199	0.02%	0.002%
28	4.902	1198	1201	1203	rBV2	581	415	0.04%	0.005%
29	4.963	1203	1220	1245	rBV2	401593	1073973	100.00%	13.209%
30	5.474	1376	1379	1382	rBV2	656	435	0.04%	0.005%
31	5.500	1384	1387	1388	rBV	591	306	0.03%	0.004%
32	5.539	1388	1399	1425	rBV	302040	633239	58.96%	7.788%
33	5.828	1477	1489	1508	rBV2	46004	98967	9.22%	1.217%
34	5.995	1528	1541	1569	rBV	246107	519589	48.38%	6.390%
35	6.211	1606	1608	1610	rBV2	581	354	0.03%	0.004%
36	6.256	1620	1622	1624	rBV	428	219	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031429.D
 Acq On : 08 Jun 2023 03:53
 Operator : SY/MD
 Sample : 03077-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.346	1648	1650	1654	rVB2	624	408	0.04%	0.005%
38	6.368	1654	1657	1659	rBV2	451	328	0.03%	0.004%
39	6.384	1659	1662	1665	rVV3	421	282	0.03%	0.003%
40	6.474	1687	1690	1694	rVB3	499	357	0.03%	0.004%
41	6.494	1694	1696	1701	rBV	259	187	0.02%	0.002%
42	6.516	1701	1703	1706	rBV2	513	276	0.03%	0.003%
43	6.564	1716	1718	1722	rVB2	343	195	0.02%	0.002%
44	6.593	1722	1727	1728	rBV2	657	500	0.05%	0.006%
45	6.670	1747	1751	1754	rBV4	429	270	0.03%	0.003%
46	6.693	1756	1758	1760	rVV3	474	212	0.02%	0.003%
47	6.741	1772	1773	1778	rVB	448	245	0.02%	0.003%
48	6.834	1799	1802	1804	rVB2	647	378	0.04%	0.005%
49	6.847	1804	1806	1812	rVB	500	370	0.03%	0.005%
50	6.918	1816	1828	1853	rBV	117896	227531	21.19%	2.798%
51	7.137	1895	1896	1901	rVB3	706	520	0.05%	0.006%
52	7.249	1919	1931	1952	rBV	429670	763701	71.11%	9.393%
53	7.522	2013	2016	2017	rBV	653	349	0.03%	0.004%
54	7.558	2018	2027	2052	rVV	86428	159611	14.86%	1.963%
55	7.738	2081	2083	2091	rVB3	828	694	0.06%	0.009%
56	7.908	2134	2136	2147	rVB6	1437	1771	0.16%	0.022%
57	7.953	2147	2150	2152	rBV2	646	385	0.04%	0.005%
58	7.998	2162	2164	2165	rBV2	513	222	0.02%	0.003%
59	8.034	2165	2175	2213	rVV2	221589	514449	47.90%	6.327%
60	8.374	2278	2281	2285	rBV3	771	790	0.07%	0.010%
61	8.416	2292	2294	2296	rBV	387	249	0.02%	0.003%
62	8.603	2350	2352	2357	rVB3	480	358	0.03%	0.004%
63	8.635	2357	2362	2366	rBV4	854	864	0.08%	0.011%
64	8.693	2375	2380	2382	rBV3	375	249	0.02%	0.003%
65	8.789	2398	2410	2436	rBV	480360	803649	74.83%	9.884%
66	9.130	2510	2516	2517	rBV4	426	365	0.03%	0.004%
67	9.262	2554	2557	2559	rVB2	821	297	0.03%	0.004%
68	9.297	2566	2568	2572	rVB3	491	288	0.03%	0.004%
69	9.352	2582	2585	2589	rVB5	447	312	0.03%	0.004%
70	9.432	2608	2610	2613	rBV	350	253	0.02%	0.003%
71	9.583	2655	2657	2663	rBV4	408	324	0.03%	0.004%
72	9.612	2663	2666	2668	rBV2	377	270	0.03%	0.003%
73	9.770	2711	2715	2716	rBV	422	286	0.03%	0.004%
74	9.850	2738	2740	2742	rBV2	419	222	0.02%	0.003%
75	9.879	2745	2749	2750	rBV2	568	369	0.03%	0.005%
76	9.937	2764	2767	2771	rVV2	388	263	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031429.D
 Acq On : 08 Jun 2023 03:53
 Operator : SY/MD
 Sample : 03077-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	9.982	2777	2781	2786	rBV2	548	618	0.06%	0.008%
78	10.021	2791	2793	2800	rVB3	419	220	0.02%	0.003%
79	10.053	2800	2803	2804	rBV2	381	240	0.02%	0.003%
80	10.117	2819	2823	2824	rBV2	430	229	0.02%	0.003%
81	10.159	2824	2836	2860	rVV	259782	418929	39.01%	5.152%
82	10.255	2863	2866	2867	rBV	718	360	0.03%	0.004%
83	10.336	2879	2891	2898	rBV5	3168	5122	0.48%	0.063%
84	10.481	2933	2936	2937	rBV	387	227	0.02%	0.003%
85	10.564	2959	2962	2965	rBV	395	294	0.03%	0.004%
86	10.683	2995	2999	3002	rBV	380	335	0.03%	0.004%
87	10.911	3067	3070	3073	rBV2	426	270	0.03%	0.003%
88	11.040	3107	3110	3114	rVV3	469	317	0.03%	0.004%
89	11.072	3118	3120	3126	rVB2	444	348	0.03%	0.004%
90	11.098	3126	3128	3133	rBV3	427	325	0.03%	0.004%
91	11.191	3146	3157	3182	rBV	454446	723680	67.38%	8.900%
92	11.339	3201	3203	3207	rBV2	804	534	0.05%	0.007%
93	11.468	3240	3243	3245	rBV3	596	352	0.03%	0.004%
94	11.567	3262	3274	3294	rBV	441541	706586	65.79%	8.690%
95	12.133	3448	3450	3452	rBV2	457	225	0.02%	0.003%
96	12.821	3662	3664	3668	rVB3	342	257	0.02%	0.003%
97	12.844	3668	3671	3673	rBV	433	302	0.03%	0.004%
98	12.911	3689	3692	3695	rBV4	570	391	0.04%	0.005%
99	13.648	3920	3921	3923	rBV	428	235	0.02%	0.003%
100	13.937	4002	4011	4016	rBV6	877	1420	0.13%	0.017%




Sum of corrected areas: 8130836

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031429.D
Acq On : 08 Jun 2023 03:53
Operator : SY/MD
Sample : 03077-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

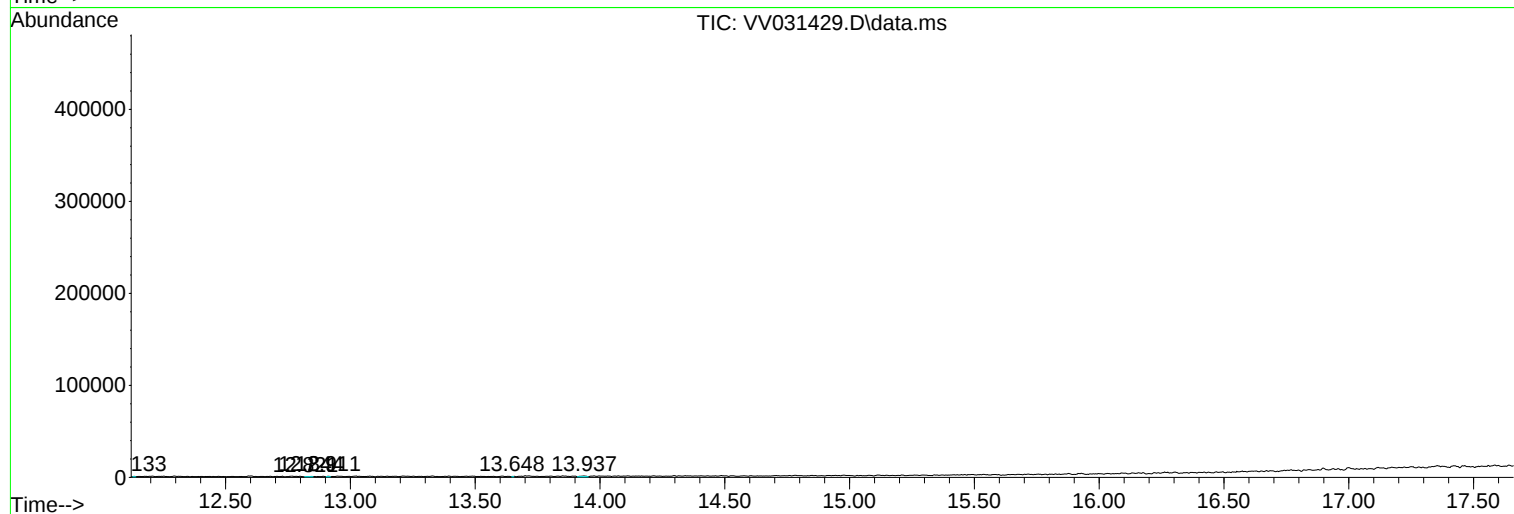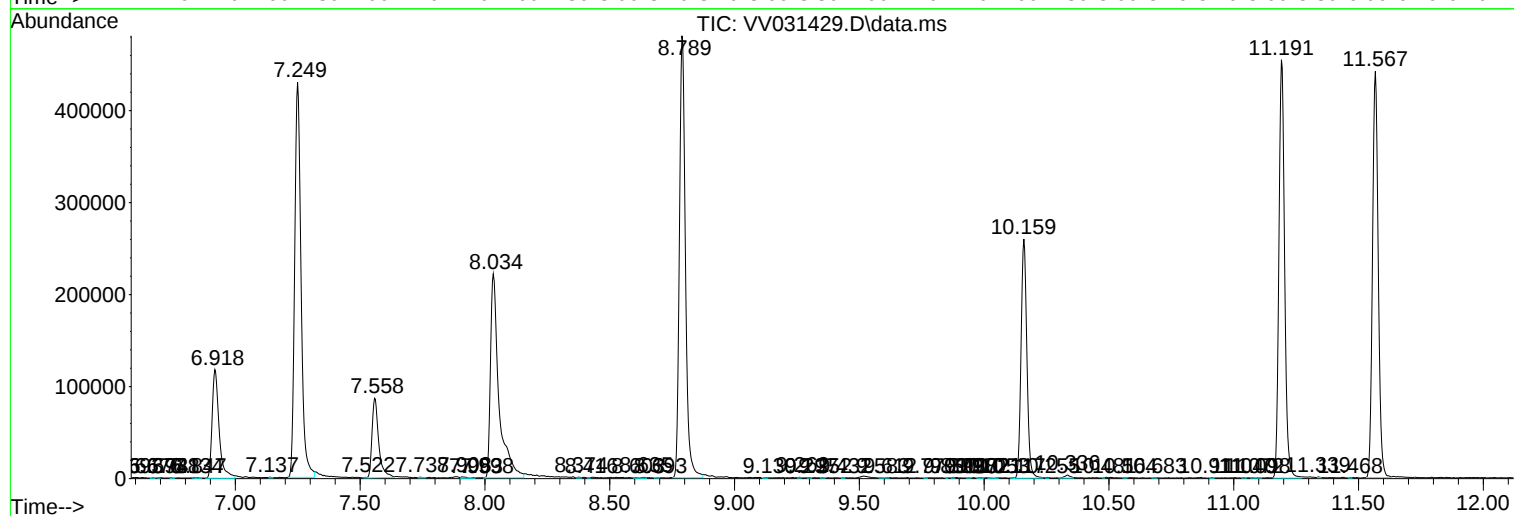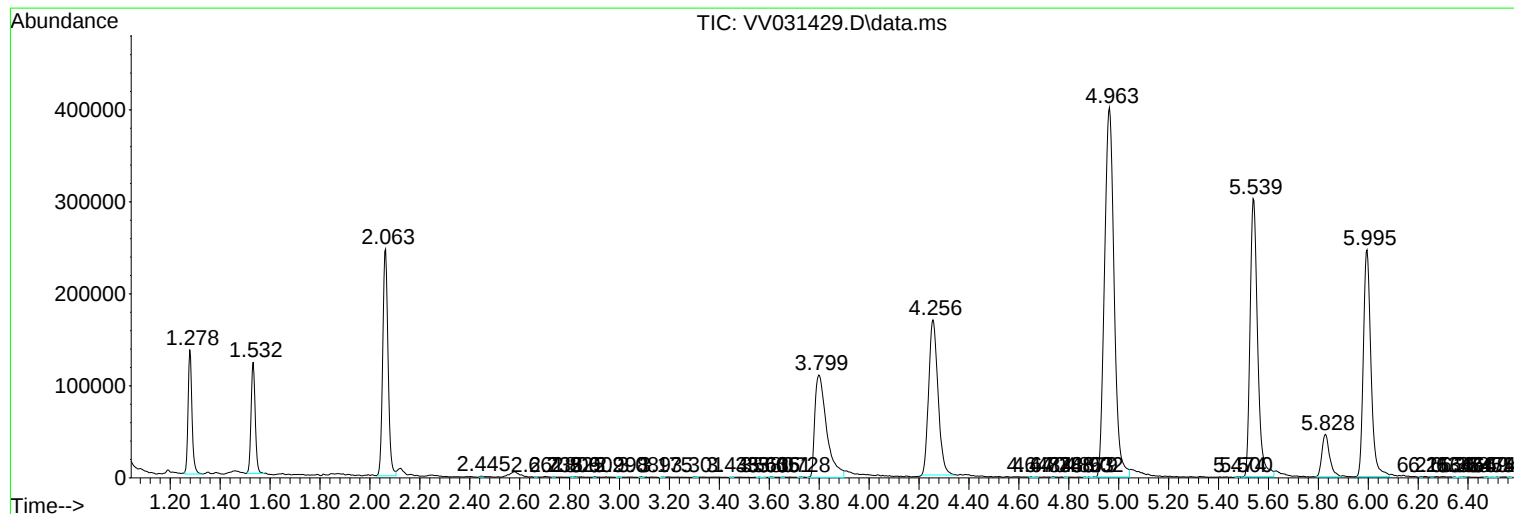

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031429.D
Acq On : 08 Jun 2023 03:53
Operator : SY/MD
Sample : 03077-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031429.D
Acq On : 08 Jun 2023 03:53
Operator : SY/MD
Sample : 03077-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------