

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031431.D
 Acq On : 08 Jun 2023 04:40
 Operator : SY/MD
 Sample : 03077-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	87	rVB	135180	142830	13.34%	1.603%
2	1.532	146	153	166	rVB	117358	138482	12.94%	1.554%
3	2.063	308	318	330	rBV2	262678	400523	37.42%	4.494%
4	2.558	470	472	474	rBV3	919	456	0.04%	0.005%
5	2.632	490	495	498	rBV3	562	434	0.04%	0.005%
6	2.696	512	515	516	rBV3	537	305	0.03%	0.003%
7	2.880	571	572	574	rBV	393	187	0.02%	0.002%
8	2.928	584	587	590	rBV3	377	325	0.03%	0.004%
9	2.966	597	599	603	rVB2	376	202	0.02%	0.002%
10	3.050	622	625	626	rBV	379	213	0.02%	0.002%
11	3.114	641	645	648	rBV3	1253	1156	0.11%	0.013%
12	3.166	660	661	665	rVB2	402	196	0.02%	0.002%
13	3.191	667	669	673	rVB2	495	272	0.03%	0.003%
14	3.214	673	676	680	rVB3	412	293	0.03%	0.003%
15	3.240	680	684	686	rBV	346	234	0.02%	0.003%
16	3.294	698	701	706	rBV2	252	194	0.02%	0.002%
17	3.507	764	767	772	rVB4	428	310	0.03%	0.003%
18	3.593	790	794	799	rVB3	522	422	0.04%	0.005%
19	3.619	799	802	803	rBV	312	182	0.02%	0.002%
20	3.754	841	844	845	rBV	408	184	0.02%	0.002%
21	3.793	846	856	887	rBV2	86590	296313	27.68%	3.325%
22	4.175	969	975	978	rBV5	725	760	0.07%	0.009%
23	4.256	984	1000	1026	rBV	177403	453781	42.40%	5.091%
24	4.523	1070	1083	1098	rBV2	13025	31759	2.97%	0.356%
25	4.606	1106	1109	1114	rVB4	797	518	0.05%	0.006%
26	4.677	1125	1131	1133	rBV2	435	369	0.03%	0.004%
27	4.693	1133	1136	1137	rVB2	364	185	0.02%	0.002%
28	4.783	1159	1164	1166	rBV3	449	356	0.03%	0.004%
29	4.867	1184	1190	1191	rBV2	523	457	0.04%	0.005%
30	4.886	1195	1196	1199	rVB2	471	215	0.02%	0.002%
31	4.963	1201	1220	1242	rBV3	404291	1070360	100.00%	12.009%
32	5.310	1326	1328	1334	rVB3	695	471	0.04%	0.005%
33	5.394	1351	1354	1359	rBV3	886	609	0.06%	0.007%
34	5.539	1387	1399	1419	rBV	300177	620592	57.98%	6.963%
35	5.838	1475	1492	1509	rBV2	412917	848368	79.26%	9.519%
36	5.995	1529	1541	1560	rBV	244862	498583	46.58%	5.594%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031431.D
 Acq On : 08 Jun 2023 04:40
 Operator : SY/MD
 Sample : 03077-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.278	1626	1629	1630	rBV2	539	238	0.02%	0.003%
38	6.400	1664	1667	1669	rBV2	356	259	0.02%	0.003%
39	6.532	1705	1708	1710	rBV4	358	223	0.02%	0.003%
40	6.619	1732	1735	1736	rBV2	429	209	0.02%	0.002%
41	6.642	1740	1742	1745	rBV2	404	268	0.03%	0.003%
42	6.667	1748	1750	1752	rBV	370	188	0.02%	0.002%
43	6.805	1789	1793	1796	rBV3	416	445	0.04%	0.005%
44	6.841	1801	1804	1807	rVV	433	250	0.02%	0.003%
45	6.918	1818	1828	1850	rBV	116019	220405	20.59%	2.473%
46	7.249	1918	1931	1968	rBV	434462	785625	73.40%	8.815%
47	7.558	2017	2027	2058	rBV	88158	161086	15.05%	1.807%
48	7.777	2094	2095	2102	rVB4	966	837	0.08%	0.009%
49	7.857	2118	2120	2124	rBV3	438	294	0.03%	0.003%
50	7.918	2134	2139	2144	rVB5	1210	1117	0.10%	0.013%
51	7.969	2153	2155	2159	rBV2	445	338	0.03%	0.004%
52	8.031	2164	2174	2208	rBV2	225506	499123	46.63%	5.600%
53	8.429	2296	2298	2302	rBV4	510	290	0.03%	0.003%
54	8.526	2326	2328	2330	rBV3	463	201	0.02%	0.002%
55	8.542	2330	2333	2335	rBV	883	497	0.05%	0.006%
56	8.600	2347	2351	2354	rBV4	510	519	0.05%	0.006%
57	8.789	2399	2410	2441	rBV	481119	803896	75.11%	9.020%
58	9.047	2487	2490	2492	rBV2	509	297	0.03%	0.003%
59	9.082	2499	2501	2505	rVB3	929	453	0.04%	0.005%
60	9.227	2543	2546	2547	rBV	459	290	0.03%	0.003%
61	9.265	2555	2558	2559	rBV2	441	202	0.02%	0.002%
62	9.275	2559	2561	2564	rVV	556	323	0.03%	0.004%
63	9.339	2578	2581	2587	rVB3	319	328	0.03%	0.004%
64	9.365	2587	2589	2592	rBV2	379	286	0.03%	0.003%
65	9.487	2624	2627	2628	rBV	461	254	0.02%	0.003%
66	9.596	2657	2661	2665	rBV4	537	429	0.04%	0.005%
67	9.651	2676	2678	2680	rBV2	365	181	0.02%	0.002%
68	9.728	2699	2702	2703	rBV	433	237	0.02%	0.003%
69	9.838	2733	2736	2739	rBV3	431	269	0.03%	0.003%
70	9.905	2755	2757	2763	rVB4	403	321	0.03%	0.004%
71	10.040	2796	2799	2802	rBV3	318	238	0.02%	0.003%
72	10.159	2824	2836	2858	rBV	291107	461899	43.15%	5.182%
73	10.439	2919	2923	2925	rBV3	249	196	0.02%	0.002%
74	10.464	2929	2931	2933	rBV2	361	192	0.02%	0.002%
75	10.542	2952	2955	2956	rBV	480	263	0.02%	0.003%
76	10.619	2978	2979	2983	rBV2	397	214	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031431.D
 Acq On : 08 Jun 2023 04:40
 Operator : SY/MD
 Sample : 03077-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.812	3035	3039	3041	rBV4	860	588	0.05%	0.007%
78	10.882	3059	3061	3066	rVB4	849	576	0.05%	0.006%
79	10.918	3066	3072	3076	rBV3	581	607	0.06%	0.007%
80	10.947	3076	3081	3083	rBV4	450	358	0.03%	0.004%
81	10.973	3086	3089	3092	rVB3	381	221	0.02%	0.002%
82	10.989	3092	3094	3096	rBV3	308	184	0.02%	0.002%
83	11.133	3134	3139	3141	rBV3	663	539	0.05%	0.006%
84	11.191	3146	3157	3180	rBV	462099	730448	68.24%	8.195%
85	11.567	3262	3274	3291	rBV	456455	720104	67.28%	8.079%
86	11.760	3332	3334	3337	rBV2	516	258	0.02%	0.003%
87	11.776	3337	3339	3340	rBV2	495	233	0.02%	0.003%
88	12.226	3476	3479	3483	rBV3	376	249	0.02%	0.003%
89	12.387	3527	3529	3532	rVB2	503	242	0.02%	0.003%
90	12.532	3572	3574	3576	rBV	372	222	0.02%	0.002%
91	12.603	3593	3596	3597	rBV2	664	394	0.04%	0.004%
92	12.786	3649	3653	3658	rBV2	686	588	0.05%	0.007%
93	12.812	3658	3661	3662	rBV	545	273	0.03%	0.003%
94	12.879	3675	3682	3685	rBV3	582	664	0.06%	0.007%
95	12.969	3708	3710	3714	rBV2	601	393	0.04%	0.004%
96	13.088	3746	3747	3749	rBV2	394	188	0.02%	0.002%
97	13.452	3858	3860	3862	rBV2	478	205	0.02%	0.002%
98	13.667	3924	3927	3929	rBV3	540	411	0.04%	0.005%
99	13.783	3961	3963	3965	rVB3	613	183	0.02%	0.002%
100	13.815	3970	3973	3974	rBV3	606	398	0.04%	0.004%



Sum of corrected areas: 8912802

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031431.D
Acq On : 08 Jun 2023 04:40
Operator : SY/MD
Sample : 03077-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

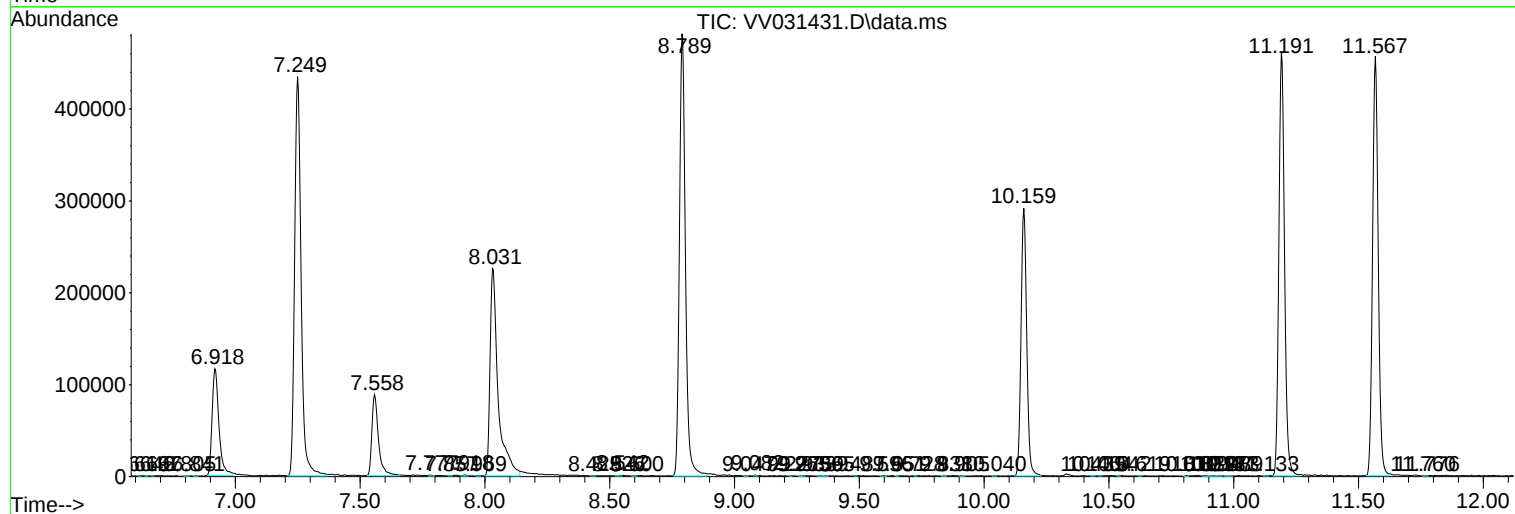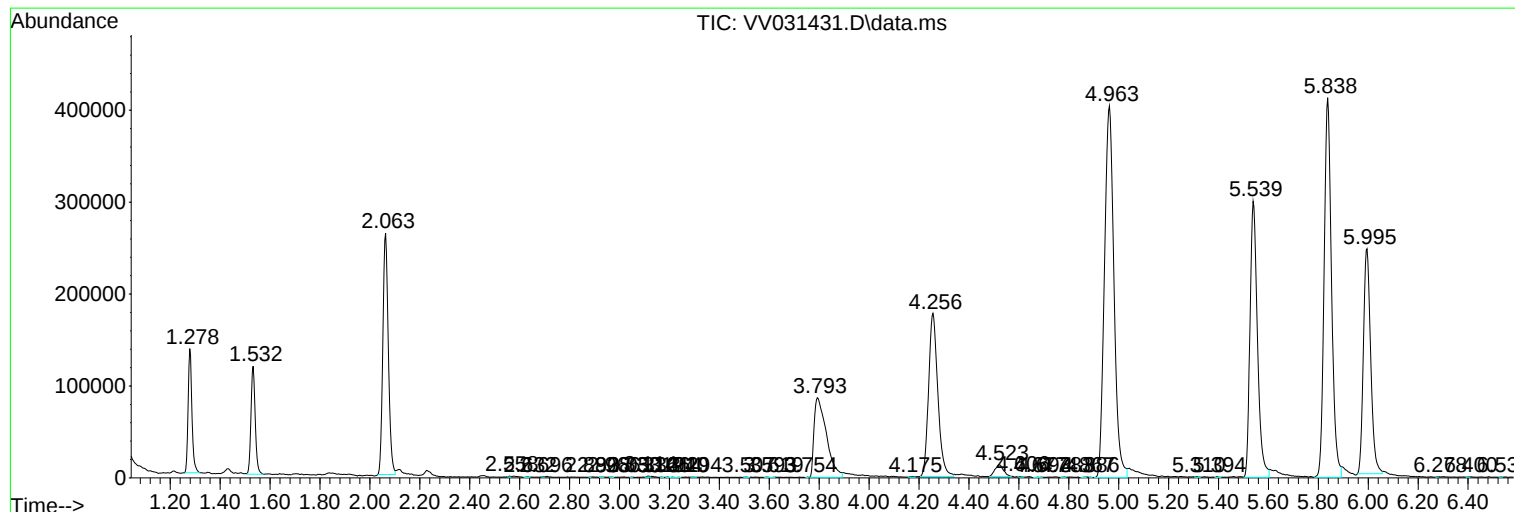

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031431.D
Acq On : 08 Jun 2023 04:40
Operator : SY/MD
Sample : 03077-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031431.D
Acq On : 08 Jun 2023 04:40
Operator : SY/MD
Sample : 03077-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc