

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031432.D
 Acq On : 08 Jun 2023 05:04
 Operator : SY/MD
 Sample : 03077-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

Signal : TIC: VV031432.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	85	rVB	129291	133909	12.72%	1.694%
2	1.532	146	153	167	rVB	118802	138465	13.15%	1.752%
3	2.063	307	318	330	rBV	241050	358553	34.05%	4.536%
4	2.523	459	461	462	rBV	475	175	0.02%	0.002%
5	2.552	468	470	471	rBV2	490	185	0.02%	0.002%
6	2.680	507	510	512	rBV	453	248	0.02%	0.003%
7	2.700	512	516	517	rBV3	768	474	0.05%	0.006%
8	2.799	542	547	550	rVB4	487	414	0.04%	0.005%
9	2.864	565	567	570	rBV	542	216	0.02%	0.003%
10	2.973	598	601	604	rBV2	411	343	0.03%	0.004%
11	3.069	626	631	632	rBV3	329	271	0.03%	0.003%
12	3.121	644	647	648	rBV	425	199	0.02%	0.003%
13	3.253	685	688	690	rBV3	422	217	0.02%	0.003%
14	3.301	699	703	705	rBV2	261	180	0.02%	0.002%
15	3.388	728	730	733	rBV3	473	291	0.03%	0.004%
16	3.722	831	834	837	rVB3	728	484	0.05%	0.006%
17	3.790	844	855	883	rBV	79191	220716	20.96%	2.792%
18	4.256	985	1000	1022	rBV	169245	440993	41.88%	5.579%
19	4.696	1133	1137	1139	rBV4	630	279	0.03%	0.004%
20	4.815	1172	1174	1177	rVB3	476	274	0.03%	0.003%
21	4.835	1177	1180	1181	rBV2	352	190	0.02%	0.002%
22	4.963	1202	1220	1243	rBV2	394154	1052867	100.00%	13.319%
23	5.240	1305	1306	1312	rBV4	484	433	0.04%	0.005%
24	5.458	1370	1374	1378	rBV4	852	703	0.07%	0.009%
25	5.484	1380	1382	1385	rBV3	494	309	0.03%	0.004%
26	5.539	1387	1399	1420	rBV	299157	618742	58.77%	7.827%
27	5.828	1478	1489	1508	rBV2	31179	68809	6.54%	0.870%
28	5.947	1524	1526	1527	rBV2	357	180	0.02%	0.002%
29	5.995	1527	1541	1569	rBV	241976	515377	48.95%	6.520%
30	6.195	1601	1603	1608	rVB3	897	761	0.07%	0.010%
31	6.269	1623	1626	1628	rBV2	397	189	0.02%	0.002%
32	6.278	1628	1629	1631	rBV	504	211	0.02%	0.003%
33	6.375	1655	1659	1660	rBV2	391	239	0.02%	0.003%
34	6.404	1664	1668	1671	rBV	321	274	0.03%	0.003%
35	6.436	1673	1678	1680	rBV2	630	472	0.04%	0.006%
36	6.478	1689	1691	1694	rBV2	228	173	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW060723\
 Data File : VW031432.D
 Acq On : 08 Jun 2023 05:04
 Operator : SY/MD
 Sample : 03077-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

37	6.519	1701	1704	1706	rBV2	361	210	0.02%	0.003%
38	6.532	1706	1708	1713	rVV2	569	427	0.04%	0.005%
39	6.622	1732	1736	1740	rBV4	581	524	0.05%	0.007%
40	6.661	1744	1748	1753	rBV3	404	532	0.05%	0.007%
41	6.703	1758	1761	1765	rVB3	304	282	0.03%	0.004%
42	6.741	1770	1773	1776	rBV3	624	373	0.04%	0.005%
43	6.757	1776	1778	1781	rBV	294	207	0.02%	0.003%
44	6.815	1793	1796	1798	rVB2	397	232	0.02%	0.003%
45	6.838	1798	1803	1808	rBV3	379	422	0.04%	0.005%
46	6.870	1808	1813	1816	rBV2	452	402	0.04%	0.005%
47	6.918	1817	1828	1858	rBV	115155	220851	20.98%	2.794%
48	7.249	1919	1931	1955	rBV	419354	756610	71.86%	9.571%
49	7.558	2017	2027	2052	rBV	87888	160308	15.23%	2.028%
50	7.699	2068	2071	2073	rBV	606	439	0.04%	0.006%
51	7.944	2145	2147	2149	rBV	520	264	0.03%	0.003%
52	8.031	2161	2174	2204	rBV2	221304	488173	46.37%	6.176%
53	8.497	2317	2319	2323	rBV2	496	244	0.02%	0.003%
54	8.529	2327	2329	2332	rBV	665	464	0.04%	0.006%
55	8.651	2366	2367	2372	rVB2	812	395	0.04%	0.005%
56	8.683	2372	2377	2384	rBV4	742	990	0.09%	0.013%
57	8.789	2398	2410	2435	rBV	482364	803039	76.27%	10.159%
58	9.256	2554	2555	2557	rBV2	550	225	0.02%	0.003%
59	9.301	2566	2569	2571	rBV	619	278	0.03%	0.004%
60	9.330	2574	2578	2579	rBV2	353	234	0.02%	0.003%
61	9.358	2585	2587	2589	rBV2	446	198	0.02%	0.003%
62	9.368	2589	2590	2592	rVV2	543	197	0.02%	0.002%
63	9.397	2596	2599	2601	rBV2	624	307	0.03%	0.004%
64	9.487	2623	2627	2631	rVV3	814	713	0.07%	0.009%
65	9.722	2698	2700	2706	rBV	294	274	0.03%	0.003%
66	9.764	2710	2713	2716	rBV2	452	246	0.02%	0.003%
67	9.838	2734	2736	2738	rBV	346	176	0.02%	0.002%
68	9.870	2743	2746	2752	rBV4	713	766	0.07%	0.010%
69	9.931	2762	2765	2766	rBV	640	270	0.03%	0.003%
70	10.088	2810	2814	2817	rBV2	264	267	0.03%	0.003%
71	10.159	2823	2836	2857	rBV	285240	460005	43.69%	5.819%
72	10.313	2881	2884	2885	rBV2	609	352	0.03%	0.004%
73	10.326	2885	2888	2897	rVB5	1830	2559	0.24%	0.032%
74	10.429	2916	2920	2925	rVB3	515	450	0.04%	0.006%
75	10.487	2934	2938	2941	rBV4	577	456	0.04%	0.006%
76	10.519	2944	2948	2949	rBV2	488	307	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
 Data File : VV031432.D
 Acq On : 08 Jun 2023 05:04
 Operator : SY/MD
 Sample : 03077-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0FB7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
 Title : VOC Analysis

77	10.567	2958	2963	2965	rBV3	401	381	0.04%	0.005%
78	10.616	2973	2978	2980	rBV2	482	430	0.04%	0.005%
79	10.654	2987	2990	2996	rVB3	376	321	0.03%	0.004%
80	10.686	2999	3000	3005	rVB2	382	258	0.02%	0.003%
81	10.744	3016	3018	3020	rVB2	513	195	0.02%	0.002%
82	10.773	3025	3027	3029	rBV2	581	280	0.03%	0.004%
83	10.838	3044	3047	3051	rVB2	336	275	0.03%	0.003%
84	10.860	3051	3054	3055	rBV	326	206	0.02%	0.003%
85	11.021	3102	3104	3106	rBV2	428	196	0.02%	0.002%
86	11.124	3132	3136	3139	rBV2	347	331	0.03%	0.004%
87	11.191	3145	3157	3176	rBV	458982	728398	69.18%	9.214%
88	11.448	3235	3237	3242	rBV2	446	426	0.04%	0.005%
89	11.567	3262	3274	3297	rVV	444797	708695	67.31%	8.965%
90	12.072	3428	3431	3435	rBV3	519	472	0.04%	0.006%
91	12.564	3581	3584	3588	rVB3	462	253	0.02%	0.003%
92	12.596	3590	3594	3595	rBV3	758	430	0.04%	0.005%
93	12.715	3629	3631	3639	rVB3	555	462	0.04%	0.006%
94	12.850	3671	3673	3674	rBV	393	197	0.02%	0.002%
95	13.030	3727	3729	3731	rVB2	641	285	0.03%	0.004%
96	13.162	3766	3770	3773	rVB2	544	362	0.03%	0.005%
97	13.313	3815	3817	3820	rBV2	312	201	0.02%	0.003%
98	13.355	3828	3830	3832	rBV2	464	203	0.02%	0.003%
99	13.821	3971	3975	3978	rBV2	613	566	0.05%	0.007%
100	14.243	4103	4106	4108	rBV	942	666	0.06%	0.008%




Sum of corrected areas: 7904972

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031432.D
Acq On : 08 Jun 2023 05:04
Operator : SY/MD
Sample : 03077-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

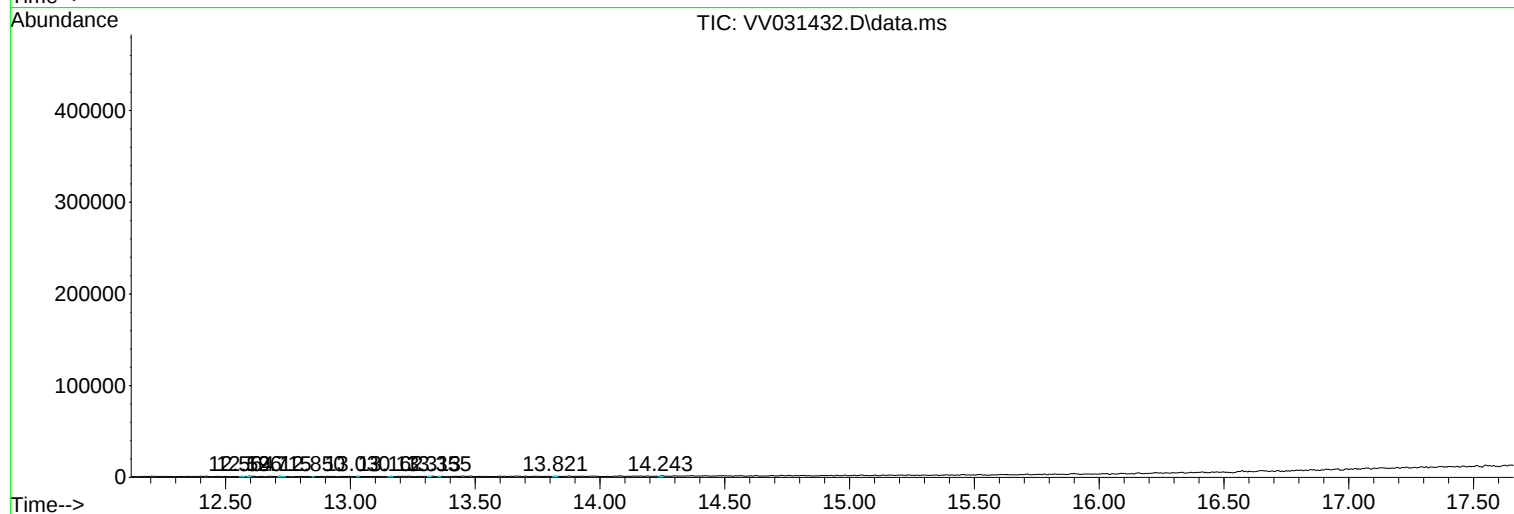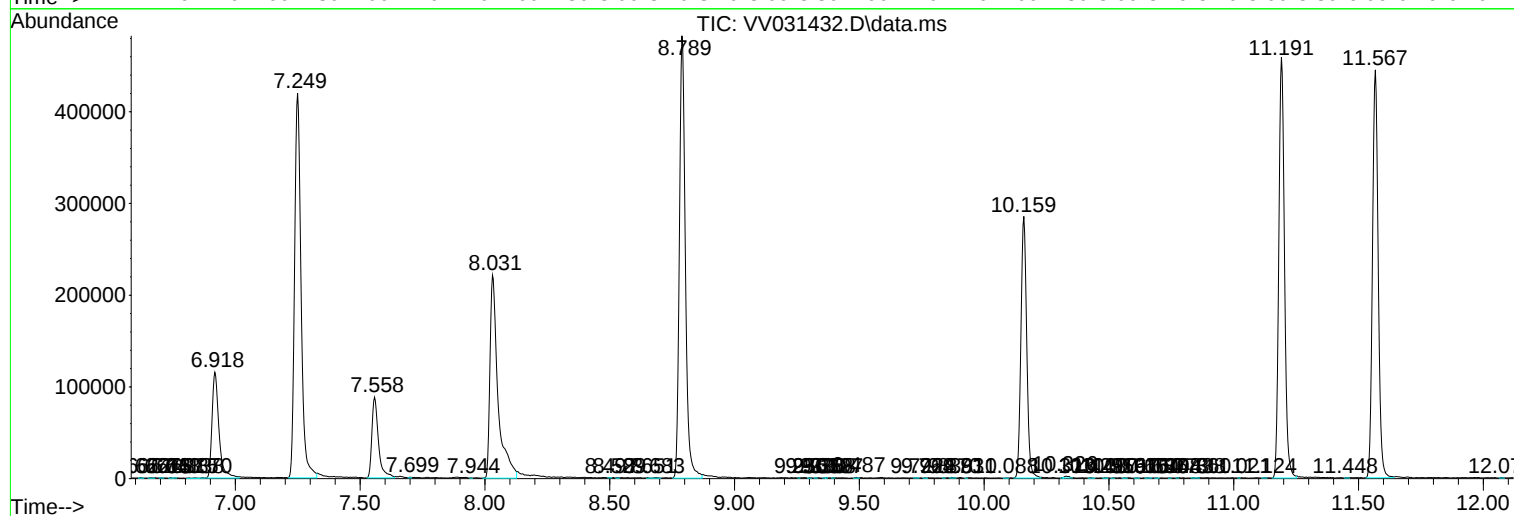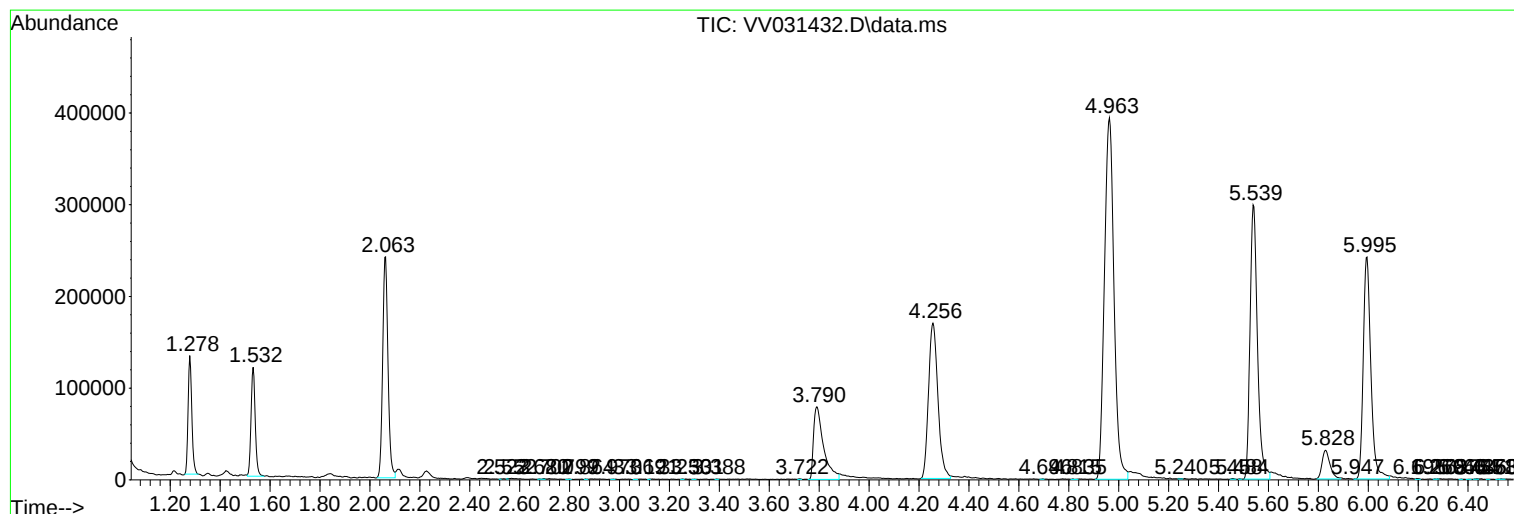

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031432.D
Acq On : 08 Jun 2023 05:04
Operator : SY/MD
Sample : 03077-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031432.D
Acq On : 08 Jun 2023 05:04
Operator : SY/MD
Sample : 03077-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 50 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0FB7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc