


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV060723\
Data File : VV031386.D
Acq On : 07 Jun 2023 08:40
Operator : SY/MD
Sample : BFB382
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB382

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM060723WMA.M
Title : VOC Analysis
Last Update : Thu Jun 08 05:16:53 2023

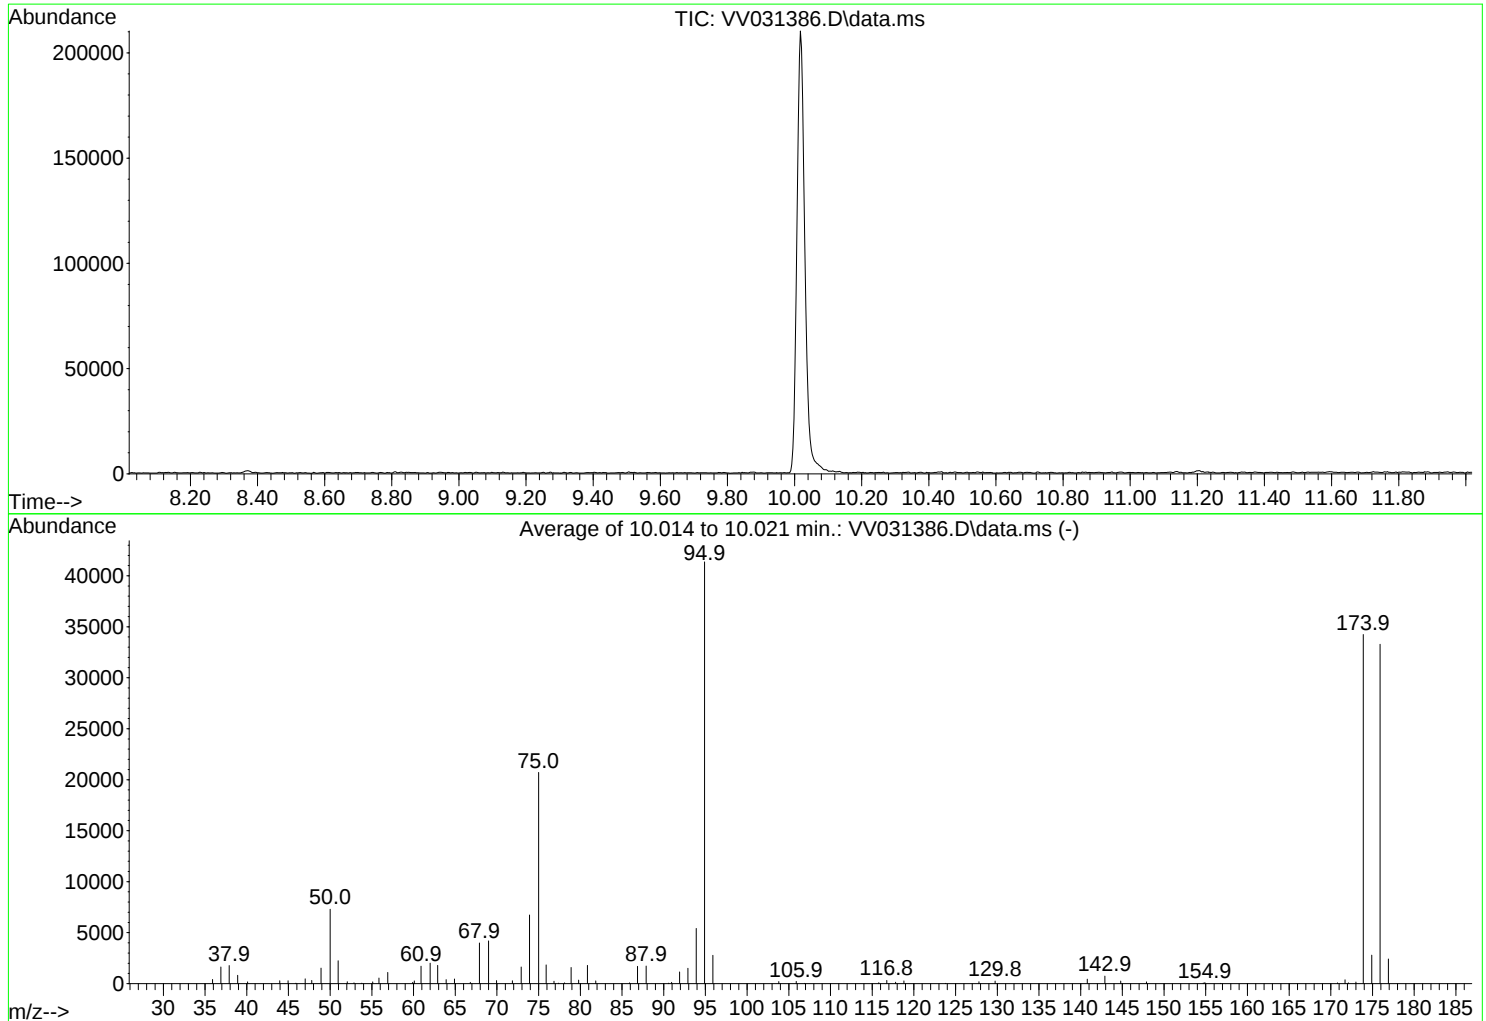

AutoFind: Scans 2791, 2792, 2793; Background Corrected with Scan 2781

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	7302	PASS
75	95	30	80	50.1	20712	PASS
95	95	100	100	100.0	41368	PASS
96	95	5	9	6.7	2784	PASS
173	174	0.00	2	0.4	154	PASS
174	95	50	120	82.8	34243	PASS
175	174	5	9	8.2	2798	PASS
176	174	95	105	97.2	33291	PASS
177	176	5	10	7.3	2421	PASS

m/z	Abundance
39.70	181.0
43.60	223.0
44.10	166.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
35.90	413.0
36.90	1673.0
37.90	1709.0
38.90	721.0
40.20	165.0
43.90	467.0
44.90	271.0
45.90	145.0
47.00	472.0
47.80	299.0
48.90	1641.0
50.00	7154.0
51.00	2041.0
52.00	170.0
55.10	178.0
55.90	571.0
56.90	1027.0
59.90	363.0
60.90	1710.0
62.00	1990.0
62.90	1646.0
63.90	383.0
64.90	466.0
66.80	132.0
67.90	4125.0
69.00	4004.0
69.90	294.0
71.80	281.0
72.90	1633.0
73.90	6837.0
75.00	20352.0
75.90	1808.0
76.90	257.0
78.10	219.0
78.90	1464.0
79.80	341.0
80.90	1752.0
81.90	252.0
85.90	107.0
86.90	1721.0
87.90	1637.0
91.00	105.0
91.90	1027.0
92.90	1340.0
93.90	4957.0
94.90	40760.0
95.90	2792.0
103.80	198.0
105.90	208.0
115.80	167.0
116.70	333.0
117.80	168.0
118.80	284.0
123.80	102.0
127.80	209.0
129.80	212.0
140.80	421.0
142.90	677.0
144.80	255.0
148.00	172.0
154.70	167.0
170.90	120.0
171.70	295.0
172.10	227.0
173.00	462.0
173.90	33048.0
174.90	2642.0
175.90	31392.0
176.90	2157.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
35.90	431.0
36.90	1666.0
37.90	1842.0
38.90	856.0
39.80	158.0
40.10	177.0
43.90	458.0
45.00	304.0
47.00	480.0
47.80	341.0
48.90	1552.0
50.00	7472.0
50.90	2342.0
52.00	201.0
52.90	102.0
55.10	194.0
55.90	564.0
56.90	1123.0
60.10	399.0
60.90	1768.0
62.00	2081.0
62.90	1827.0
63.90	400.0
64.90	446.0
66.80	123.0
67.90	4043.0
69.00	4351.0
70.00	313.0
71.80	299.0
72.90	1643.0
73.90	6898.0
75.00	21296.0
75.90	1922.0
76.80	250.0
77.40	130.0
78.90	1610.0
79.80	333.0
80.90	1888.0
81.80	275.0
85.90	123.0
86.90	1740.0
87.90	1806.0
90.60	120.0
91.00	142.0
91.90	1177.0
92.90	1530.0
93.90	5642.0
94.90	43072.0
95.90	2918.0
103.80	228.0
105.90	237.0
115.80	141.0
116.70	333.0
117.80	143.0
118.80	272.0
127.80	206.0
129.70	277.0
140.80	449.0
142.90	816.0
144.80	260.0
147.90	177.0
154.90	165.0
156.80	103.0
171.70	390.0
173.90	35304.0
174.90	2915.0
175.90	34616.0
176.90	2545.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382

m/z	Abundance
35.90	391.0
36.90	1565.0
37.90	1775.0
38.90	880.0
40.00	202.0
43.90	441.0
44.90	280.0
47.00	459.0
47.80	321.0
48.90	1394.0
50.00	7279.0
50.90	2350.0
52.10	193.0
52.80	135.0
53.80	125.0
55.10	142.0
55.80	515.0
56.90	1137.0
60.10	421.0
60.90	1655.0
62.00	1934.0
62.90	1890.0
63.90	406.0
64.90	453.0
66.80	125.0
67.90	3795.0
69.00	4218.0
69.90	294.0
71.90	264.0
72.90	1601.0
73.90	6458.0
75.00	20488.0
75.90	1789.0
76.80	221.0
78.90	1673.0
79.80	346.0
80.80	1737.0
81.80	272.0
86.80	1640.0
87.90	1742.0
90.90	152.0
91.90	1224.0
92.90	1640.0
93.90	5671.0
94.90	40272.0
95.90	2643.0
103.80	211.0
105.90	210.0
106.90	106.0
116.80	298.0
117.80	125.0
118.80	254.0
127.80	172.0
129.70	256.0
140.80	468.0
142.90	736.0
144.80	261.0
147.80	187.0
154.90	176.0
170.70	123.0
171.70	457.0
173.90	34376.0
174.90	2838.0
175.90	33864.0
176.90	2561.0

Instrument :
MSVOA_V
ClientSampleId :
BFB382