

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011326.D
 Acq On : 08 Jun 2019 18:53
 Operator : SY/MD
 Sample : K3276-03
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E1

Quant Time: Jun 09 00:26:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	148057	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	133919	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	50497	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.31	65	45150	4.02	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	80.40%
7) Chloroethane-d5	1.57	69	37613	4.03	ug/L	0.02
Spiked Amount	5.000	Range	65 - 130	Recovery	=	80.60%
11) 1,1-Dichloroethene-d2	2.12	63	75917	3.39	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	67.80%
20) 2-Butanone-d5	3.95	46	120216	47.60	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	95.20%
24) Chloroform-d	4.40	84	89808	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.08	65	50925	4.77	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.40%
32) Benzene-d6	5.09	84	183271	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
36) 1,2-Dichloropropane-d6	6.12	67	56331	4.56	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	91.20%
41) Toluene-d8	7.36	98	159307	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
43) trans-1,3-Dichloropropene-	7.67	79	17014	3.62	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	72.40%
46) 2-Hexanone-d5	8.14	63	91114	45.85	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.70%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	36237	4.31	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	86.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	48901	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Ovalue
13) Acetone	2.21	43	12893	7.613 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011326.D
Acq On : 08 Jun 2019 18:53
Operator : SY/MD
Sample : K3276-03
Misc : 25ML/MSVOA V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E1

Quant Time: Jun 09 00:26:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

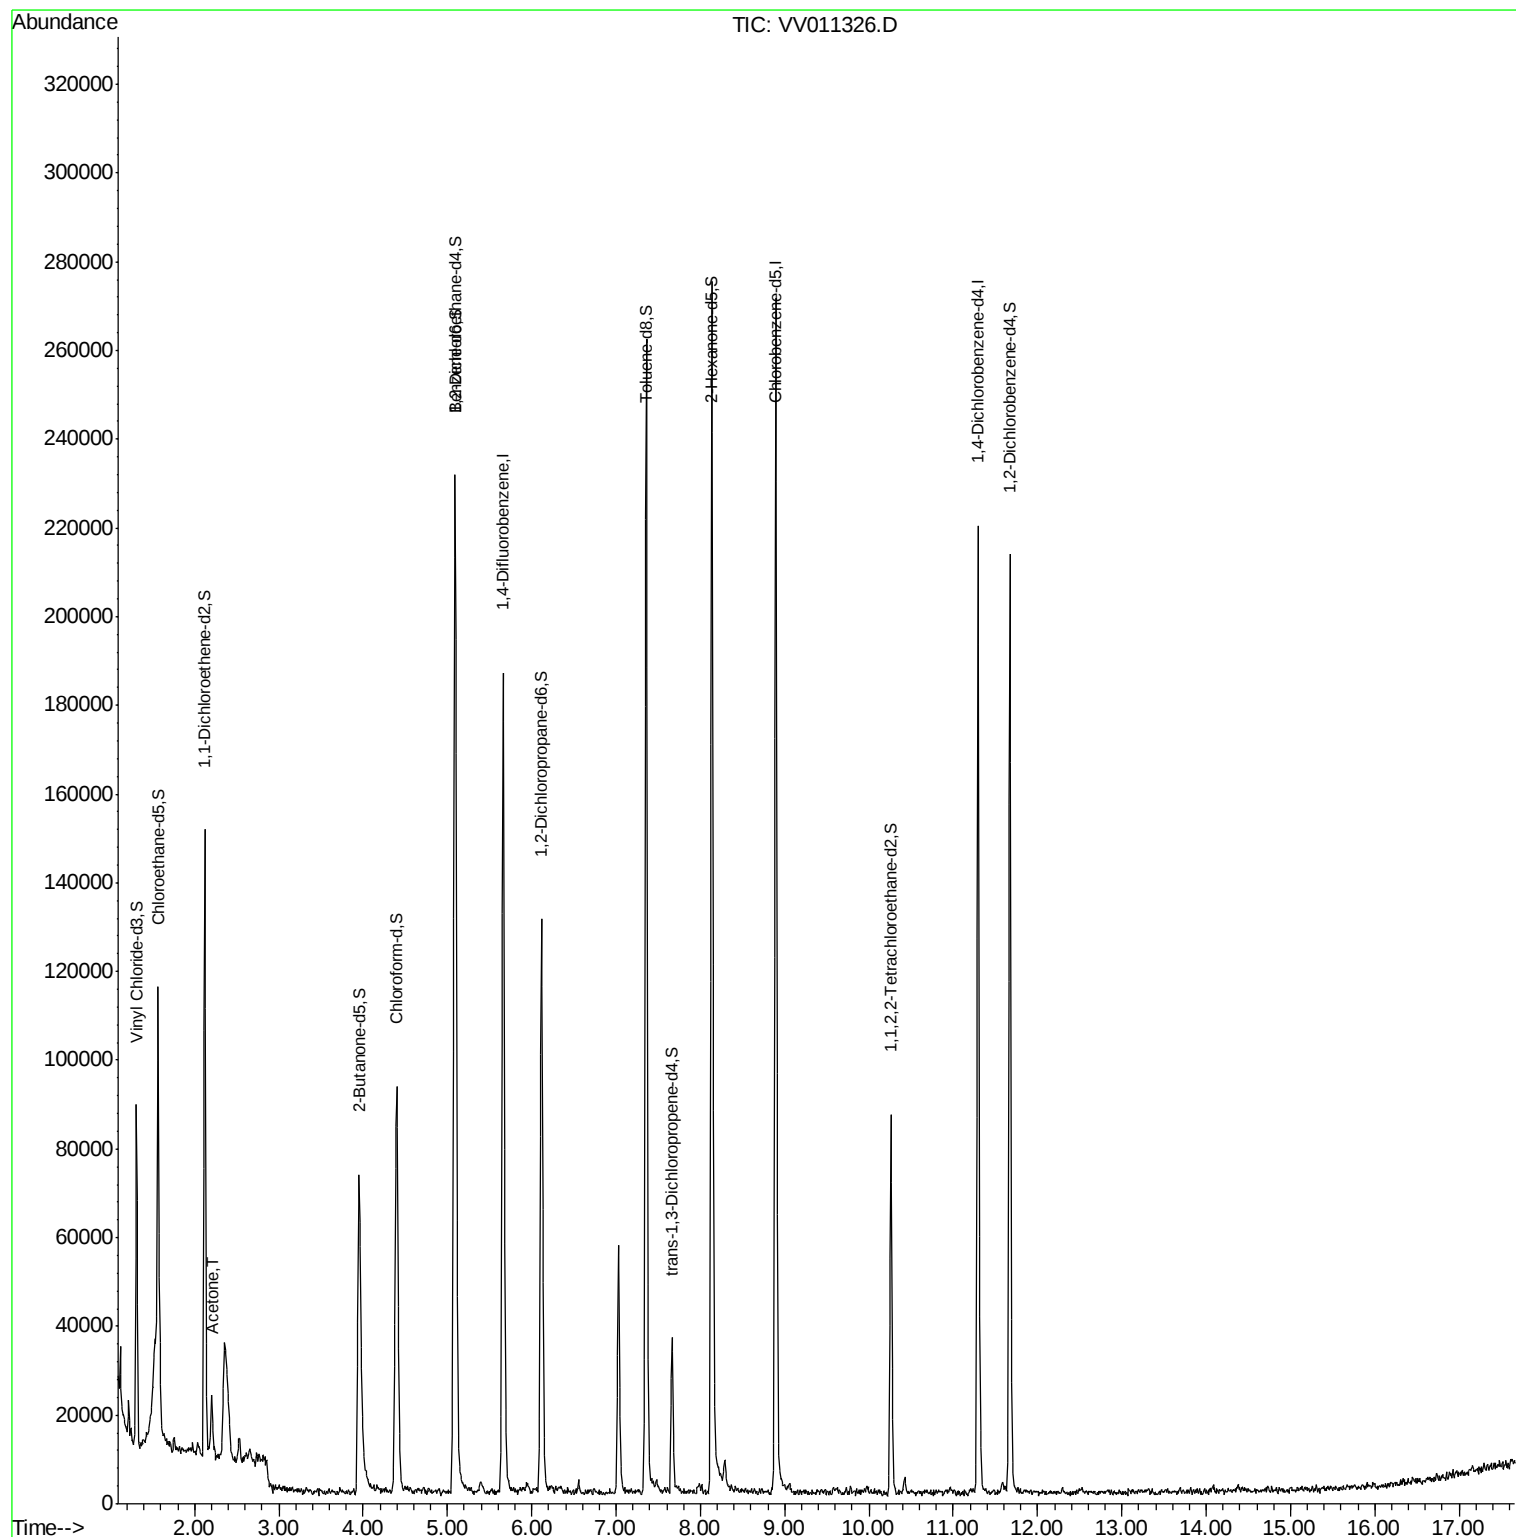

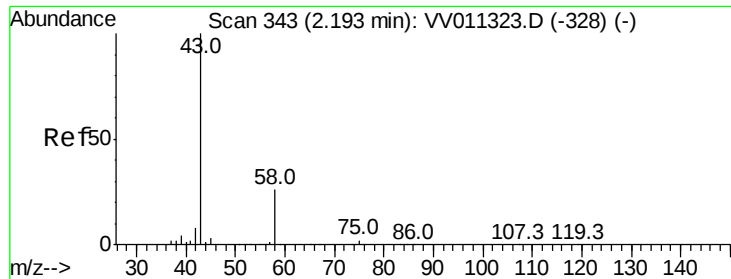

#13

Acetone

Concen: 7.613 ug/L

RT: 2.21 min Scan# 347

Delta R.T. 0.01 min

Lab File: VV011326.D

Acq: 08 Jun 2019 18:53

Instrument :

MSVOA_V

ClientSampleId :

DB8E1

Tot Ion: 43 Resp: 12893

Ion Ratio Lower Upper

43 100

58 28.8 0.0 55.2

