

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011327.D
 Acq On : 08 Jun 2019 19:21
 Operator : SY/MD
 Sample : K3276-04
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E2

Quant Time: Jun 09 00:33:42 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	136966	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	128027	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	49407	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	46328	4.46	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	89.20%
7) Chloroethane-d5	1.55	69	37759	4.38	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.60%
11) 1,1-Dichloroethene-d2	2.12	63	75699	3.65	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	73.00%
20) 2-Butanone-d5	3.94	46	121958	52.20	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	104.40%
24) Chloroform-d	4.40	84	88431	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
26) 1,2-Dichloroethane-d4	5.08	65	50622	5.13	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	102.60%
32) Benzene-d6	5.09	84	183593	4.79	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.80%
36) 1,2-Dichloropropane-d6	6.11	67	56427	4.78	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.60%
41) Toluene-d8	7.36	98	163616	4.65	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.00%
43) trans-1,3-Dichloropropene-	7.66	79	16687	3.71	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	74.20%
46) 2-Hexanone-d5	8.13	63	94419	49.70	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	99.40%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	38002	4.72	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	94.40%
64) 1,2-Dichlorobenzene-d4	11.67	152	51705	5.30	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	106.00%


Target Compounds					Ovalue
13) Acetone	2.19	43	9425	6.016 ug/L	84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011327.D
Acq On : 08 Jun 2019 19:21
Operator : SY/MD
Sample : K3276-04
Misc : 25ML/MSVOA V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E2

Quant Time: Jun 09 00:33:42 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

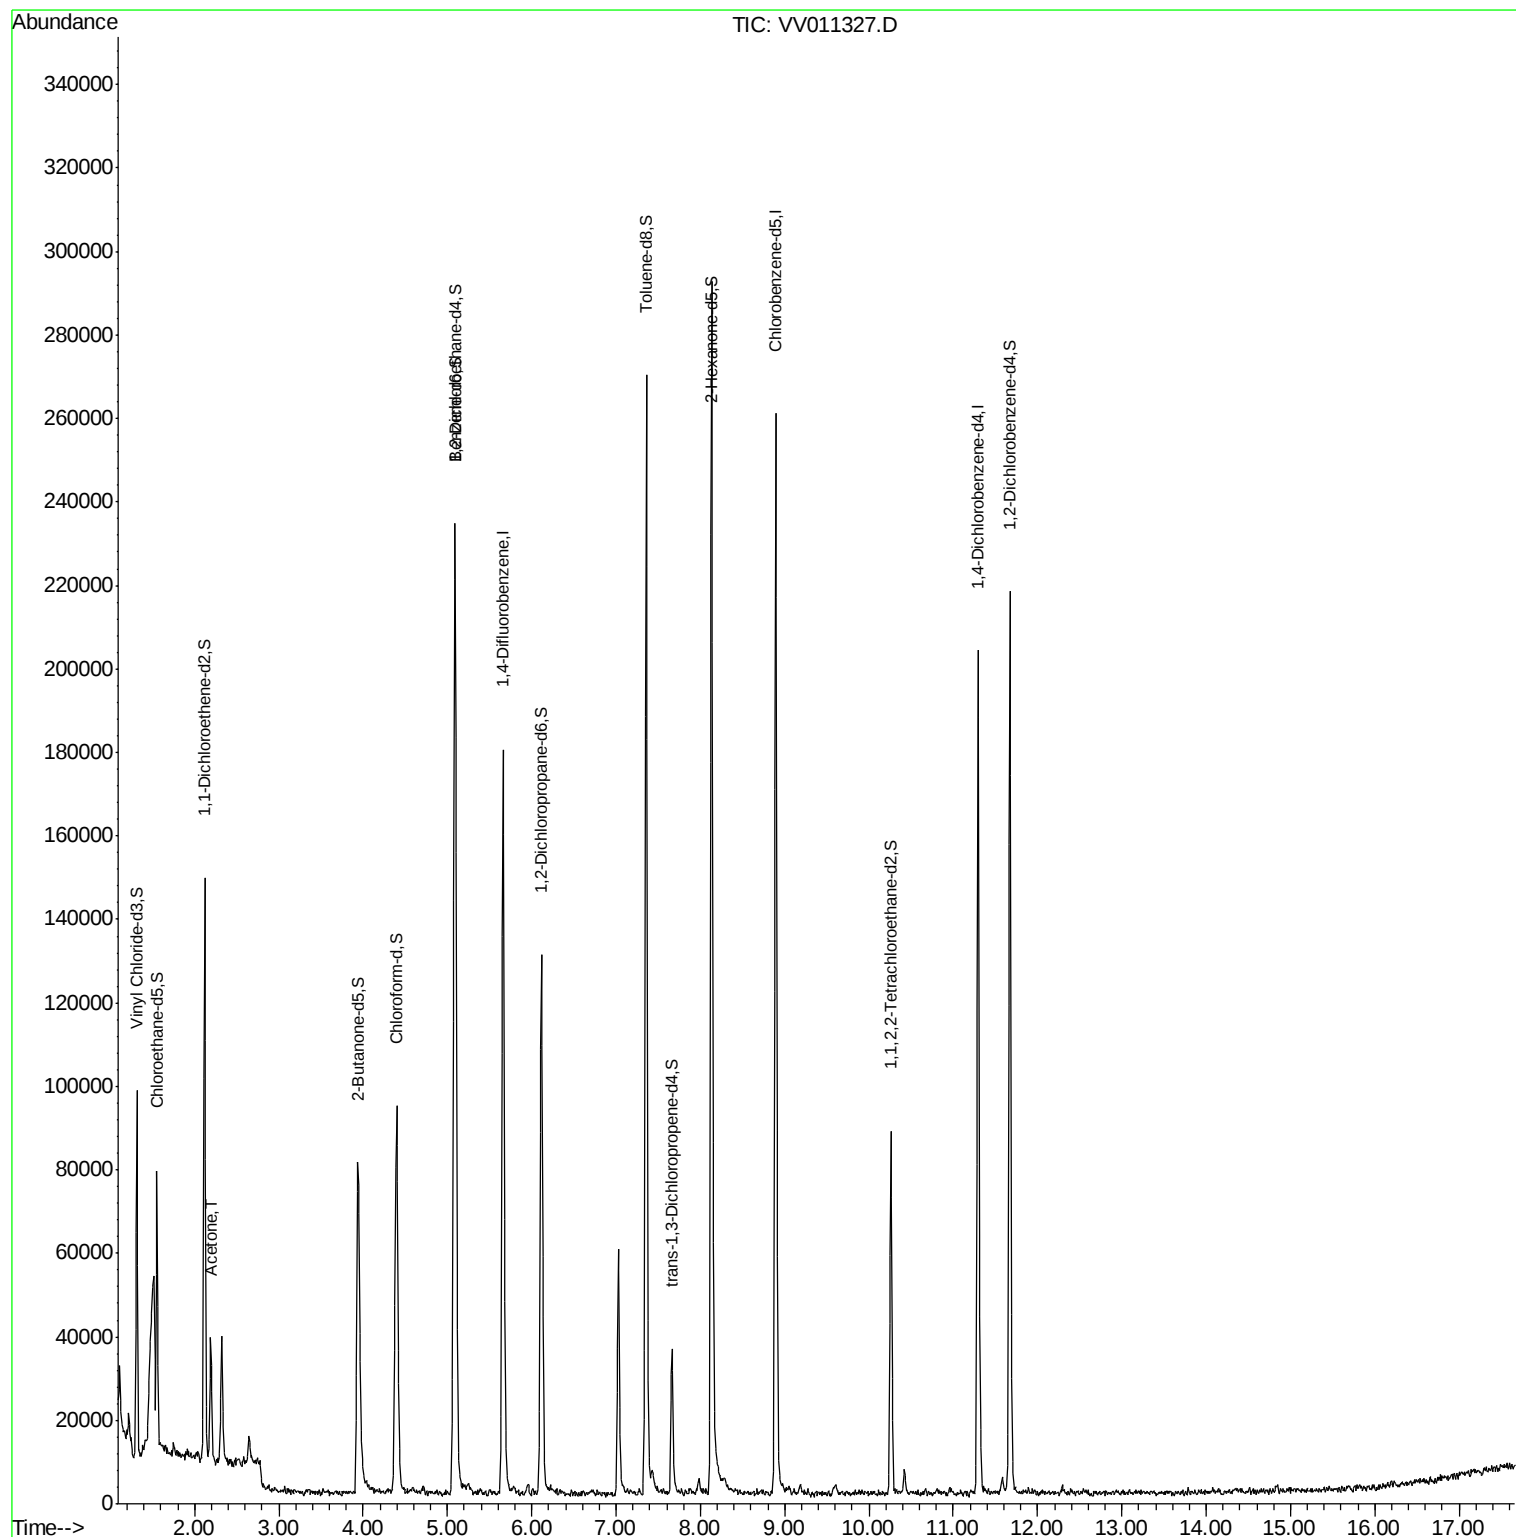

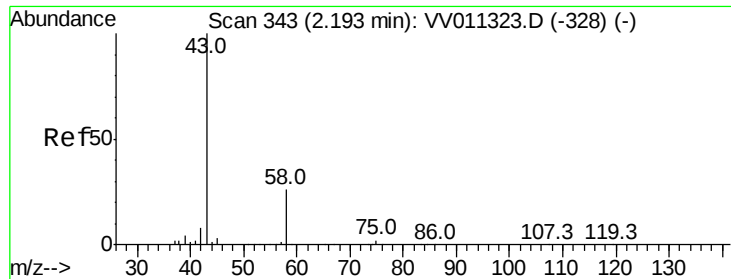

#13

Acetone

Concen: 6.016 ug/L

RT: 2.19 min Scan# 343

Delta R.T. -0.00 min

Lab File: VV011327.D

Acq: 08 Jun 2019 19:21

Instrument :
MSVOA_V
ClientSampleId :
DB8E2

Tot Ion: 43 Resp: 9425

Ion Ratio Lower Upper

43 100

58 35.9 0.0 55.2

