

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV060819\
 Data File : VV011331.D
 Acq On : 08 Jun 2019 21:13
 Operator : SY/MD
 Sample : K3276-09
 Misc : 25ML/MSVOA V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E5

Quant Time: Jun 09 00:41:28 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sun Jun 09 00:10:13 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.66	114	139852	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.89	117	129489	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.29	152	50489	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	44104	4.16	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	83.20%
7) Chloroethane-d5	1.55	69	37434	4.25	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	85.00%
11) 1,1-Dichloroethene-d2	2.12	63	72495	3.42	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.40%
20) 2-Butanone-d5	3.94	46	117717	49.34	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	98.68%
24) Chloroform-d	4.40	84	85903	4.61	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.20%
26) 1,2-Dichloroethane-d4	5.08	65	49446	4.90	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.00%
32) Benzene-d6	5.09	84	177656	4.59	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.80%
36) 1,2-Dichloropropane-d6	6.11	67	53123	4.45	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	89.00%
41) Toluene-d8	7.36	98	155703	4.38	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	87.60%
43) trans-1,3-Dichloropropene-	7.66	79	15660	3.44	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	68.80%
46) 2-Hexanone-d5	8.13	63	89905	46.79	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.58%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	35778	4.40	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	88.00%
64) 1,2-Dichlorobenzene-d4	11.67	152	49361	4.95	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	99.00%


Target Compounds				Ovalue
13) Acetone	2.19	43	10993	6.872 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV060819\
Data File : VV011331.D
Acq On : 08 Jun 2019 21:13
Operator : SY/MD
Sample : K3276-09
Misc : 25ML/MSVOA V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
DB8E5

Quant Time: Jun 09 00:41:28 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR060419WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sun Jun 09 00:10:13 2019
Response via : Initial Calibration

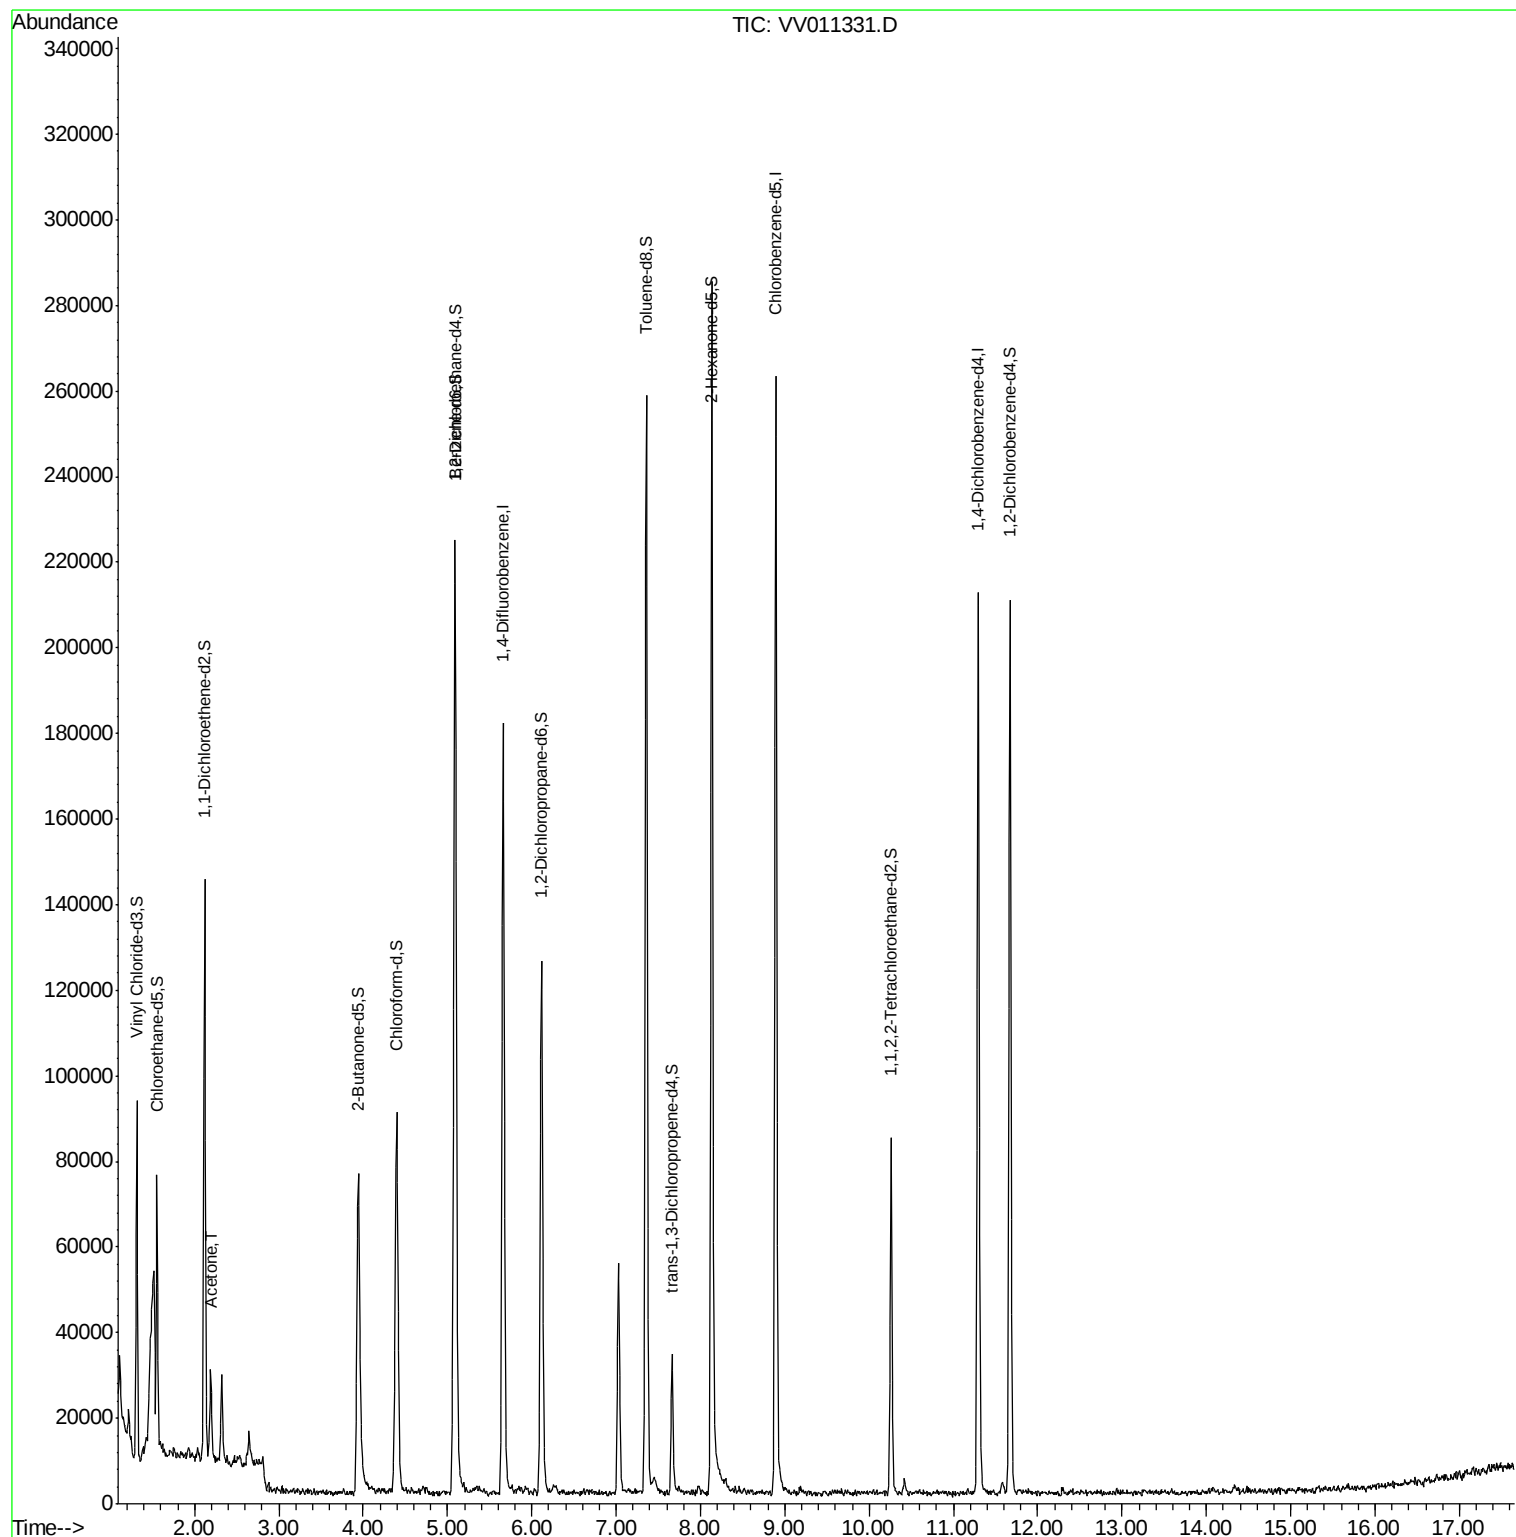

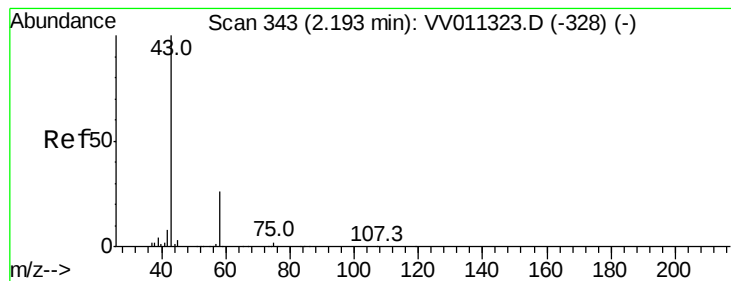

#13
 Acetone
 Concen: 6.872 ug/L
 RT: 2.19 min Scan# 343
 Delta R.T. -0.00 min
 Lab File: VV011331.D
 Acq: 08 Jun 2019 21:13

Instrument :
 MSVOA_V
 ClientSampleId :
 DB8E5

Tot Ion: 43 Resp: 10993
 Ion Ratio Lower Upper
 43 100
 58 25.8 0.0 55.2

